

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
 Data File : PL080250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 22:32
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 00:58:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 00:48:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.690	148.8E6	205.1E6	72.644	72.801
28)	SA Decachlor...	8.786	7.840	107.9E6	162.1E6	72.528	72.670
Target Compounds							
23)	Chlordane-1	4.499	3.688	57693223	60075688	725.525	726.817
24)	Chlordane-2	5.025	4.266	62871711	75646013	729.477	726.916
25)	Chlordane-3	5.730	4.896	245.6E6	216.5E6	732.637	728.830
26)	Chlordane-4	5.812	4.958	302.3E6	214.6E6	738.777	725.592
27)	Chlordane-5	6.653	5.626	50488173	55672884	723.829	724.488



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 22:32
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 00:58:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 00:48:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

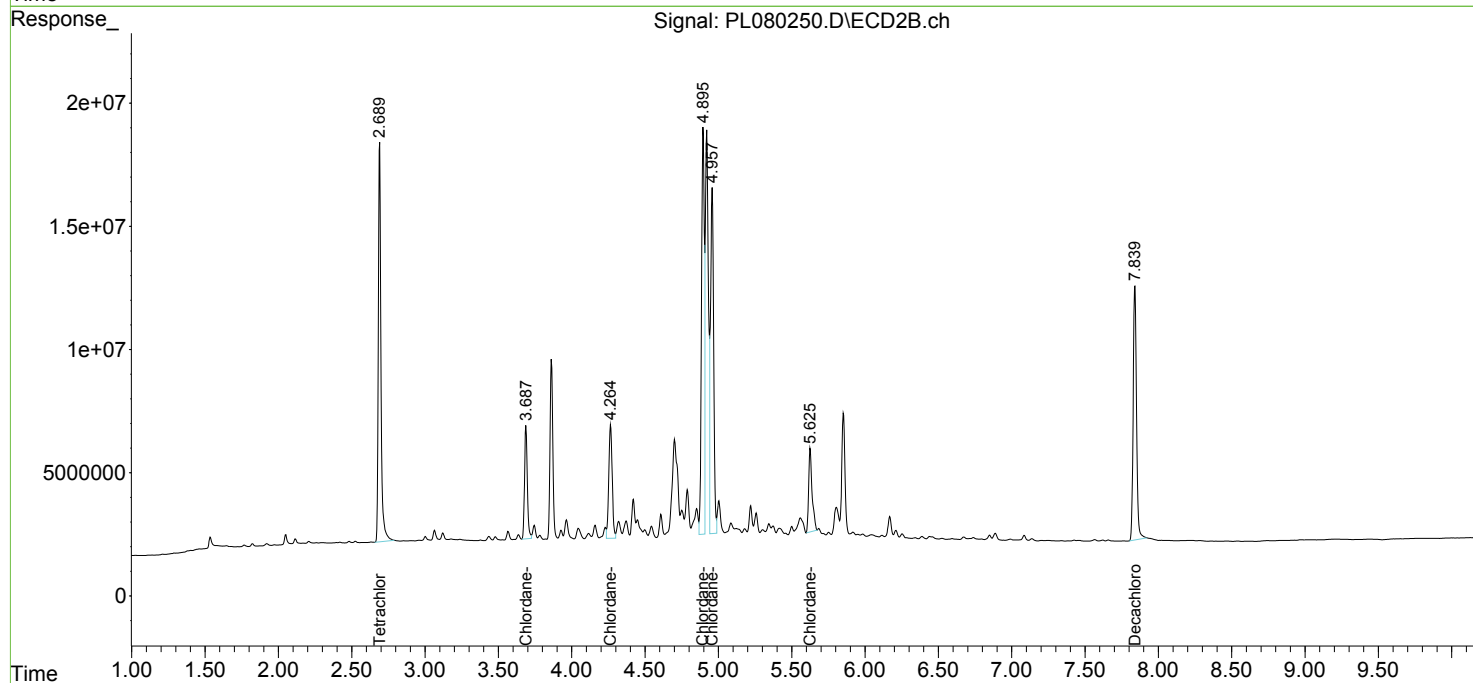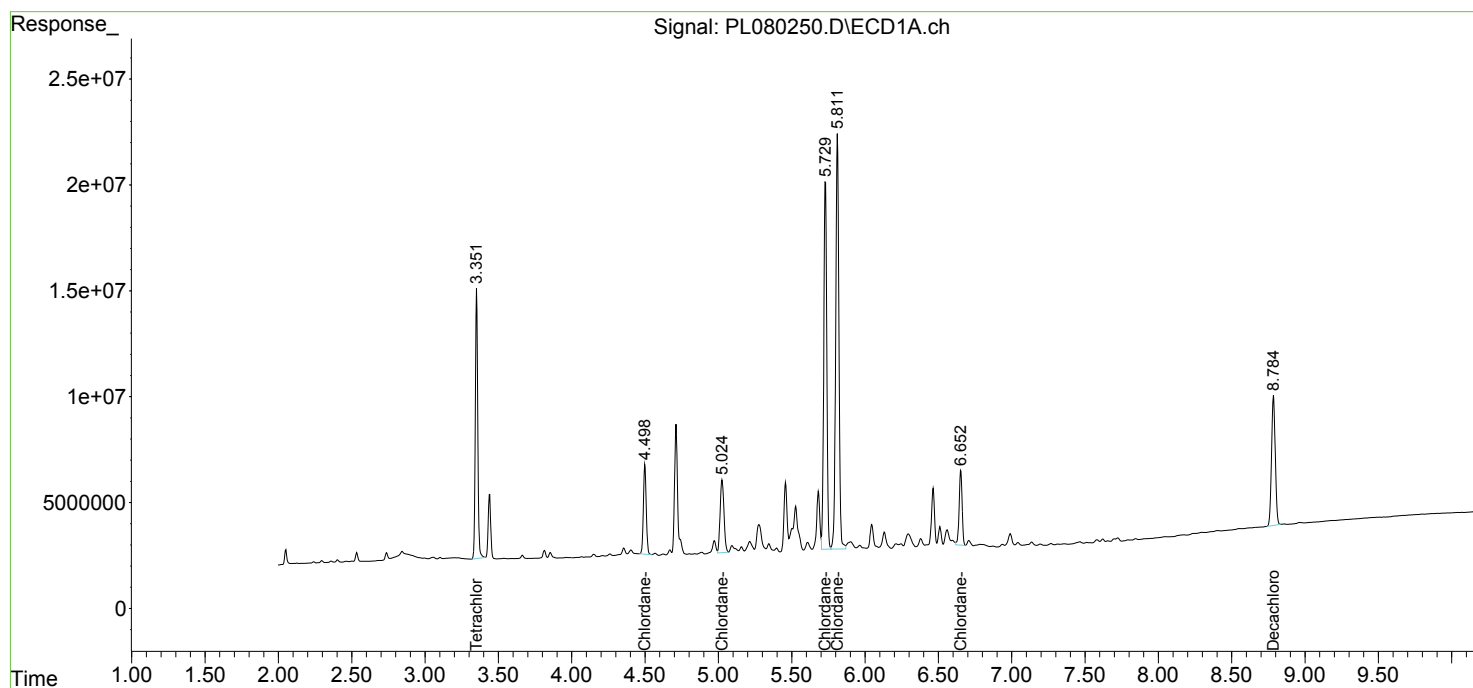


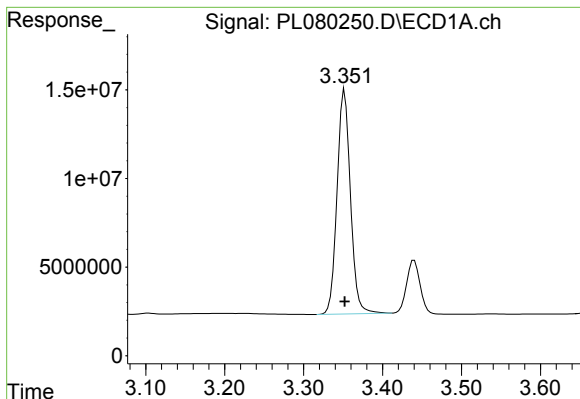

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 148839043
Conc: 72.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

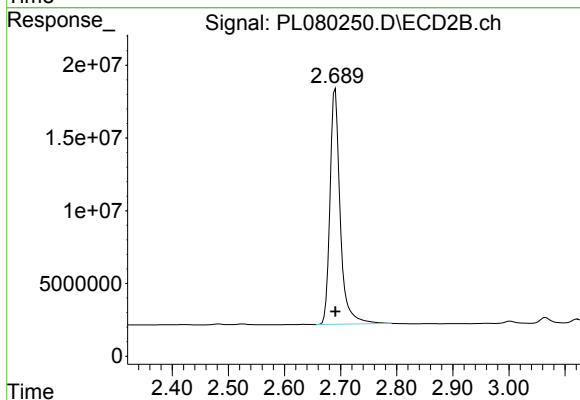


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: 0.000 min
Response: 205133793
Conc: 72.80 ng/ml

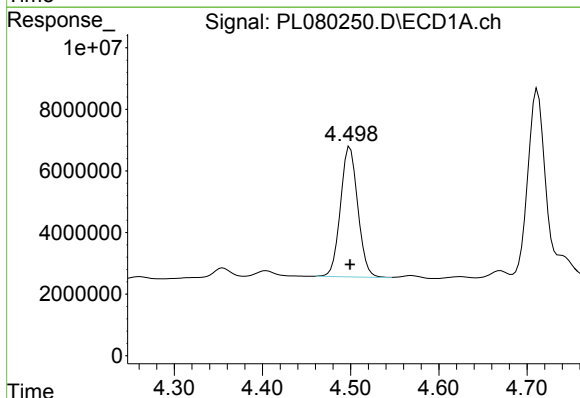


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 57693223
Conc: 725.53 ng/ml

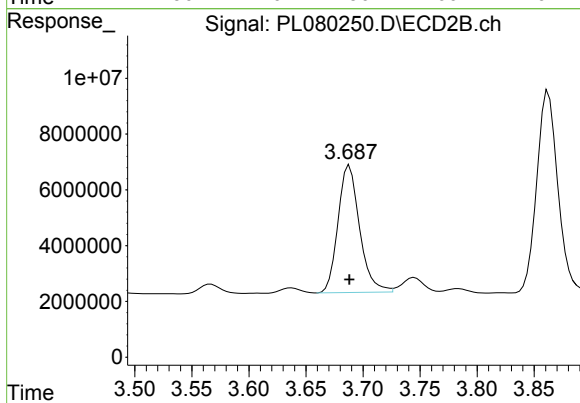

#23 Chlordane-1


R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 60075688
Conc: 726.82 ng/ml

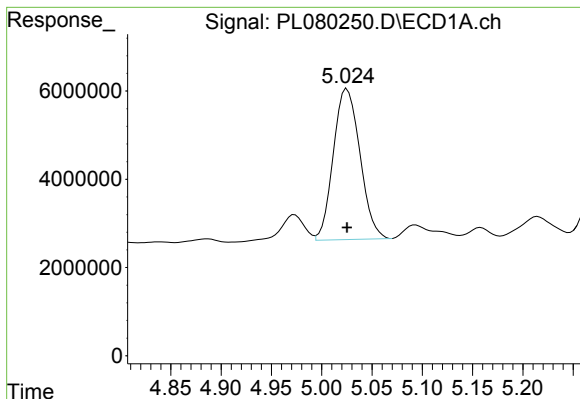

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 62871711
Conc: 729.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

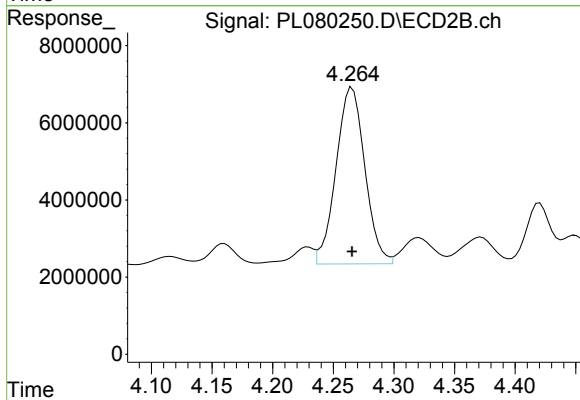


#24 Chlordane-2

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 75646013
Conc: 726.92 ng/ml

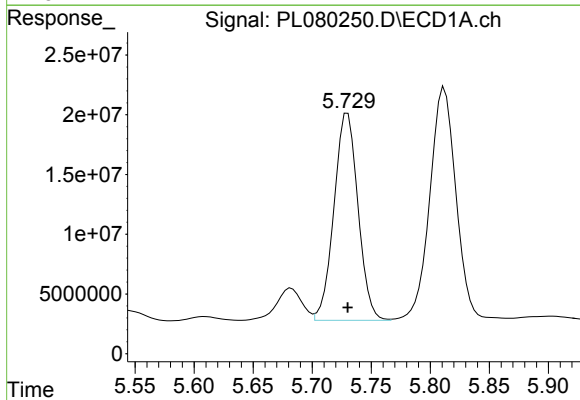


#25 Chlordane-3

R.T.: 5.730 min
Delta R.T.: 0.000 min
Response: 245553553
Conc: 732.64 ng/ml

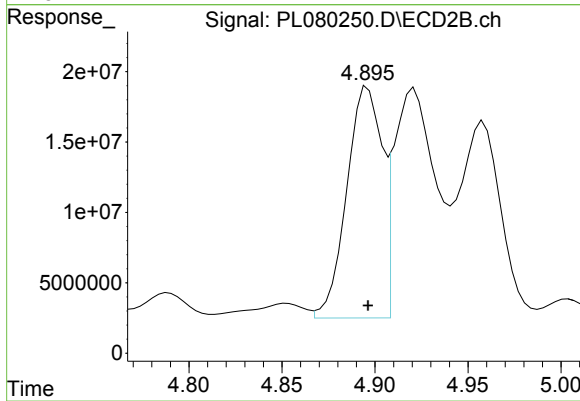

#25 Chlordane-3


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 216491547
Conc: 728.83 ng/ml

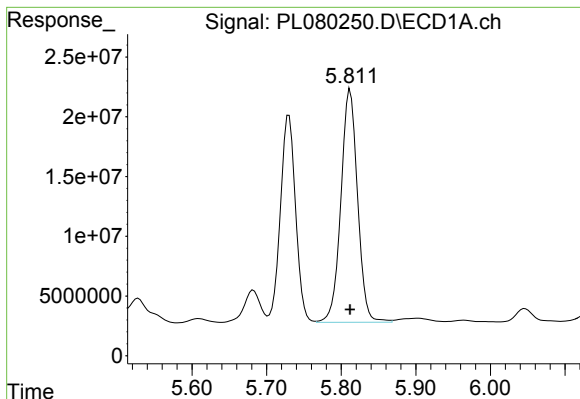

#26 Chlordane-4


R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 302270499
Conc: 738.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

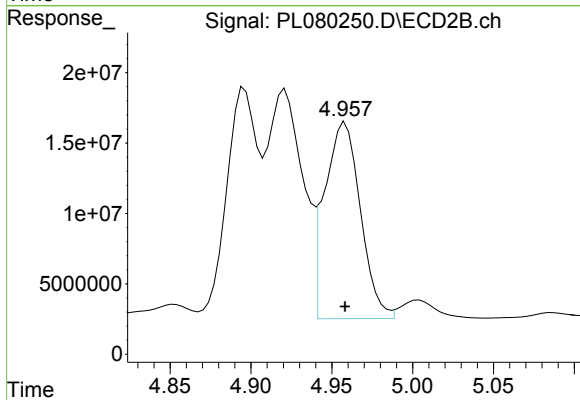


#26 Chlordane-4

R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 214615057
Conc: 725.59 ng/ml

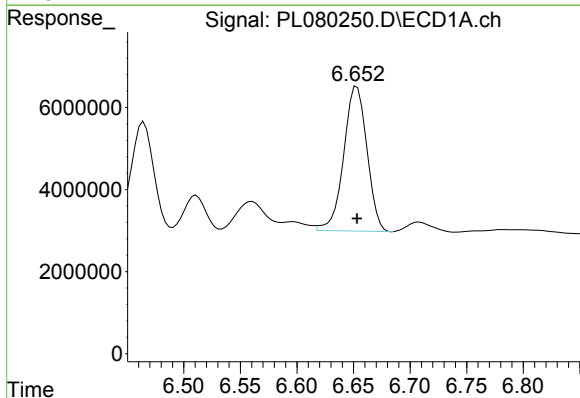


#27 Chlordane-5

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 50488173
Conc: 723.83 ng/ml

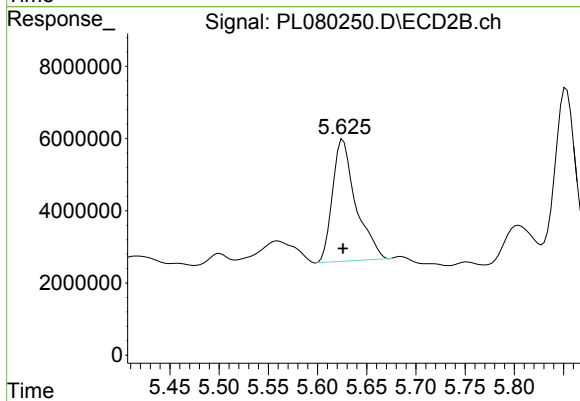

#27 Chlordane-5


R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 55672884
Conc: 724.49 ng/ml

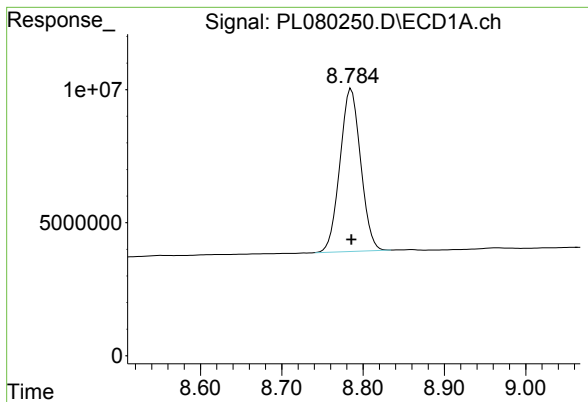

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 107896035
Conc: 72.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

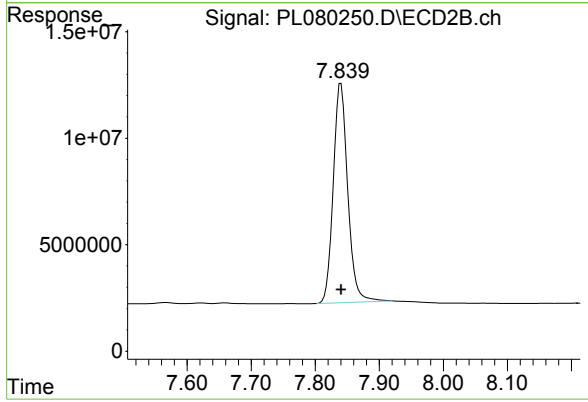

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 162079111
Conc: 72.67 ng/ml