

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
 Data File : PL080251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 22:45
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 00:52:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 00:48:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.690	102.8E6	140.4E6	50.000	50.000
28)	SA Decachlor...	8.786	7.840	76244977	115.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.499	3.688	40139954	41370756	500.000	500.000
24)	Chlordane-2	5.025	4.265	44221381	53451296	500.000	500.000
25)	Chlordane-3	5.730	4.896	166.0E6	146.4E6	500.000	500.000
26)	Chlordane-4	5.812	4.958	203.4E6	146.8E6	500.000	500.000
27)	Chlordane-5	6.654	5.626	35551923	38885025	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 22:45
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 00:52:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 00:48:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

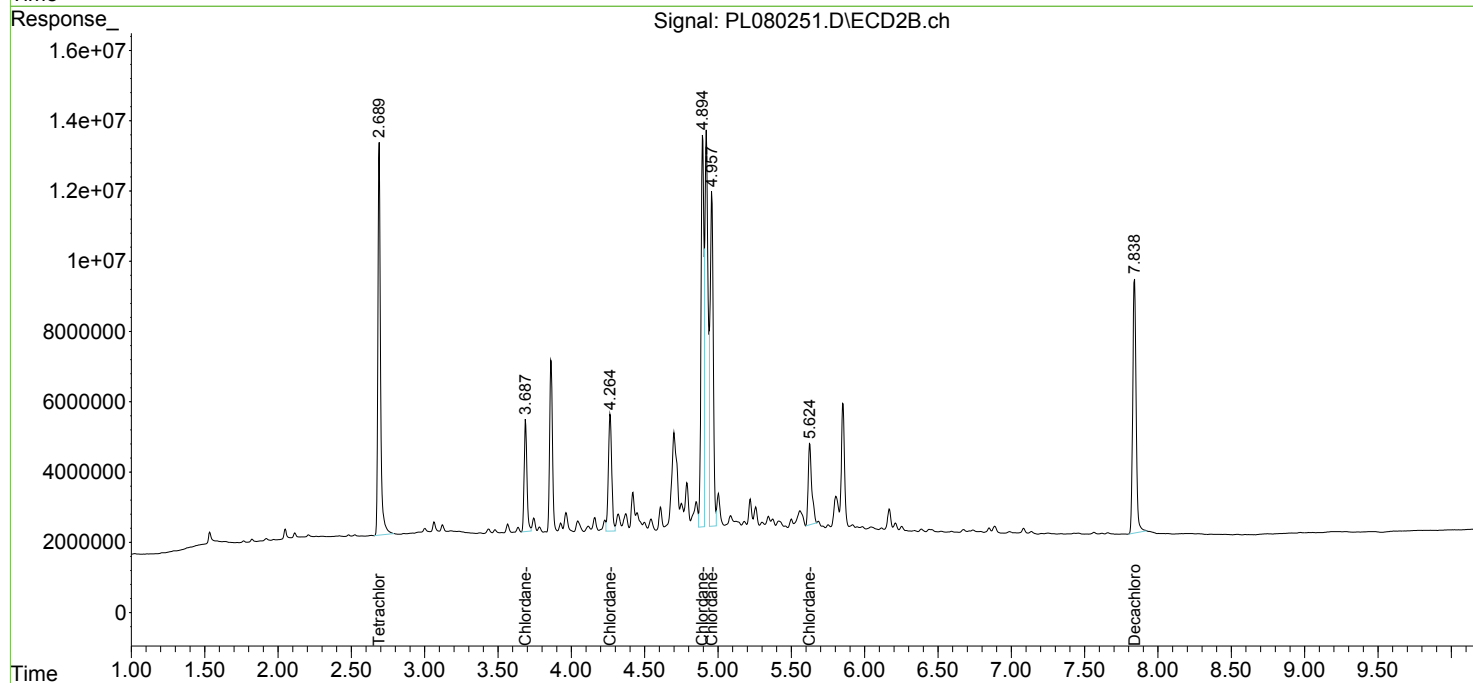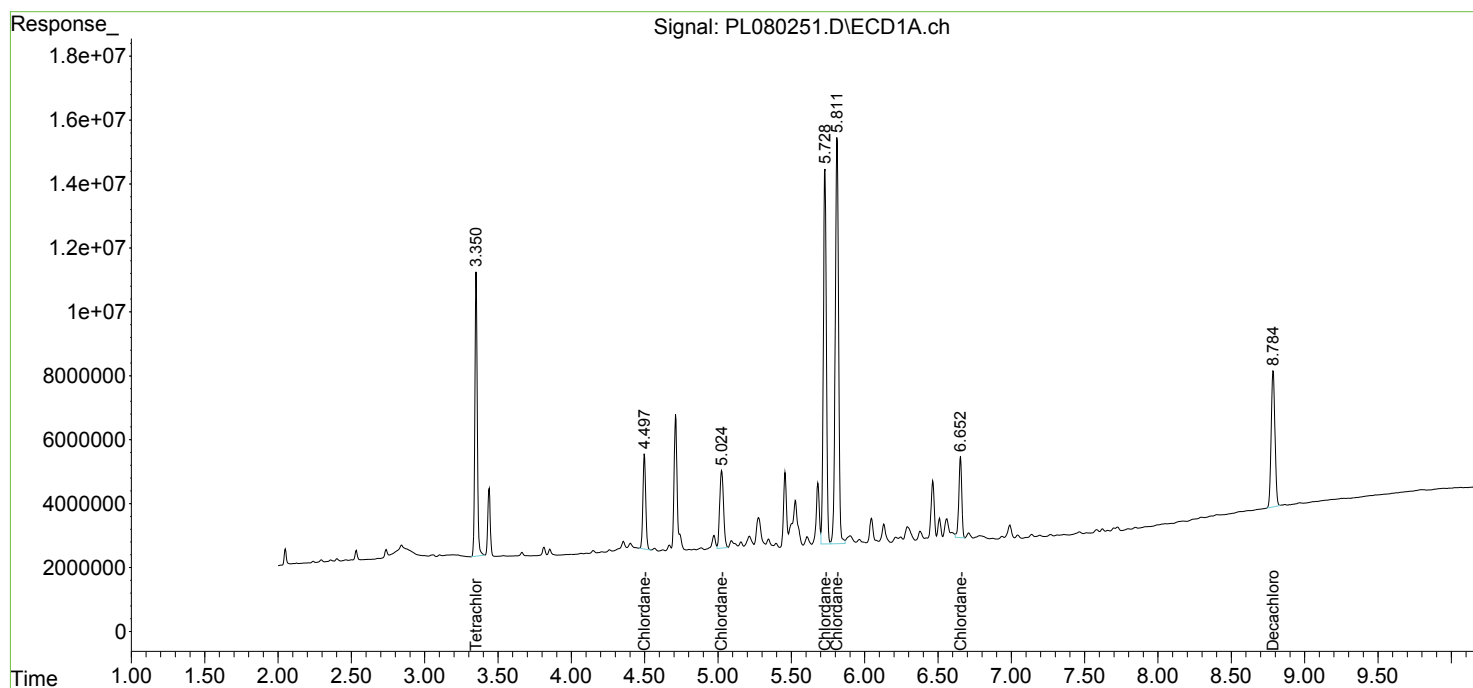


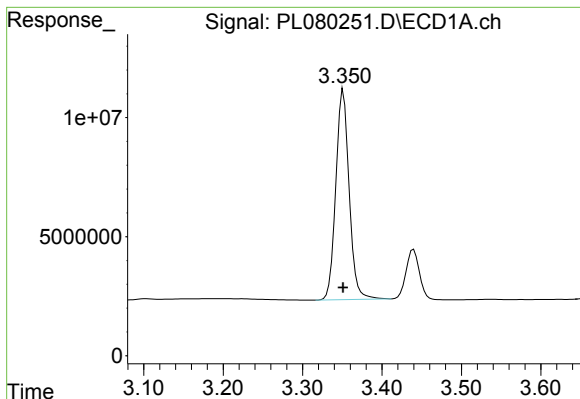

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 102801265
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

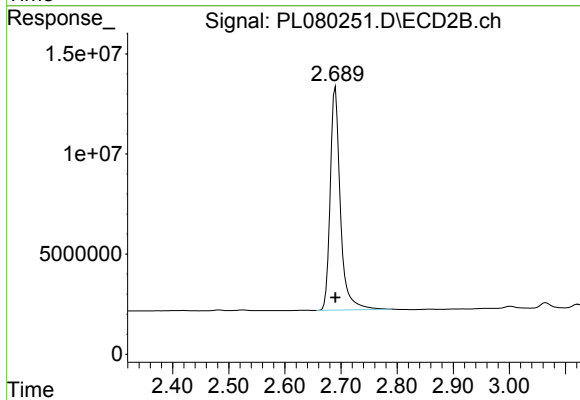


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: 0.000 min
Response: 140432654
Conc: 50.00 ng/ml

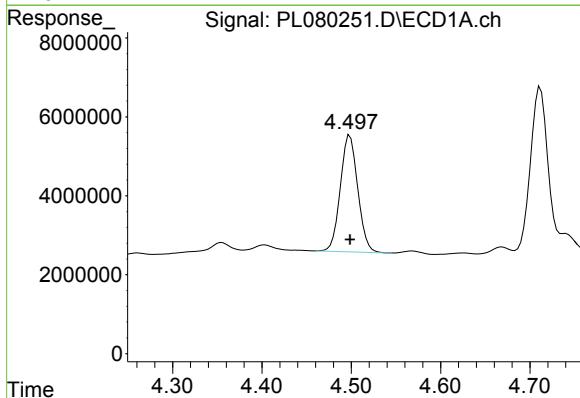


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 40139954
Conc: 500.00 ng/ml

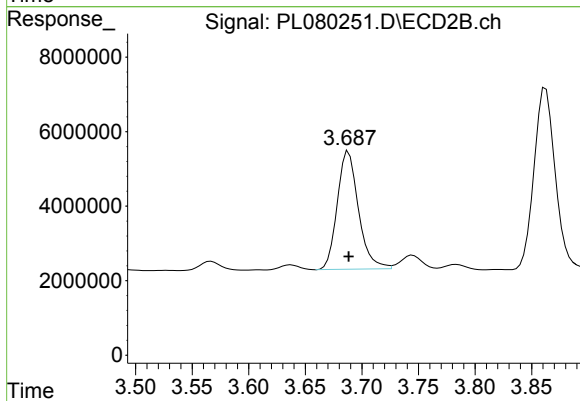

#23 Chlordane-1


R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 41370756
Conc: 500.00 ng/ml

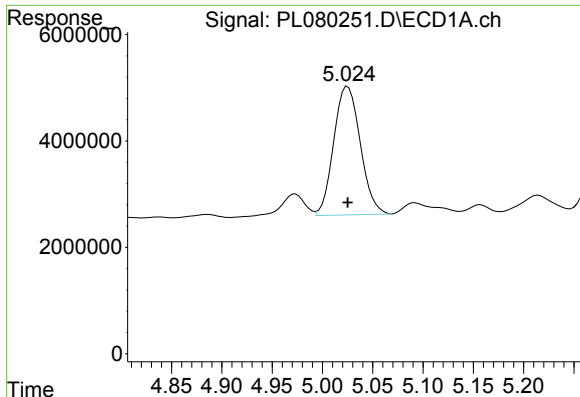

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 44221381
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

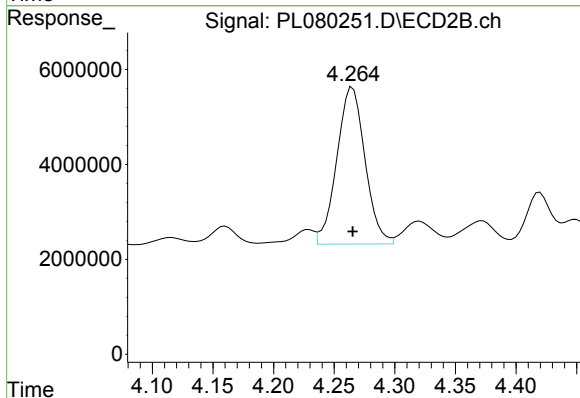


#24 Chlordane-2

R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 53451296
Conc: 500.00 ng/ml

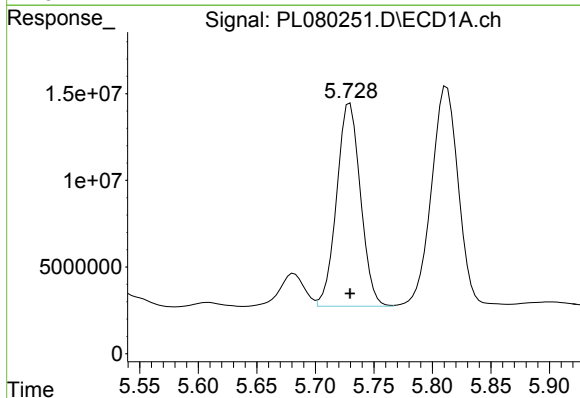


#25 Chlordane-3

R.T.: 5.730 min
Delta R.T.: 0.000 min
Response: 166023878
Conc: 500.00 ng/ml

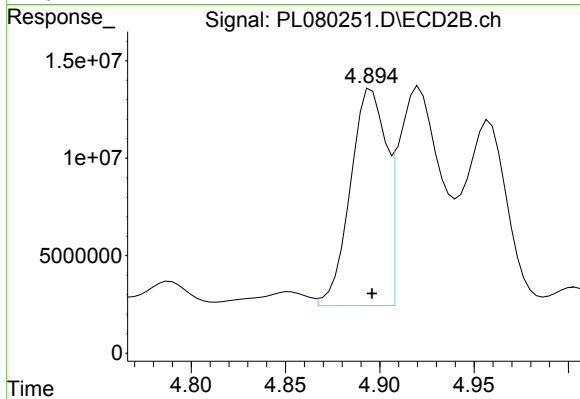

#25 Chlordane-3


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 146447152
Conc: 500.00 ng/ml

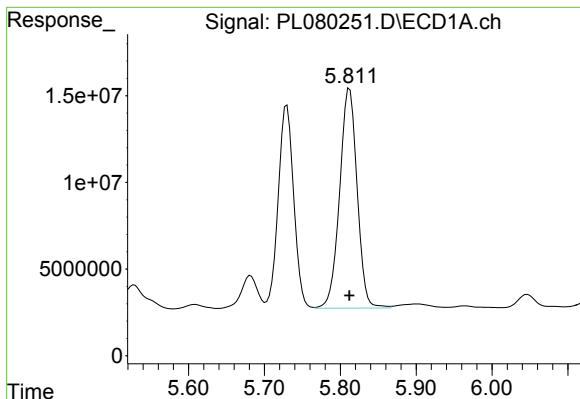

#26 Chlordane-4


R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 203397730
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

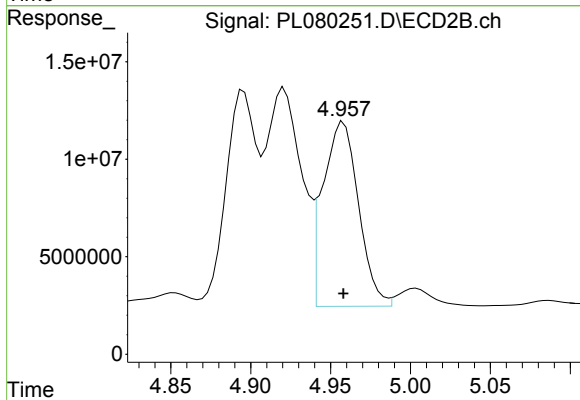


#26 Chlordane-4

R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 146751043
Conc: 500.00 ng/ml

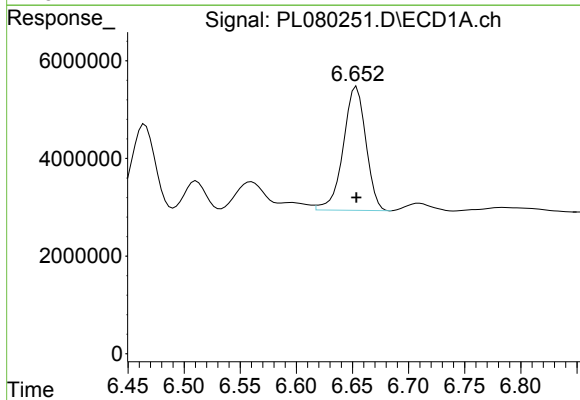


#27 Chlordane-5

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 35551923
Conc: 500.00 ng/ml

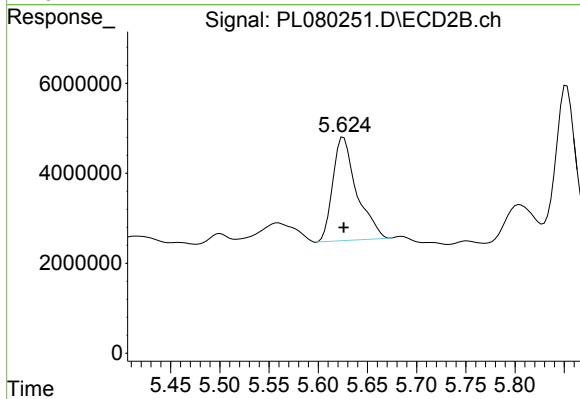

#27 Chlordane-5


R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 38885025
Conc: 500.00 ng/ml

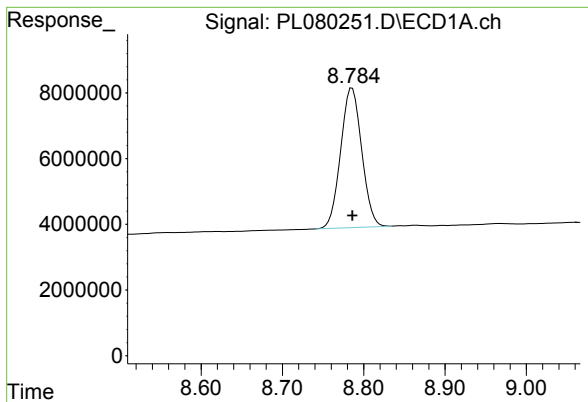

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 76244977
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

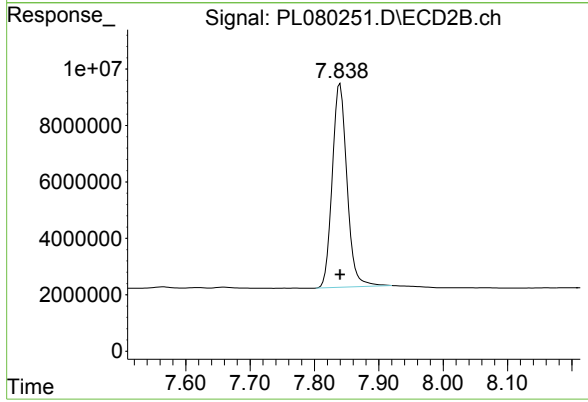

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 115029007
Conc: 50.00 ng/ml