

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
 Data File : PL080252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 22:59
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 01:00:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 00:48:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.690	50190567	67386018	24.620	24.177
28)	SA Decachlor...	8.787	7.841	38196440	59156428	25.504	26.125
Target Compounds							
23)	Chlordane-1	4.498	3.688	19187474	20089890	243.413	244.754
24)	Chlordane-2	5.025	4.265	22061999	26878038	254.456	256.161
25)	Chlordane-3	5.730	4.896	78405256	68132456	237.751	234.203
26)	Chlordane-4	5.812	4.958	97285413	68889665	240.718	236.959
27)	Chlordane-5	6.654	5.626	18327462	19159096	259.445	249.492



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 22:59
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 01:00:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 00:48:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

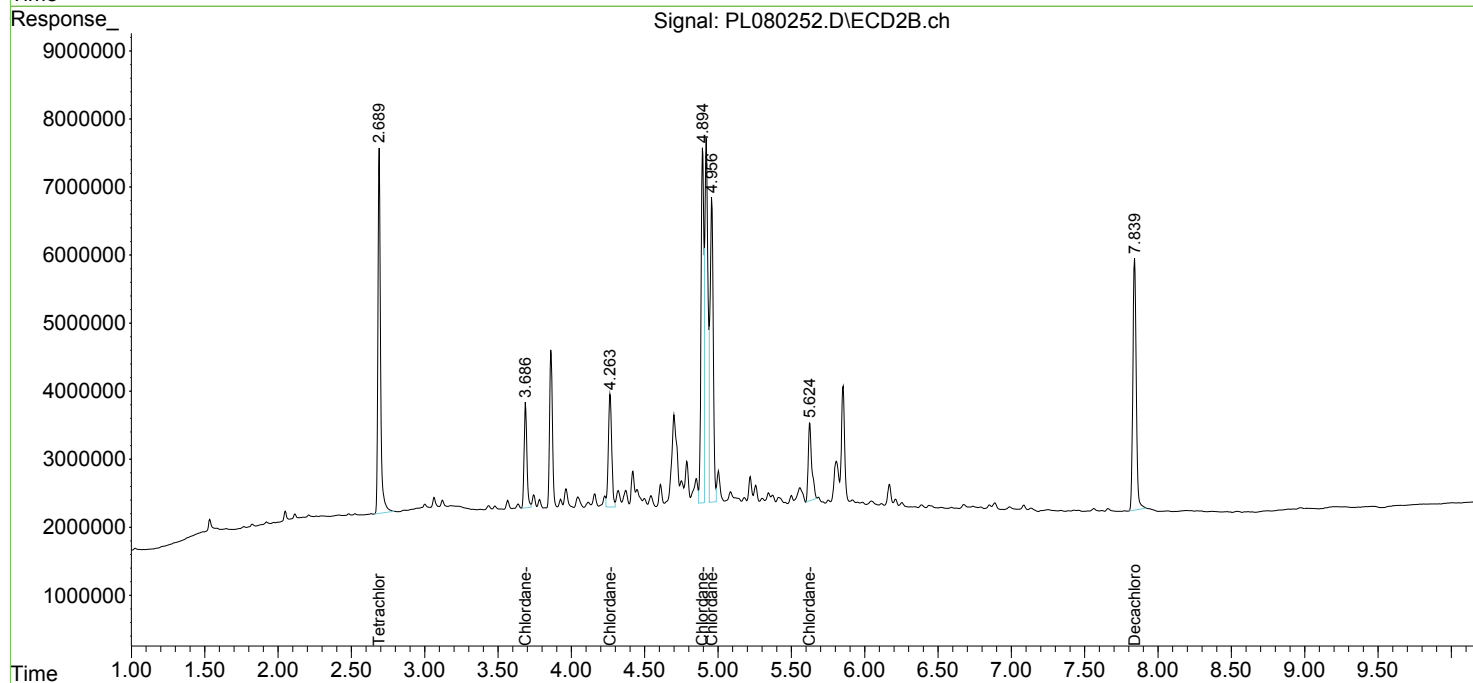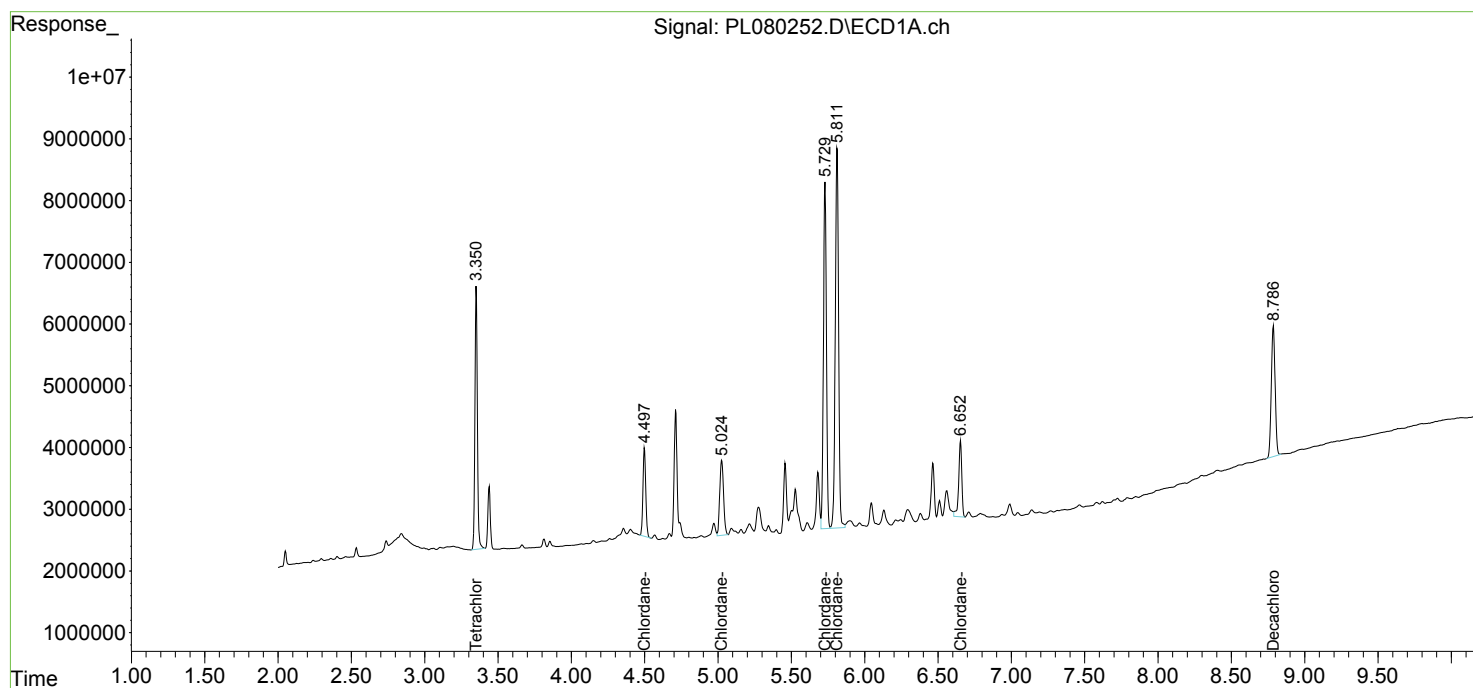


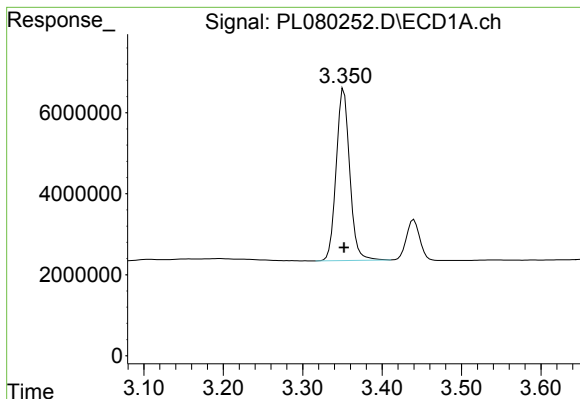

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 50190567
Conc: 24.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

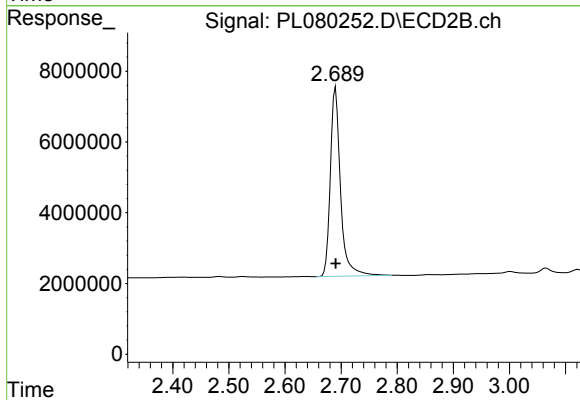


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: 0.000 min
Response: 67386018
Conc: 24.18 ng/ml

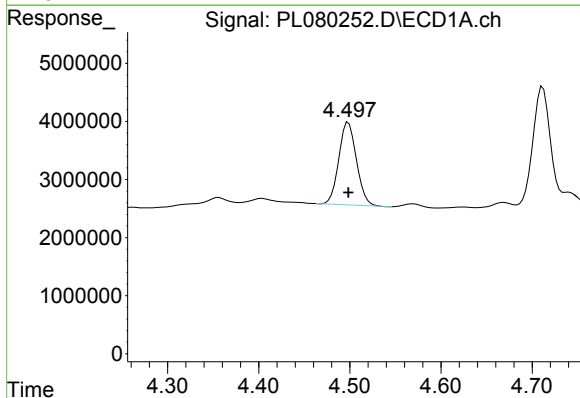


#23 Chlordane-1

R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 19187474
Conc: 243.41 ng/ml

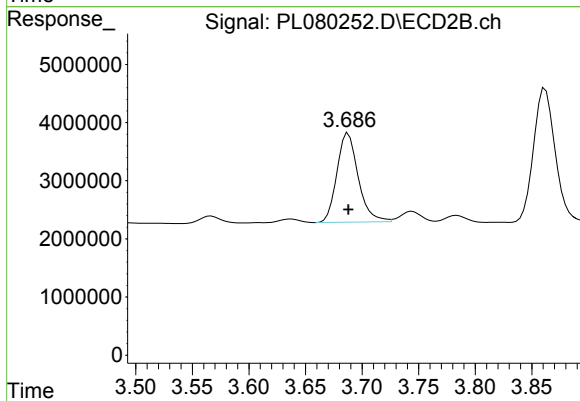

#23 Chlordane-1


R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 20089890
Conc: 244.75 ng/ml

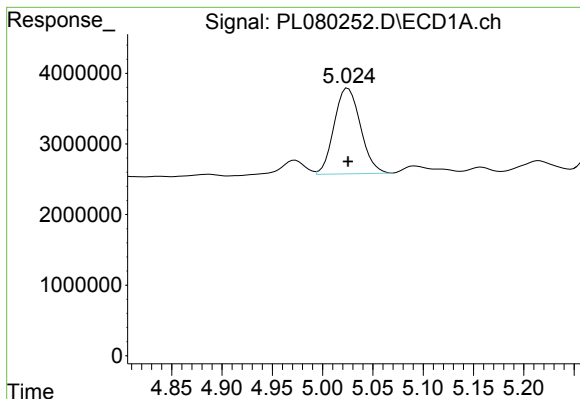

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 22061999
Conc: 254.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

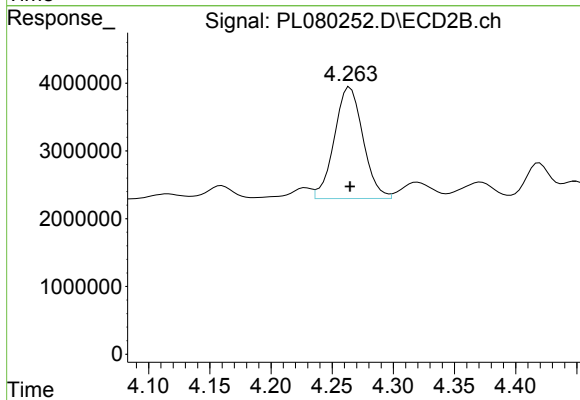


#24 Chlordane-2

R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 26878038
Conc: 256.16 ng/ml

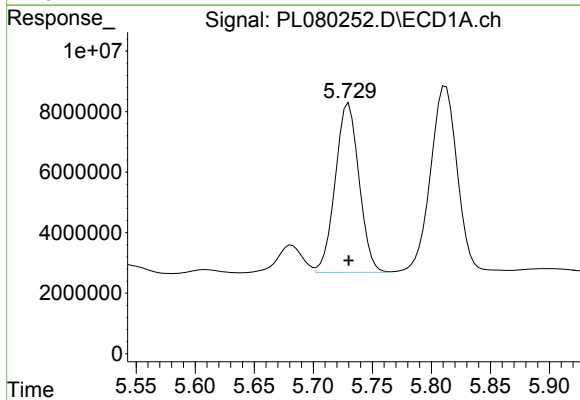


#25 Chlordane-3

R.T.: 5.730 min
Delta R.T.: 0.000 min
Response: 78405256
Conc: 237.75 ng/ml

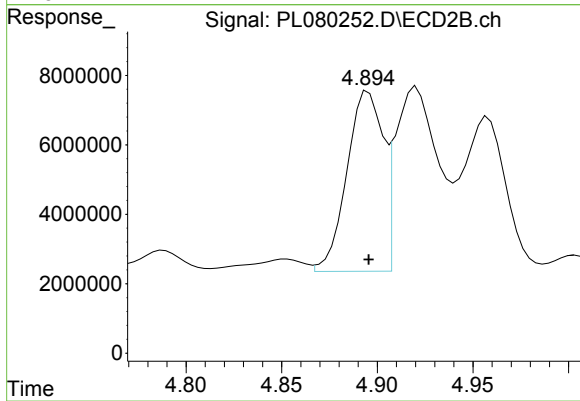

#25 Chlordane-3


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 68132456
Conc: 234.20 ng/ml

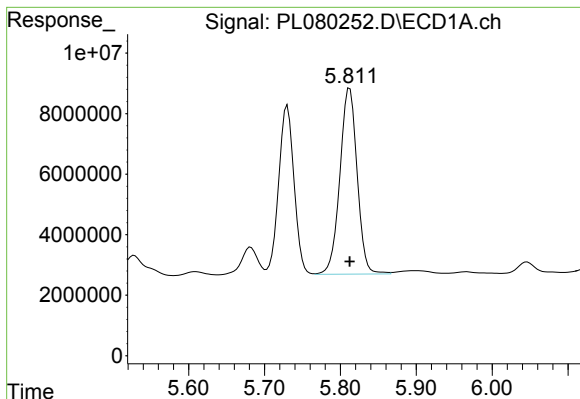

#26 Chlordane-4


R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 97285413
Conc: 240.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

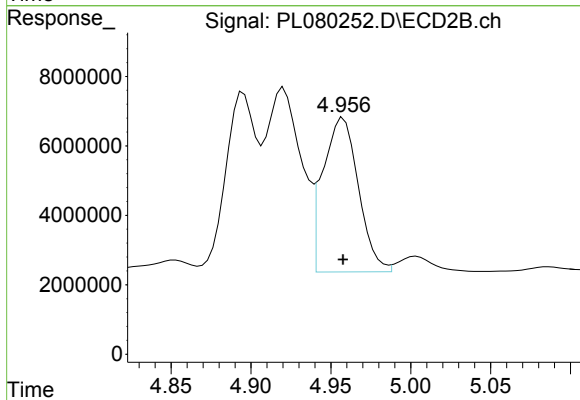


#26 Chlordane-4

R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 68889665
Conc: 236.96 ng/ml

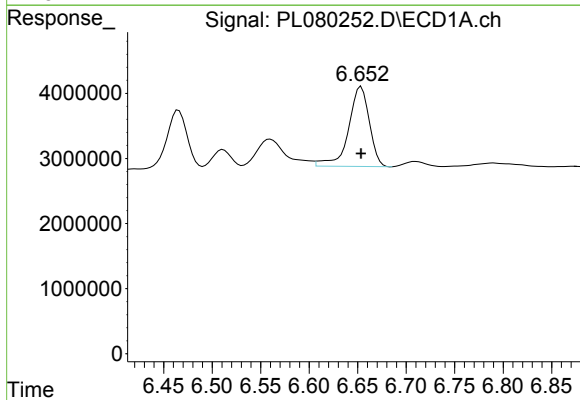


#27 Chlordane-5

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 18327462
Conc: 259.44 ng/ml

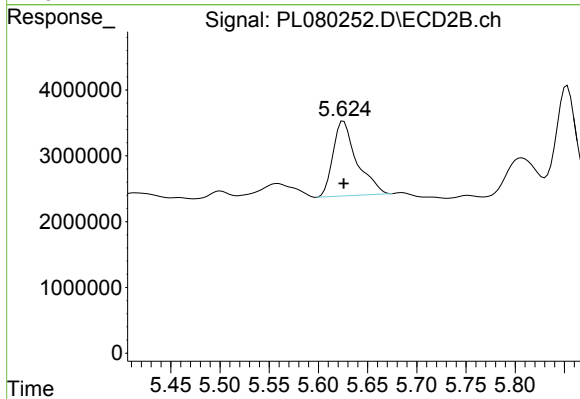

#27 Chlordane-5


R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 19159096
Conc: 249.49 ng/ml

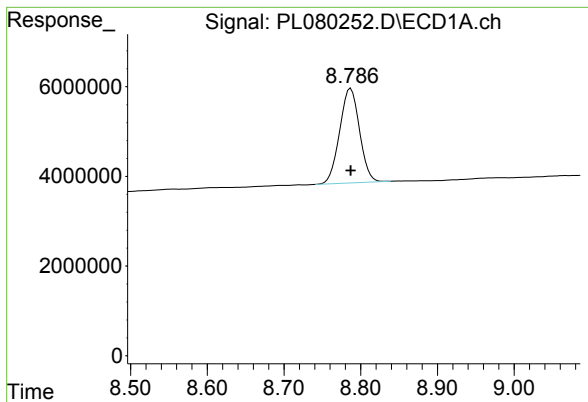

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 38196440
Conc: 25.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

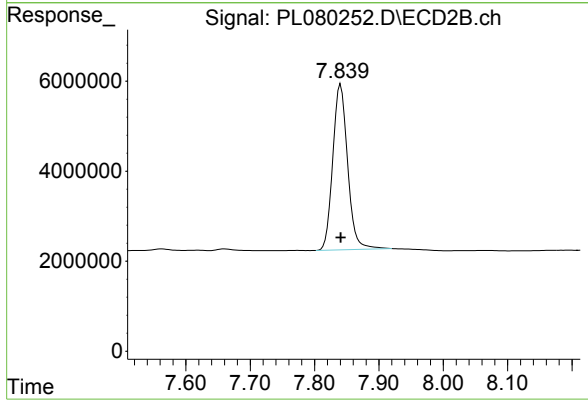

#28 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 59156428
Conc: 26.13 ng/ml