

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
 Data File : PL080275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 06:54
 Operator : AR\AJ
 Sample : 01094-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 STOCKPILE-A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/12/2023
 Supervised By :Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 07:09:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.691	42903237	45542957	21.477m	20.363
28) SA Decachlor...	8.787	7.840	22971805	33906878	15.570	15.084

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 06:54
Operator : AR\AJ
Sample : 01094-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
STOCKPILE-A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/12/2023
Supervised By : Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 07:09:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

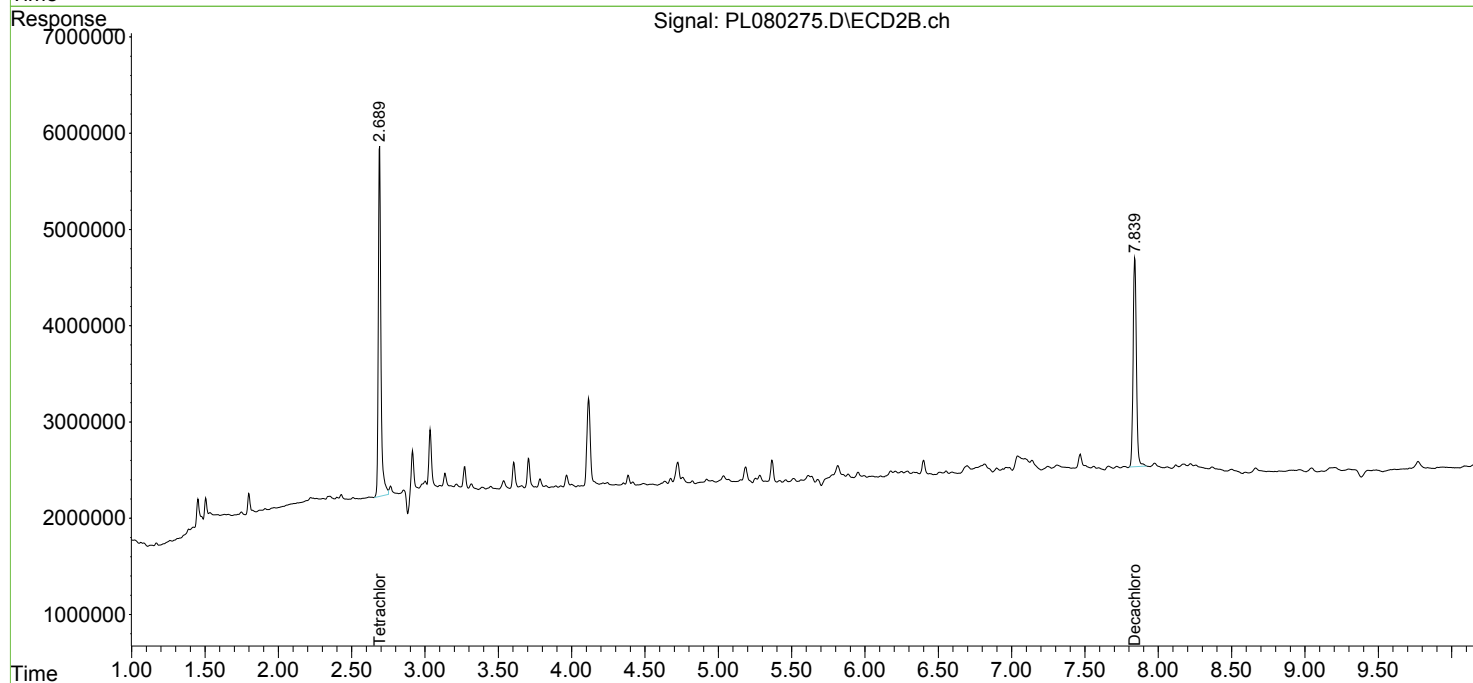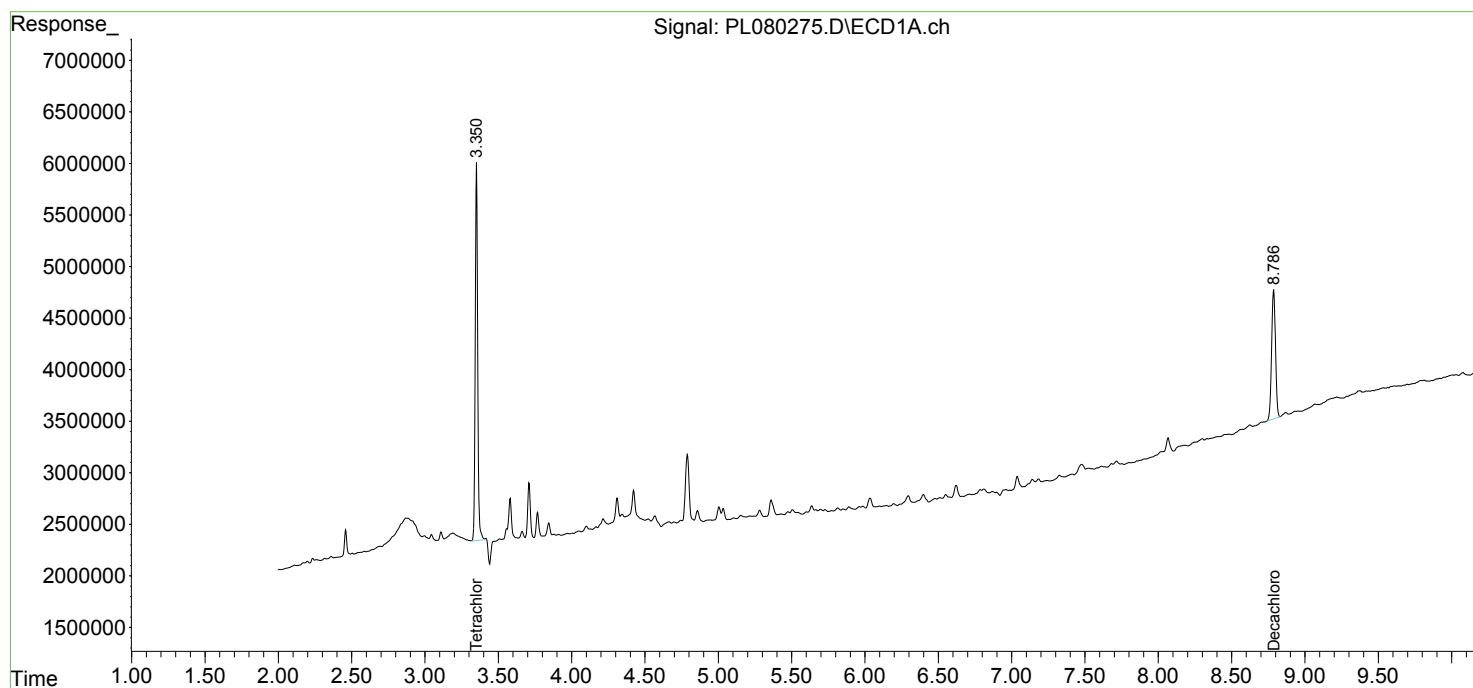

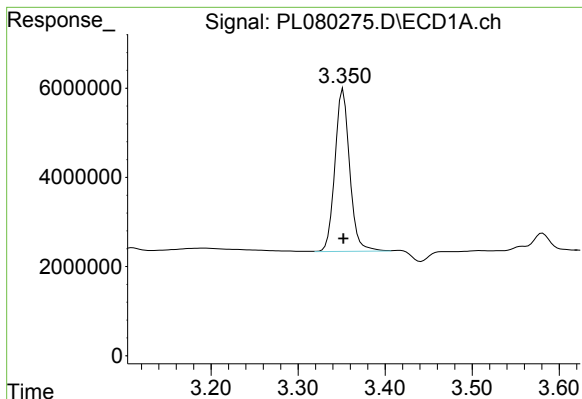


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 42903237
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE-A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/12/2023
Supervised By :Ankita Jodhani 01/12/2023

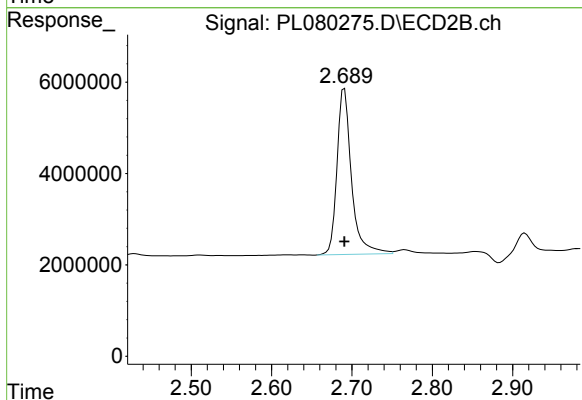


#1 Tetrachloro-m-xylene

R.T.: 2.691 min
Delta R.T.: 0.000 min
Response: 45542957
Conc: 20.36 ng/ml

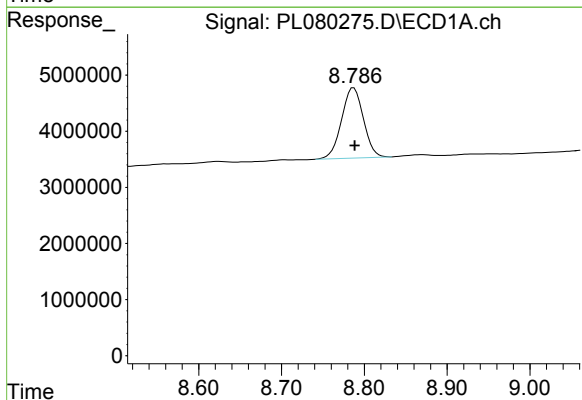

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.001 min
Response: 22971805
Conc: 15.57 ng/ml

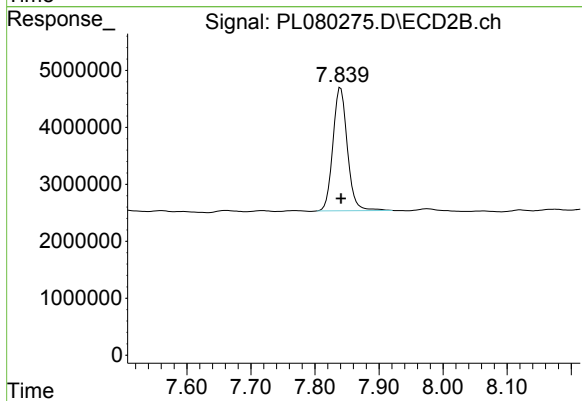

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 33906878
Conc: 15.08 ng/ml