

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011320\
 Data File : PL055695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2020 13:26
 Operator : AJ\MA
 Sample : L1014-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 16:24:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	3.967	173.6E6	34873267	18.784	13.164 #
28)	SA Decachlor...	8.237	8.955	137.6E6	33585714	15.673	16.154
Target Compounds							
2)	A alpha-BHC	3.944	0.000	13081872	0	0.828	N.D. #
4)	MA Heptachlor	4.485f	0.000	16345662	0	1.143	N.D. #
6)	B beta-BHC	4.485f	4.829f	16345662	8904464	2.675	5.832 #
10)	B gamma-Chl...	5.423	6.041	8472904	4179296	0.633	1.484 #
11)	B alpha-Chl...	0.000	6.114	0	7146318	N.D.	2.543 #
23)	Chlordane-1	4.361	0.000	22832695	0	66.013	N.D. #
24)	Chlordane-2	0.000	5.401	0	6849109	N.D.	71.434 #
25)	Chlordane-3	5.423	6.041	8472904	4179296	7.198	12.237 #
26)	Chlordane-4	0.000	6.114	0	7146318	N.D.	17.816 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011320\
Data File : PL055695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2020 13:26
Operator : AJ\MA
Sample : L1014-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 16:24:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

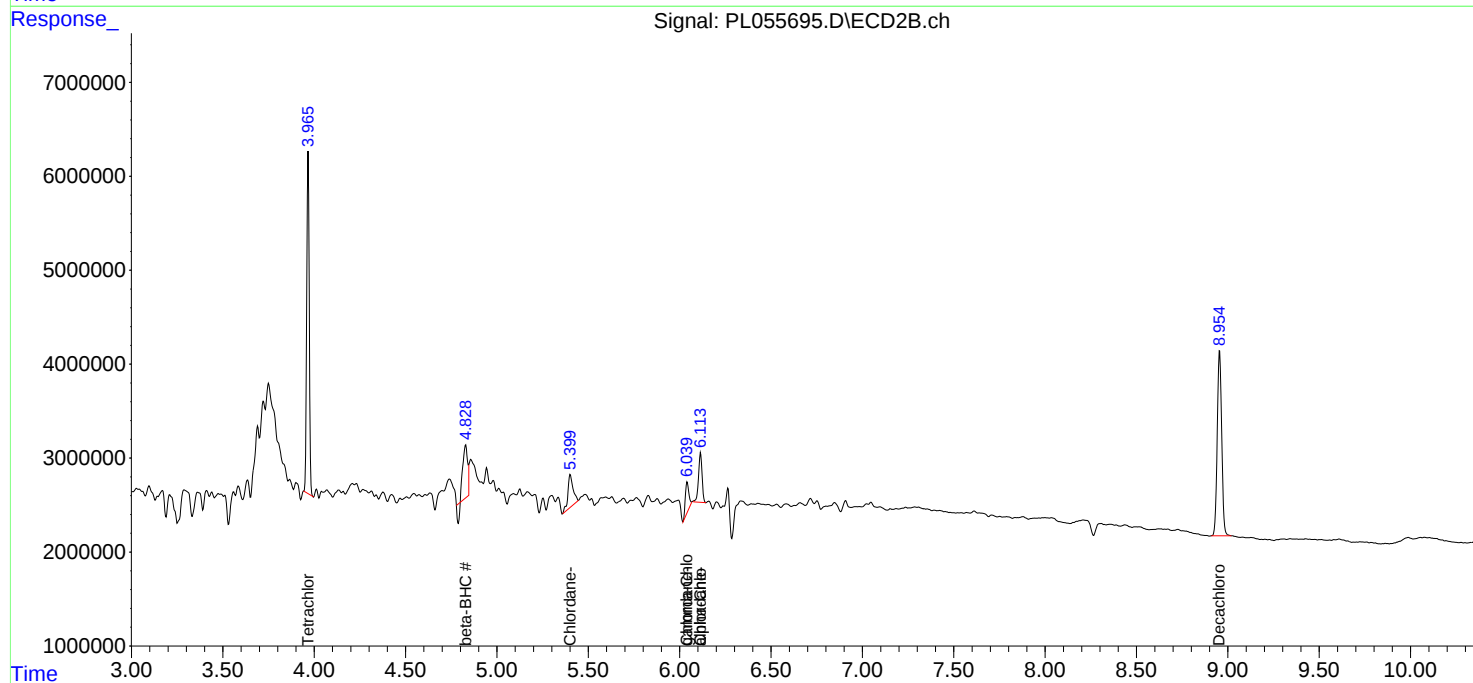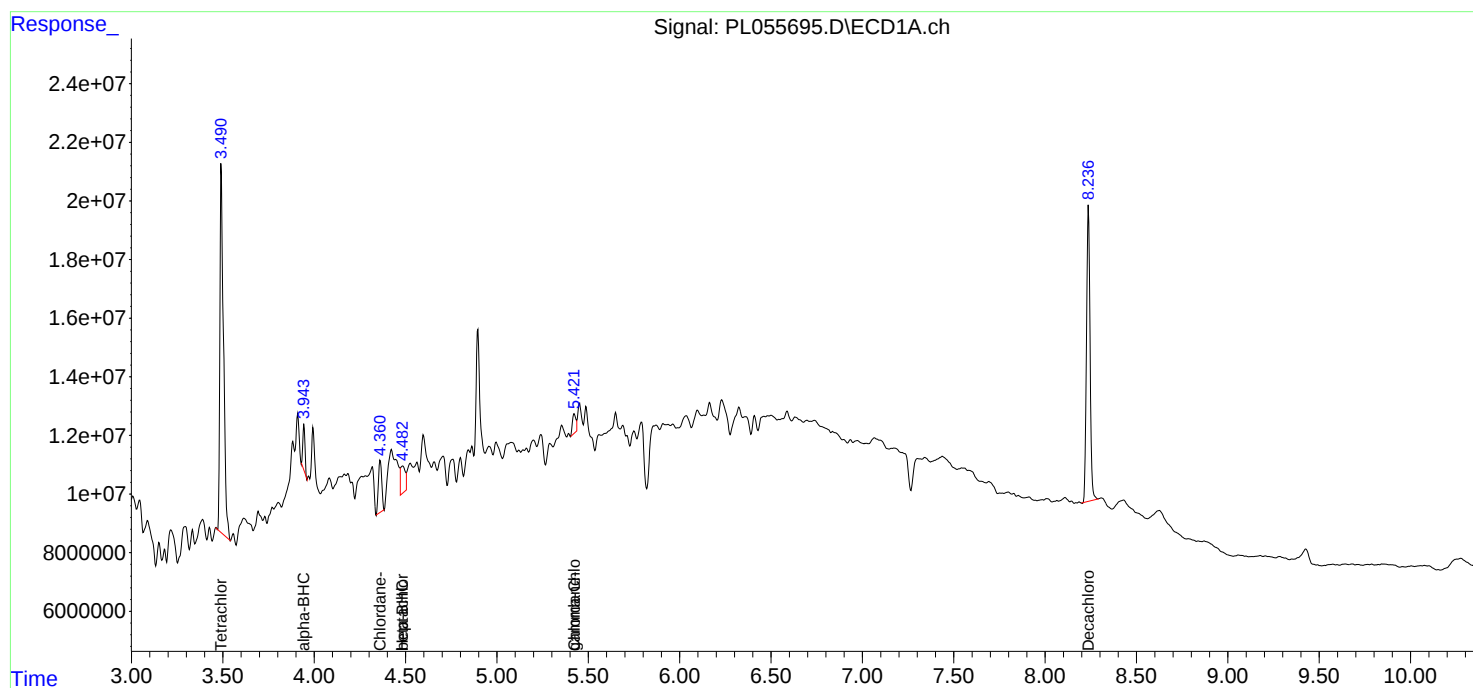


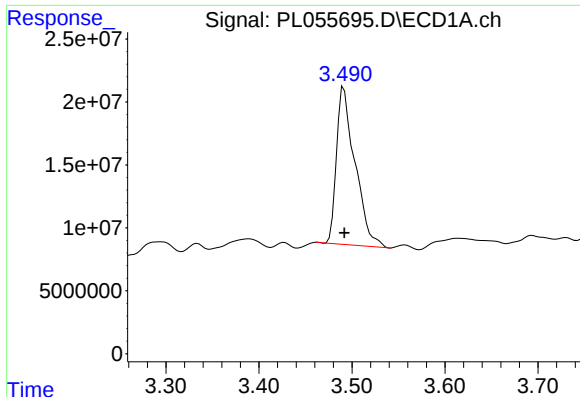

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 173576046
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

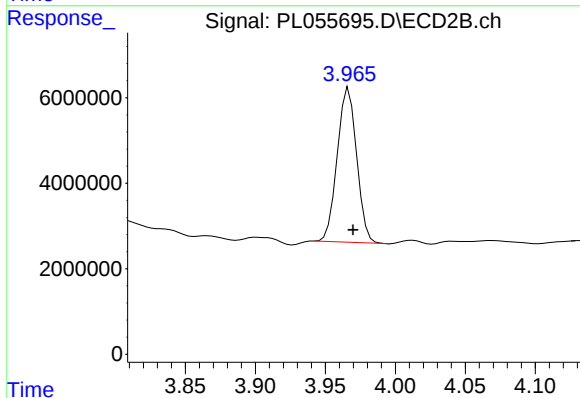


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.003 min
Response: 34873267
Conc: 13.16 ng/ml

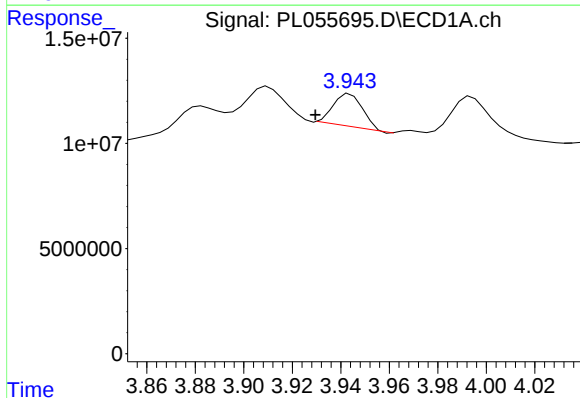


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.014 min
Response: 13081872
Conc: 0.83 ng/ml

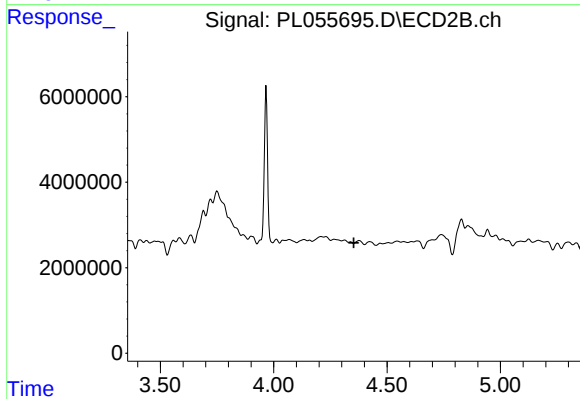

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.354 min
Response: 0
Conc: N.D.

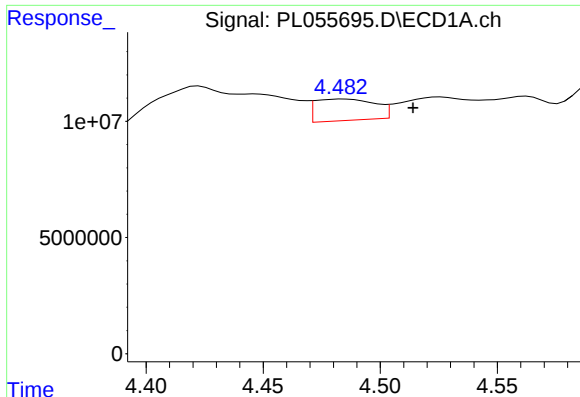

#4 Heptachlor


R.T.: 4.485 min
Delta R.T.: -0.029 min
Response: 16345662
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

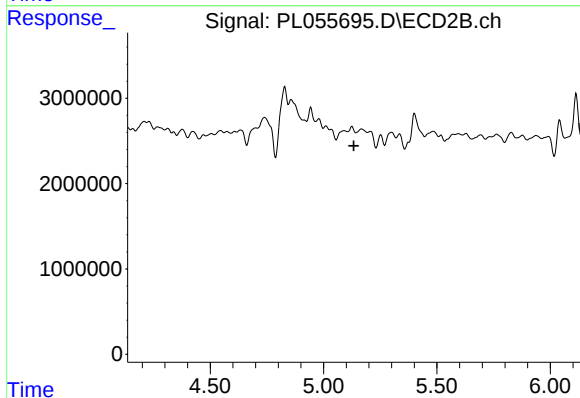


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.134 min
Response: 0
Conc: N.D.

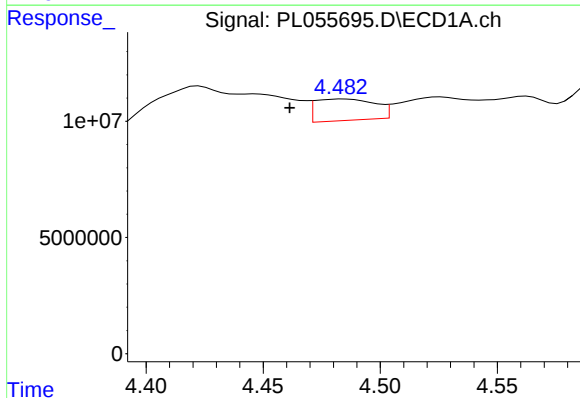


#6 beta-BHC

R.T.: 4.485 min
Delta R.T.: 0.023 min
Response: 16345662
Conc: 2.67 ng/ml

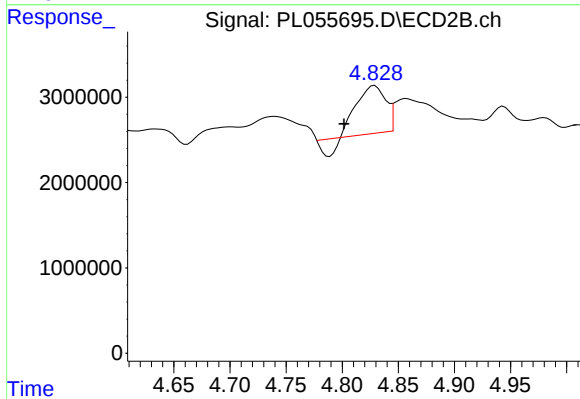

#6 beta-BHC


R.T.: 4.829 min
Delta R.T.: 0.027 min
Response: 8904464
Conc: 5.83 ng/ml

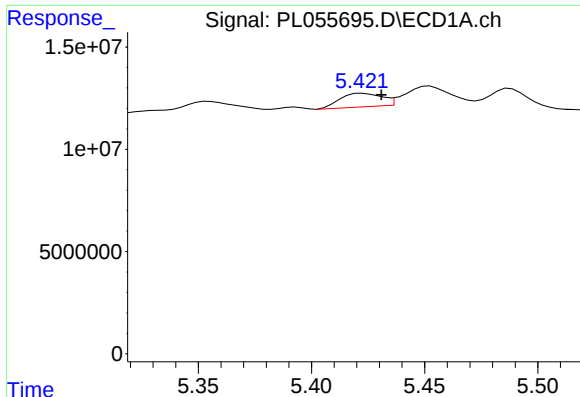

#10 gamma-Chlordane


R.T.: 5.423 min
Delta R.T.: -0.008 min
Response: 8472904
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

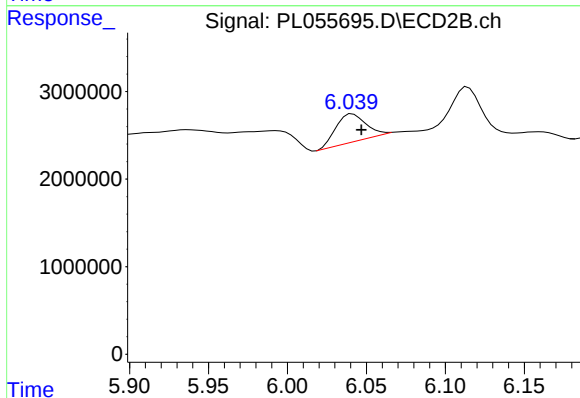


#10 gamma-Chlordane

R.T.: 6.041 min
Delta R.T.: -0.006 min
Response: 4179296
Conc: 1.48 ng/ml

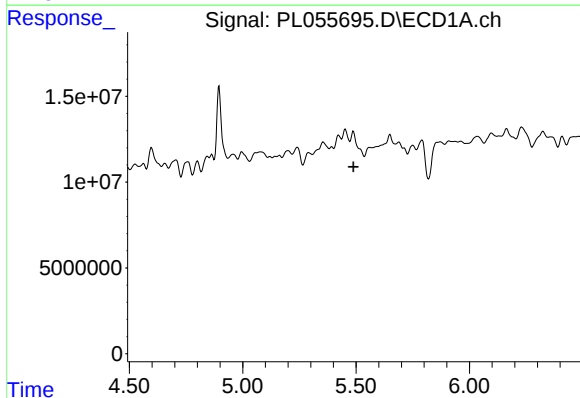


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.489 min
Response: 0
Conc: N.D.

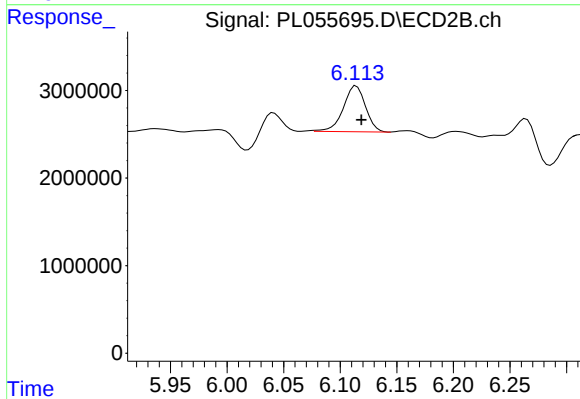

#11 alpha-Chlordane


R.T.: 6.114 min
Delta R.T.: -0.004 min
Response: 7146318
Conc: 2.54 ng/ml

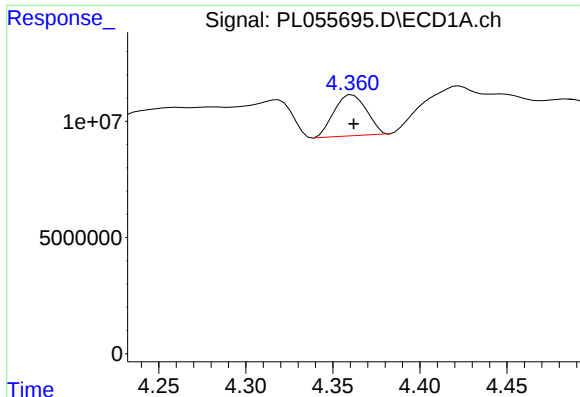

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 22832695
Conc: 66.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

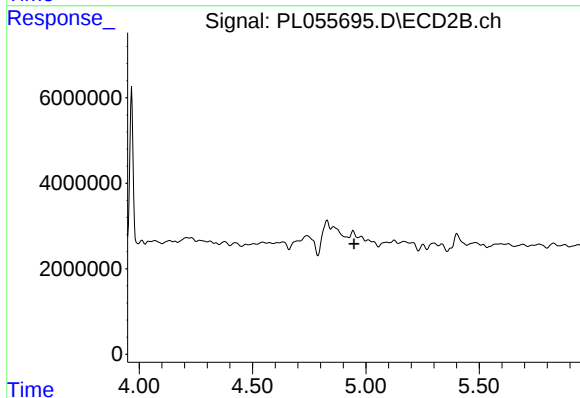


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.947 min
Response: 0
Conc: N.D.

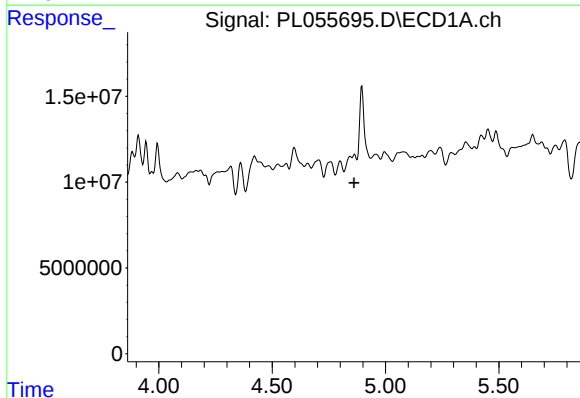


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.862 min
Response: 0
Conc: N.D.

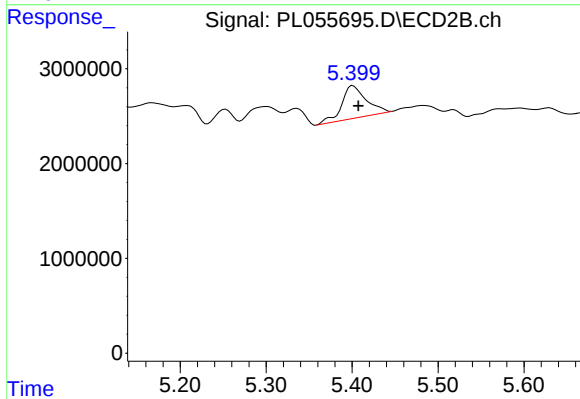

#24 Chlordane-2


R.T.: 5.401 min
Delta R.T.: -0.006 min
Response: 6849109
Conc: 71.43 ng/ml

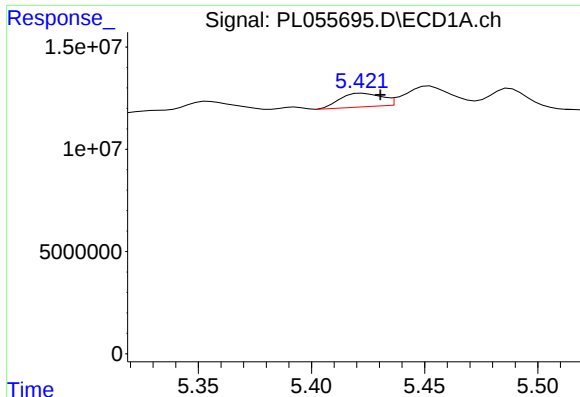

#25 Chlordane-3


R.T.: 5.423 min
Delta R.T.: -0.008 min
Response: 8472904
Conc: 7.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

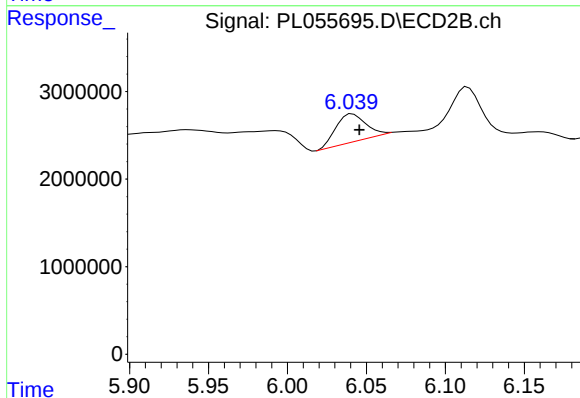


#25 Chlordane-3

R.T.: 6.041 min
Delta R.T.: -0.004 min
Response: 4179296
Conc: 12.24 ng/ml

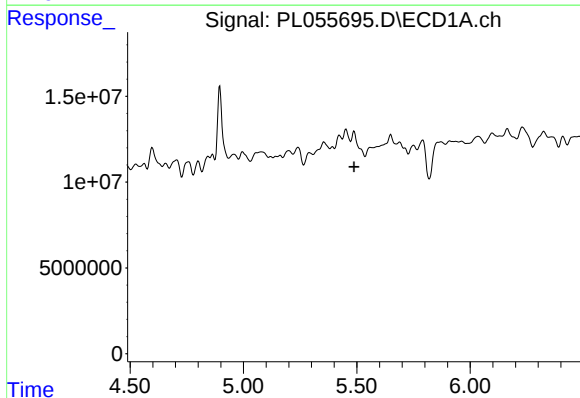


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.488 min
Response: 0
Conc: N.D.

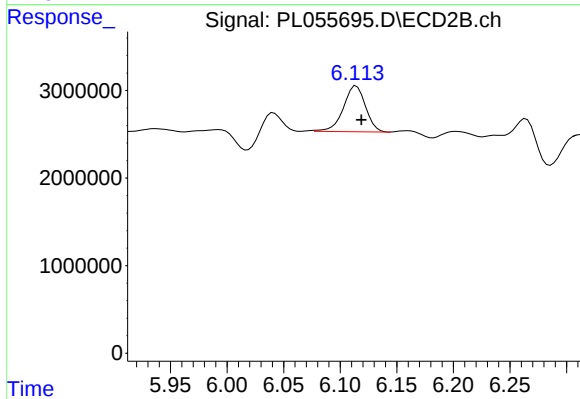

#26 Chlordane-4


R.T.: 6.114 min
Delta R.T.: -0.005 min
Response: 7146318
Conc: 17.82 ng/ml

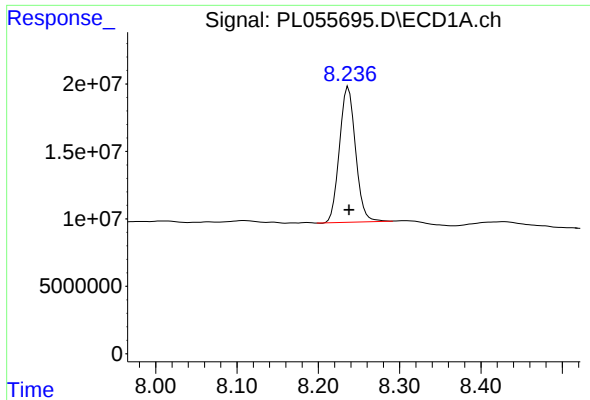

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 137636377
Conc: 15.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

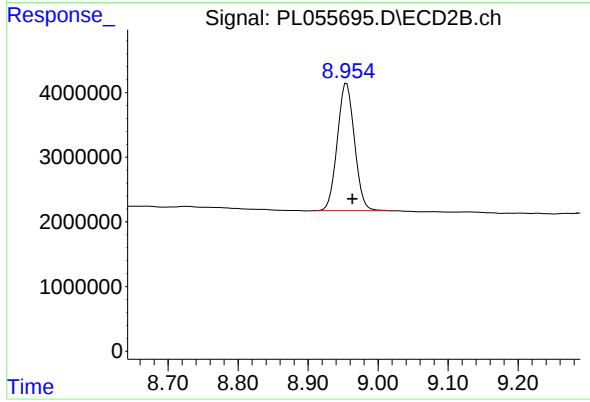

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.008 min
Response: 33585714
Conc: 16.15 ng/ml