

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011320\
 Data File : PL055711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2020 17:13
 Operator : AJ\MA
 Sample : L1074-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 08:39:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	3.969	199.4E6	61278784	21.574	23.132
28)	SA Decachlor...	8.236	8.955	154.6E6	38364623	17.606	18.453
Target Compounds							
9)	A Endosulfan I	5.552	0.000	3022795	0	0.245	N.D. #
10)	B gamma-Chl...	5.446f	0.000	50580038	0	3.778	N.D. #
11)	B alpha-Chl...	5.484	0.000	21799926	0	1.660	N.D. #
25)	Chlordane-3	5.446f	0.000	50580038	0	42.971	N.D. #
26)	Chlordane-4	5.484	0.000	21799926	0	22.327	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011320\
Data File : PL055711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2020 17:13
Operator : AJ\MA
Sample : L1074-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 08:39:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

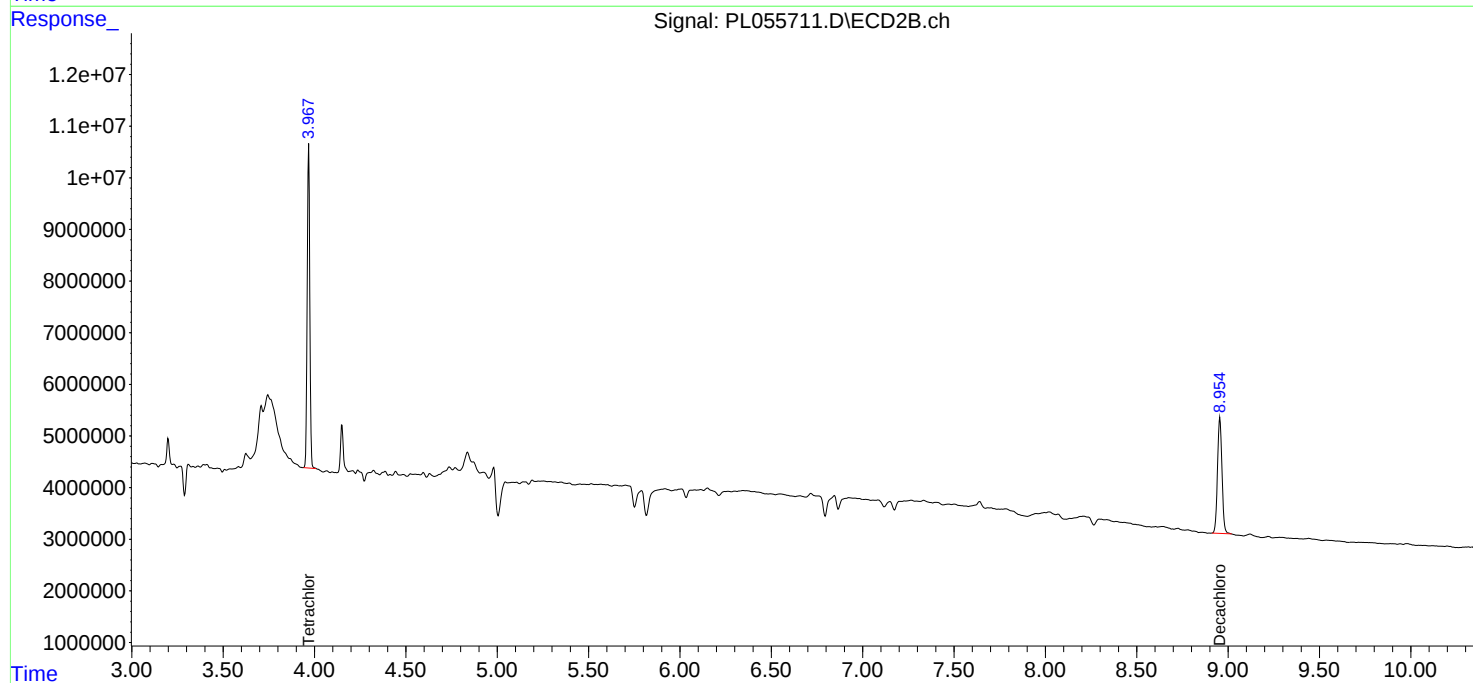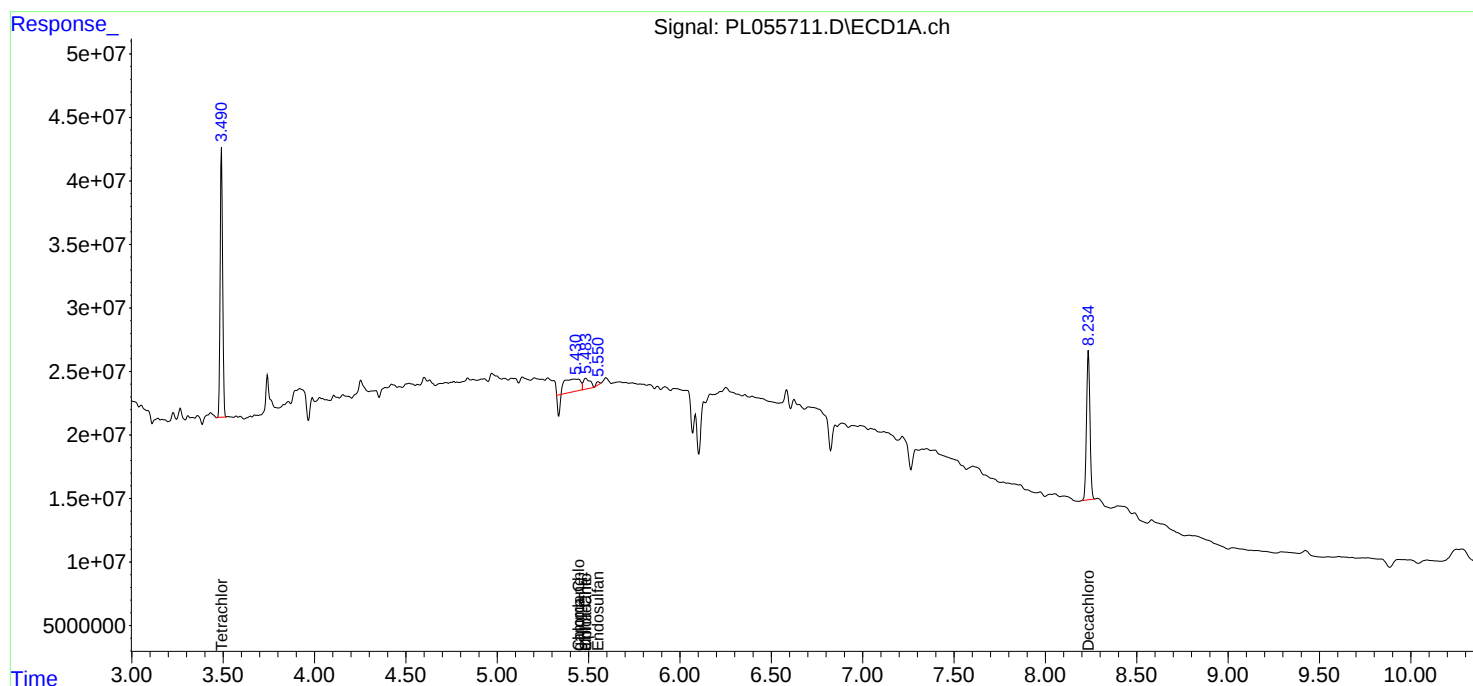


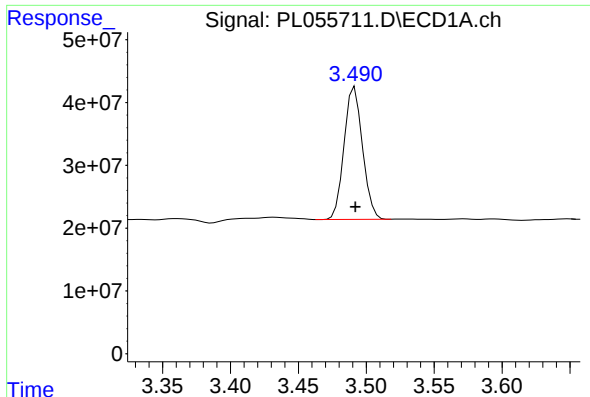

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 199361088
Conc: 21.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

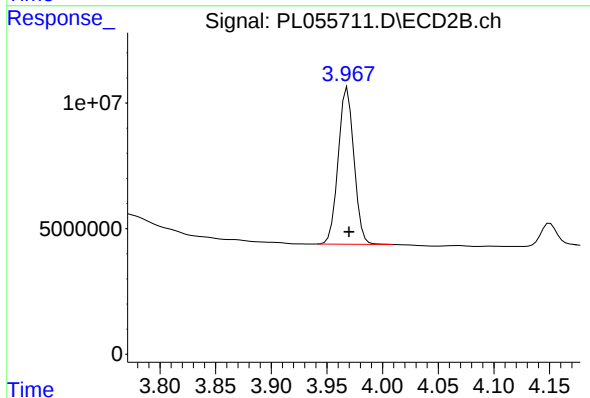


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 61278784
Conc: 23.13 ng/ml

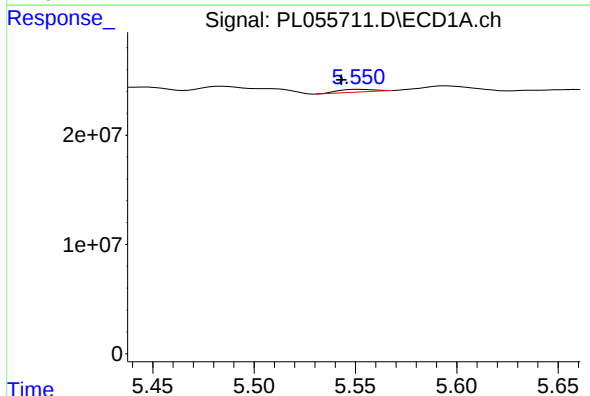


#9 Endosulfan I

R.T.: 5.552 min
Delta R.T.: 0.008 min
Response: 3022795
Conc: 0.24 ng/ml

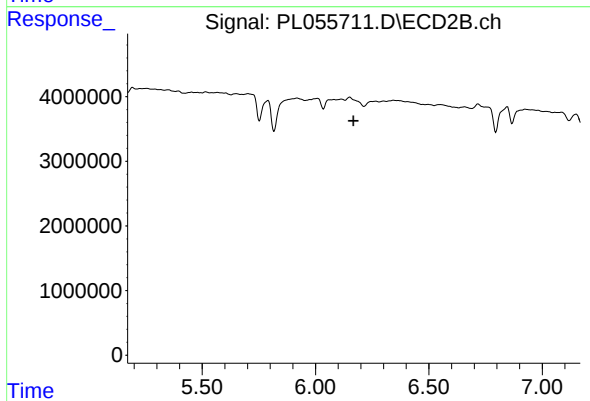

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

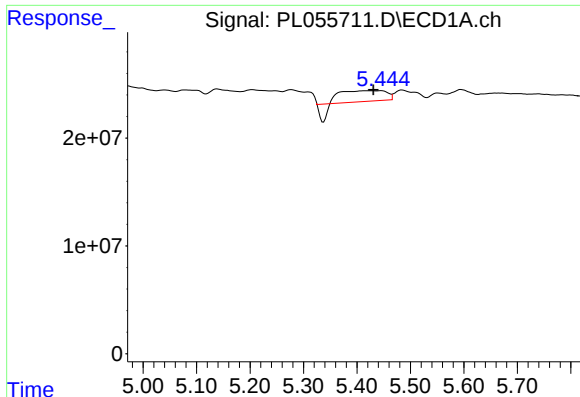

#10 gamma-Chlordane


R.T.: 5.446 min
Delta R.T.: 0.015 min
Response: 50580038
Conc: 3.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

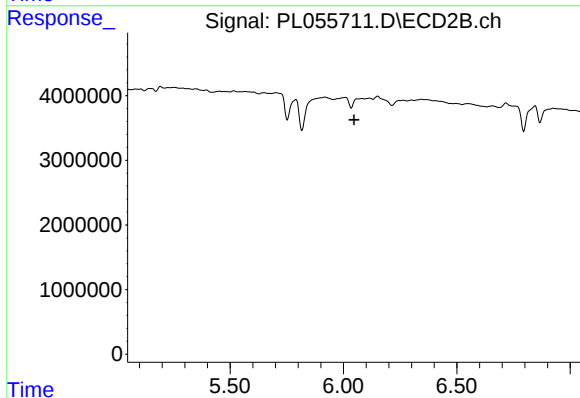


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.047 min
Response: 0
Conc: N.D.

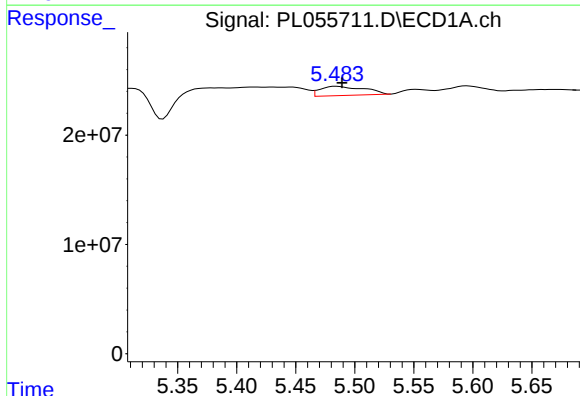


#11 alpha-Chlordane

R.T.: 5.484 min
Delta R.T.: -0.005 min
Response: 21799926
Conc: 1.66 ng/ml

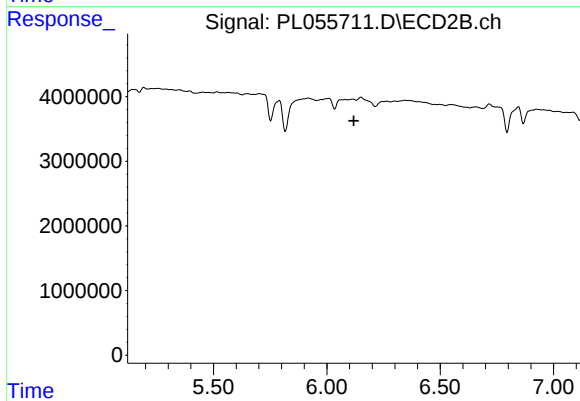

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

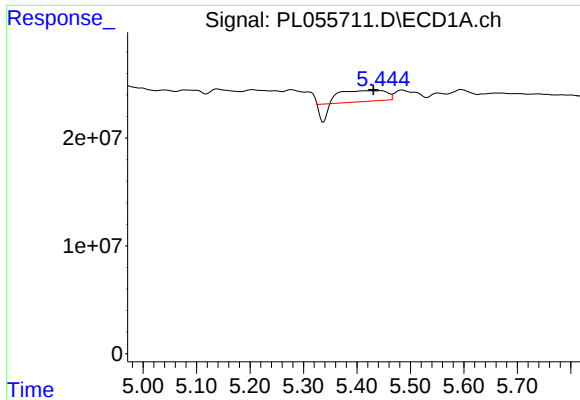

#25 Chlordane-3


R.T.: 5.446 min
Delta R.T.: 0.016 min
Response: 50580038
Conc: 42.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

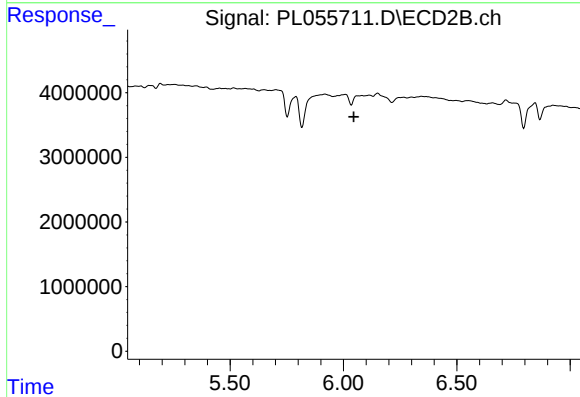


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

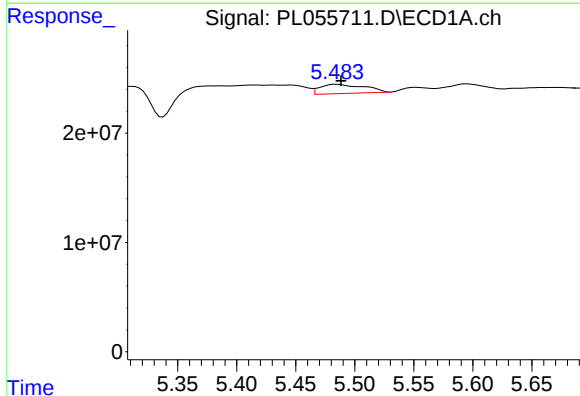


#26 Chlordane-4

R.T.: 5.484 min
Delta R.T.: -0.004 min
Response: 21799926
Conc: 22.33 ng/ml

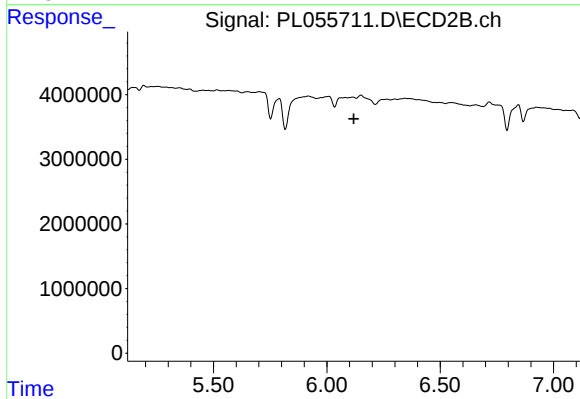

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

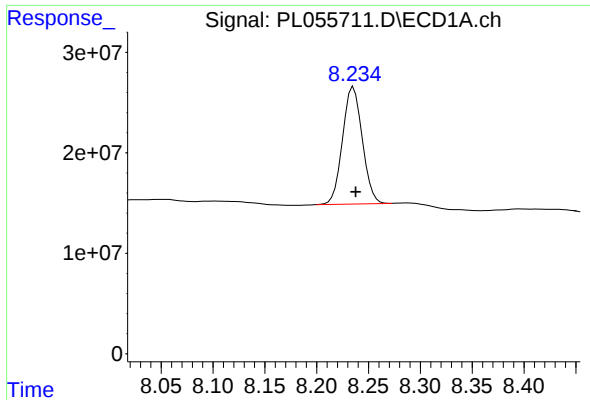

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: -0.002 min
Response: 154608038
Conc: 17.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

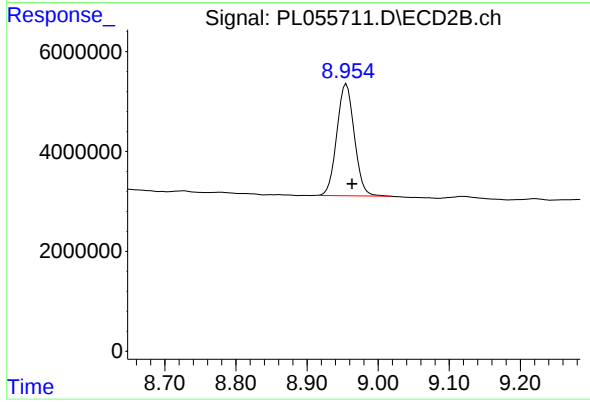

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.008 min
Response: 38364623
Conc: 18.45 ng/ml