

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
 Data File : PL064092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2021 16:14
 Operator : AR\AJ
 Sample : M1058-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 19:02:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.107	48686960	54614833	16.237	21.364 #
28)	SA Decachlor...	8.170	9.267	16782566	12821396	5.499	5.402
Target Compounds							
2)	A alpha-BHC	3.853f	0.000	6727886	0	1.353	N.D. #
3)	MA gamma-BHC...	4.150	0.000	35423925	0	7.640	N.D. #
4)	MA Heptachlor	4.455	0.000	5820281	0	1.328	N.D. #
6)	B beta-BHC	4.374f	0.000	5759530	0	0.085	N.D. #
11)	B alpha-Chl...	5.410	6.337	14083746	6579387	3.681	2.161 #
26)	Chlordane-4	5.410	6.337	14083746	6579387	47.293	13.571 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
Data File : PL064092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2021 16:14
Operator : AR\AJ
Sample : M1058-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 19:02:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

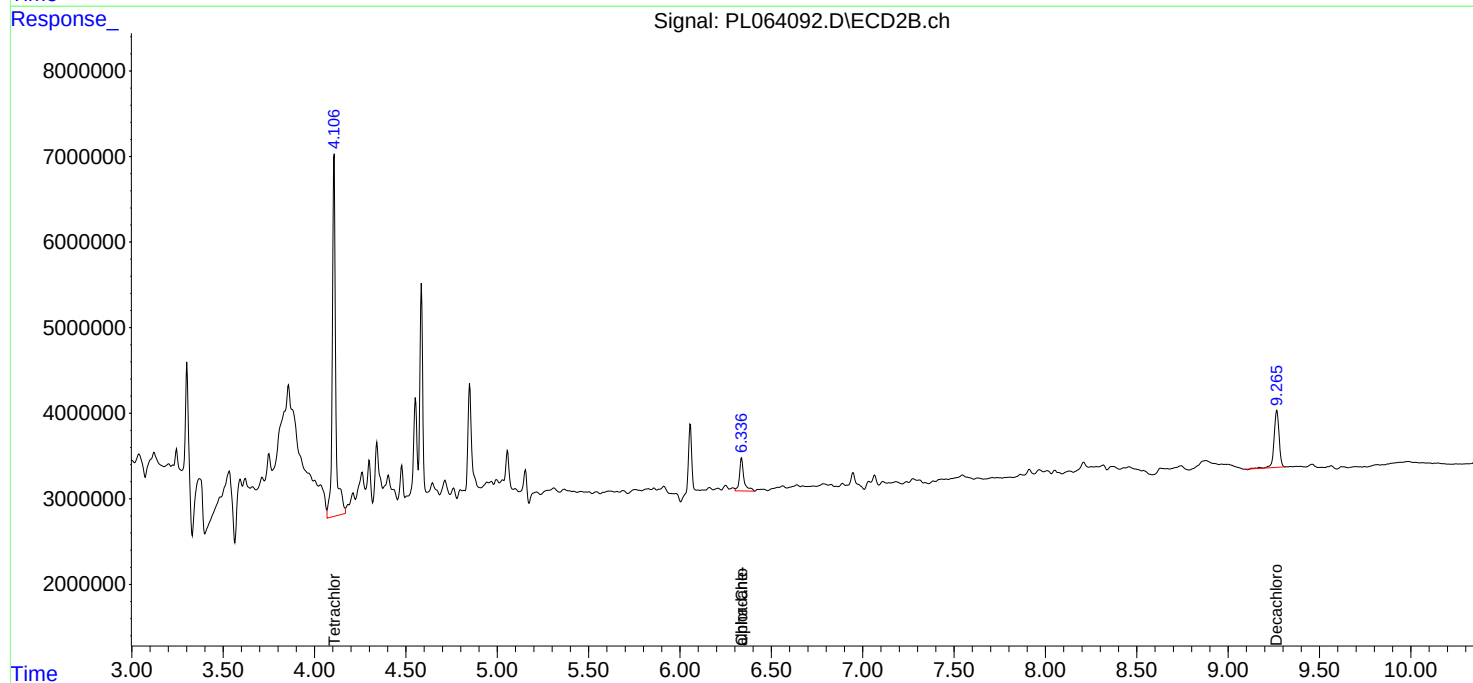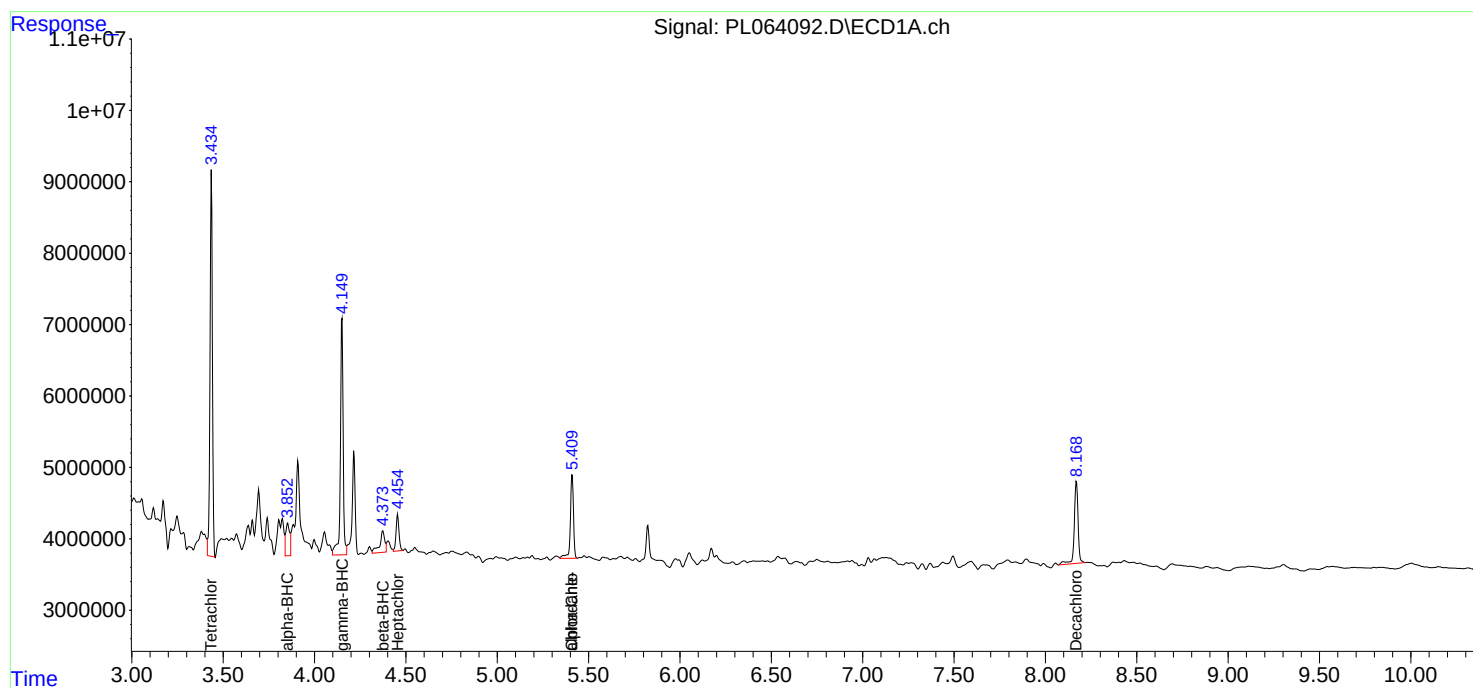


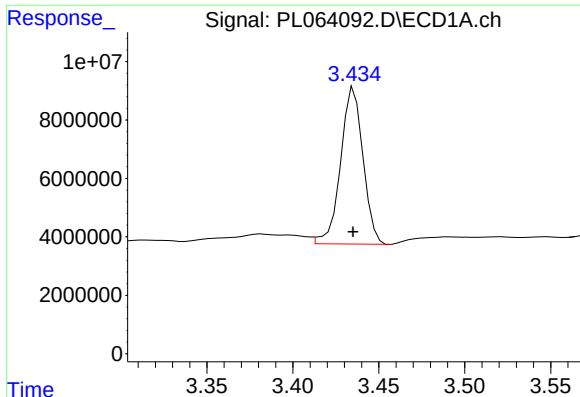

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 48686960
Conc: 16.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

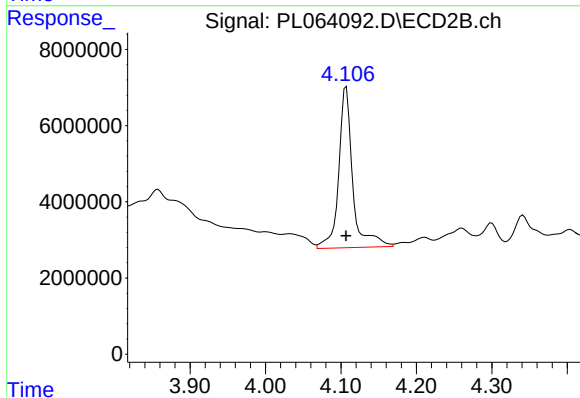


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 54614833
Conc: 21.36 ng/ml

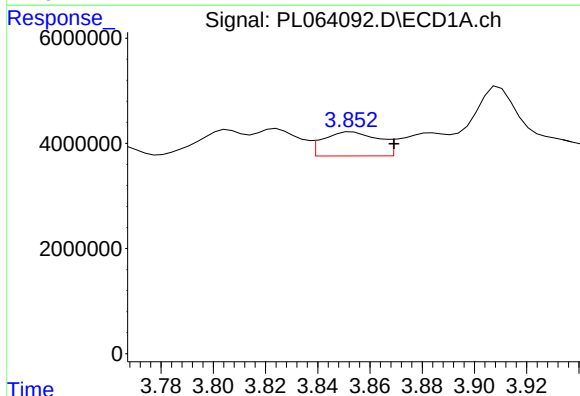


#2 alpha-BHC

R.T.: 3.853 min
Delta R.T.: -0.016 min
Response: 6727886
Conc: 1.35 ng/ml

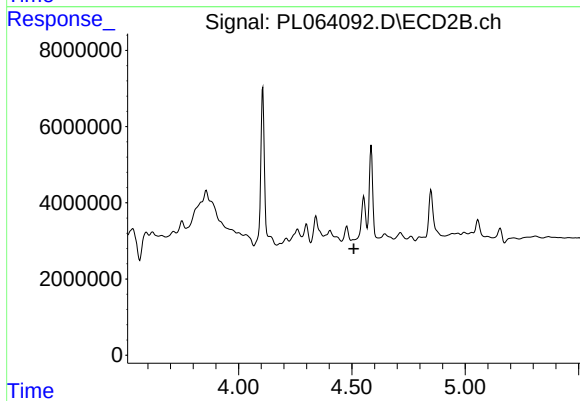

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.508 min
Response: 0
Conc: N.D.

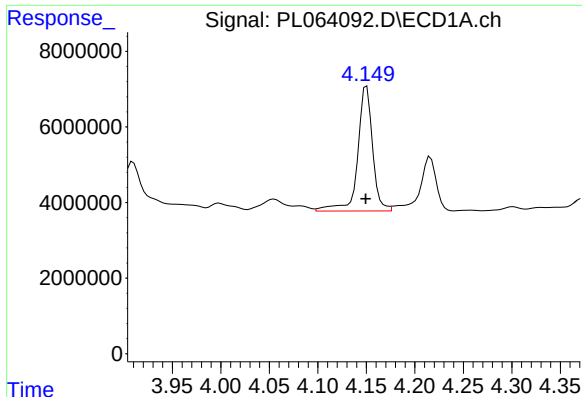

#3 gamma-BHC (Lindane)


R.T.: 4.150 min
Delta R.T.: 0.000 min
Response: 35423925
Conc: 7.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

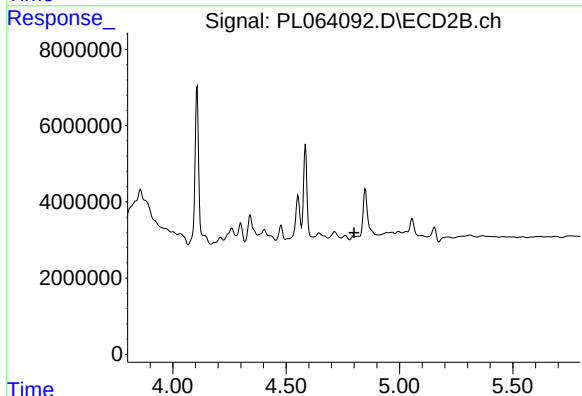


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

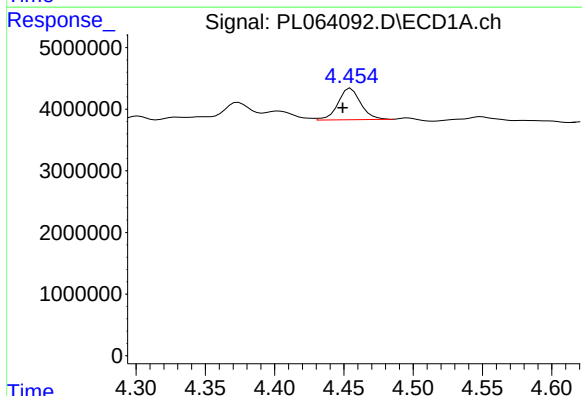


#4 Heptachlor

R.T.: 4.455 min
Delta R.T.: 0.006 min
Response: 5820281
Conc: 1.33 ng/ml

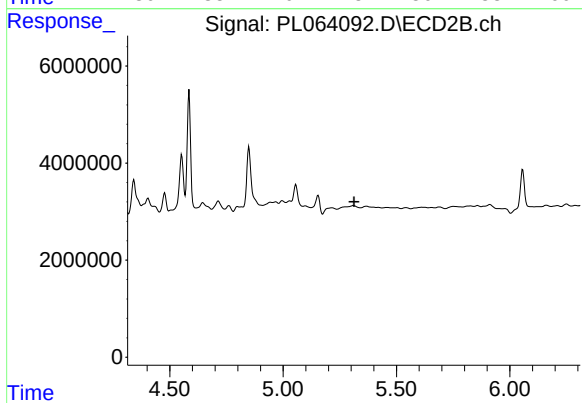

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.313 min
Response: 0
Conc: N.D.

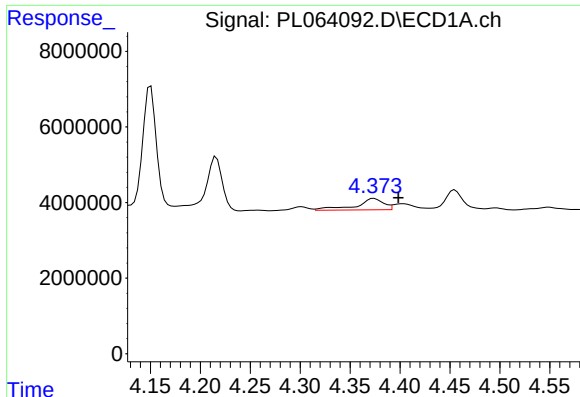

#6 beta-BHC


R.T.: 4.374 min
Delta R.T.: -0.024 min
Response: 5759530
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

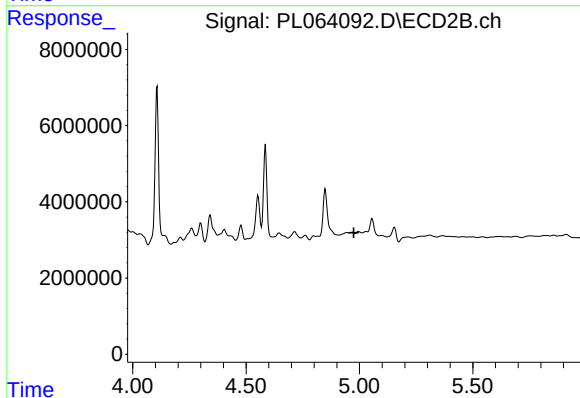


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.976 min
Response: 0
Conc: N.D.

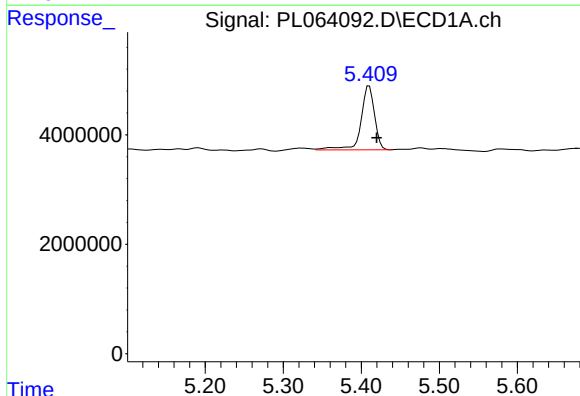


#11 alpha-Chlordane

R.T.: 5.410 min
Delta R.T.: -0.010 min
Response: 14083746
Conc: 3.68 ng/ml

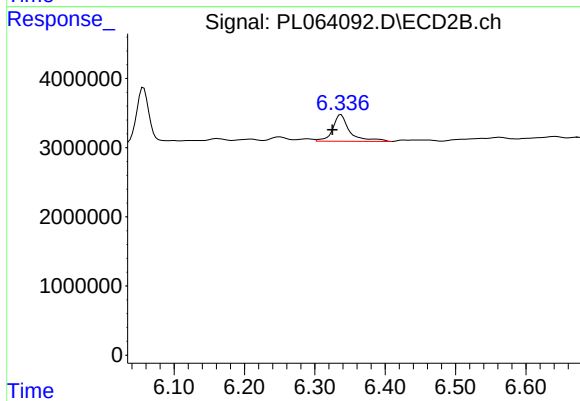

#11 alpha-Chlordane


R.T.: 6.337 min
Delta R.T.: 0.012 min
Response: 6579387
Conc: 2.16 ng/ml

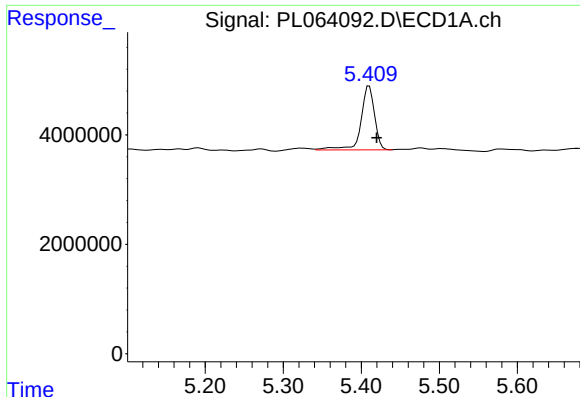

#26 Chlordane-4


R.T.: 5.410 min
Delta R.T.: -0.009 min
Response: 14083746
Conc: 47.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

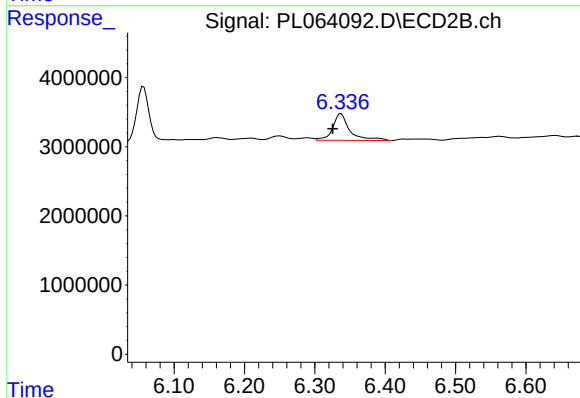


#26 Chlordane-4

R.T.: 6.337 min
Delta R.T.: 0.012 min
Response: 6579387
Conc: 13.57 ng/ml

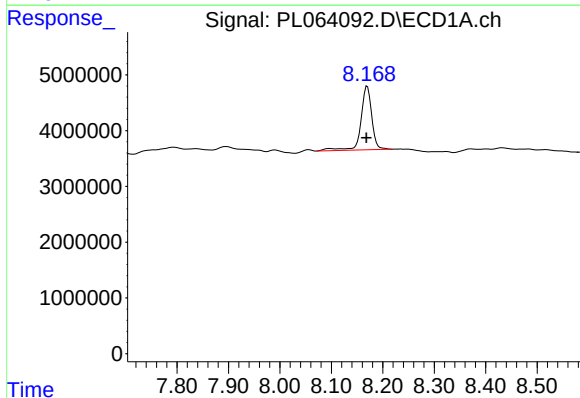

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.002 min
Response: 16782566
Conc: 5.50 ng/ml

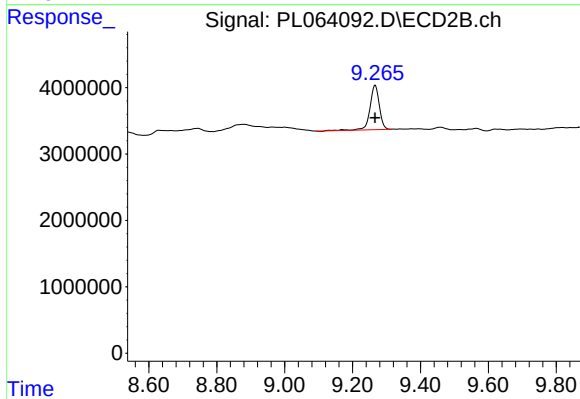

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 12821396
Conc: 5.40 ng/ml