

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
 Data File : PL064083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2021 13:04
 Operator : AR\AJ
 Sample : M1075-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 72-11977

Manual Integrations
 APPROVED

Ankita
 1/14/2021 4:37:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 19:00:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.435	4.108	68940544	63115357	22.992	24.689
28) SA Decachlor...	8.169	9.266	60918889	46322036	19.960m	19.517m
Target Compounds						
10) B gamma-Chl...	5.361	6.253	1900286	7001143	0.491m	2.330m#
11) B alpha-Chl...	5.415	6.324	3033674	4343907	0.793m	1.427m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
Data File : PL064083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2021 13:04
Operator : AR\AJ
Sample : M1075-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
72-11977


Manual Integrations
APPROVED

Ankita
1/14/2021 4:37:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 19:00:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

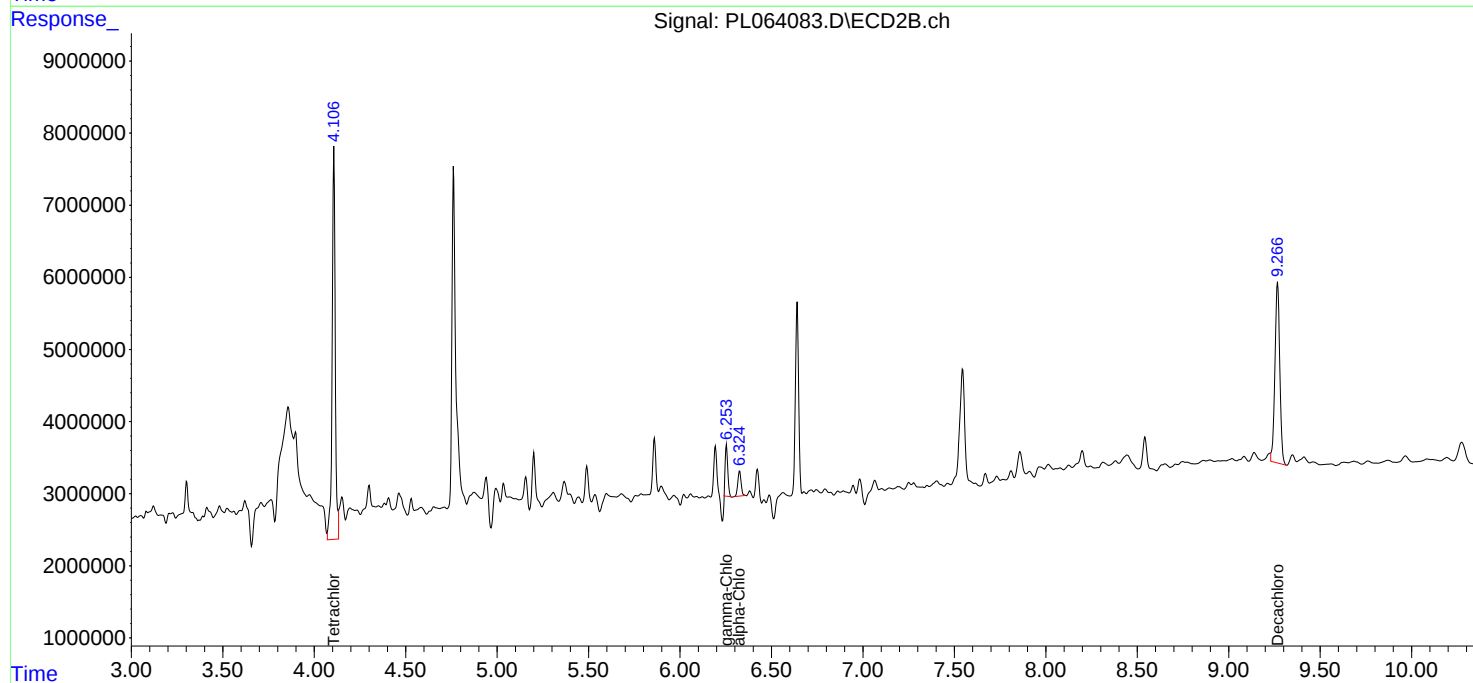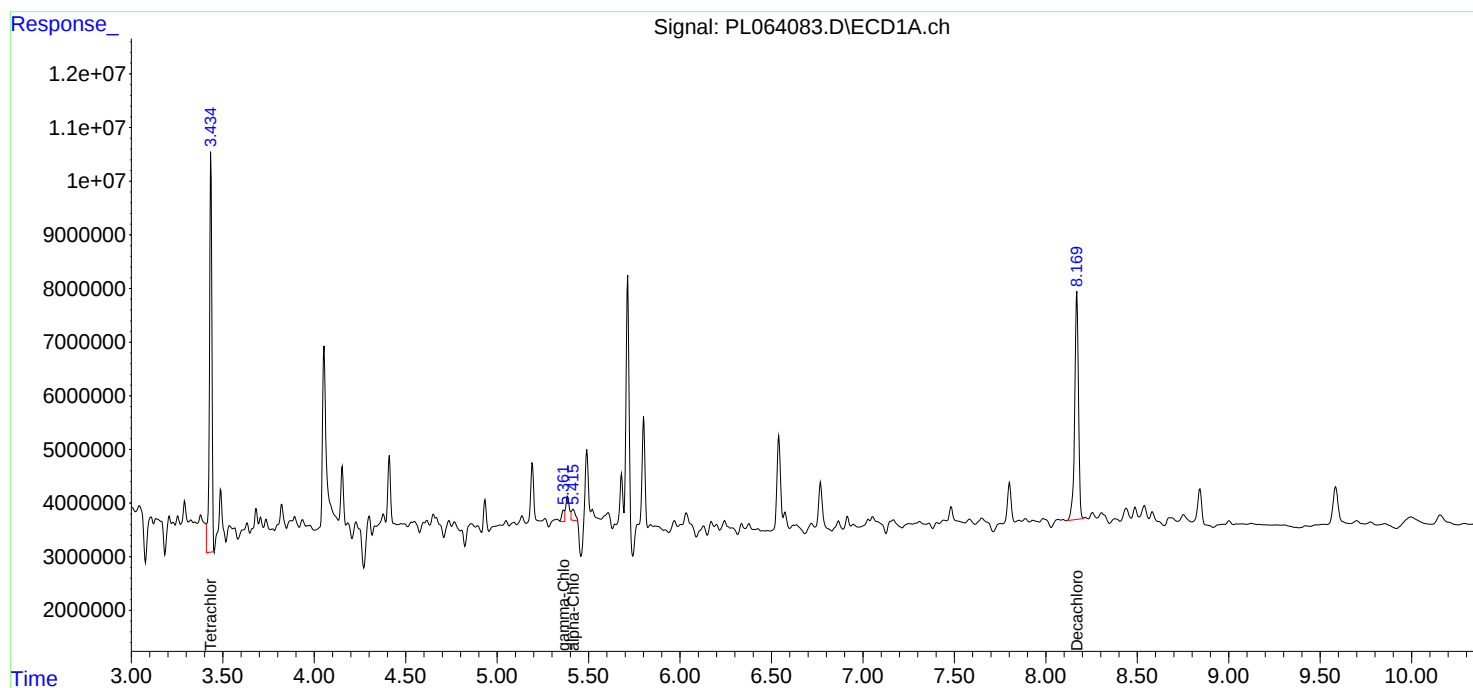

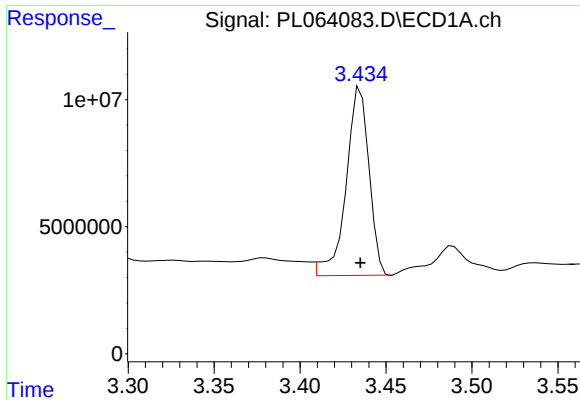


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 68940544
Conc: 22.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
72-11977


Manual Integrations
APPROVED

Ankita
1/14/2021 4:37:25 PM

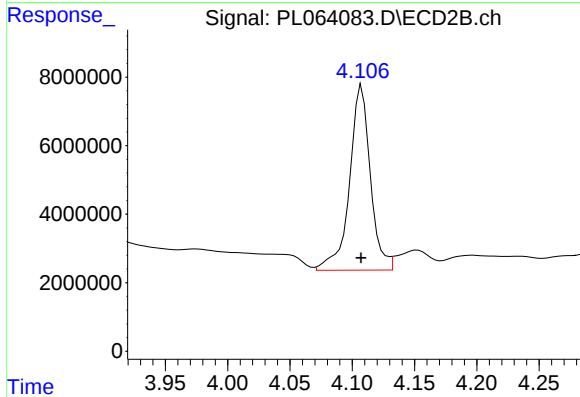


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 63115357
Conc: 24.69 ng/ml

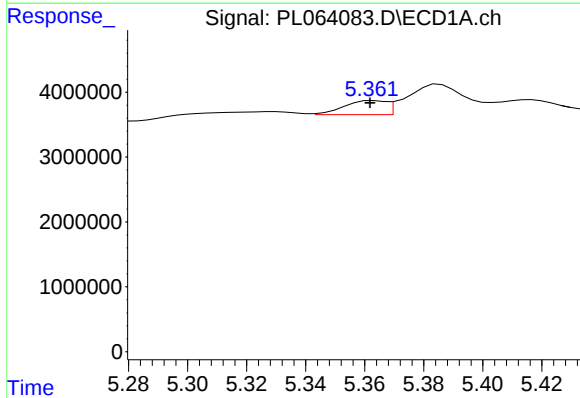


#10 gamma-Chlordane

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 1900286
Conc: 0.49 ng/ml m

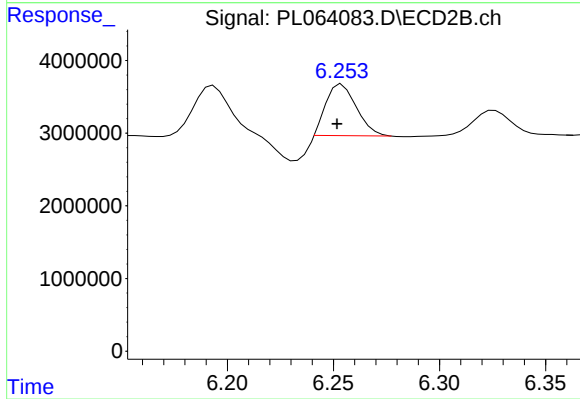

#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 7001143
Conc: 2.33 ng/ml m

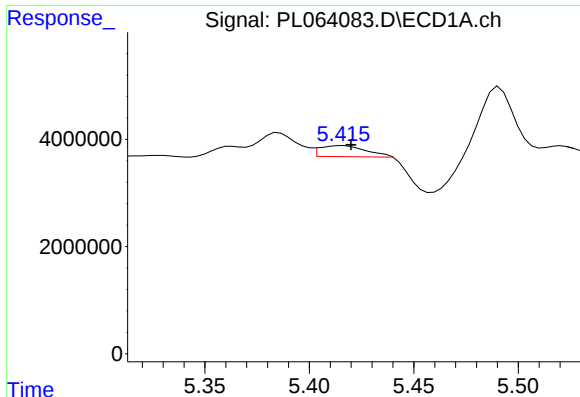


#11 alpha-Chlordane

R.T.: 5.415 min
Delta R.T.: -0.005 min
Response: 3033674
Conc: 0.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
72-11977


Manual Integrations
APPROVED

Ankita
1/14/2021 4:37:25 PM

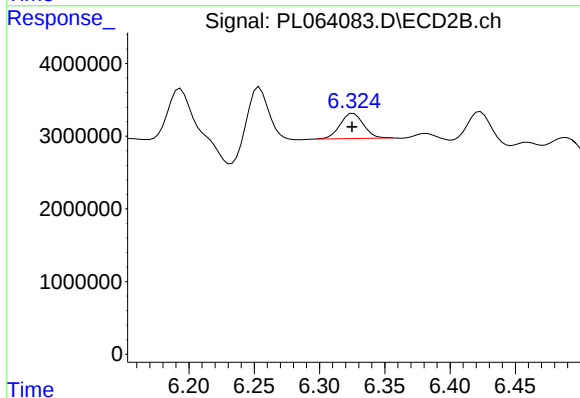


#11 alpha-Chlordane

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 4343907
Conc: 1.43 ng/ml m

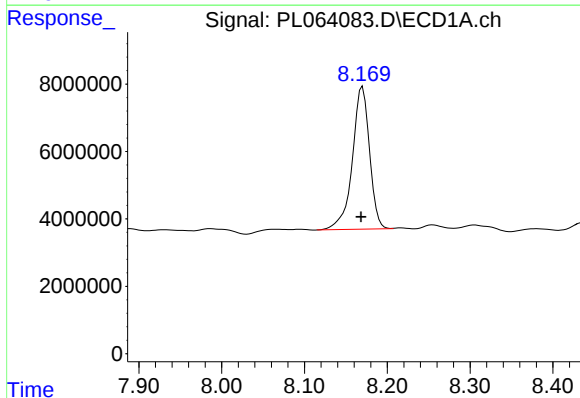

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 60918889
Conc: 19.96 ng/ml m

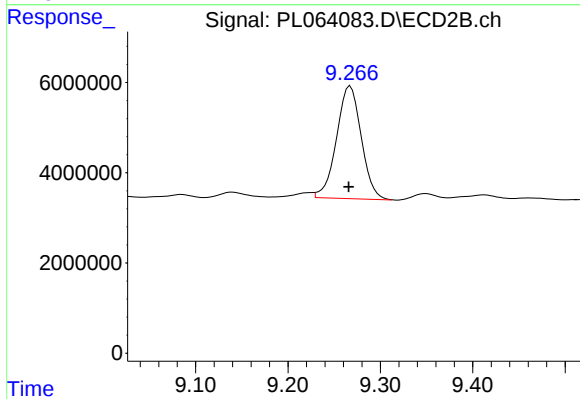

#28 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: 0.000 min
Response: 46322036
Conc: 19.52 ng/ml m