

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
 Data File : PL064103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2021 19:01
 Operator : AR\AJ
 Sample : M1023-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Field Sampling Hourly Rate

Manual Integrations
 APPROVED

Ankita
 1/14/2021 2:20:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:37:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	26710606	22791013	8.908	8.915
28)	SA Decachlor...	8.167	9.268	26237556	21429553	8.597m	9.029

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011321\
Data File : PL064103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2021 19:01
Operator : AR\AJ
Sample : M1023-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
Field Sampling Hourly Rate


Manual Integrations
APPROVED

Ankita
1/14/2021 2:20:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:37:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

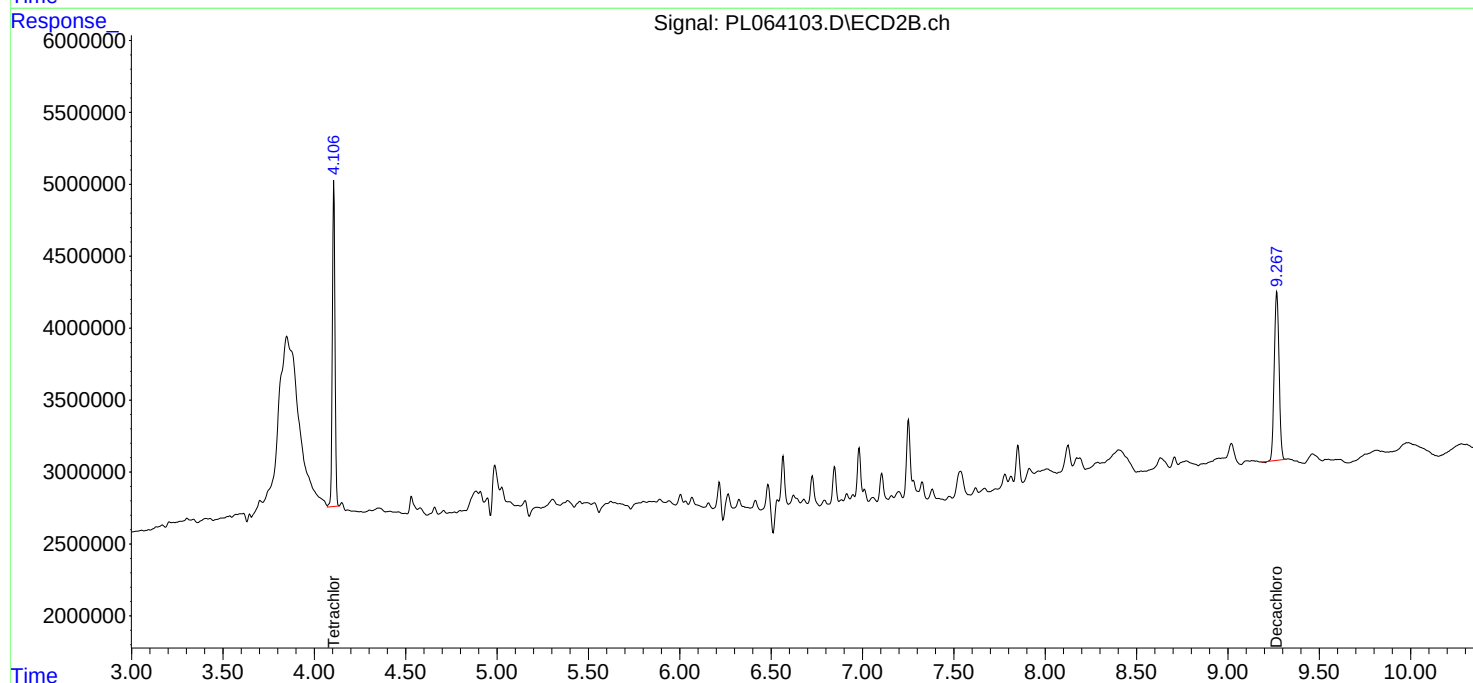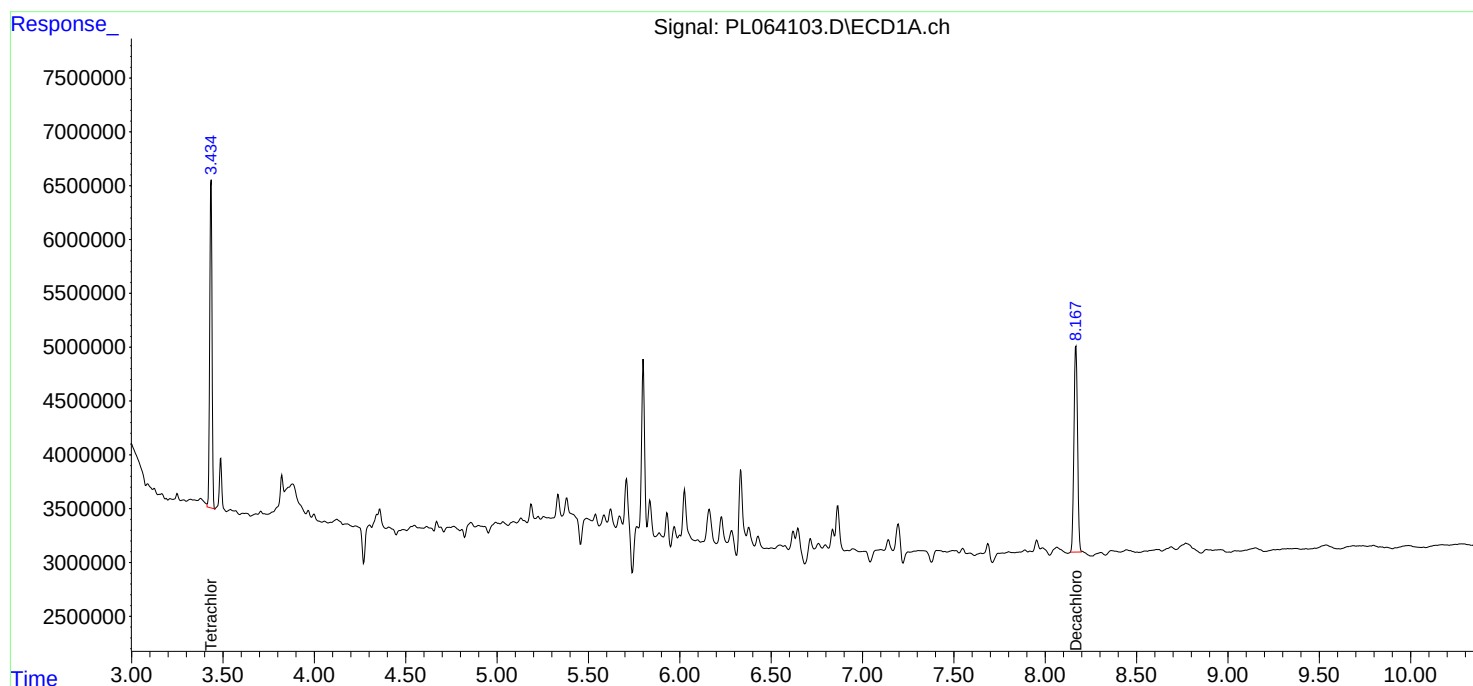

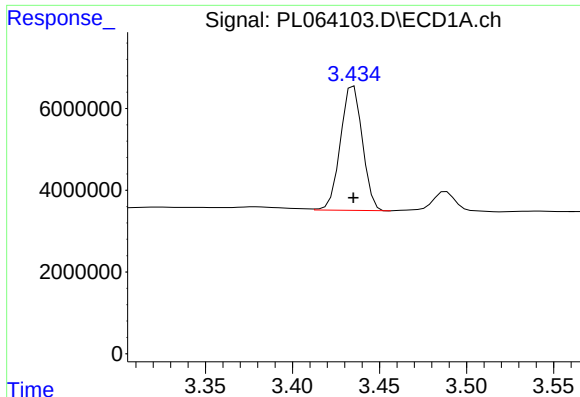


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 26710606
Conc: 8.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
Field Sampling Hourly Rate


Manual Integrations
APPROVED

Ankita
1/14/2021 2:20:48 PM

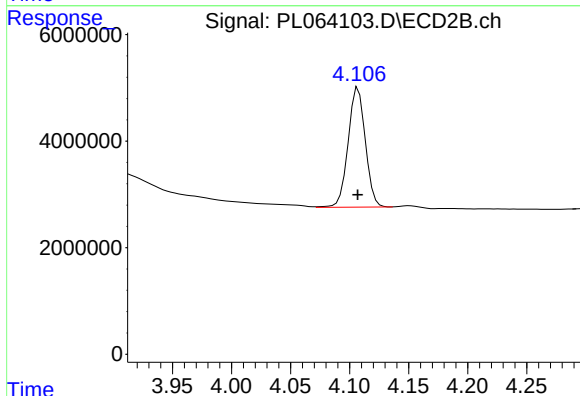


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 22791013
Conc: 8.92 ng/ml

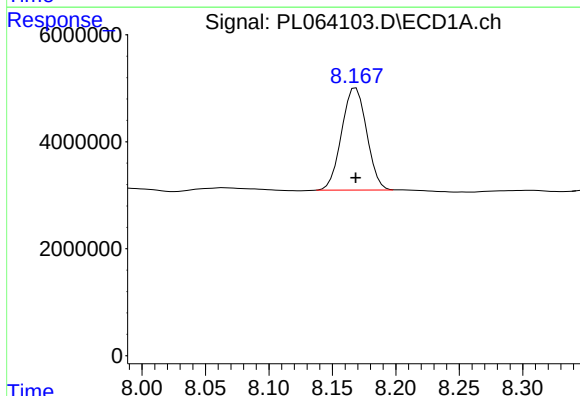

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 26237556
Conc: 8.60 ng/ml m

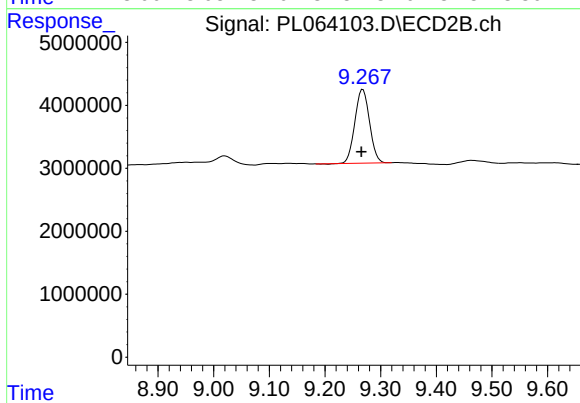

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 21429553
Conc: 9.03 ng/ml