

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
 Data File : PL071970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 08:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:14:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.494	10006045	27588375	21.660	22.454
28)	SA Decachlor...	10.322	11.389	14821210	25573964	20.499	21.581
Target Compounds							
7)	B delta-BHC	0.000	6.973f	0	400182	N.D.	0.261 #
9)	A Endosulfan I	0.000	8.343	0	100847	N.D.	0.081 #
10)	B gamma-Chl...	0.000	8.226	0	122886	N.D.	0.090 #
14)	MA Endrin	0.000	8.915f	0	250745	N.D.	0.242 #
15)	B Endosulfa...	0.000	9.149f	0	345008	N.D.	0.307 #
17)	MA 4,4'-DDT	0.000	9.328f	0	257095	N.D.	0.273 #
19)	B Endosulfa...	0.000	9.506	0	47672	N.D.	0.046 #
25)	Chlordane-3	0.000	8.226	0	122886	N.D.	0.602 #
27)	Chlordane-5	0.000	9.193	0	46771	N.D.	1.168 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
Data File : PL071970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 08:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:14:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

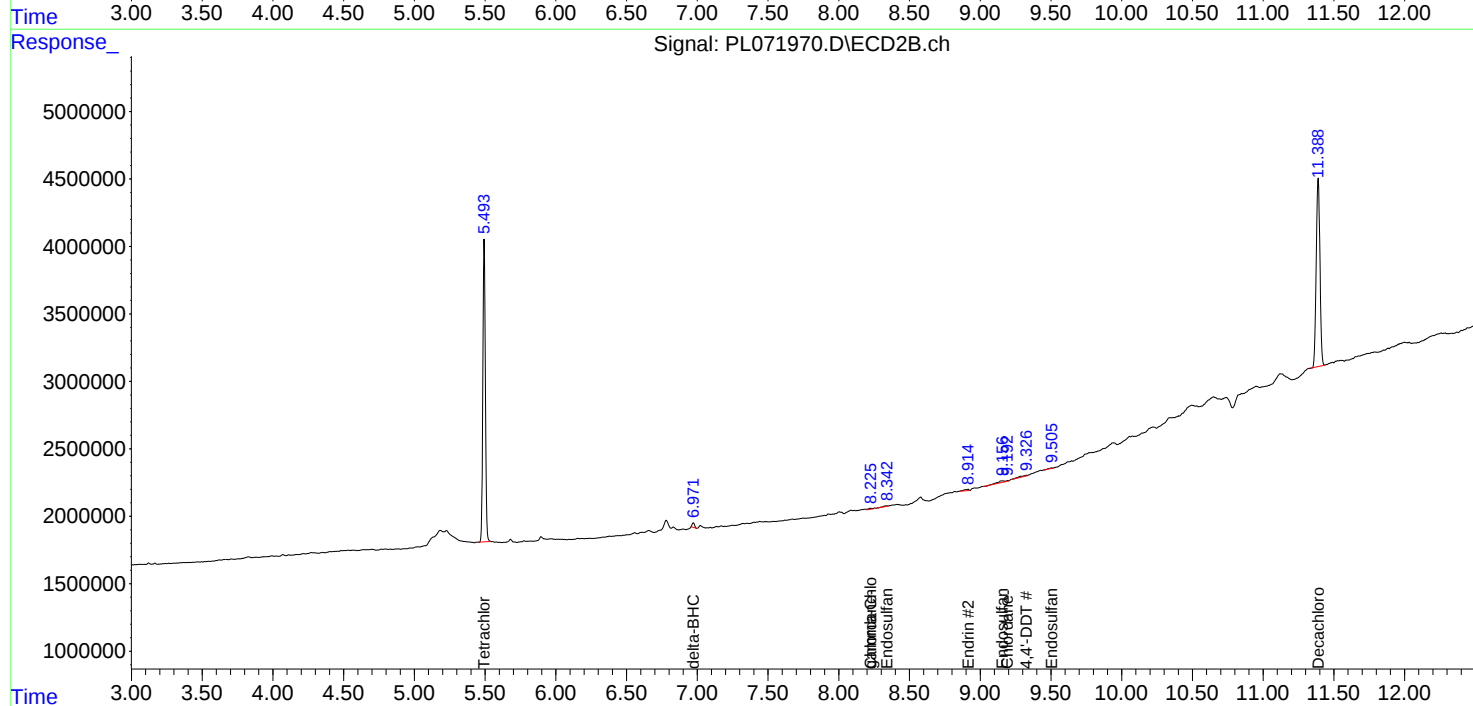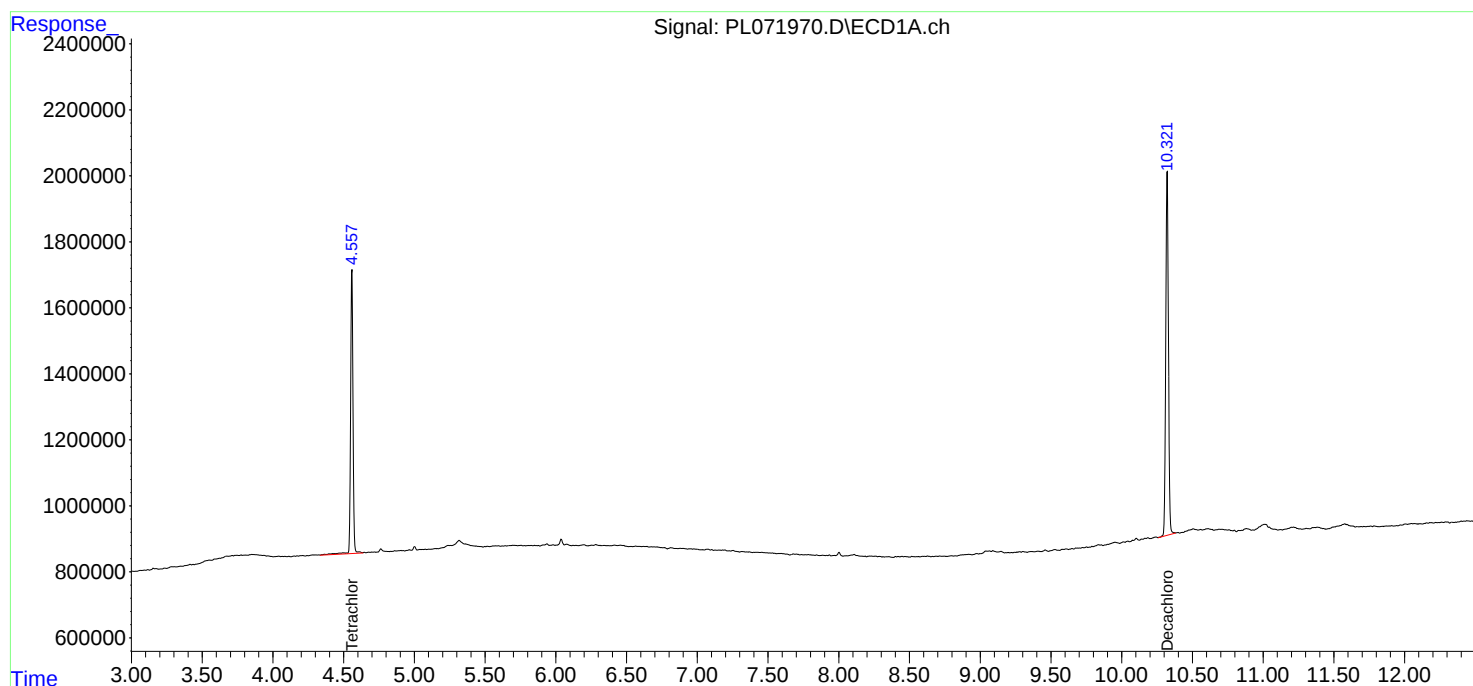


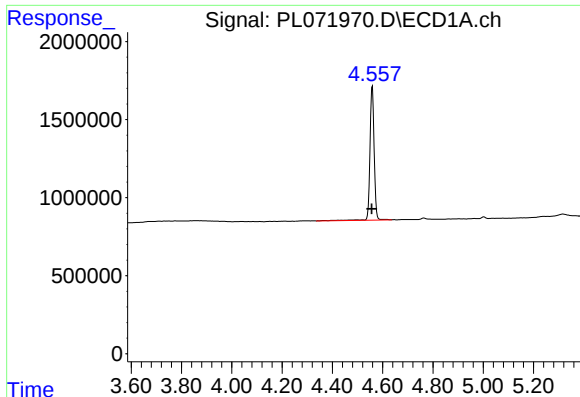

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: 0.003 min
Response: 10006045
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

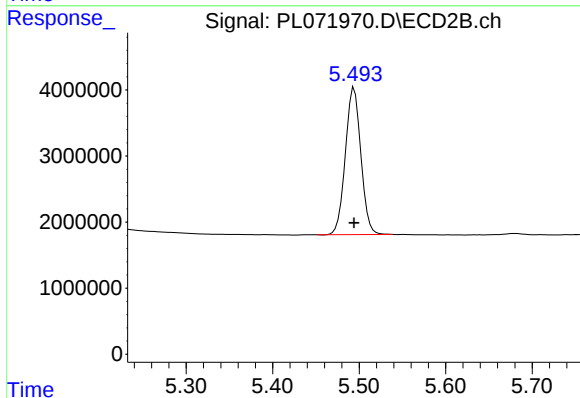


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 27588375
Conc: 22.45 ng/ml

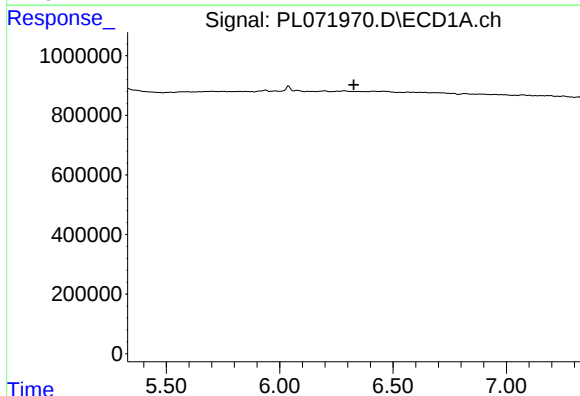


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

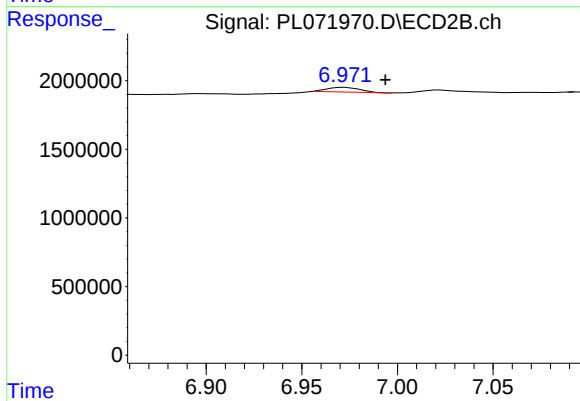

#7 delta-BHC


R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 400182
Conc: 0.26 ng/ml

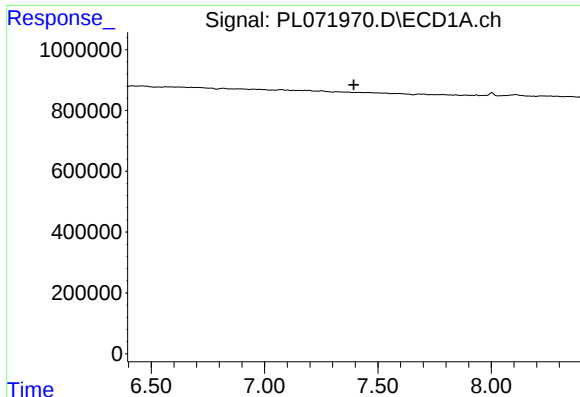

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

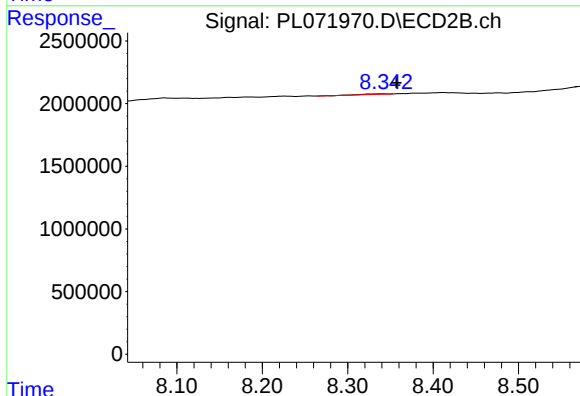


#9 Endosulfan I

R.T.: 8.343 min
Delta R.T.: -0.014 min
Response: 100847
Conc: 0.08 ng/ml

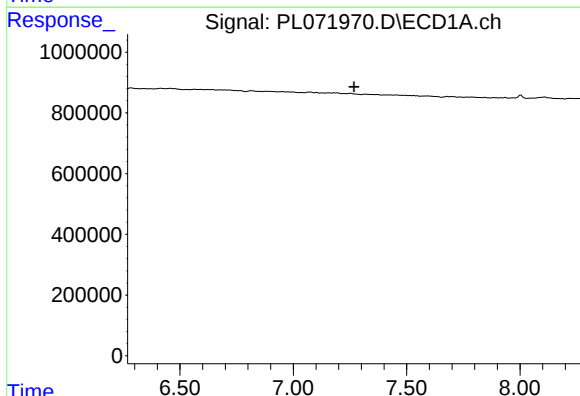


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

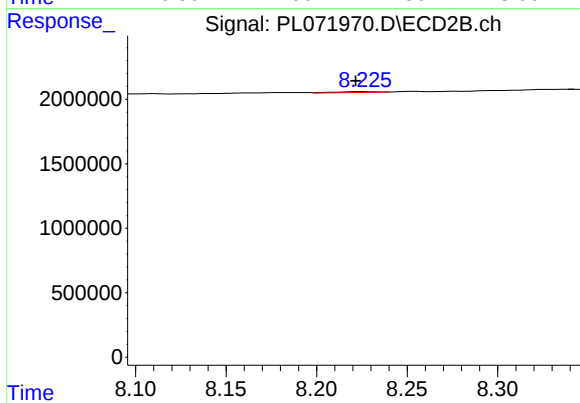

#10 gamma-Chlordane


R.T.: 8.226 min
Delta R.T.: 0.005 min
Response: 122886
Conc: 0.09 ng/ml

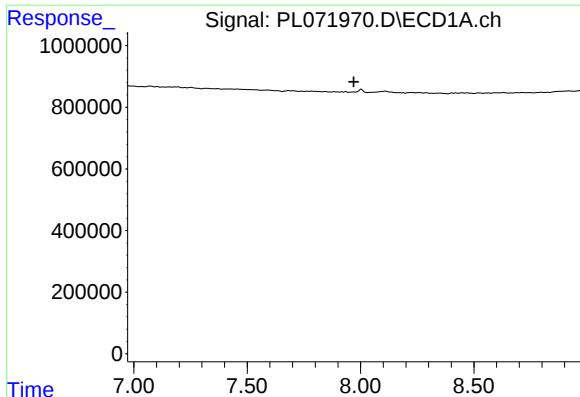

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

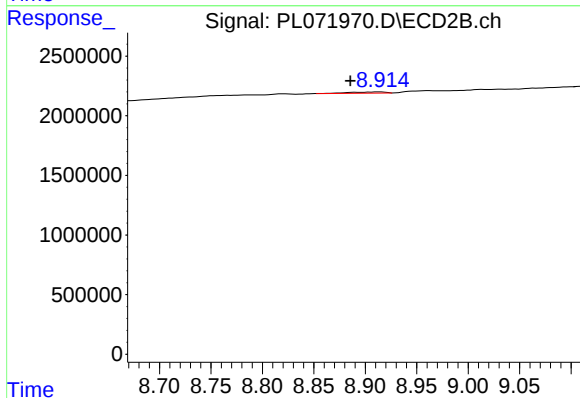


#14 Endrin

R.T.: 8.915 min
Delta R.T.: 0.030 min
Response: 250745
Conc: 0.24 ng/ml

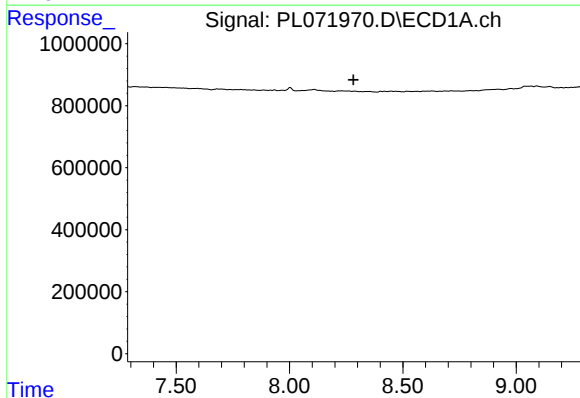


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

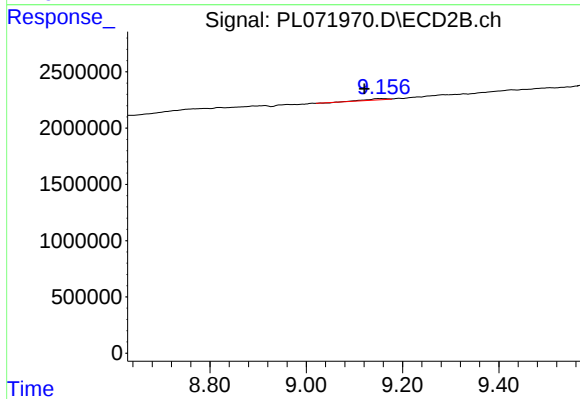

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.029 min
Response: 345008
Conc: 0.31 ng/ml

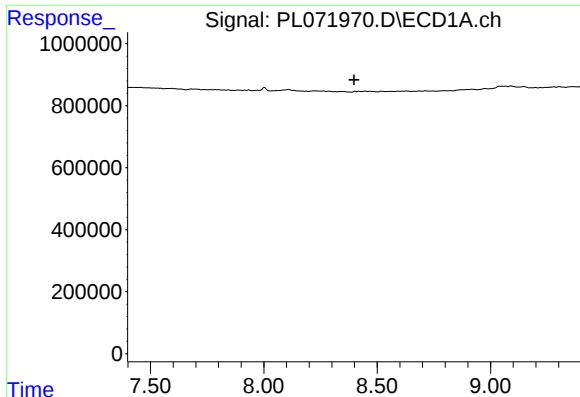

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

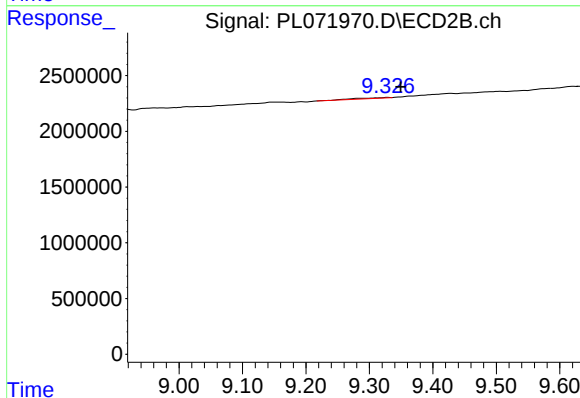


#17 4,4'-DDT

R.T.: 9.328 min
Delta R.T.: -0.021 min
Response: 257095
Conc: 0.27 ng/ml

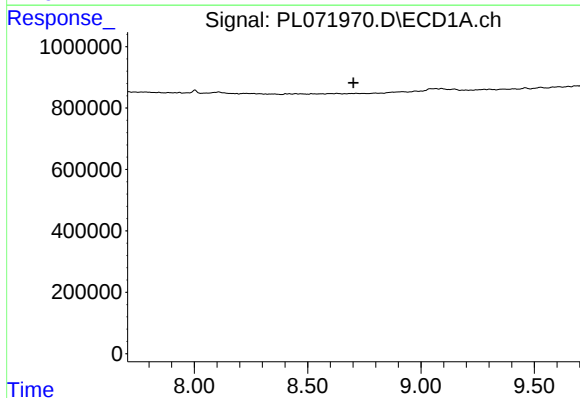


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

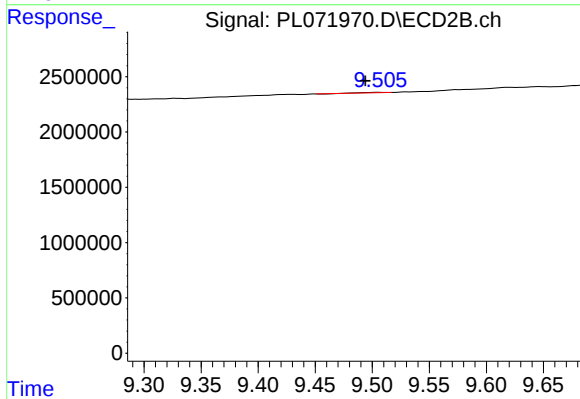

#19 Endosulfan Sulfate


R.T.: 9.506 min
Delta R.T.: 0.012 min
Response: 47672
Conc: 0.05 ng/ml

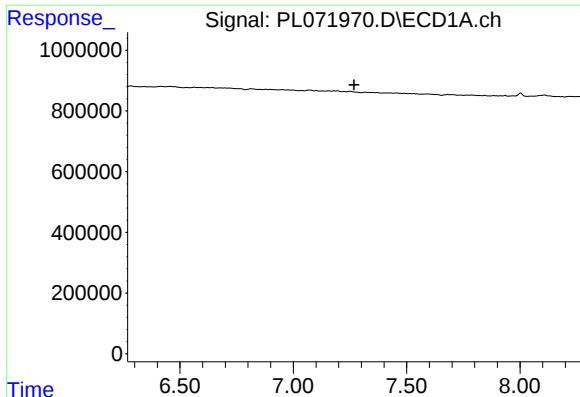

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

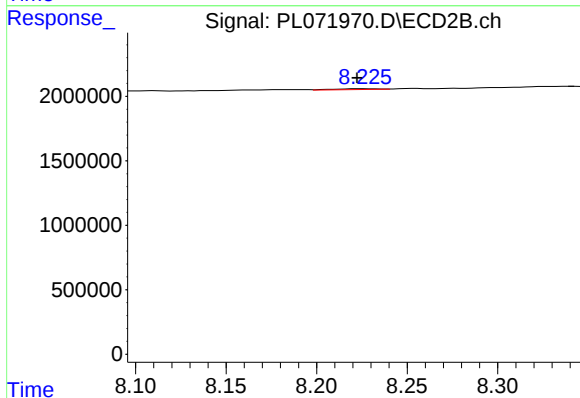


#25 Chlordane-3

R.T.: 8.226 min
Delta R.T.: 0.004 min
Response: 122886
Conc: 0.60 ng/ml

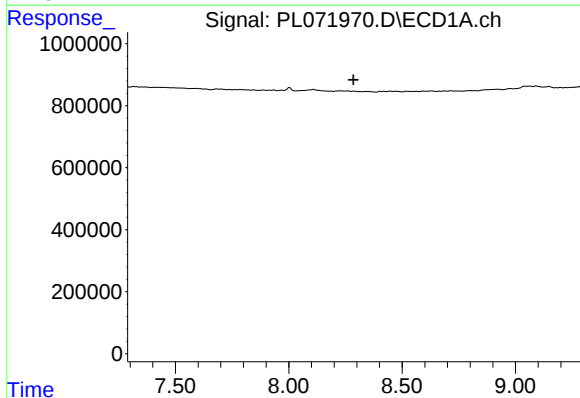


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

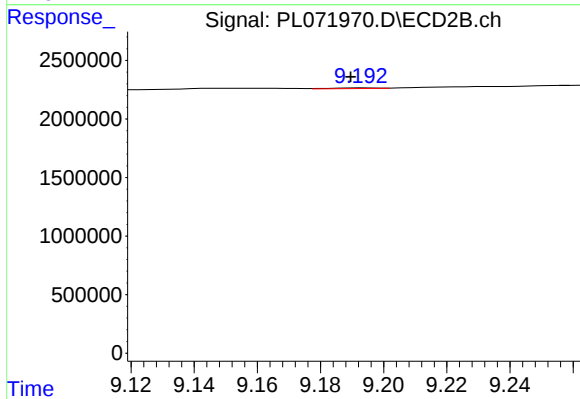

#27 Chlordane-5


R.T.: 9.193 min
Delta R.T.: 0.004 min
Response: 46771
Conc: 1.17 ng/ml

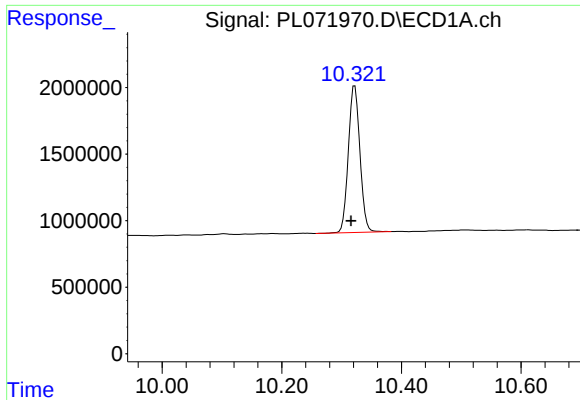

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 14821210
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

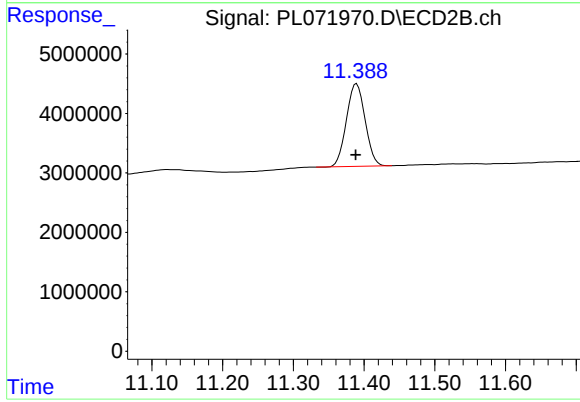

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.001 min
Response: 25573964
Conc: 21.58 ng/ml