

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
 Data File : PL071978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 14:41
 Operator : AR\AJ
 Sample : PB142001BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB142001BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:15:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	5.493	9659620	26685985	20.911	21.720
2) SA Decachlor...	10.319	11.388	15783152	27197686	21.829m	22.951

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
Data File : PL071978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 14:41
Operator : AR\AJ
Sample : PB142001BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB142001BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:15:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

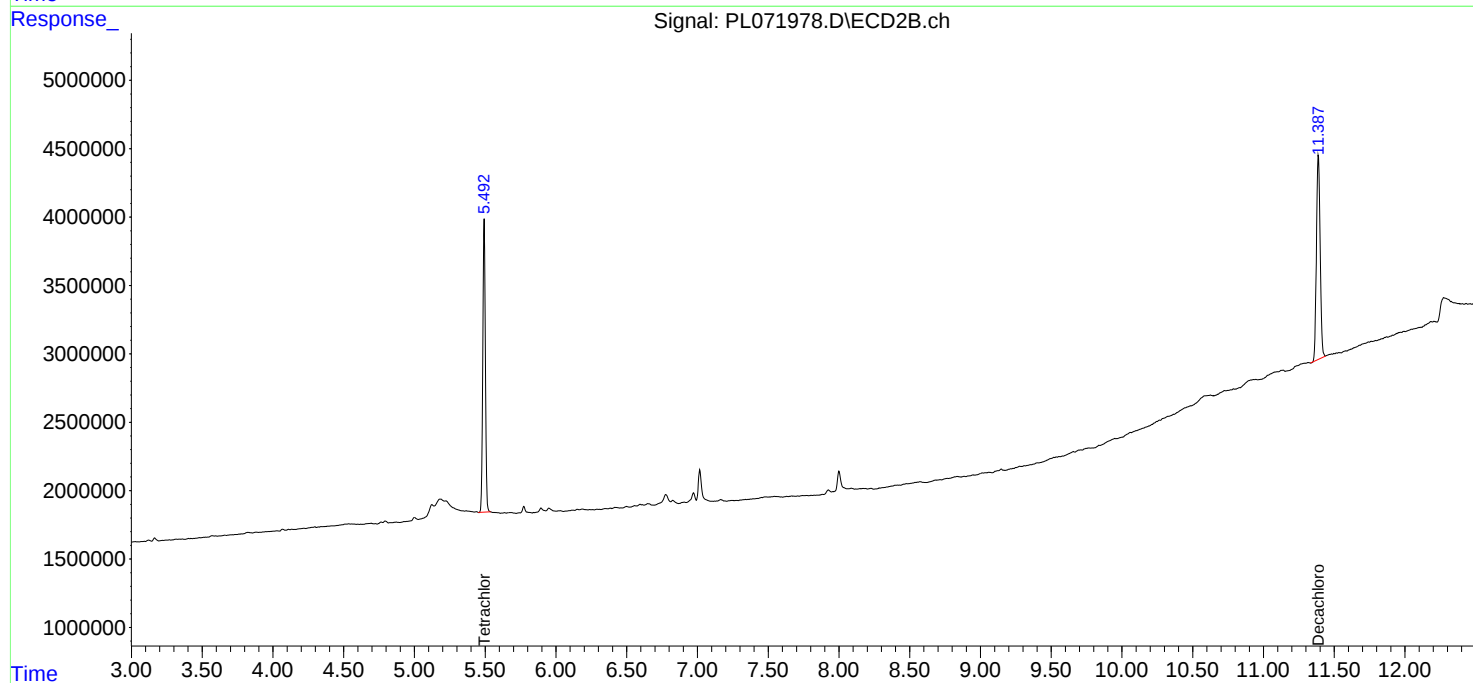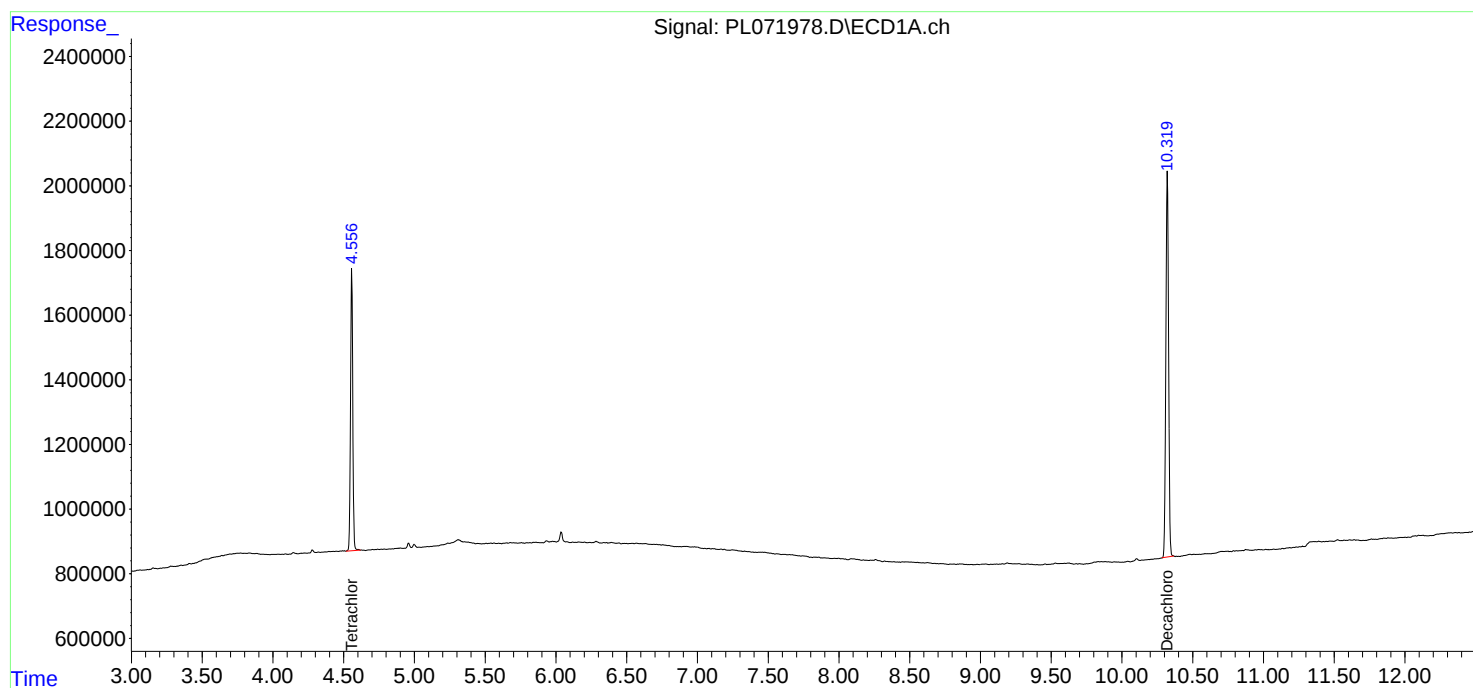

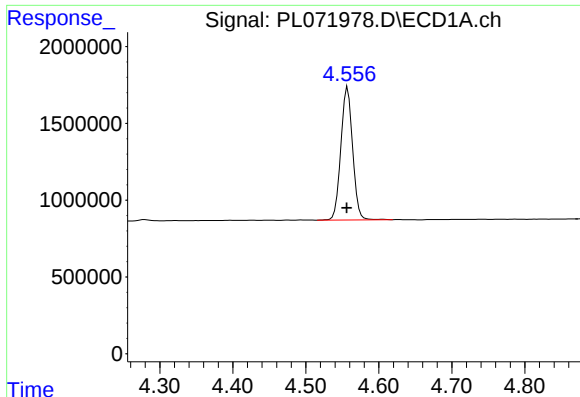


#1 Tetrachloro-m-xylene

R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 9659620
Conc: 20.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB142001BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

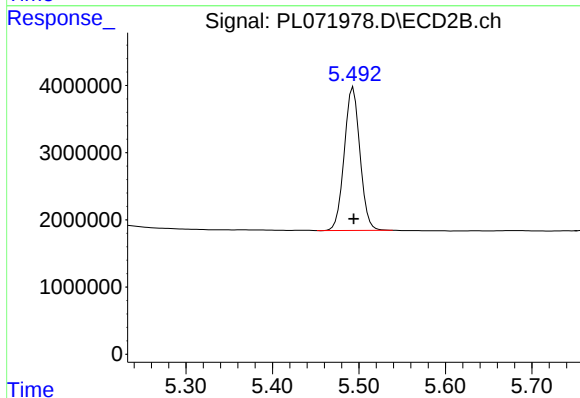


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 26685985
Conc: 21.72 ng/ml

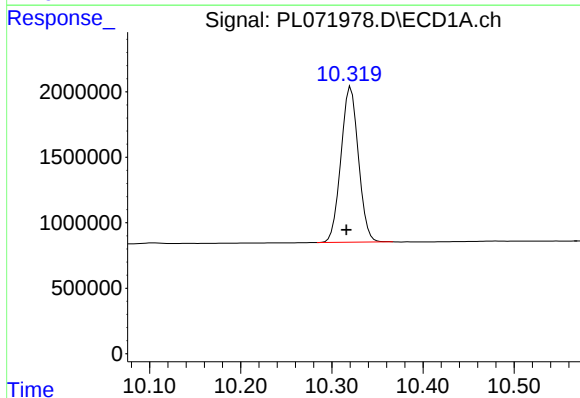

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: 0.004 min
Response: 15783152
Conc: 21.83 ng/ml m

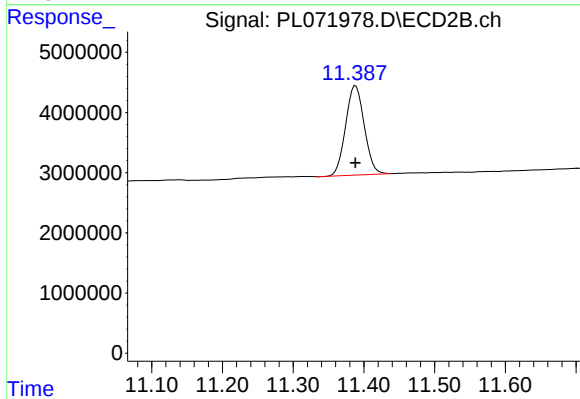

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.000 min
Response: 27197686
Conc: 22.95 ng/ml