

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
 Data File : PL071985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 16:42
 Operator : AR\AJ
 Sample : N1098-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 14-G-WATER

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:17:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	5.494	9881465	27398227	21.391	22.300
28) SA Decachlor...	10.321	11.387	10946189	19604906	15.139	16.544m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011322\
Data File : PL071985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 16:42
Operator : AR\AJ
Sample : N1098-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
14-G-WATER


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:17:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

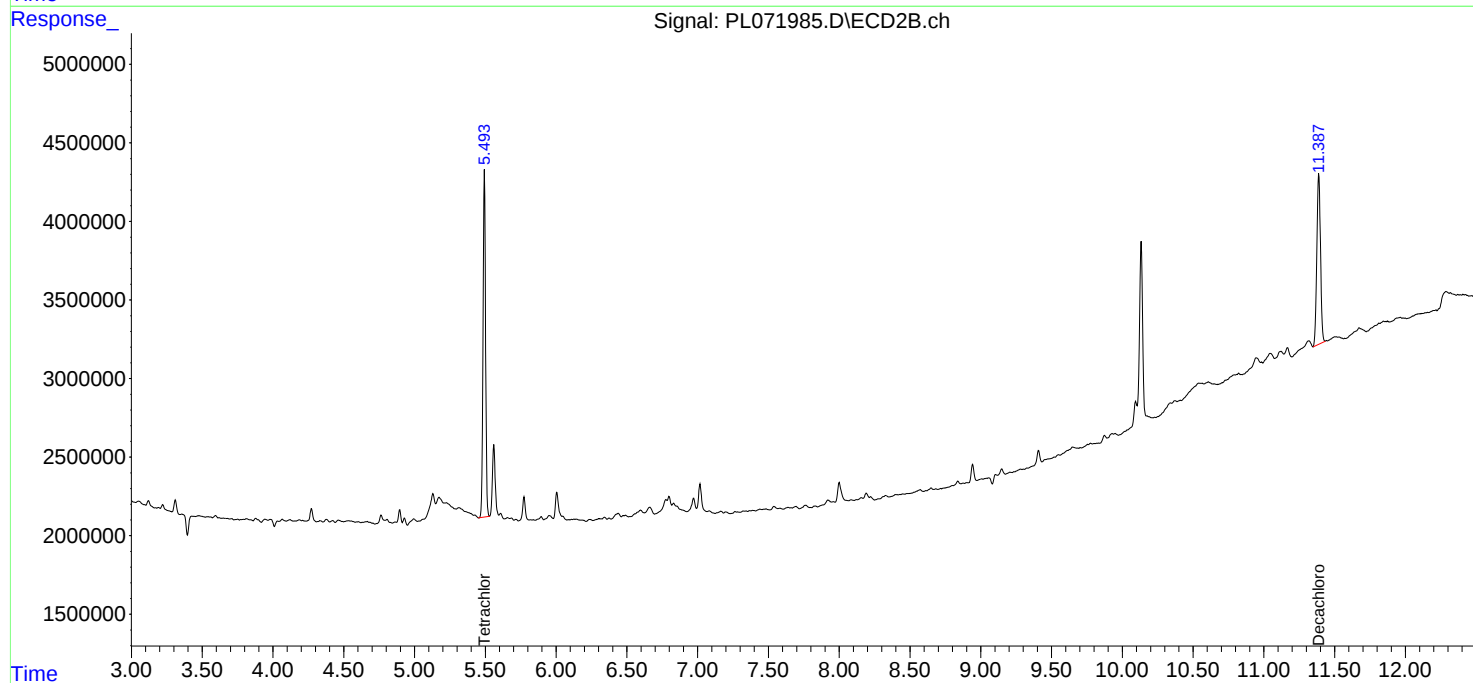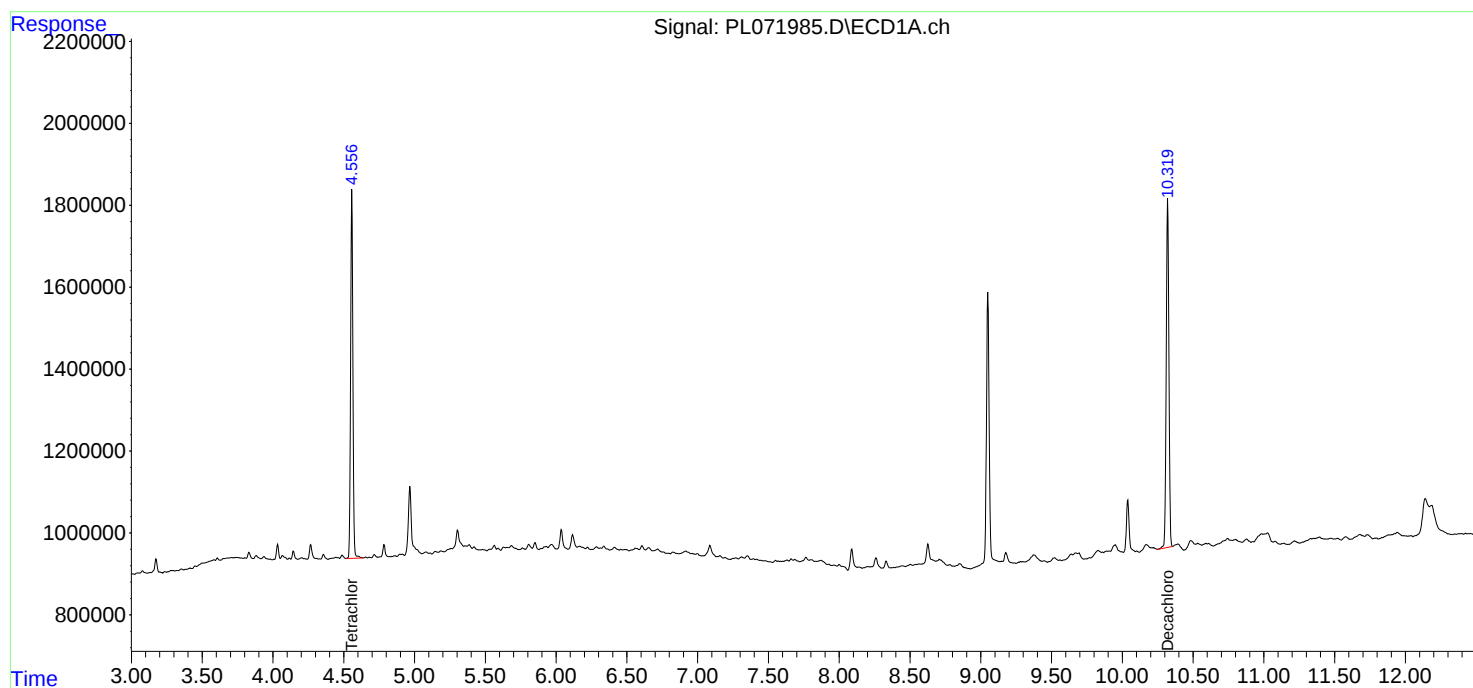

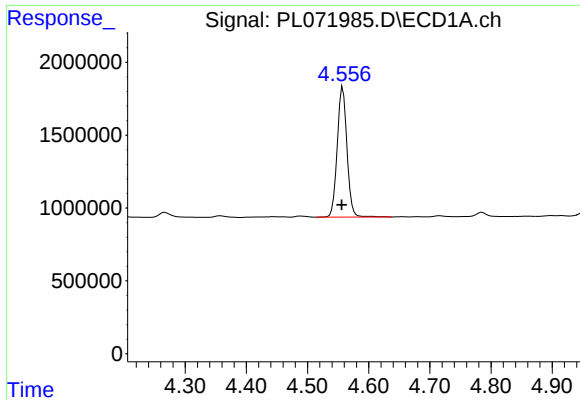


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9881465
Conc: 21.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
14-G-WATER


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

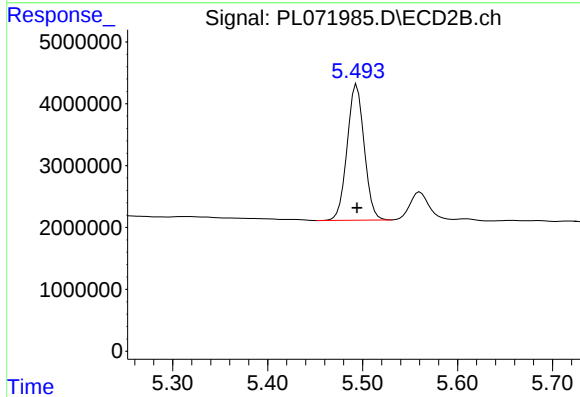


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 27398227
Conc: 22.30 ng/ml

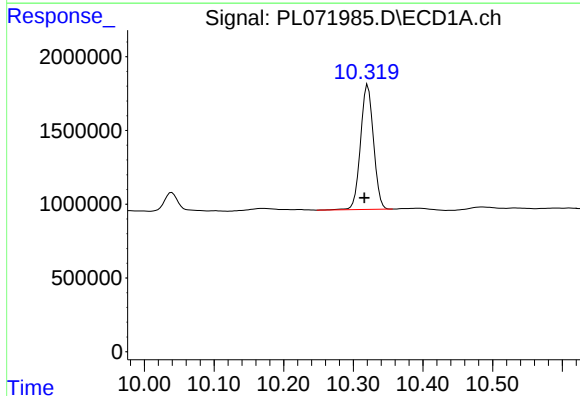

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.005 min
Response: 10946189
Conc: 15.14 ng/ml

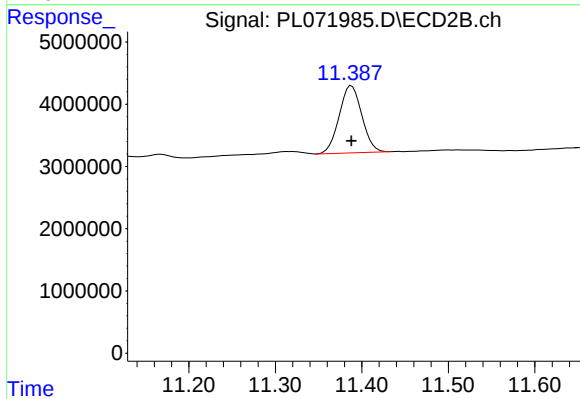

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.001 min
Response: 19604906
Conc: 16.54 ng/ml m