

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011323\
 Data File : PL080294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 13:08
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 20:33:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.691	102.1E6	130.0E6	51.094	58.136
28)	SA Decachlor...	8.788	7.840	75080455	106.0E6	50.888	47.165
Target Compounds							
23)	Chlordane-1	4.499	3.689	41466029	39404819	532.544	483.229
24)	Chlordane-2	5.025	4.266	44766283	45023324	508.746	429.625
25)	Chlordane-3	5.731	4.895	133.8E6	122.7E6	412.105	429.621m
26)	Chlordane-4	5.813	4.959	199.8E6	124.4E6	500.070	434.903
27)	Chlordane-5	6.655	5.627	35290130	35250700	498.610	440.992



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 13:08
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 20:33:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

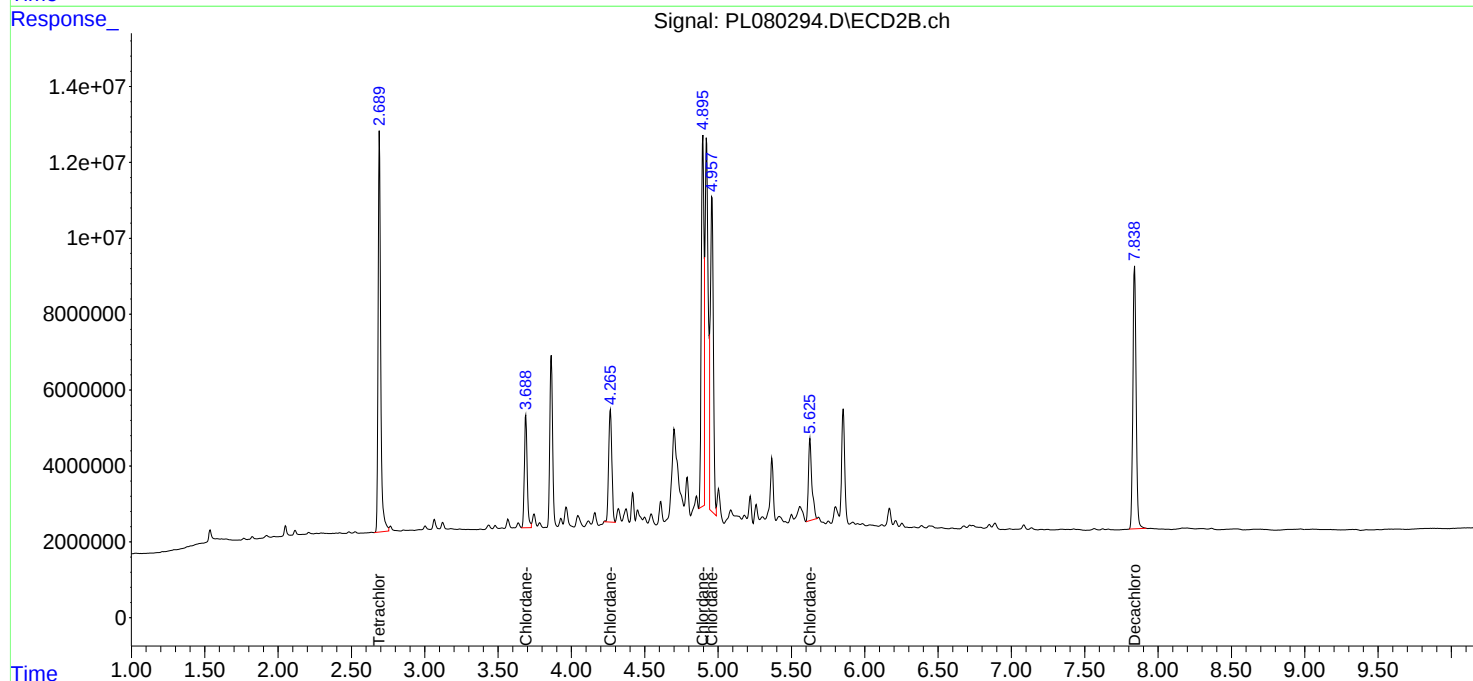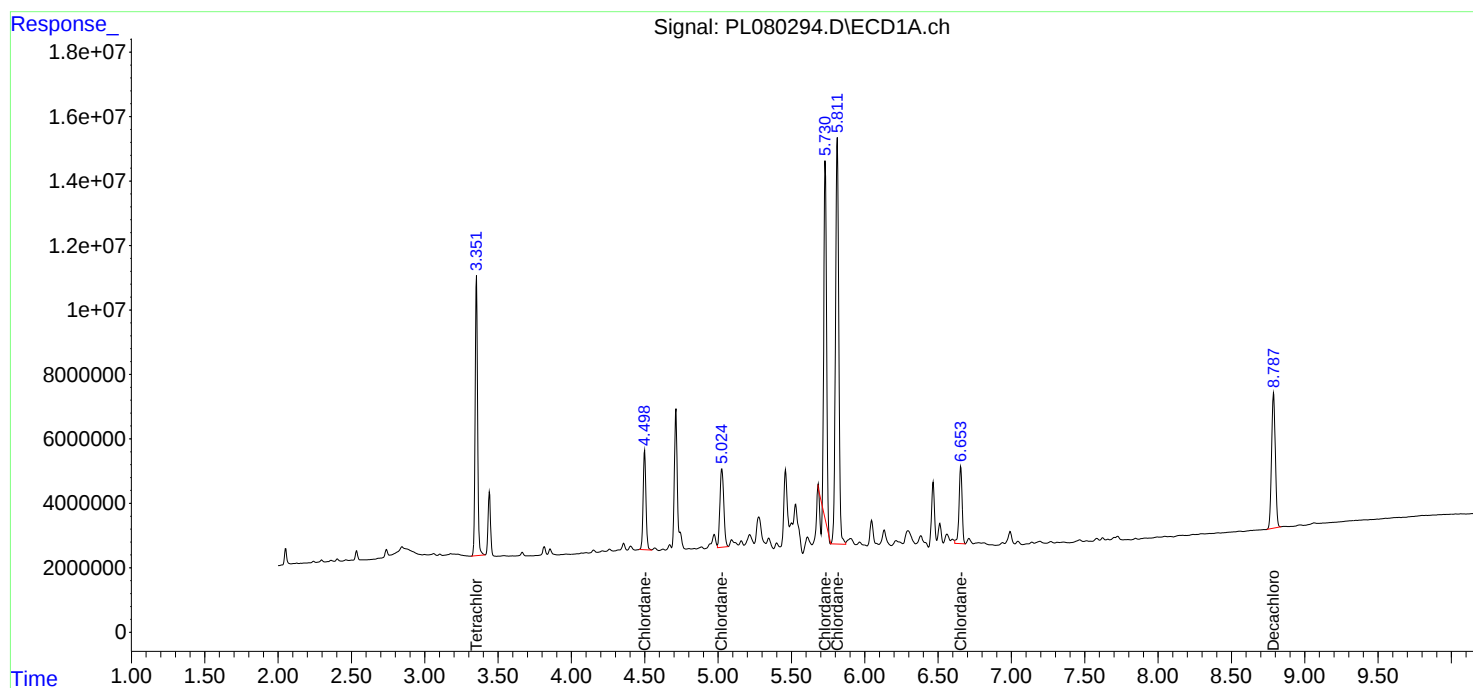


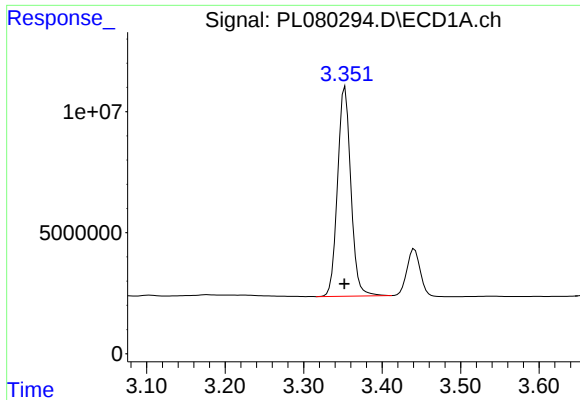

#1 Tetrachloro-m-xylene


R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 102068798
Conc: 51.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

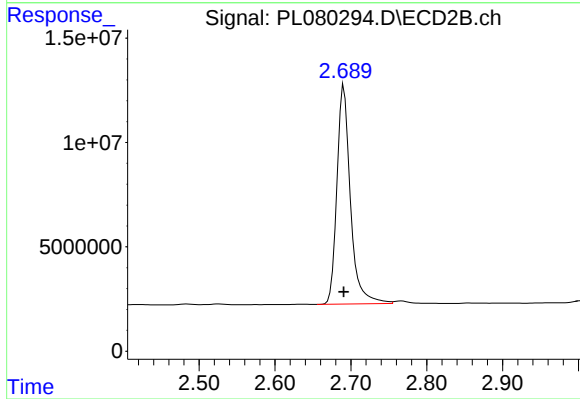


#1 Tetrachloro-m-xylene

R.T.: 2.691 min
Delta R.T.: 0.000 min
Response: 130025302
Conc: 58.14 ng/ml

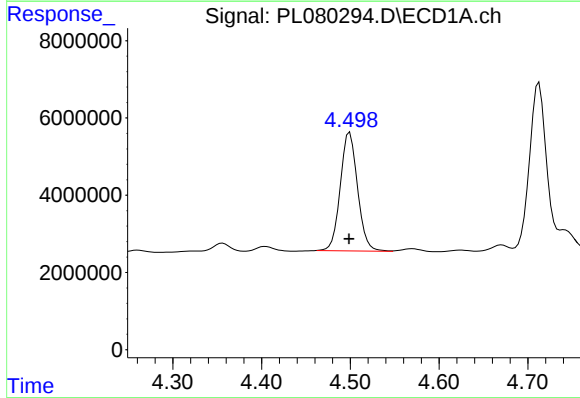


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 41466029
Conc: 532.54 ng/ml

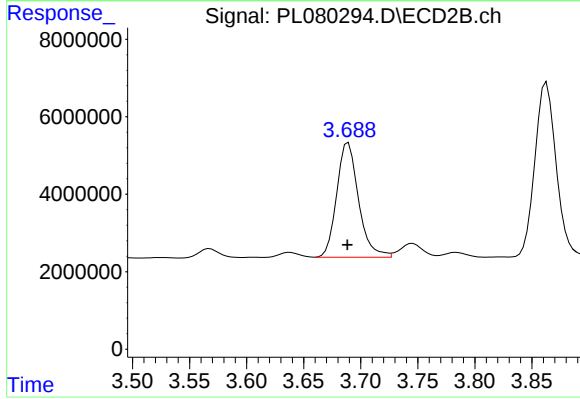

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 39404819
Conc: 483.23 ng/ml

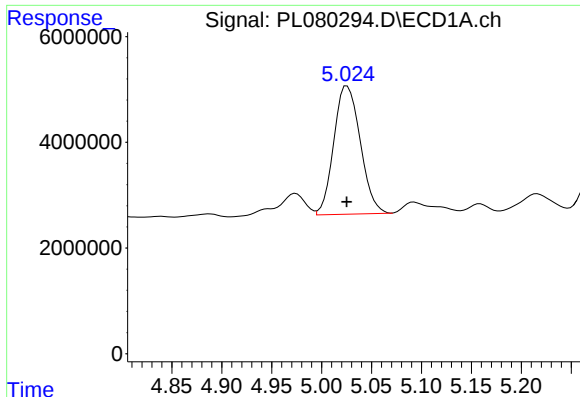

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 44766283
Conc: 508.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

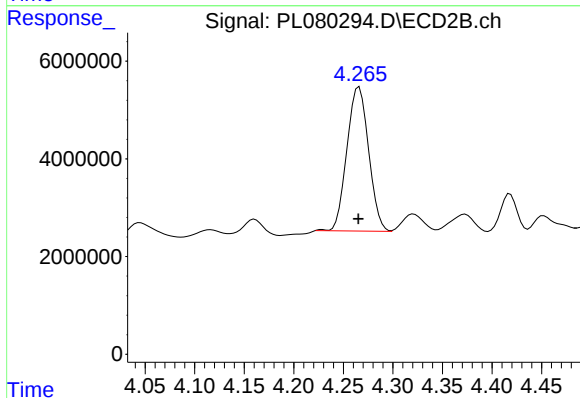


#24 Chlordane-2

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 45023324
Conc: 429.62 ng/ml

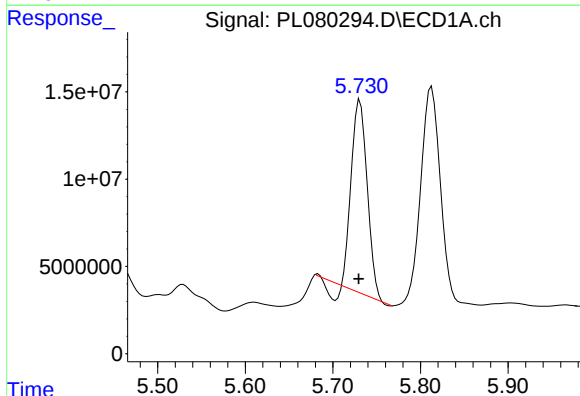


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.001 min
Response: 133753911
Conc: 412.11 ng/ml

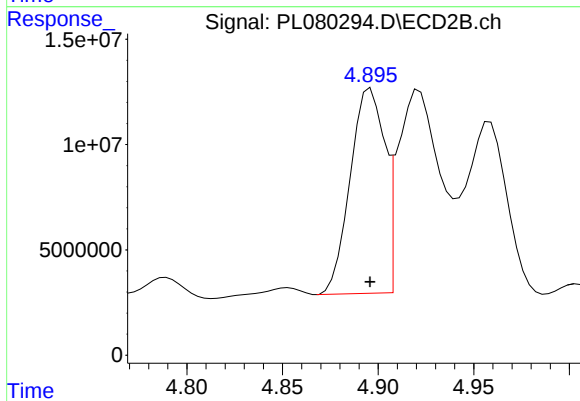

#25 Chlordane-3


R.T.: 4.895 min
Delta R.T.: -0.001 min
Response: 122651964
Conc: 429.62 ng/ml m

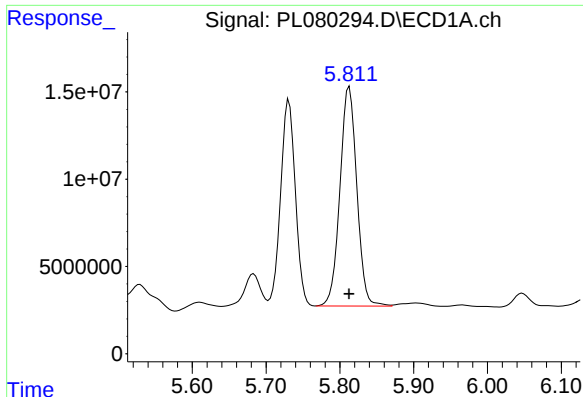

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 199771902
Conc: 500.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

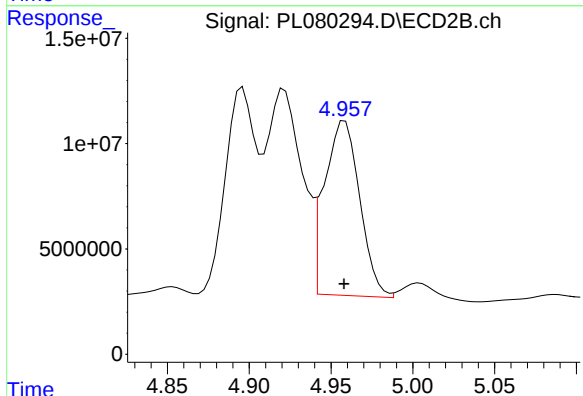


#26 Chlordane-4

R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 124400788
Conc: 434.90 ng/ml

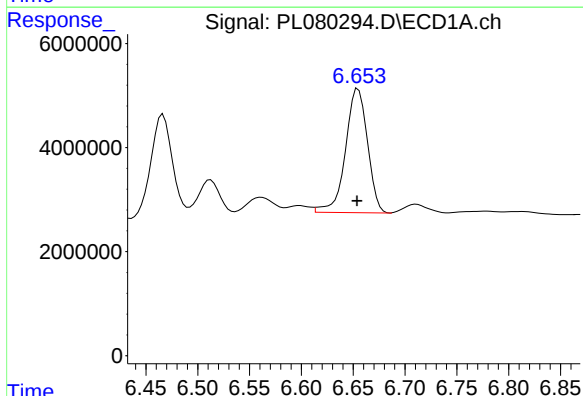


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: 0.001 min
Response: 35290130
Conc: 498.61 ng/ml

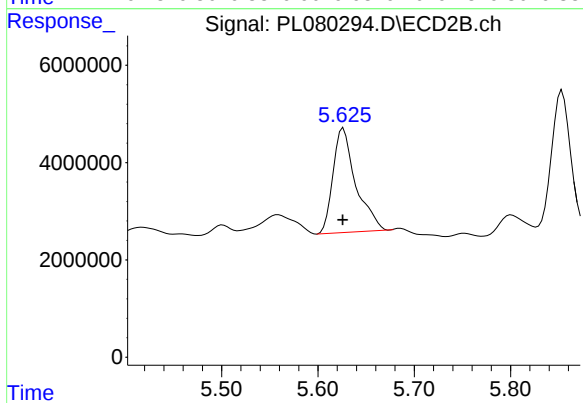

#27 Chlordane-5


R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 35250700
Conc: 440.99 ng/ml

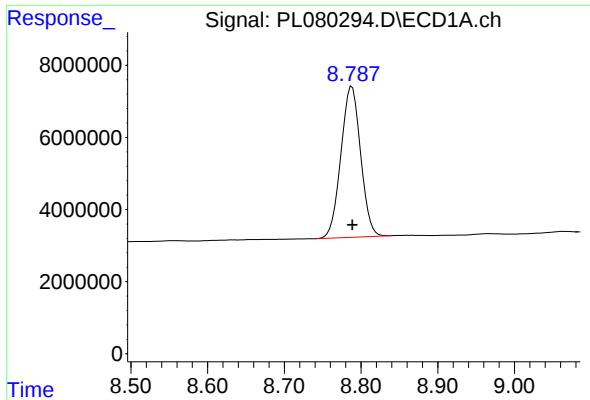

#28 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 75080455
Conc: 50.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

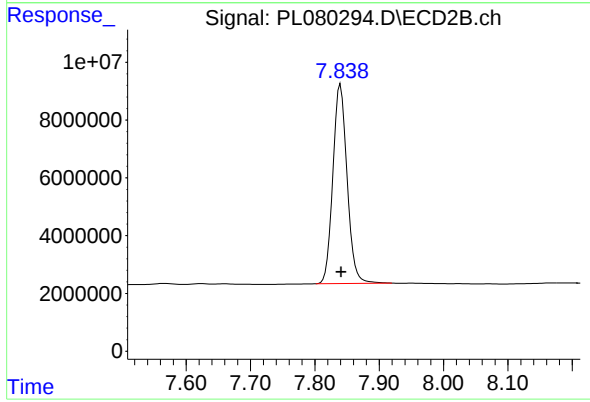

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 106019742
Conc: 47.17 ng/ml