

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011419\
 Data File : PL043859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2019 12:09
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:34:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	8.193f	0.000	1058721	0	0.187	N.D. #
Target Compounds							
3)	MA gamma-BHC...	4.263	0.000	3732687	0	0.535	N.D. #
4)	MA Heptachlor	4.475f	0.000	5001534	0	0.718	N.D. #
6)	B beta-BHC	4.475	0.000	5001534	0	1.680	N.D. #
7)	B delta-BHC	4.703	0.000	2180805	0	0.339	N.D. #
9)	A Endosulfan I	5.574	0.000	2111143	0	0.362	N.D. #
11)	B alpha-Chl...	5.574f	0.000	2111143	0	0.334	N.D. #
21)	B Endrin ke...	7.151f	0.000	3927955	0	0.652	N.D. #
23)	Chlordane-1	4.424	0.000	4086273	0	18.268	N.D. #
24)	Chlordane-2	4.900	0.000	4494966	0	18.478	N.D. #
26)	Chlordane-4	5.574	0.000	2111143	0	3.313	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011419\
Data File : PL043859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2019 12:09
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:34:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

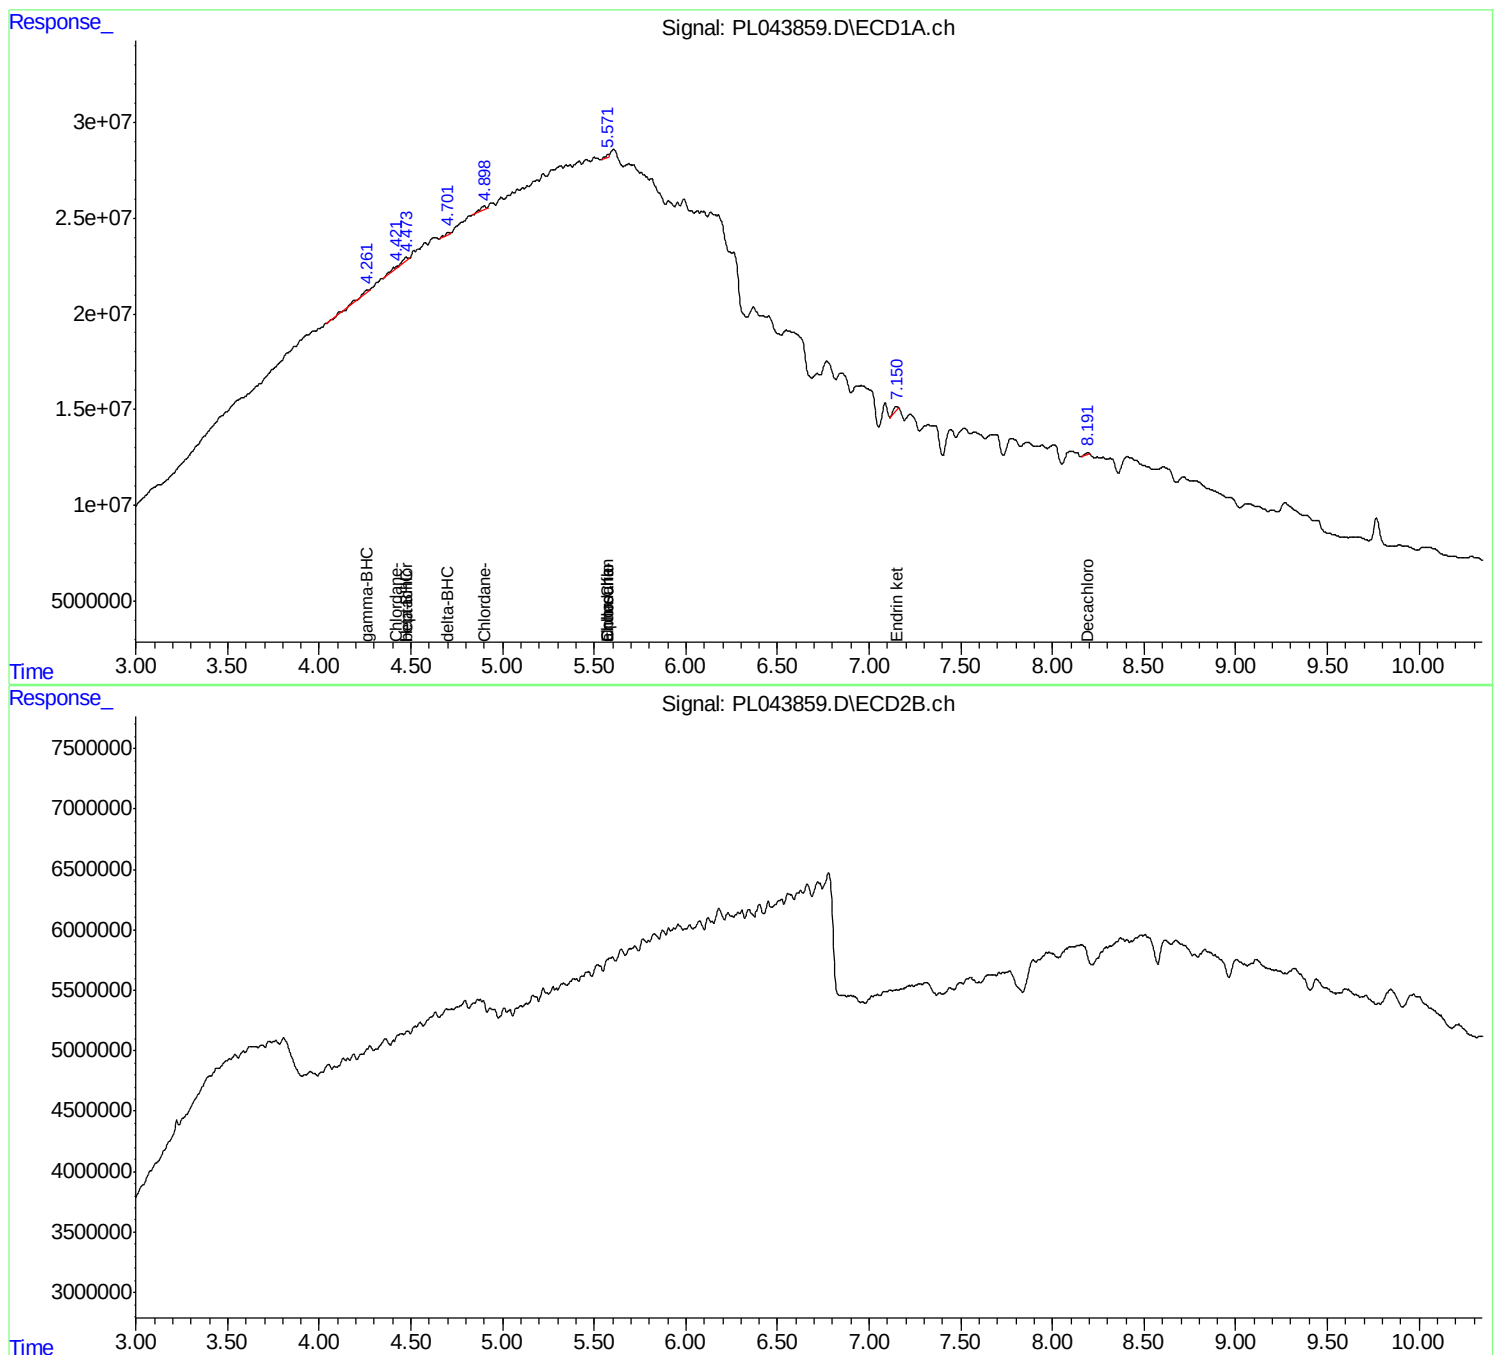


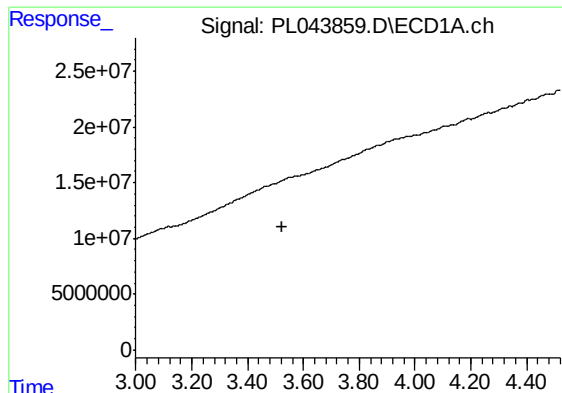

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

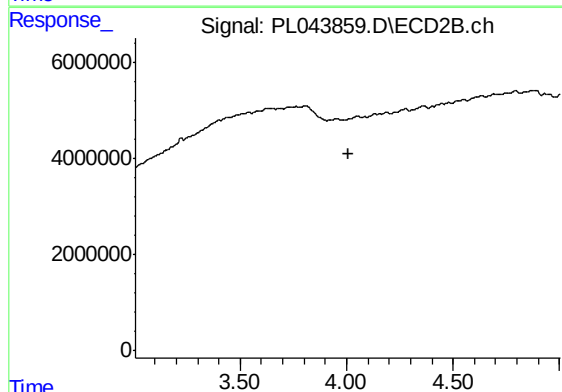


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

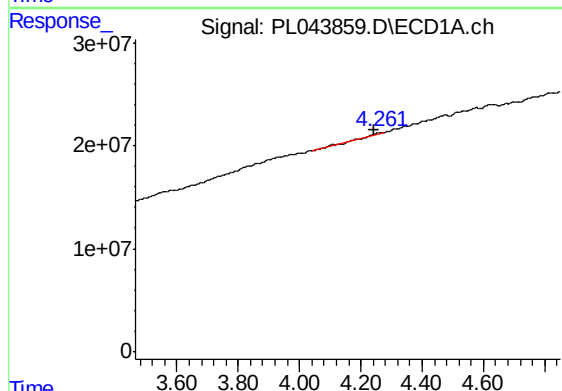


#3 gamma-BHC (Lindane)

R.T.: 4.263 min
Delta R.T.: 0.018 min
Response: 3732687
Conc: 0.54 ng/ml

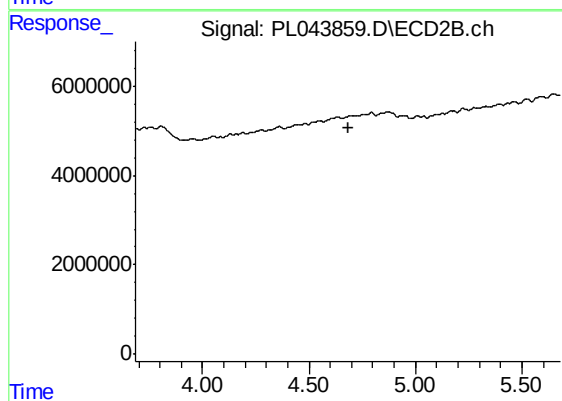

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.684 min
Response: 0
Conc: N.D.

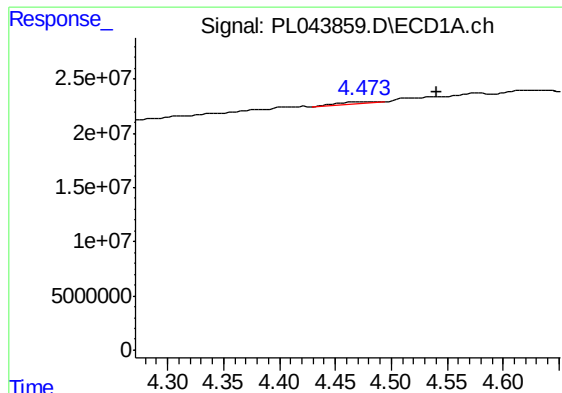

#4 Heptachlor


R.T.: 4.475 min
Delta R.T.: -0.066 min
Response: 5001534
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

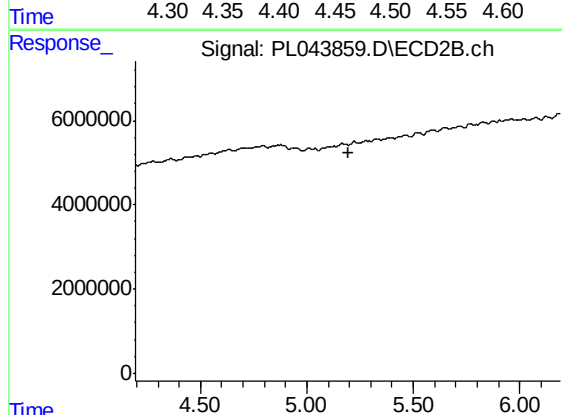


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.193 min
Response: 0
Conc: N.D.

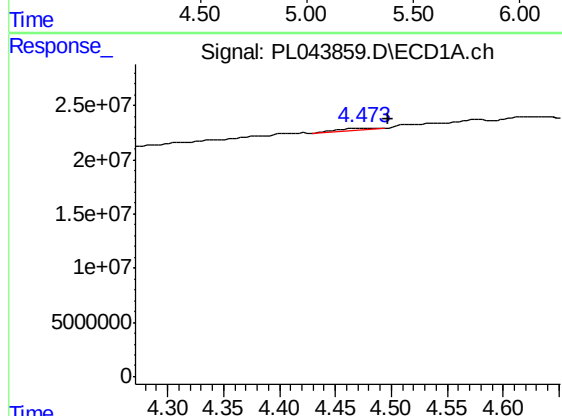


#6 beta-BHC

R.T.: 4.475 min
Delta R.T.: -0.022 min
Response: 5001534
Conc: 1.68 ng/ml

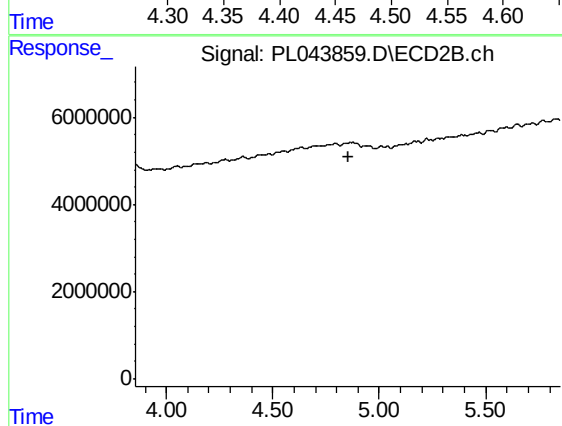

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

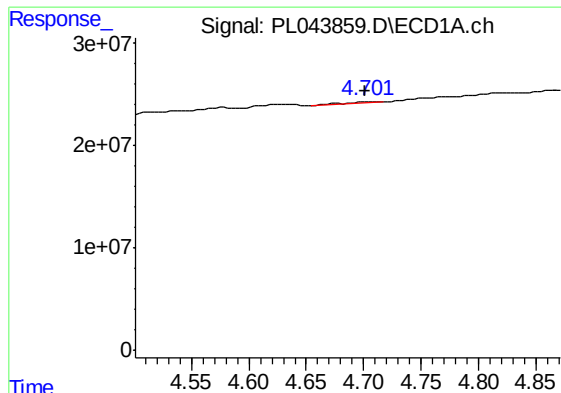

#7 delta-BHC


R.T.: 4.703 min
Delta R.T.: 0.002 min
Response: 2180805
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

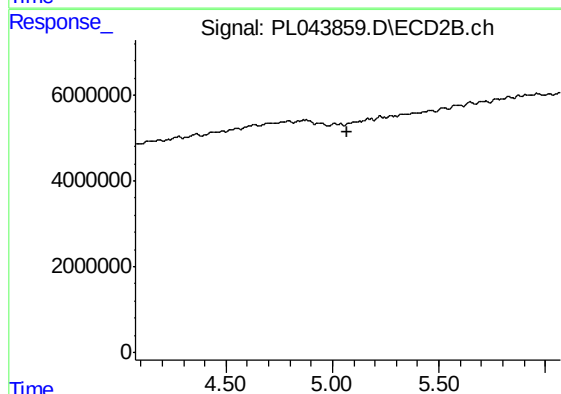


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.072 min
Response: 0
Conc: N.D.

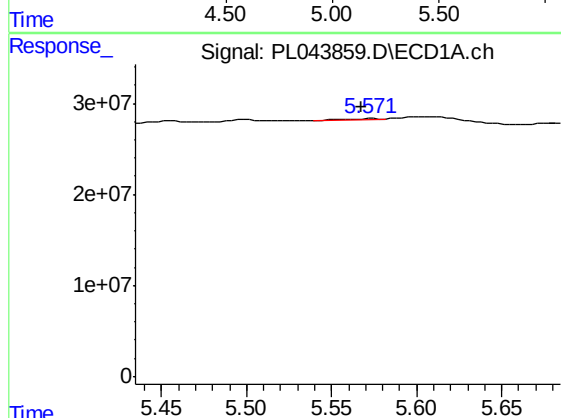


#9 Endosulfan I

R.T.: 5.574 min
Delta R.T.: 0.006 min
Response: 2111143
Conc: 0.36 ng/ml

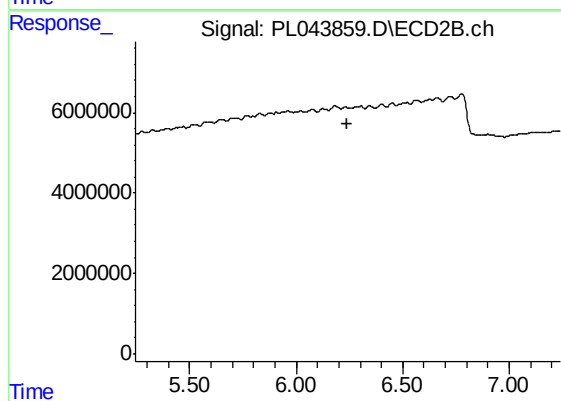

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

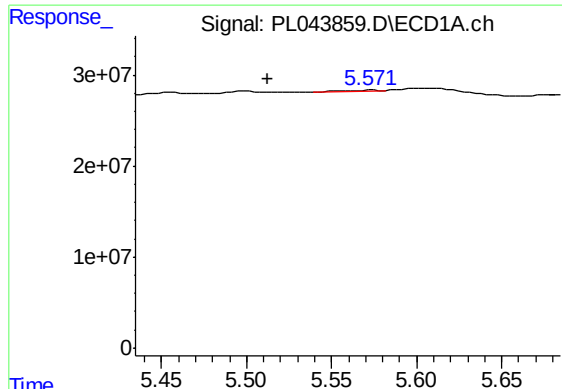

#11 alpha-Chlordane


R.T.: 5.574 min
Delta R.T.: 0.061 min
Response: 2111143
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

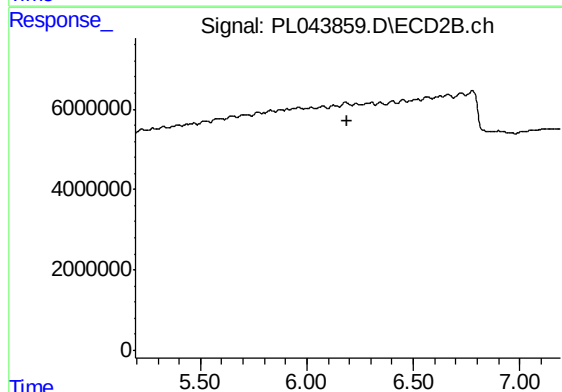


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

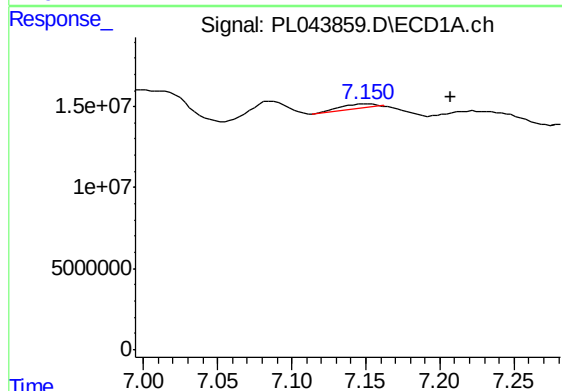


#21 Endrin ketone

R.T.: 7.151 min
Delta R.T.: -0.056 min
Response: 3927955
Conc: 0.65 ng/ml

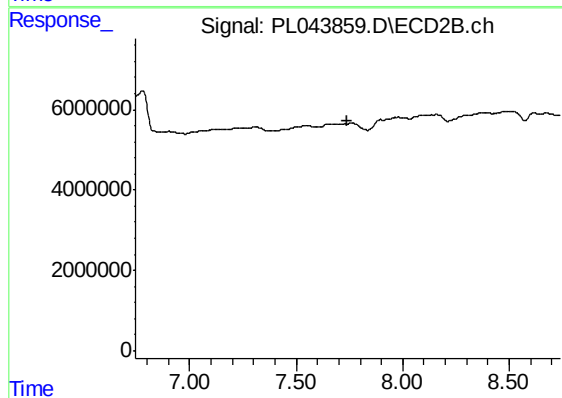

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.742 min
Response: 0
Conc: N.D.

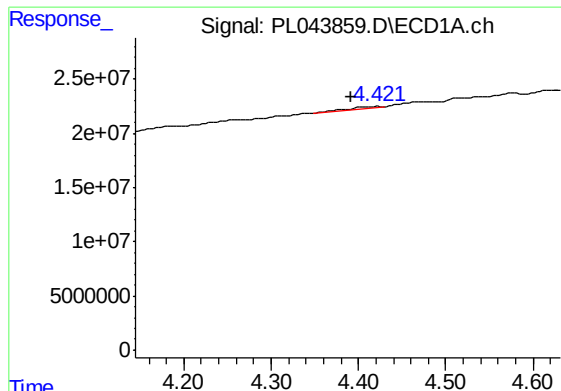

#23 Chlordane-1


R.T.: 4.424 min
Delta R.T.: 0.033 min
Response: 4086273
Conc: 18.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

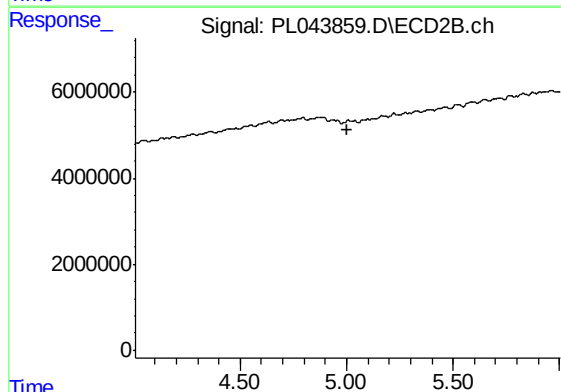


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

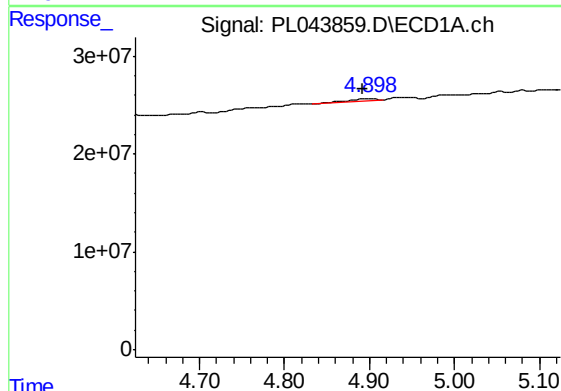


#24 Chlordane-2

R.T.: 4.900 min
Delta R.T.: 0.009 min
Response: 4494966
Conc: 18.48 ng/ml

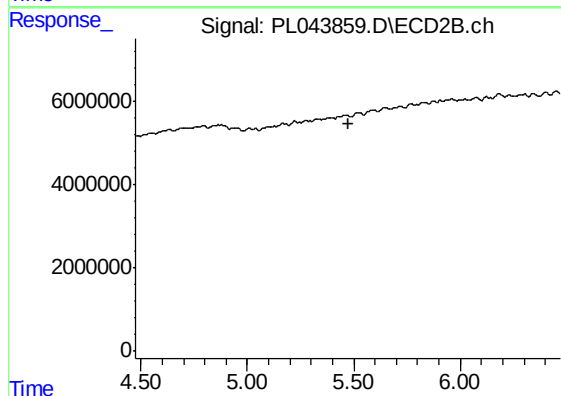

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.473 min
Response: 0
Conc: N.D.

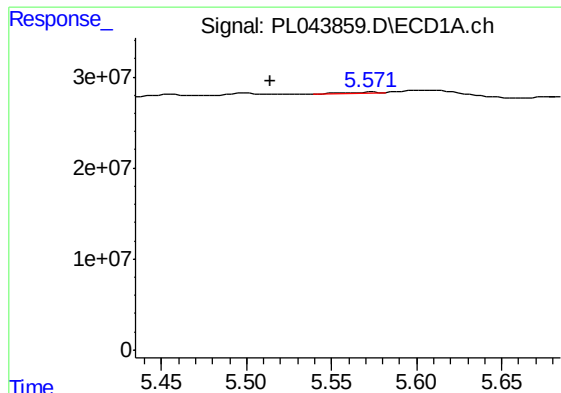

#26 Chlordane-4


R.T.: 5.574 min
Delta R.T.: 0.059 min
Response: 2111143
Conc: 3.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

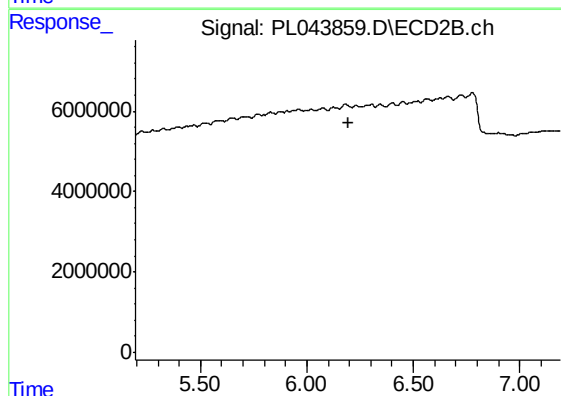


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.194 min
Response: 0
Conc: N.D.

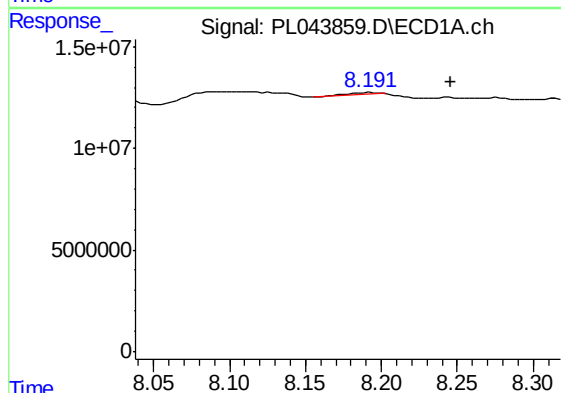

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: -0.053 min
Response: 1058721
Conc: 0.19 ng/ml

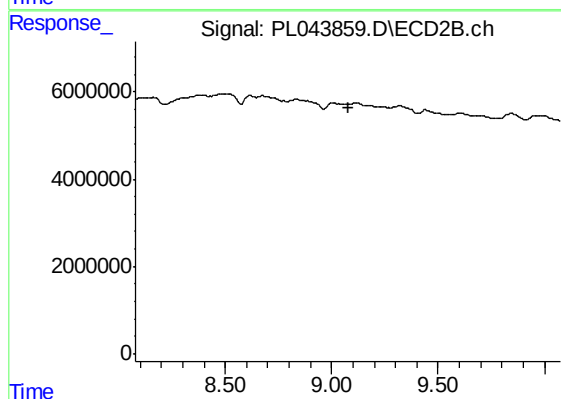

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.