

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011419\
 Data File : PL043867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2019 14:06
 Operator : AJ\SJ
 Sample : K1015-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-02-011119-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:36:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	4.007	59126122	24008320	12.045	12.319
28)	SA Decachlor...	8.250	9.078	74414925	23397140	13.168	14.728
Target Compounds							
6)	B beta-BHC	4.455f	0.000	3831678	0	1.287	N.D. #
12)	B 4,4'-DDE	5.679	6.348	31862436	12503440	5.881	6.800
14)	MA Endrin	6.067	0.000	5095931	0	0.939	N.D. #
15)	B Endosulfa...	6.274f	0.000	16590690	0	3.189	N.D. #
16)	A 4,4'-DDD	0.000	6.798f	0	4535107	N.D.	3.001 #
17)	MA 4,4'-DDT	6.431	7.136	18391195	7626540	4.032	4.624
23)	Chlordane-1	4.455	0.000	3831678	0	17.130	N.D. #
24)	Chlordane-2	4.896	0.000	5930444	0	24.378	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011419\
Data File : PL043867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2019 14:06
Operator : AJ\SJ
Sample : K1015-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:36:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

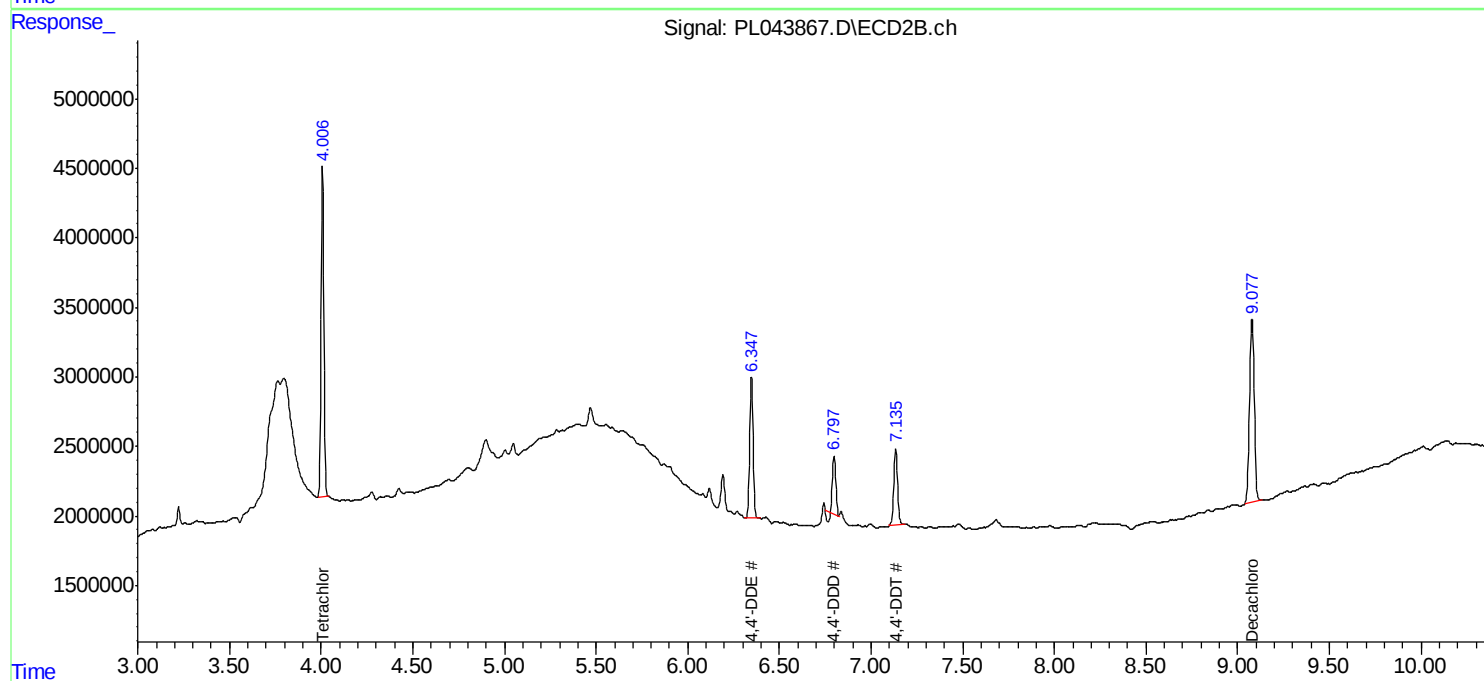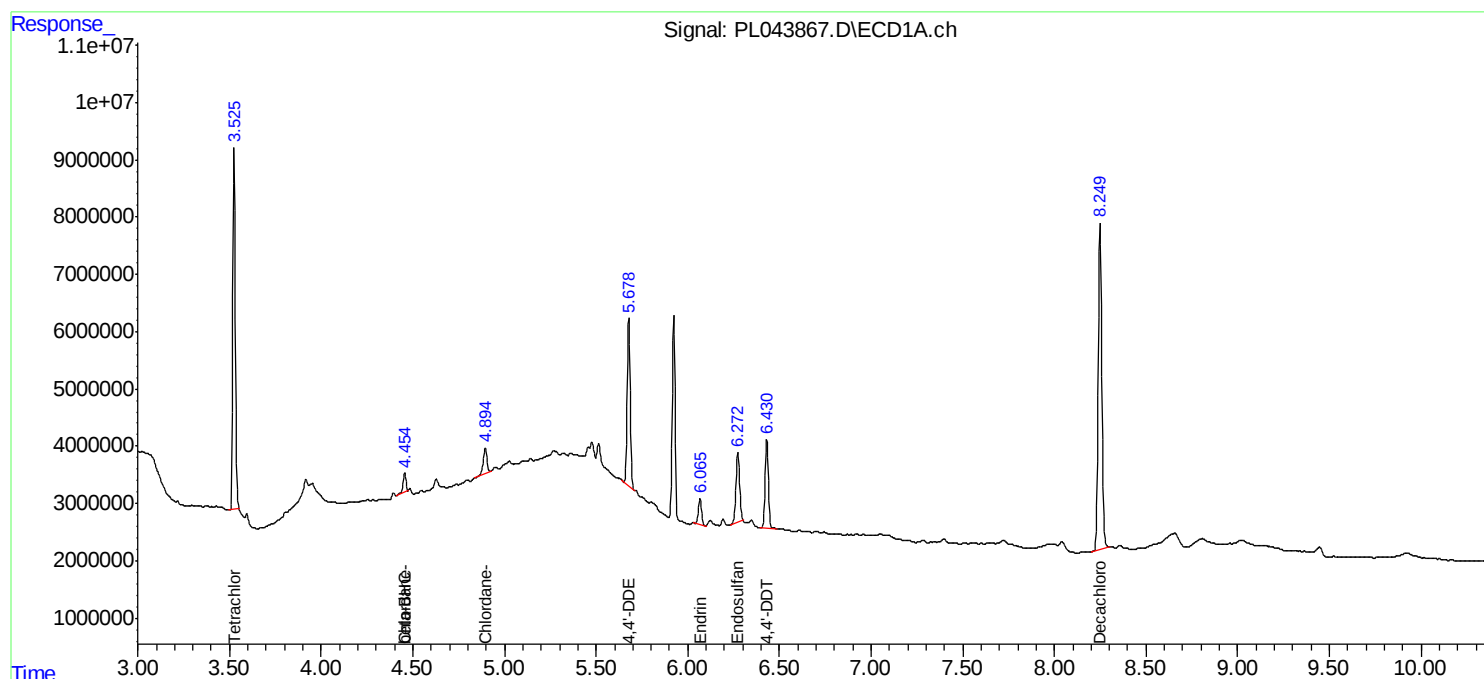


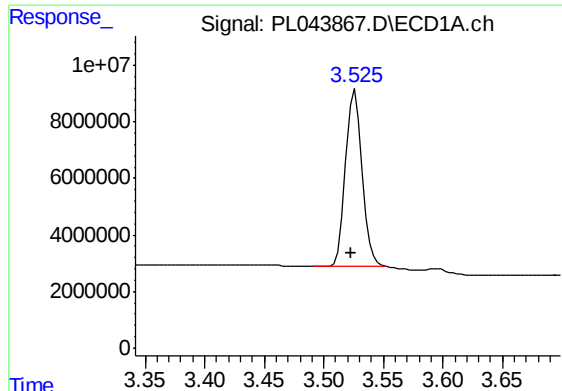

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.003 min
Response: 59126122
Conc: 12.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

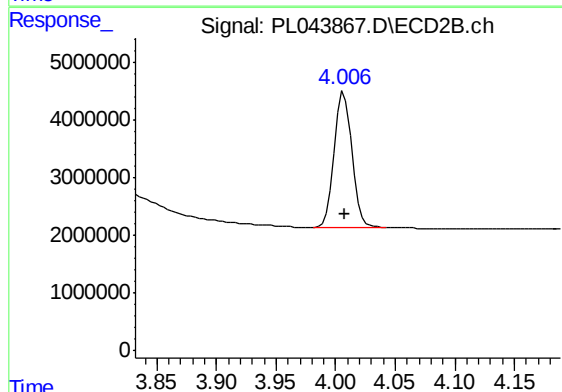


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 24008320
Conc: 12.32 ng/ml

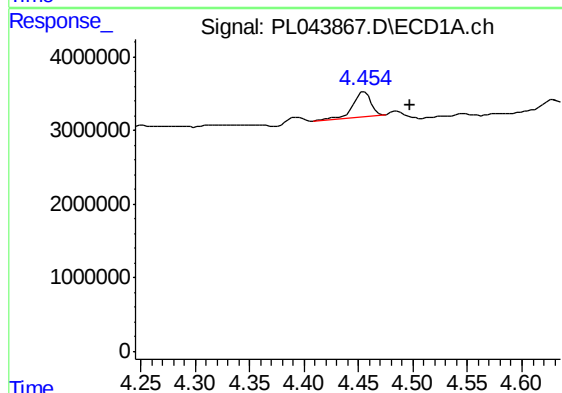


#6 beta-BHC

R.T.: 4.455 min
Delta R.T.: -0.042 min
Response: 3831678
Conc: 1.29 ng/ml

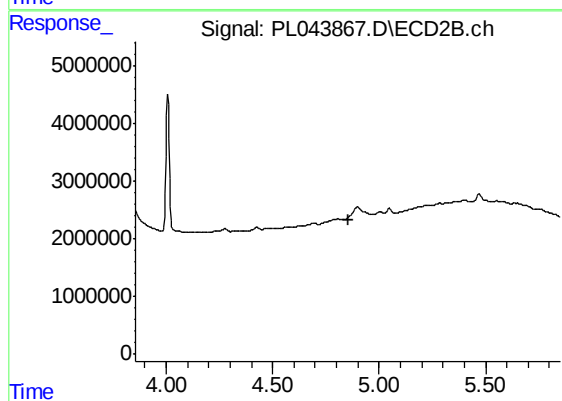

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

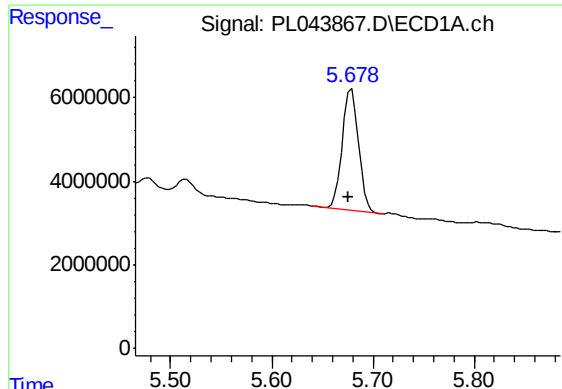

#12 4,4'-DDE


R.T.: 5.679 min
Delta R.T.: 0.002 min
Response: 31862436
Conc: 5.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

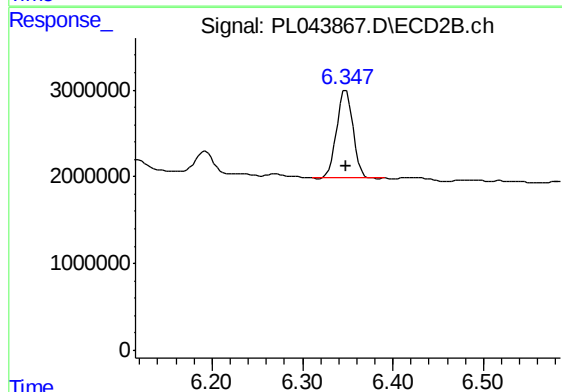


#12 4,4'-DDE

R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 12503440
Conc: 6.80 ng/ml

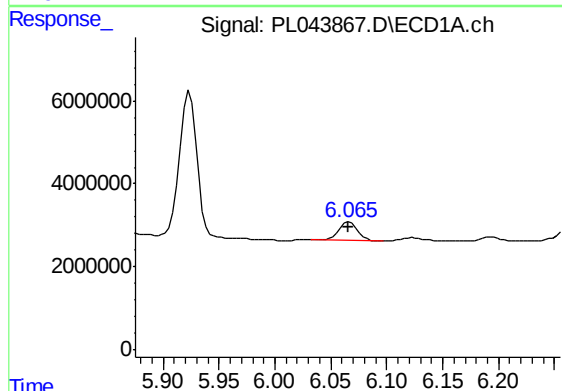


#14 Endrin

R.T.: 6.067 min
Delta R.T.: 0.000 min
Response: 5095931
Conc: 0.94 ng/ml

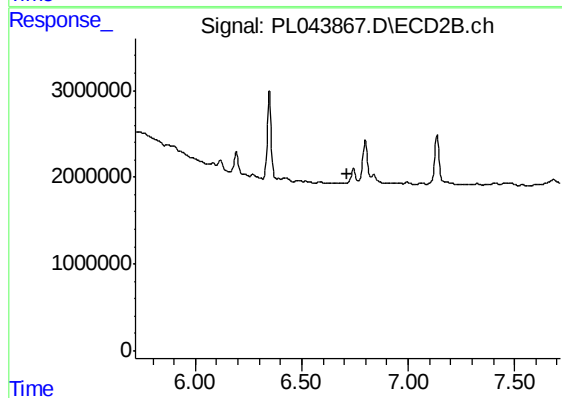

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.716 min
Response: 0
Conc: N.D.

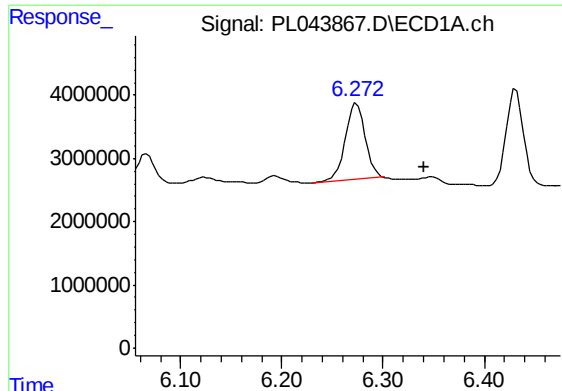

#15 Endosulfan II


R.T.: 6.274 min
Delta R.T.: -0.066 min
Response: 16590690
Conc: 3.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

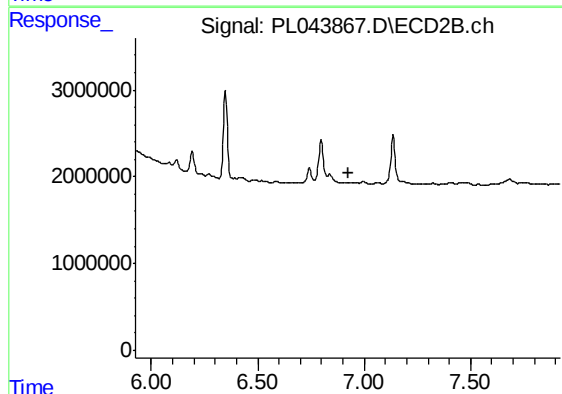


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

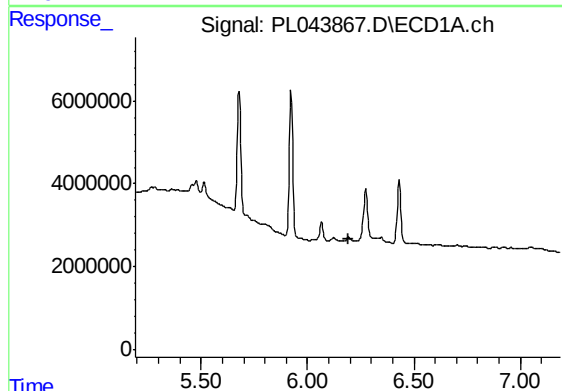


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

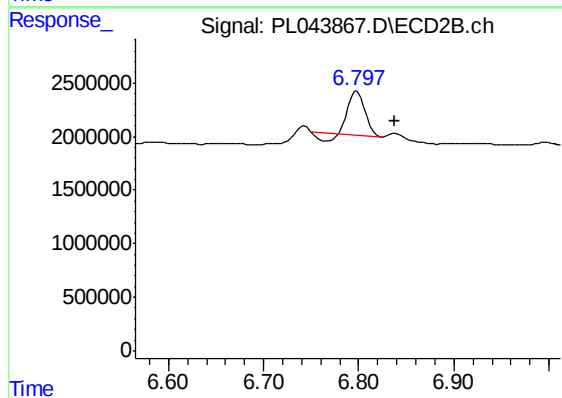

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: -0.040 min
Response: 4535107
Conc: 3.00 ng/ml

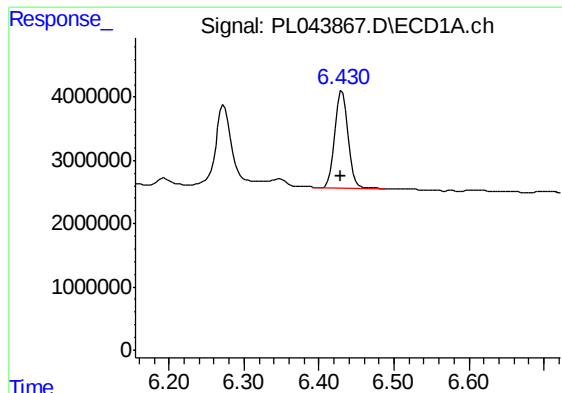

#17 4,4'-DDT


R.T.: 6.431 min
Delta R.T.: 0.002 min
Response: 18391195
Conc: 4.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

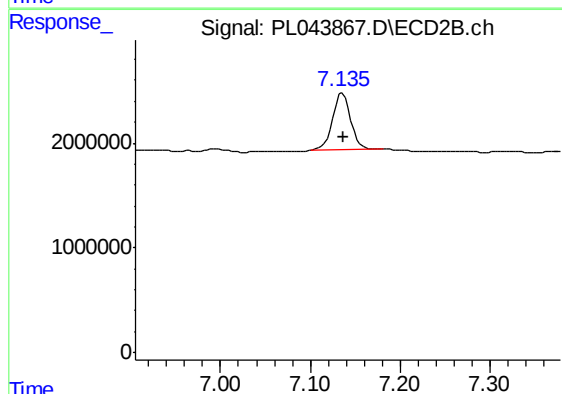


#17 4,4'-DDT

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 7626540
Conc: 4.62 ng/ml

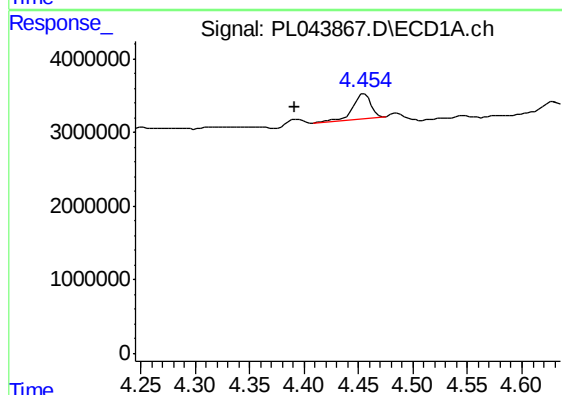


#23 Chlordane-1

R.T.: 4.455 min
Delta R.T.: 0.064 min
Response: 3831678
Conc: 17.13 ng/ml

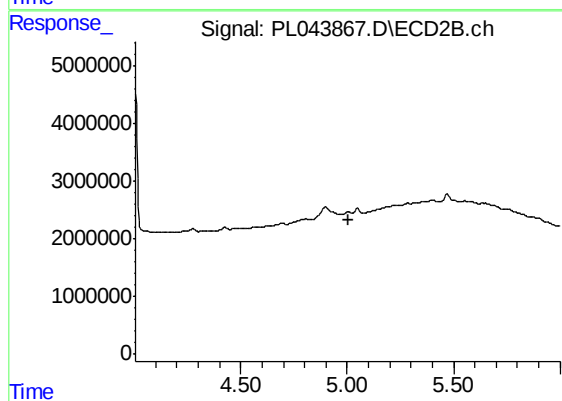

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

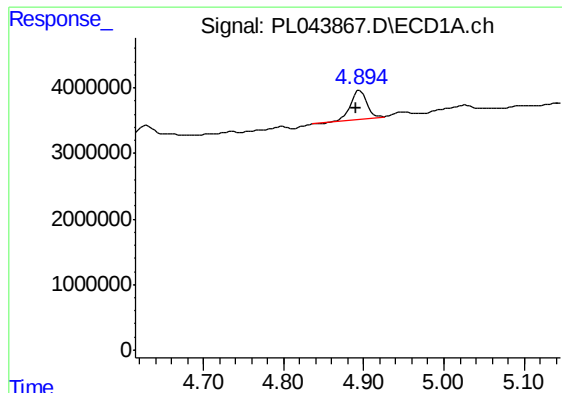

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.004 min
Response: 5930444
Conc: 24.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-02-011119-A

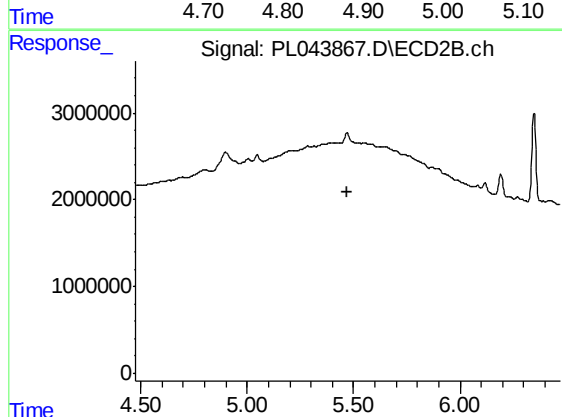


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.473 min
Response: 0
Conc: N.D.

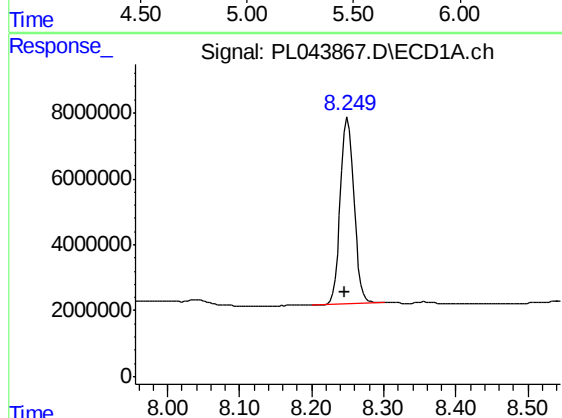

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.004 min
Response: 74414925
Conc: 13.17 ng/ml

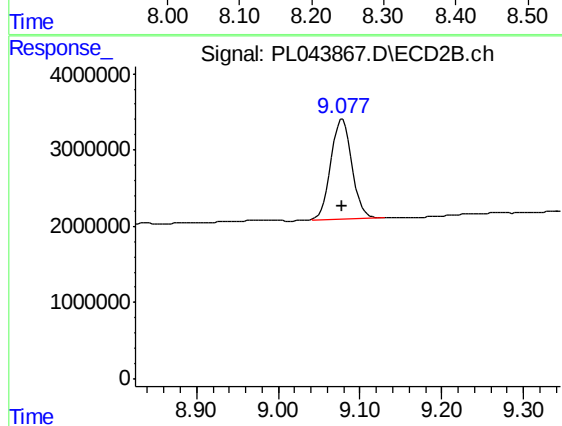

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.000 min
Response: 23397140
Conc: 14.73 ng/ml