

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL011420\  
 Data File : PL055722.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Jan 2020 10:35  
 Operator : AJ\MA  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 14 22:04:02 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL011020.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jan 10 00:58:33 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |       |          |         |       |         |
|------------------|--------------|--------|-------|----------|---------|-------|---------|
| 9) A             | Endosulfan I | 5.550  | 0.000 | 18387361 | 0       | 1.488 | N.D. #  |
| 14) MA           | Endrin       | 0.000  | 6.628 | 0        | 6760729 | N.D.  | 2.998 # |
| 15) B            | Endosulfa... | 6.292f | 0.000 | 21750298 | 0       | 2.016 | N.D. #  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL011420\  
Data File : PL055722.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Jan 2020 10:35  
Operator : AJ\MA  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 14 22:04:02 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL011020.M  
Quant Title : GC Extractables  
QLast Update : Fri Jan 10 00:58:33 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

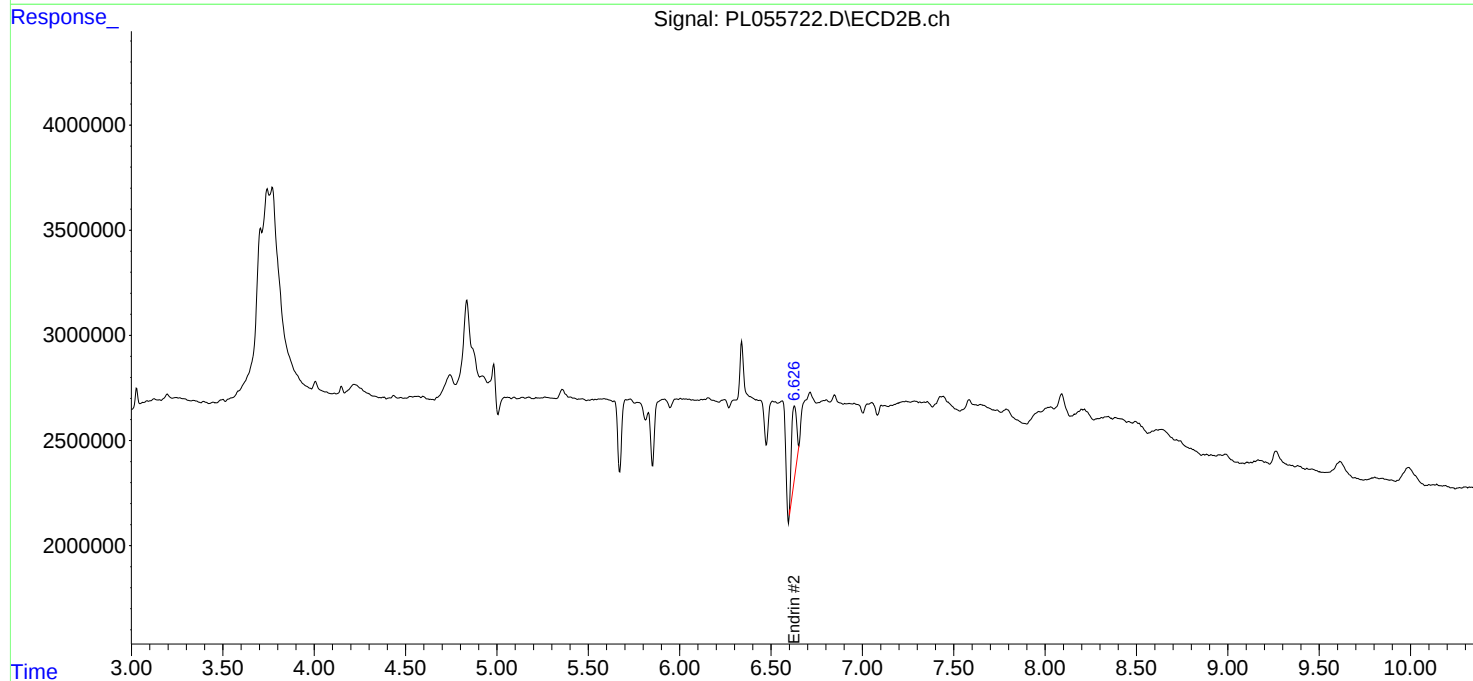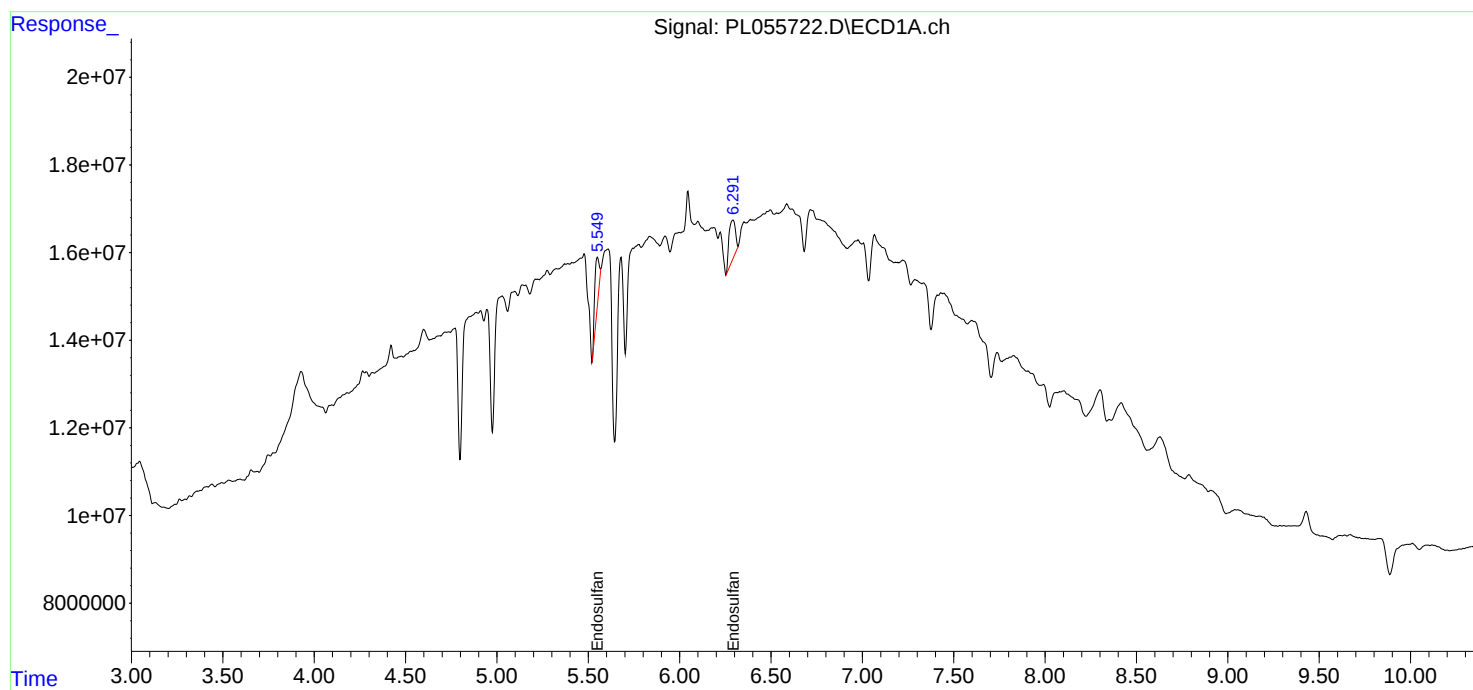


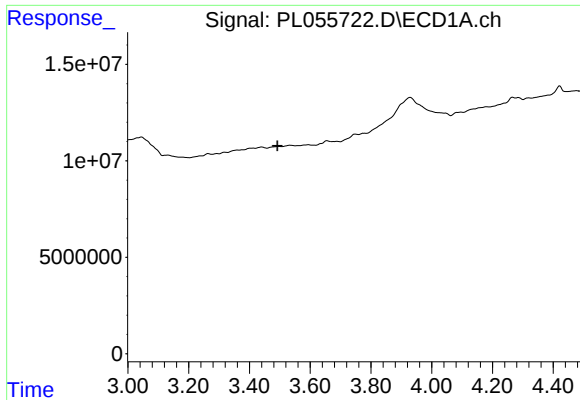

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.492 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

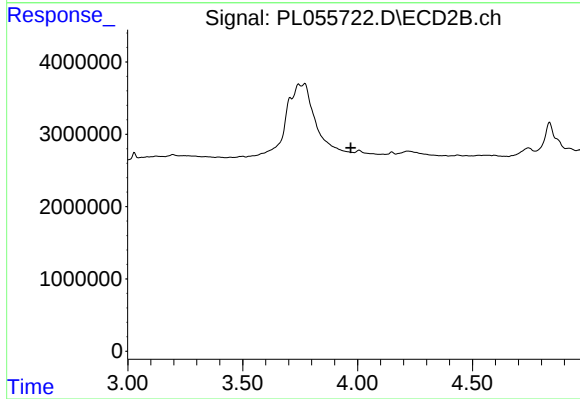


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 3.970 min  
Response: 0  
Conc: N.D.

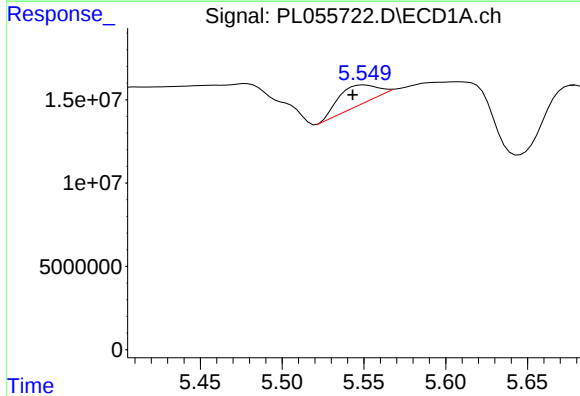


#9 Endosulfan I

R.T.: 5.550 min  
Delta R.T.: 0.007 min  
Response: 18387361  
Conc: 1.49 ng/ml

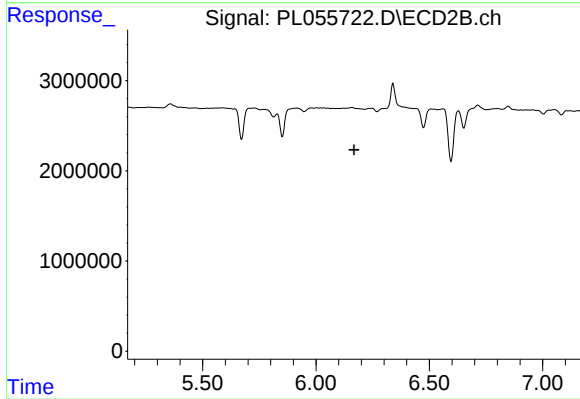

#9 Endosulfan I


R.T.: 0.000 min  
Exp R.T.: 6.168 min  
Response: 0  
Conc: N.D.

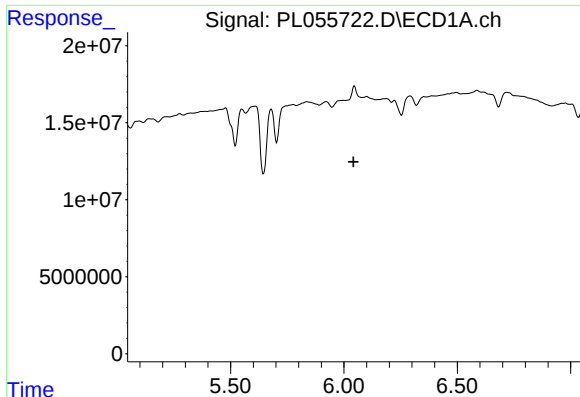

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.043 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

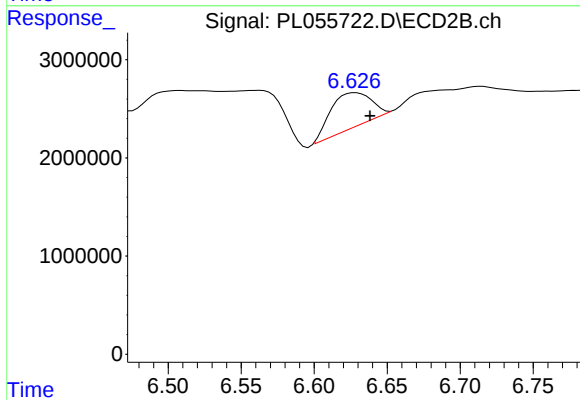


#14 Endrin

R.T.: 6.628 min  
Delta R.T.: -0.010 min  
Response: 6760729  
Conc: 3.00 ng/ml

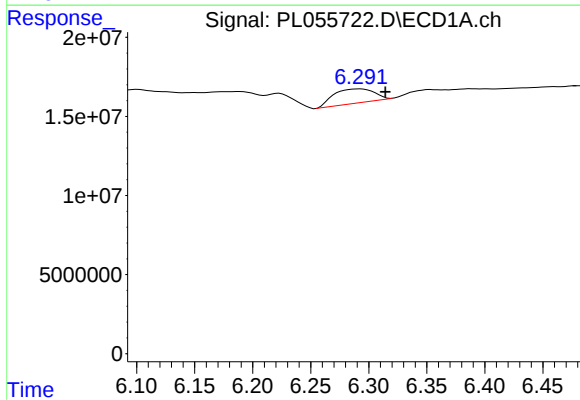


#15 Endosulfan II

R.T.: 6.292 min  
Delta R.T.: -0.022 min  
Response: 21750298  
Conc: 2.02 ng/ml

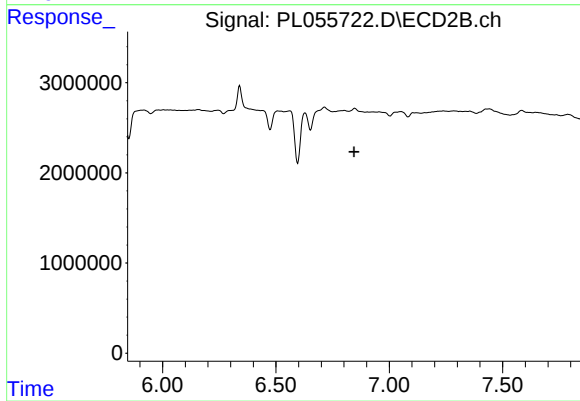

#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T.: 6.845 min  
Response: 0  
Conc: N.D.

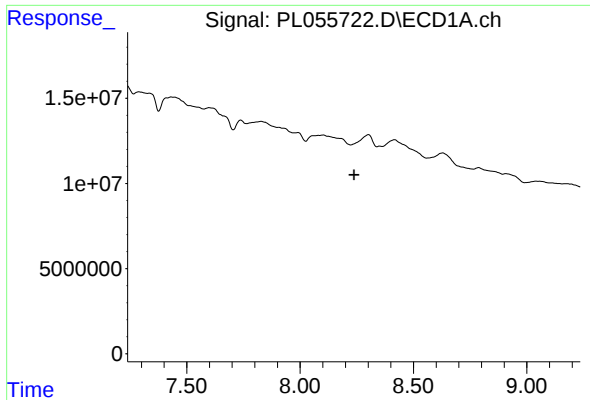

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T. : 8.238 min

Response: 0

Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

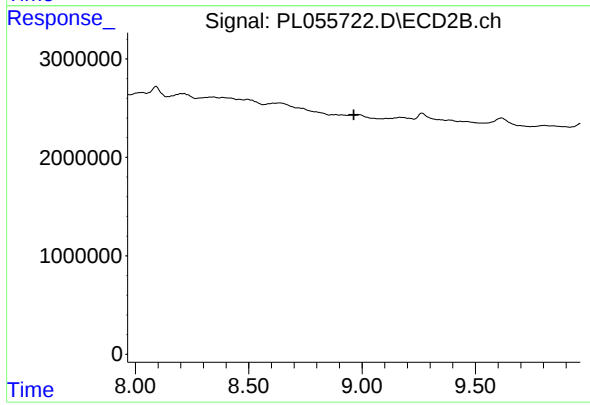

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 8.963 min

Response: 0

Conc: N.D.