

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011420\
 Data File : PL055741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2020 16:05
 Operator : AJ\MA
 Sample : L1004-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-RO-258

Manual Integrations
 APPROVED

mohammad
 1/15/2020 4:13:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 22:07:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	3.967	225.7E6	69959994	24.425	26.409m
28)	SA Decachlor...	8.236	8.957	204.9E6	52116029	23.328	25.067

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011420\
Data File : PL055741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2020 16:05
Operator : AJ\MA
Sample : L1004-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-RO-258


Manual Integrations
APPROVED

mohammad
1/15/2020 4:13:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 22:07:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

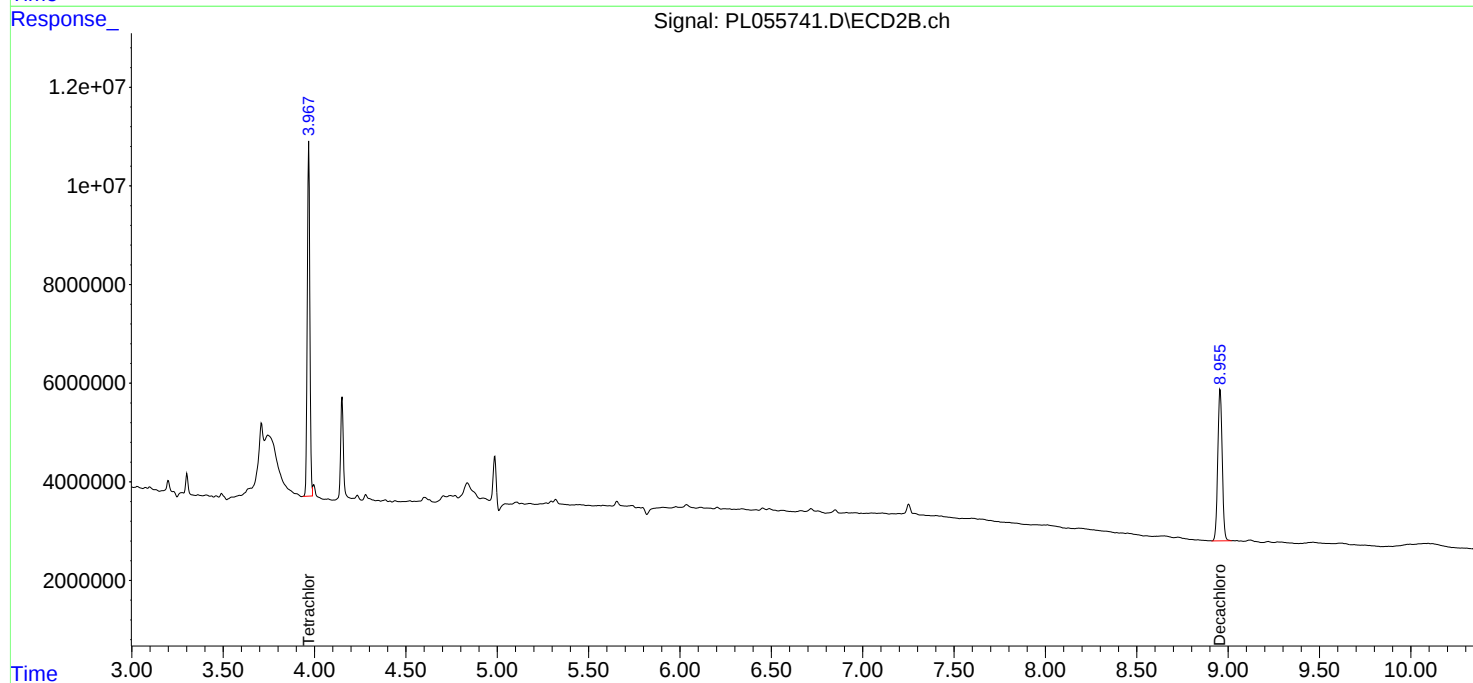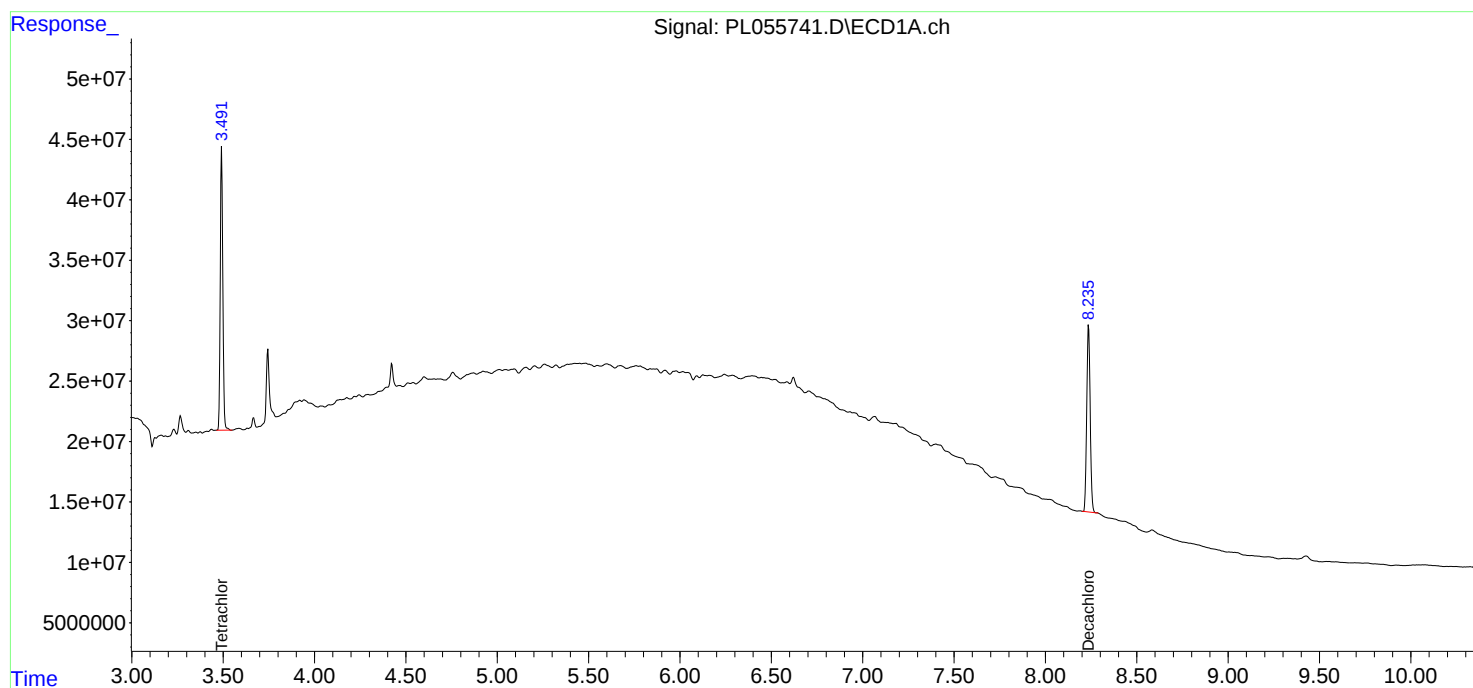

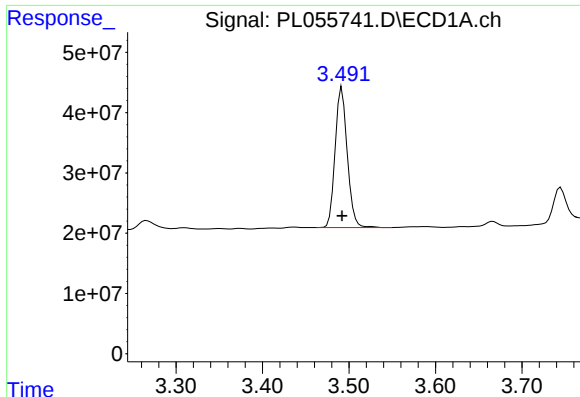


#1 Tetrachloro-m-xylene

R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 225702687
Conc: 24.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-RO-258


Manual Integrations
APPROVED

mohammad
1/15/2020 4:13:56 PM

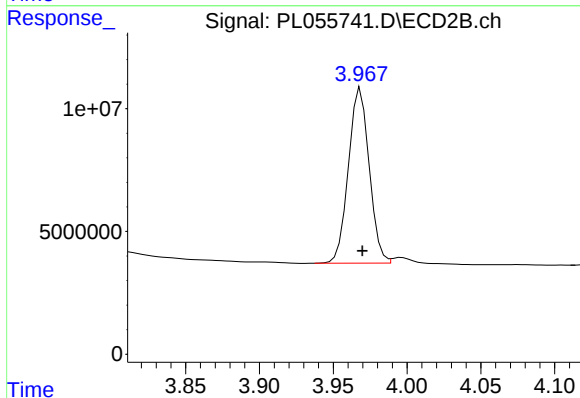


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.003 min
Response: 69959994
Conc: 26.41 ng/ml m

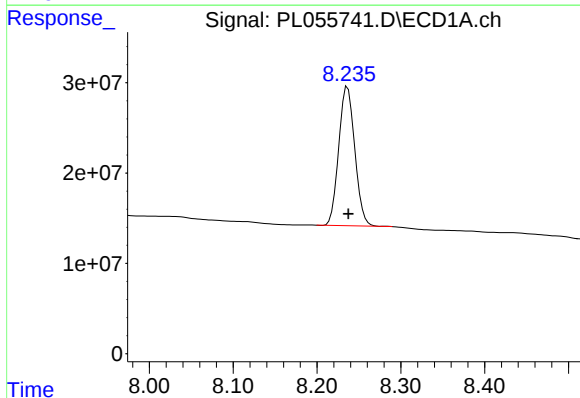

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: -0.001 min
Response: 204857213
Conc: 23.33 ng/ml

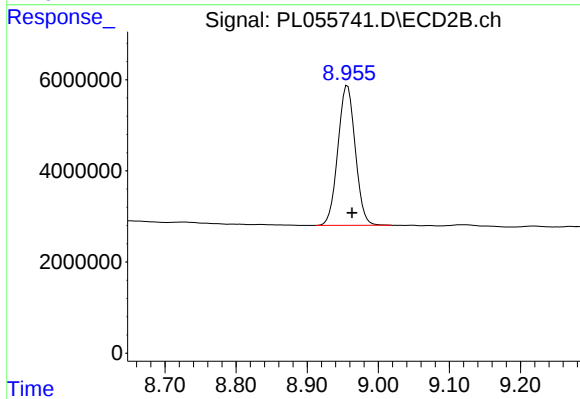

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.006 min
Response: 52116029
Conc: 25.07 ng/ml