

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
 Data File : PL064116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 14:54
 Operator : AR\AJ
 Sample : M1058-02RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:39:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.108	52516056	42442701	17.514	16.602
28)	SA Decachlor...	8.170	9.269	17714745	13255134	5.804	5.585
Target Compounds							
3)	MA gamma-BHC...	4.150	0.000	30659754	0	6.613	N.D. #
4)	MA Heptachlor	4.456	0.000	6208408	0	1.417	N.D. #
11)	B alpha-Chl...	5.410	0.000	14243497	0	3.723	N.D. #
26)	Chlordane-4	5.410	0.000	14243497	0	47.829	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
Data File : PL064116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 14:54
Operator : AR\AJ
Sample : M1058-02RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:39:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

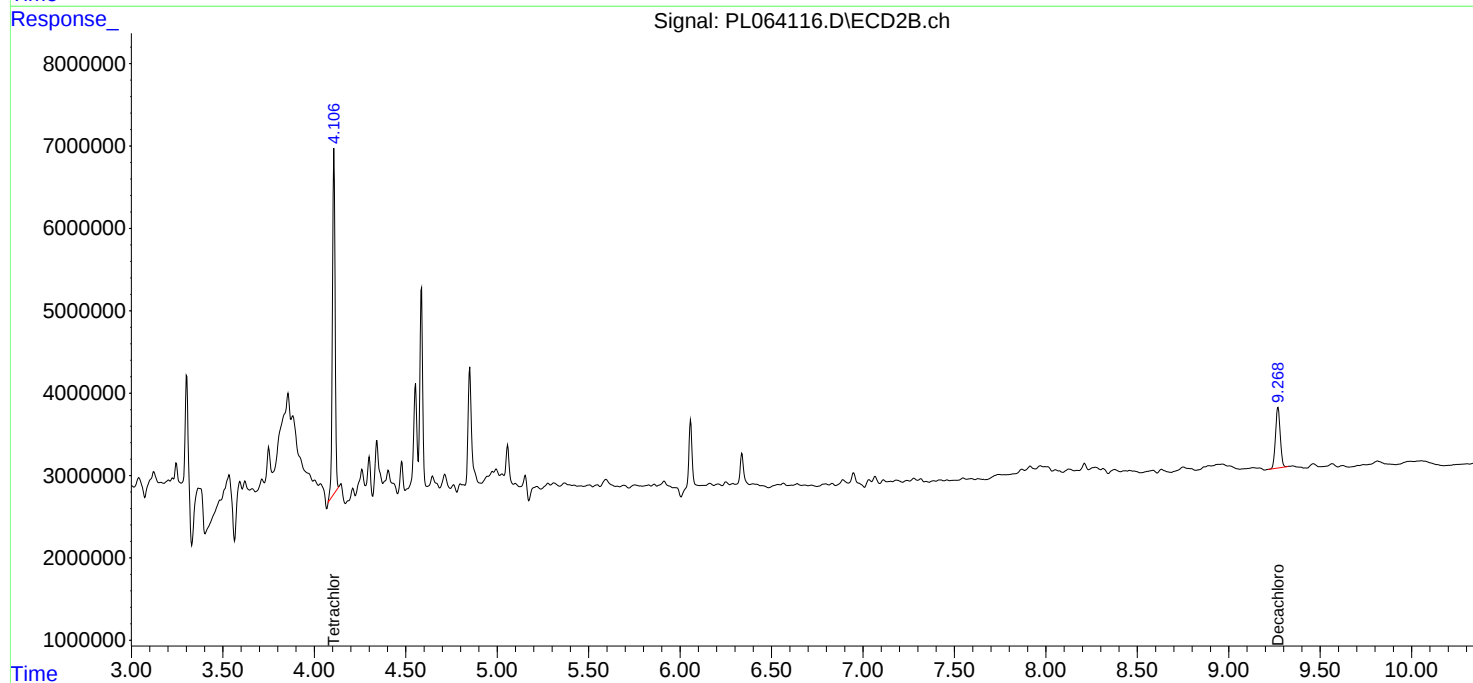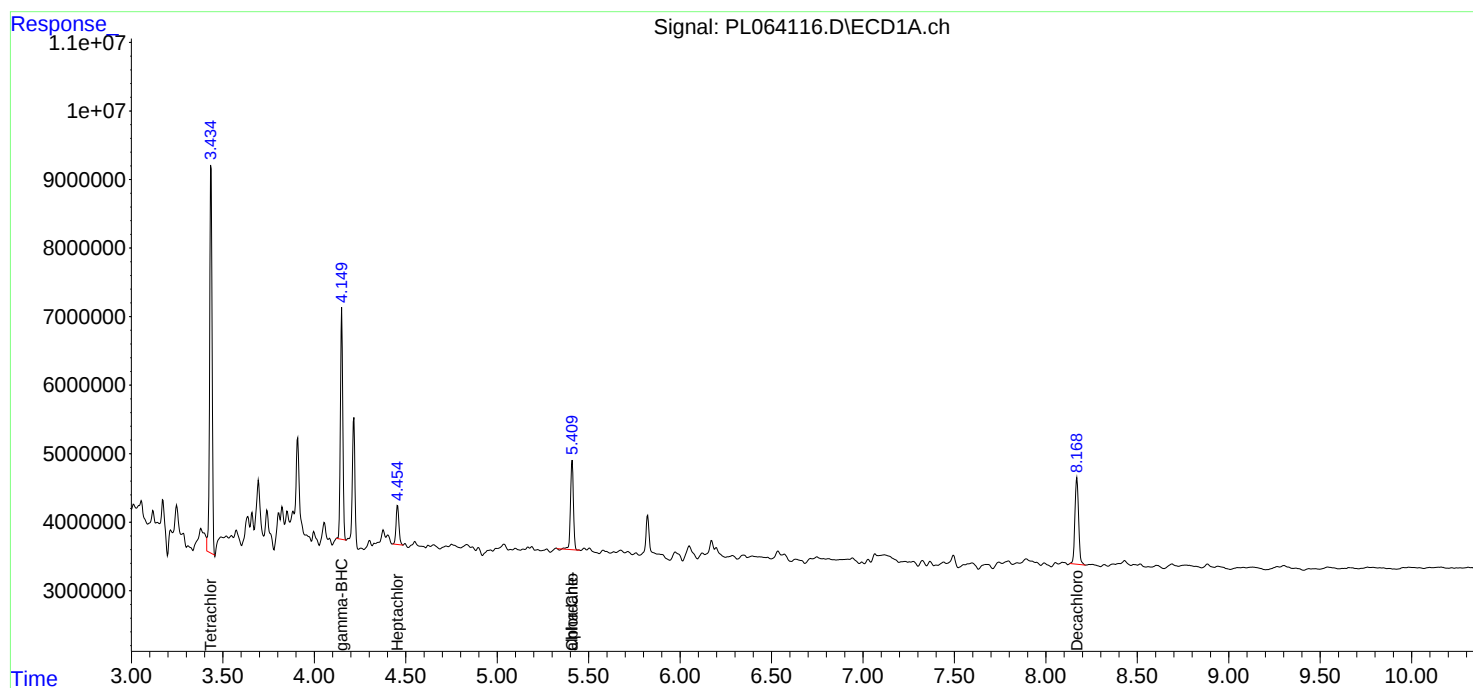


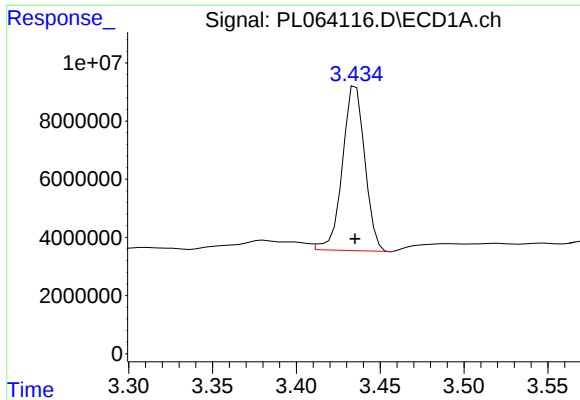

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 52516056
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

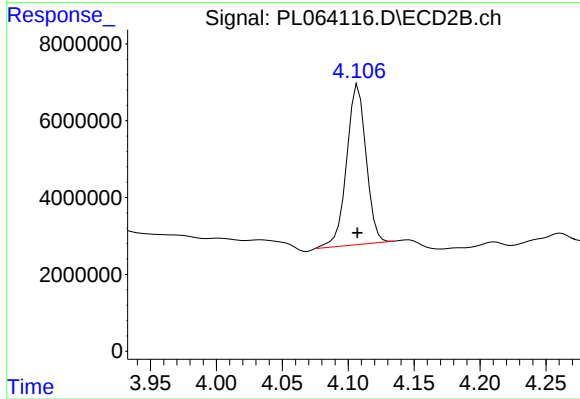


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 42442701
Conc: 16.60 ng/ml

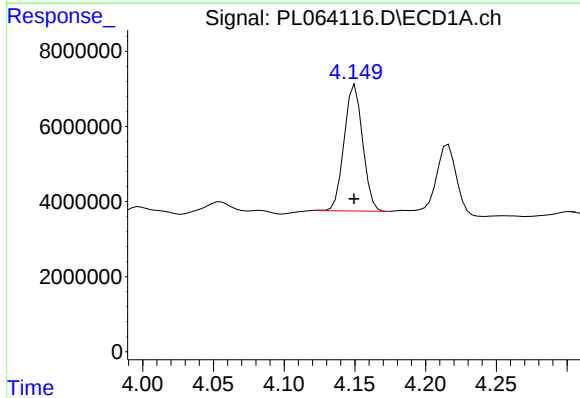


#3 gamma-BHC (Lindane)

R.T.: 4.150 min
Delta R.T.: 0.000 min
Response: 30659754
Conc: 6.61 ng/ml

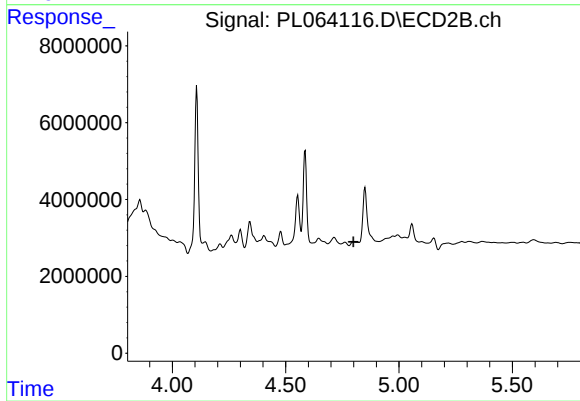

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

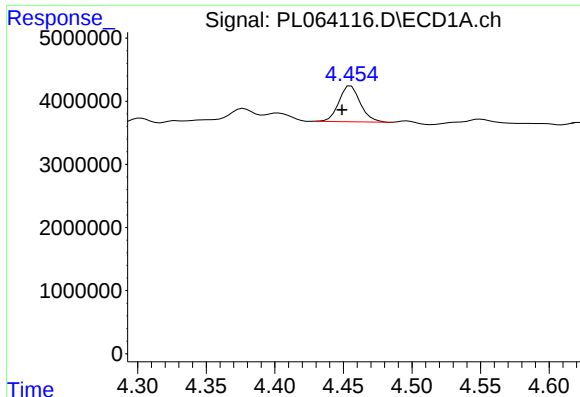

#4 Heptachlor


R.T.: 4.456 min
Delta R.T.: 0.006 min
Response: 6208408
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

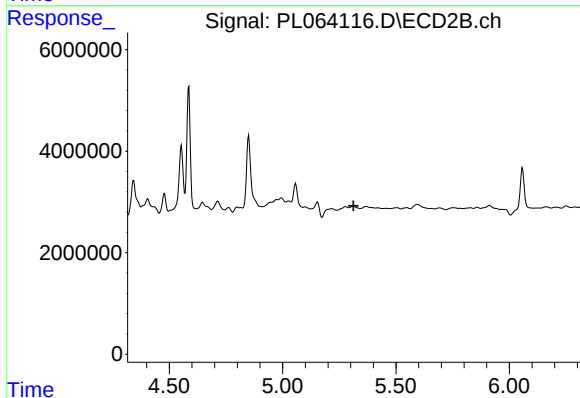


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.313 min
Response: 0
Conc: N.D.

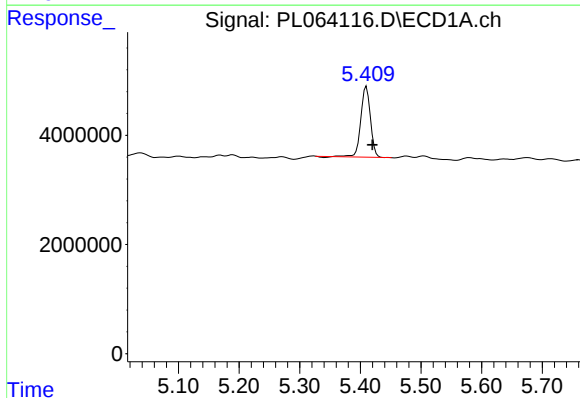


#11 alpha-Chlordane

R.T.: 5.410 min
Delta R.T.: -0.010 min
Response: 14243497
Conc: 3.72 ng/ml

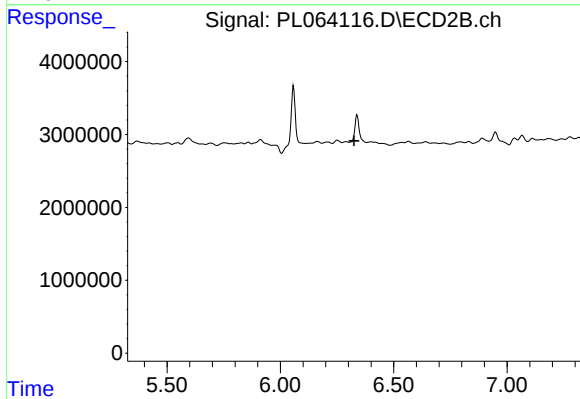

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.325 min
Response: 0
Conc: N.D.

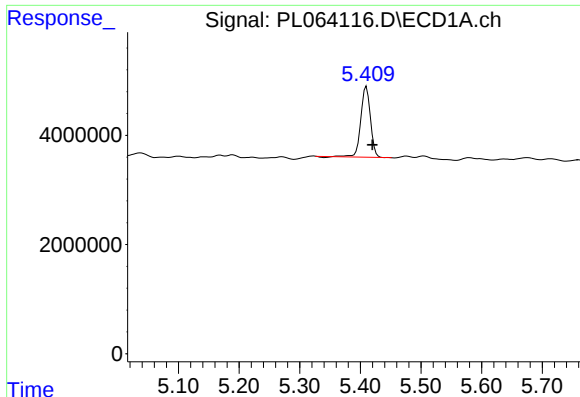

#26 Chlordane-4


R.T.: 5.410 min
Delta R.T.: -0.010 min
Response: 14243497
Conc: 47.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

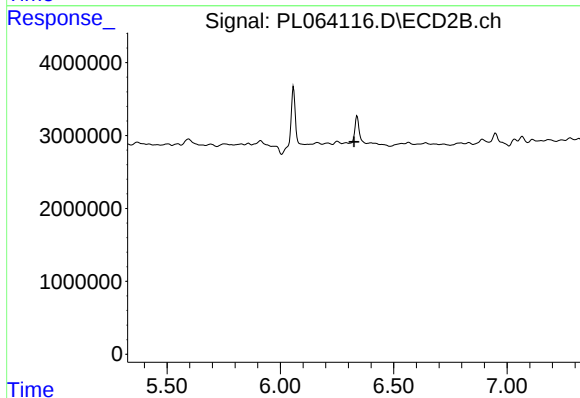


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.326 min
Response: 0
Conc: N.D.

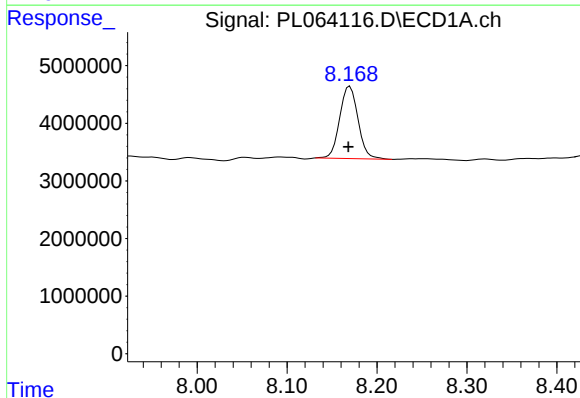

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.002 min
Response: 17714745
Conc: 5.80 ng/ml

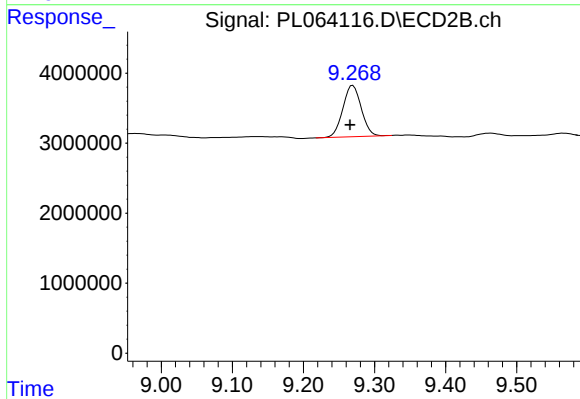

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.004 min
Response: 13255134
Conc: 5.58 ng/ml