

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
 Data File : PL064138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 20:09
 Operator : AR\AJ
 Sample : M1120-0110X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:44:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	4825341	5151948	1.609	2.015 #
28)	SA Decachlor...	8.168	0.000	6921118	0	2.268	N.D. #
Target Compounds							
9)	A Endosulfan I	5.488f	0.000	5264655	0	1.490	N.D. #
18)	B Endrin al...	6.427f	0.000	12453094	0	4.341	N.D. #
19)	B Endosulfa...	6.644f	7.406f	66006417	9125842	19.457	3.695 #
24)	Chlordane-2	4.815f	0.000	26462415	0	197.663	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
Data File : PL064138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 20:09
Operator : AR\AJ
Sample : M1120-0110X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:44:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

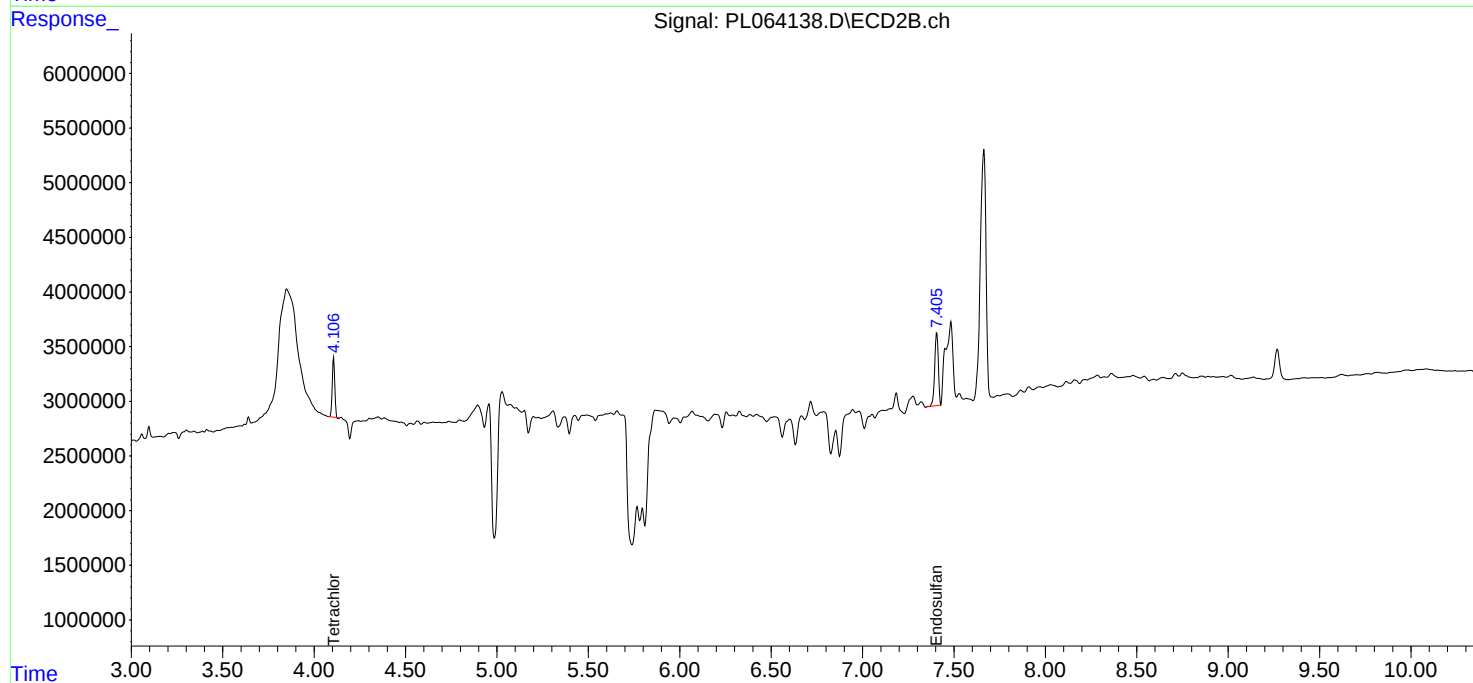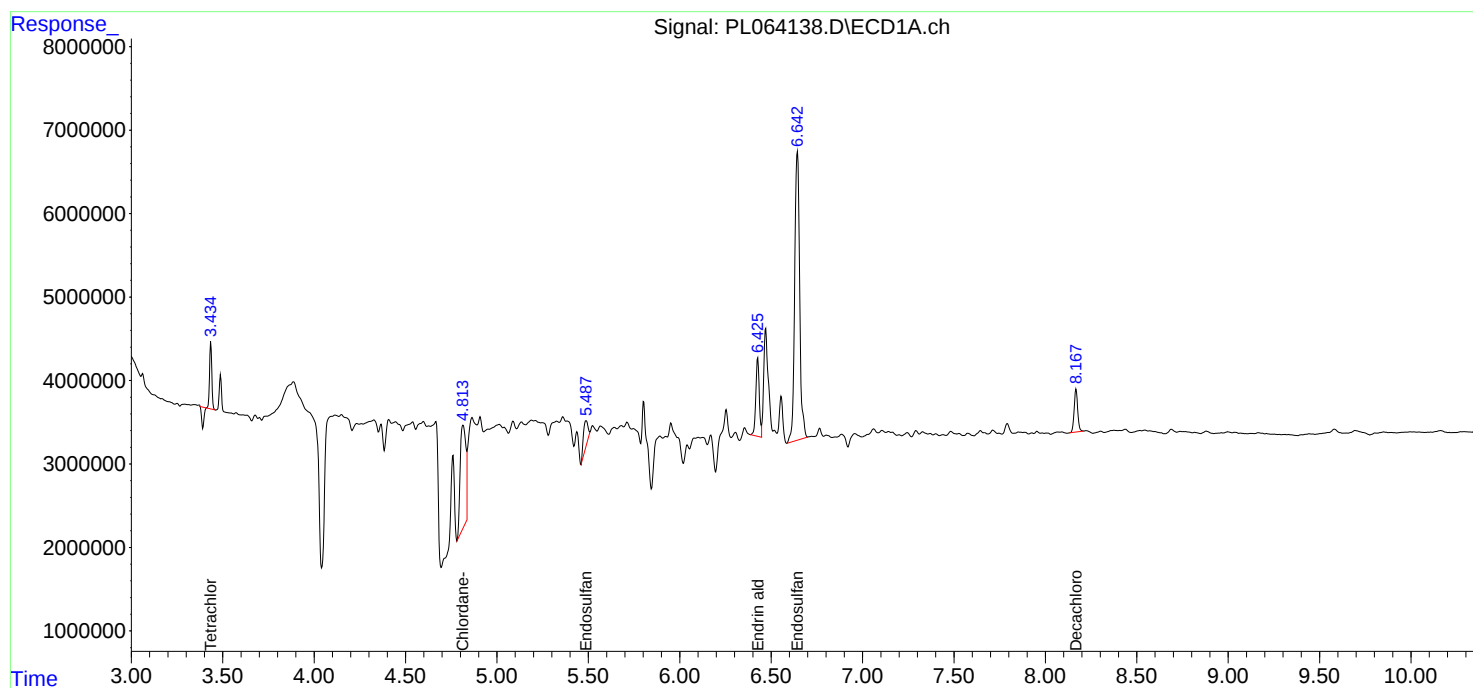


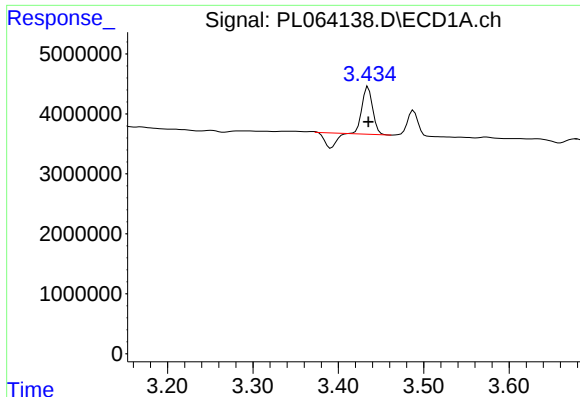

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 4825341
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

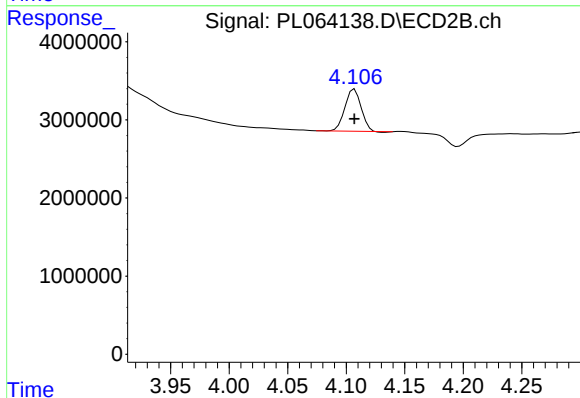


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 5151948
Conc: 2.02 ng/ml

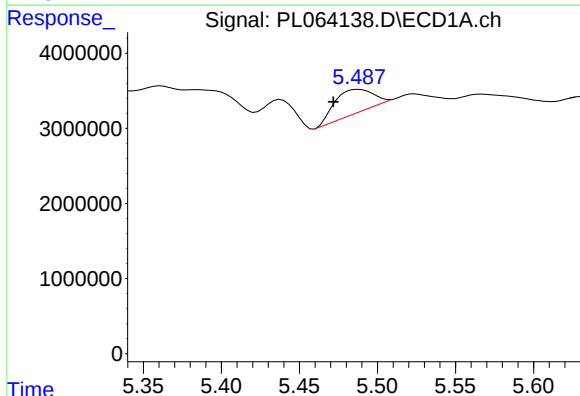


#9 Endosulfan I

R.T.: 5.488 min
Delta R.T.: 0.016 min
Response: 5264655
Conc: 1.49 ng/ml

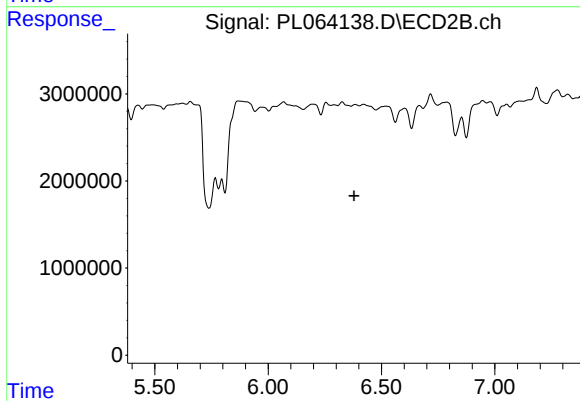

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.379 min
Response: 0
Conc: N.D.

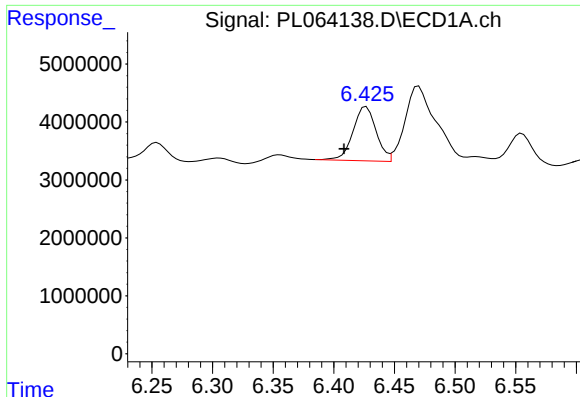

#18 Endrin aldehyde


R.T.: 6.427 min
Delta R.T.: 0.018 min
Response: 12453094
Conc: 4.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

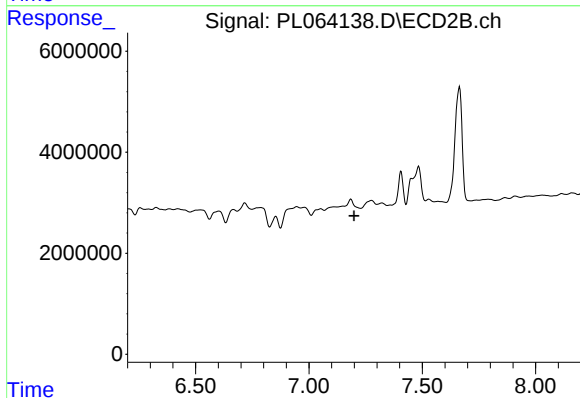


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

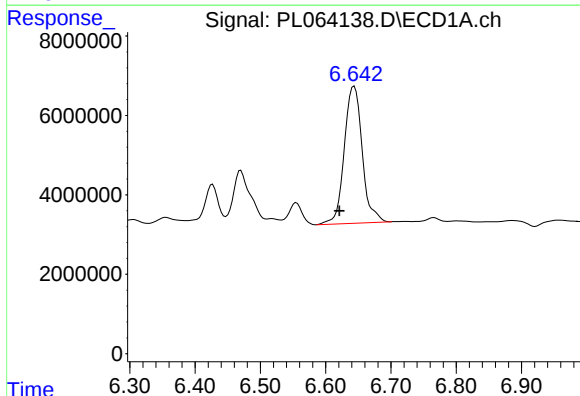


#19 Endosulfan Sulfate

R.T.: 6.644 min
Delta R.T.: 0.023 min
Response: 66006417
Conc: 19.46 ng/ml

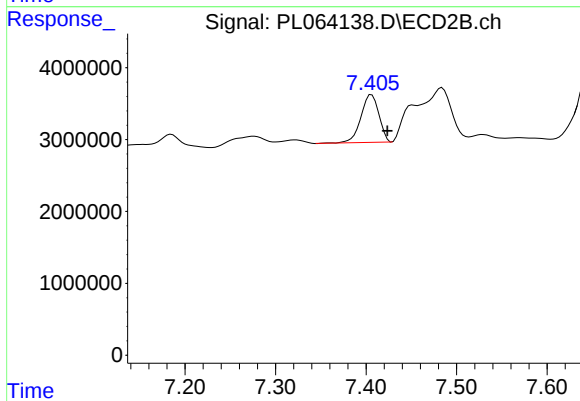

#19 Endosulfan Sulfate


R.T.: 7.406 min
Delta R.T.: -0.017 min
Response: 9125842
Conc: 3.69 ng/ml

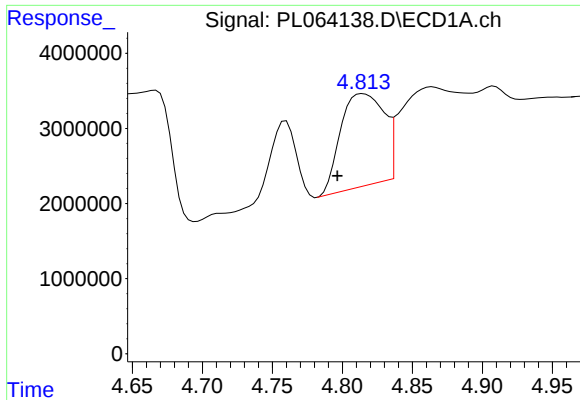

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.019 min
Response: 26462415
Conc: 197.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

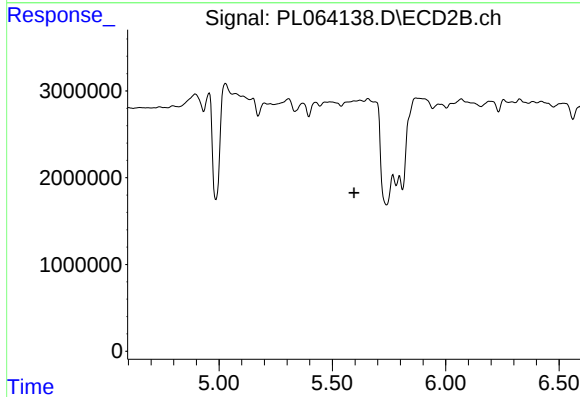


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.596 min
Response: 0
Conc: N.D.

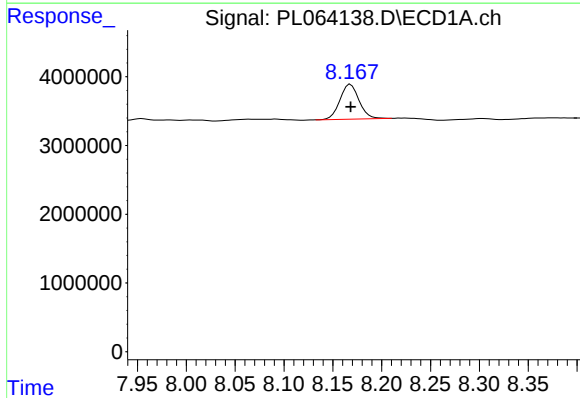

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 6921118
Conc: 2.27 ng/ml

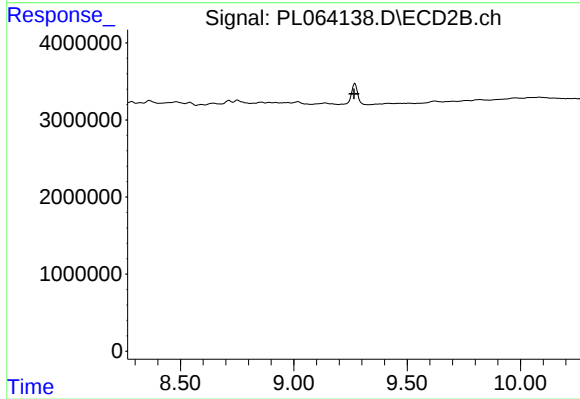

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.266 min
Response: 0
Conc: N.D.