

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
 Data File : PL064114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 14:25
 Operator : AR\AJ
 Sample : M1077-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-011121-A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 10:22:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:38:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	36443913	30302403	12.154	11.853
28)	SA Decachlor...	8.169	9.270	41190546	33117597	13.496	13.954
Target Compounds							
11)	B alpha-Chl...	5.418	6.326	2059053	2615040	0.538m	0.859m#
12)	B 4,4'-DDE	5.585	6.482	4846277	4526848	1.376m	1.700m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
Data File : PL064114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 14:25
Operator : AR\AJ
Sample : M1077-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
JC-03-011121-A


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:38:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

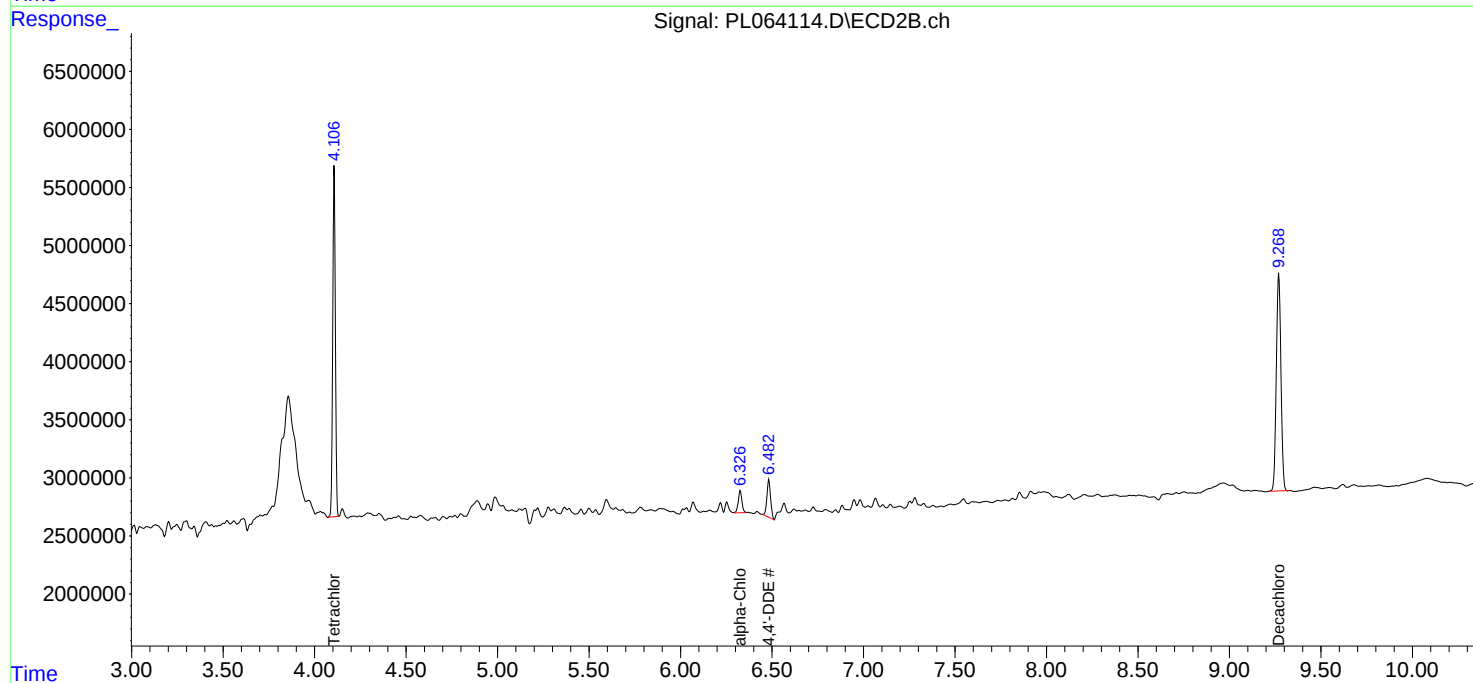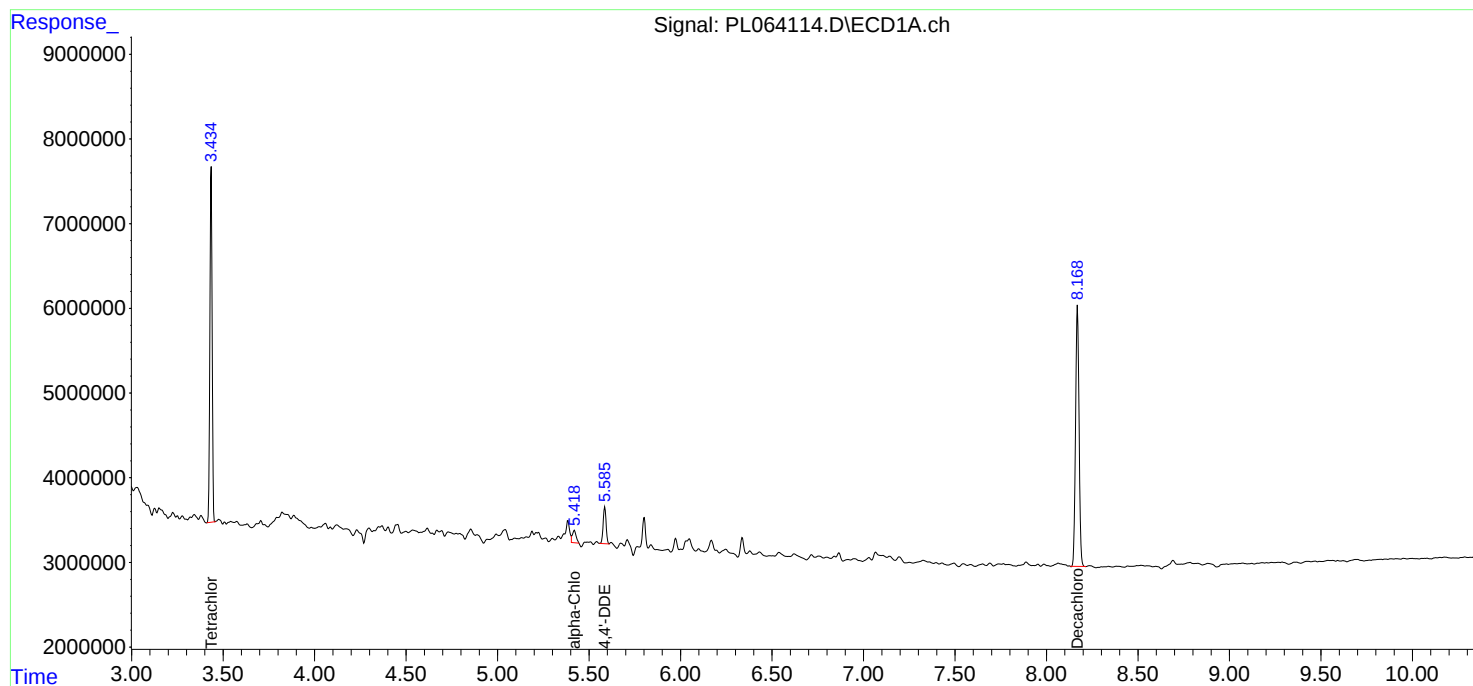

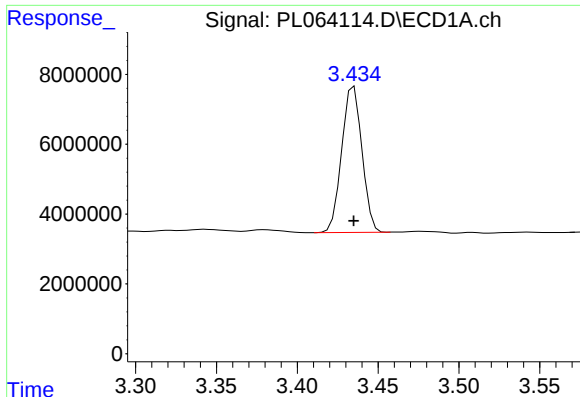


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 36443913
Conc: 12.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-011121-A


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:54 AM

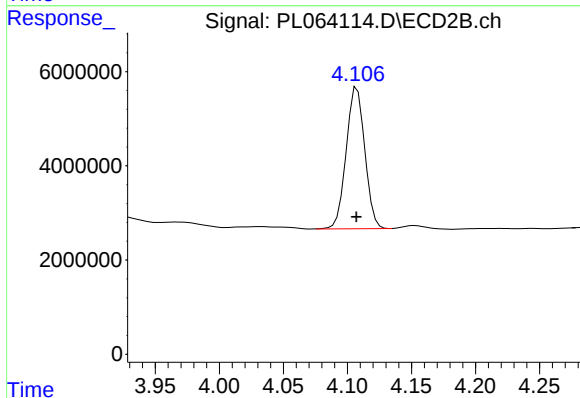


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 30302403
Conc: 11.85 ng/ml

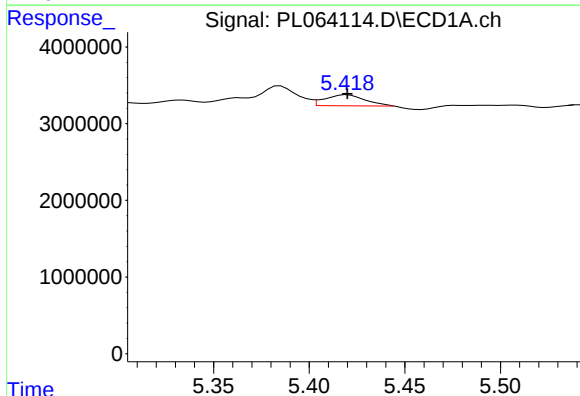


#11 alpha-Chlordane

R.T.: 5.418 min
Delta R.T.: -0.001 min
Response: 2059053
Conc: 0.54 ng/ml m

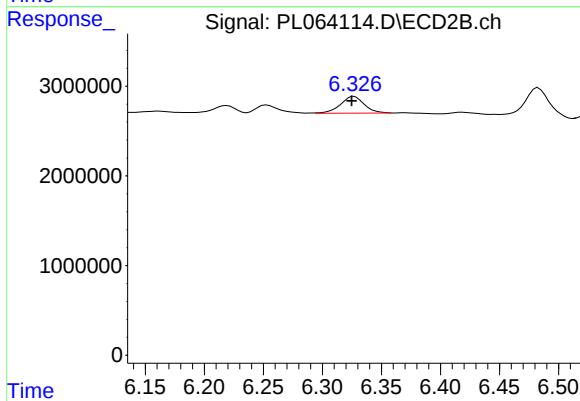

#11 alpha-Chlordane

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 2615040
Conc: 0.86 ng/ml m

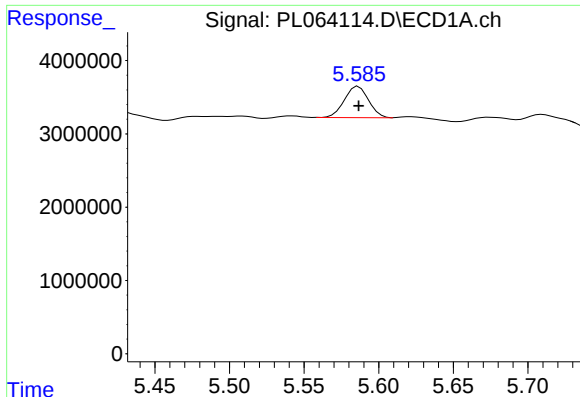


#12 4,4'-DDE

R.T.: 5.585 min
Delta R.T.: -0.002 min
Response: 4846277
Conc: 1.38 ng/ml m

Instrument :
ECD_L
ClientSampleId :
JC-03-011121-A


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:54 AM

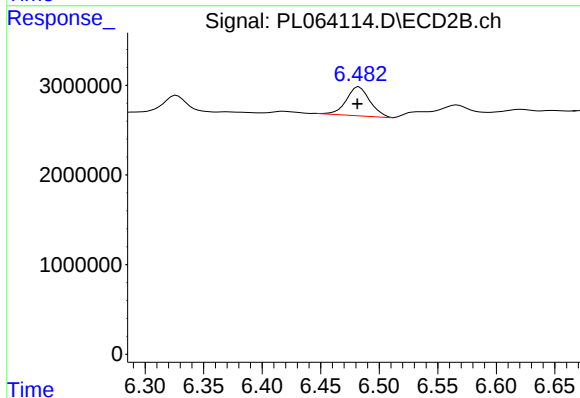


#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 4526848
Conc: 1.70 ng/ml m

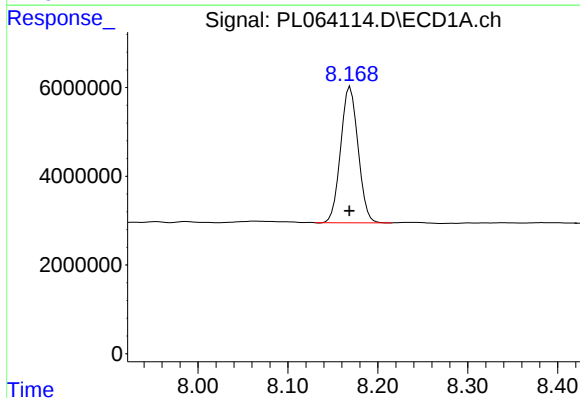

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.001 min
Response: 41190546
Conc: 13.50 ng/ml

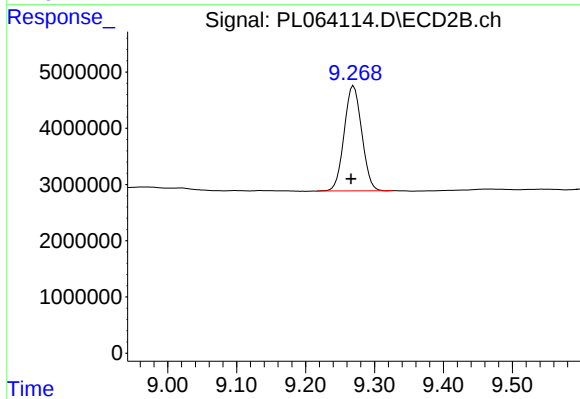

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.004 min
Response: 33117597
Conc: 13.95 ng/ml