

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
 Data File : PL064115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 14:40
 Operator : AR\AJ
 Sample : M1077-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-011121-B

Manual Integrations
 APPROVED

Ankita
 1/15/2021 10:22:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:38:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	34982653	28159920	11.667	11.015
28)	SA Decachlor...	8.171	9.269	46018644	36537920	15.078	15.395
Target Compounds							
12)	B 4,4'-DDE	5.585	6.482	6415638	5031027	1.821m	1.889m
17)	MA 4,4'-DDT	6.339	7.280	9056947	5550462	3.034	2.451m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
Data File : PL064115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 14:40
Operator : AR\AJ
Sample : M1077-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
JC-03-011121-B


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:38:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

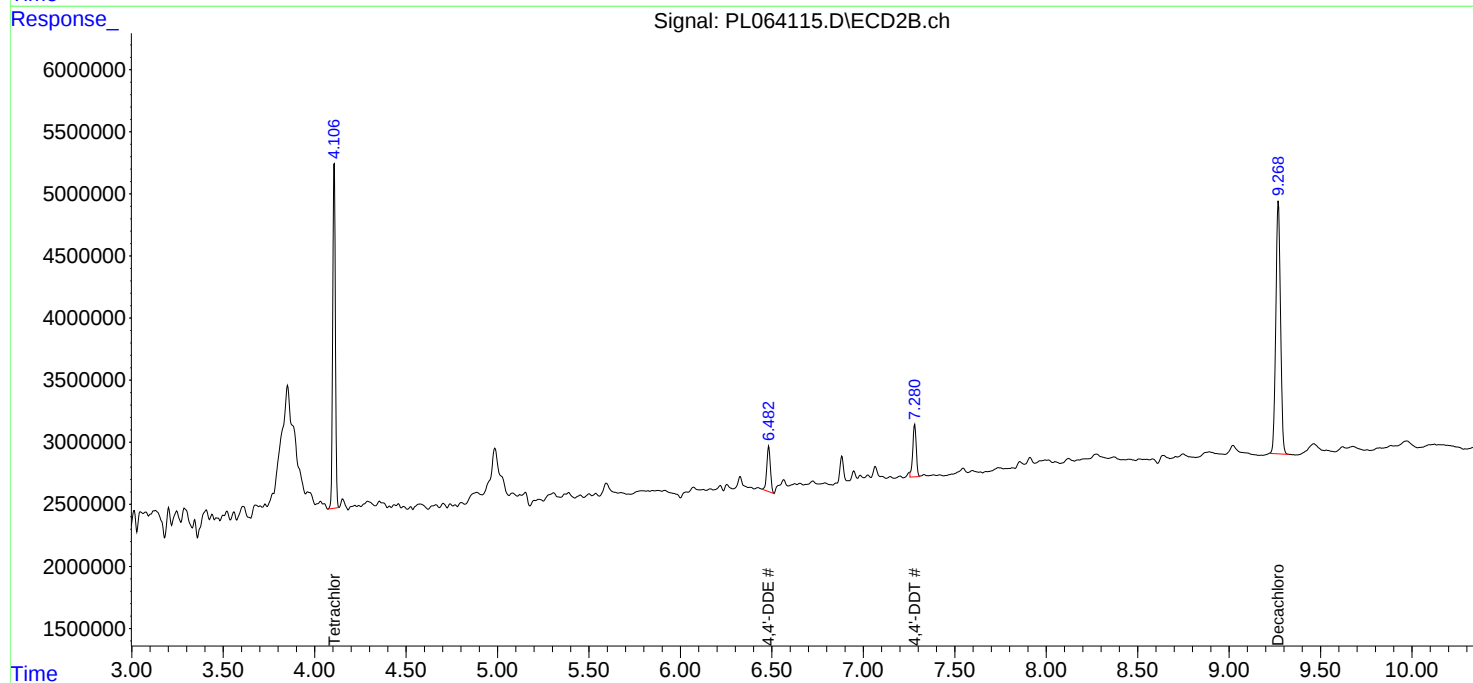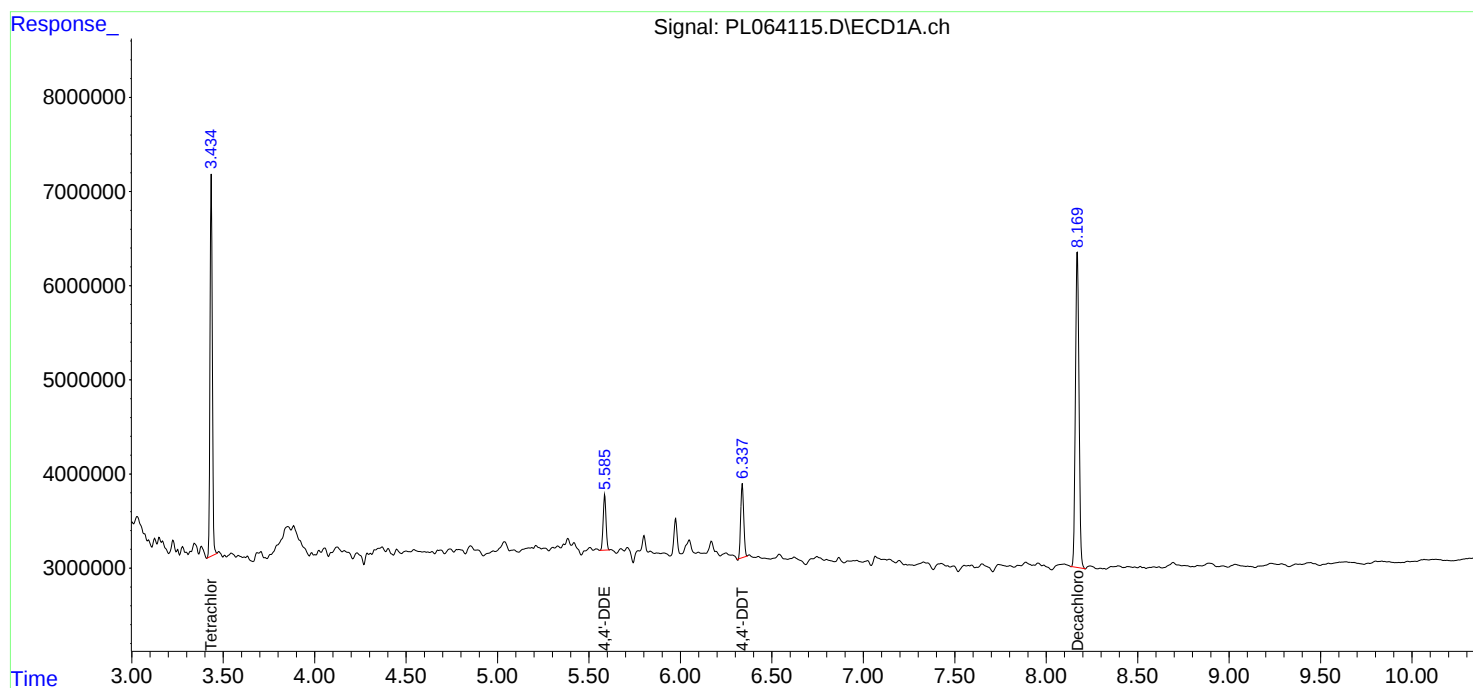

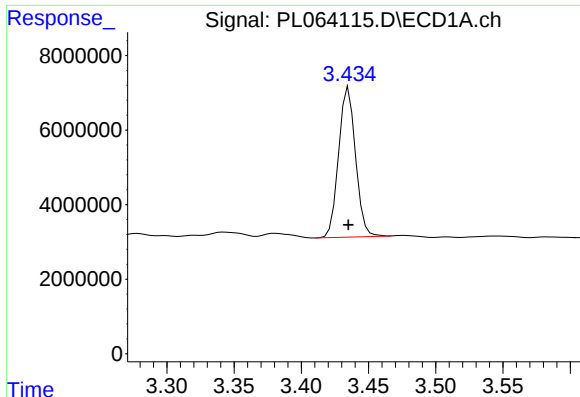


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 34982653
Conc: 11.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-011121-B


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:56 AM

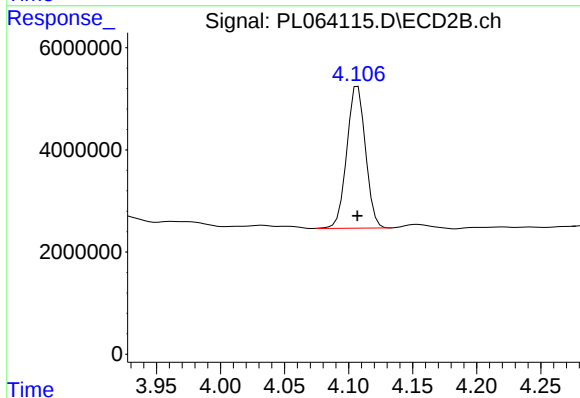


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 28159920
Conc: 11.02 ng/ml

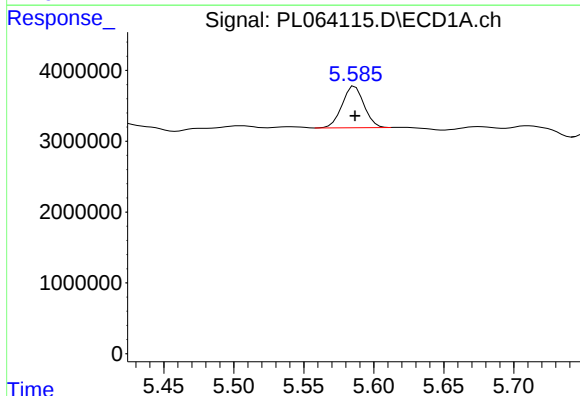


#12 4,4'-DDE

R.T.: 5.585 min
Delta R.T.: -0.002 min
Response: 6415638
Conc: 1.82 ng/ml m

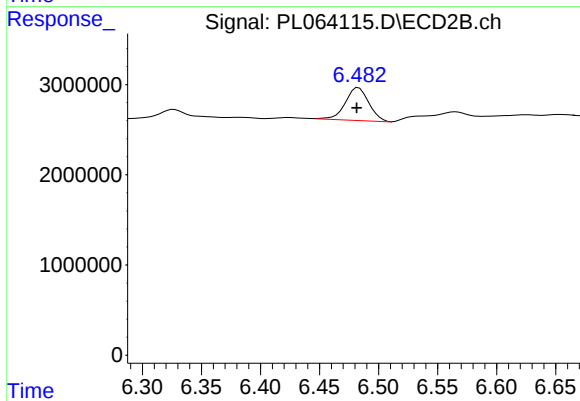

#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 5031027
Conc: 1.89 ng/ml m

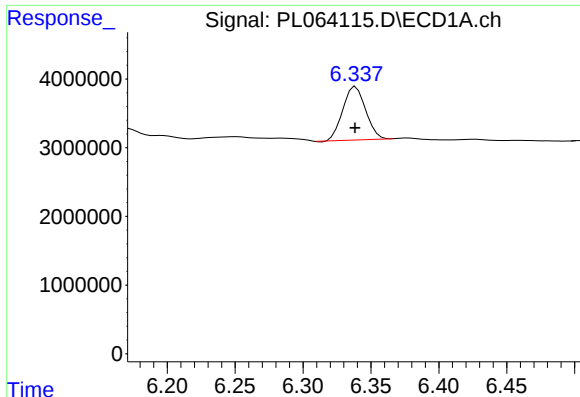


#17 4,4'-DDT

R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 9056947
Conc: 3.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-011121-B


Manual Integrations
APPROVED

Ankita
1/15/2021 10:22:56 AM

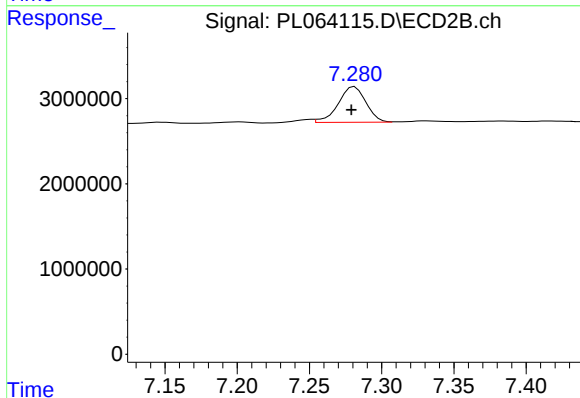


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 5550462
Conc: 2.45 ng/ml m

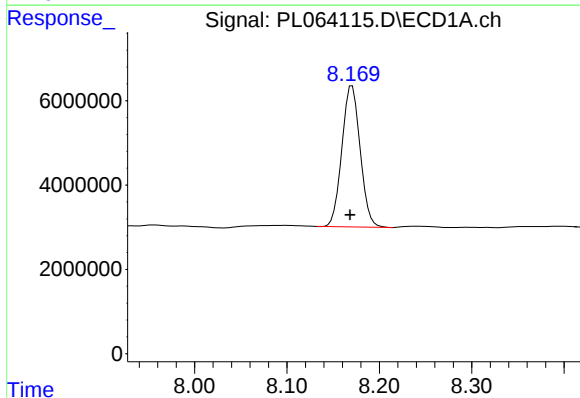

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 46018644
Conc: 15.08 ng/ml

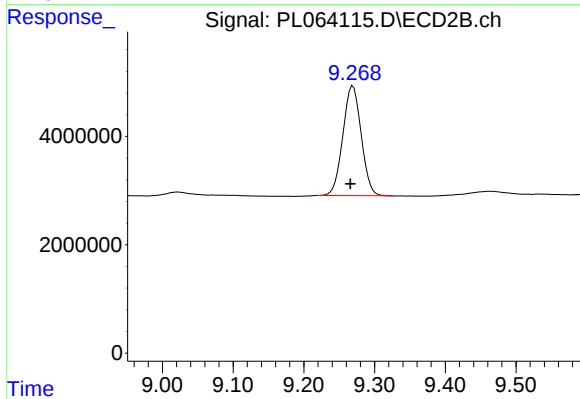

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.004 min
Response: 36537920
Conc: 15.39 ng/ml