

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
 Data File : PL064144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 21:35
 Operator : AR\AJ
 Sample : M1090-05MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BORE-3-1FT-7FTMSD

Manual Integrations
 APPROVED

Ankita
 1/15/2021 10:23:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:45:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	79696355	61645972	26.579	24.114
28)	SA Decachlor...	8.168	9.268	59713382	43552225	19.565	18.350
Target Compounds							
2)	A alpha-BHC	3.868	4.510	285.3E6	206.7E6	57.368	56.548
3)	MA gamma-BHC...	4.149	4.801	259.9E6	191.7E6	56.059	54.409
4)	MA Heptachlor	4.449	5.314	255.5E6	193.8E6	58.310	53.968
5)	MB Aldrin	4.694	5.625	245.6E6	178.7E6	61.298	57.562
6)	B beta-BHC	4.398	4.978	105.0E6	85338395	56.854	53.207
7)	B delta-BHC	4.601	5.199	253.5E6	174.1E6	54.733	54.851
8)	B Heptachlo...	5.135	6.018	230.9E6	178.0E6	60.932	68.339
9)	A Endosulfan I	5.472	6.381	191.2E6	146.7E6	54.140	53.540
10)	B gamma-Chl...	5.361	6.255	233.6E6	174.2E6	60.294	57.965
11)	B alpha-Chl...	5.419	6.327	220.7E6	158.6E6	57.688	52.086
12)	B 4,4'-DDE	5.586	6.484	205.9E6	178.7E6	58.456	67.074
13)	MA Dieldrin	5.711	6.641	298.3E6	158.9E6	80.206m	56.500 #
14)	MA Endrin	5.967	6.861	199.9E6	173.1E6	57.565m	75.804 #
15)	B Endosulfa...	6.238	7.075	219.1E6	121.9E6	64.631m	48.242m#
16)	A 4,4'-DDD	6.100	6.980	152.2E6	166.5E6	52.173	75.123m#
17)	MA 4,4'-DDT	6.337	7.281	290.5E6	135.5E6	97.303	59.838 #
18)	B Endrin al...	6.408	7.200	152.3E6	102.4E6	53.094	47.240m
19)	B Endosulfa...	6.621	7.425	191.3E6	123.5E6	56.397	50.000
20)	A Methoxychlor	6.886	7.741	112.9E6	65203288	67.542	48.257 #
21)	B Endrin ke...	7.108	7.905	183.6E6	125.7E6	51.123	50.405
22)	Mirex	7.294	8.357	142.2E6	97647162	52.283	48.134

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011421\
Data File : PL064144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 21:35
Operator : AR\AJ
Sample : M1090-05MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:45:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

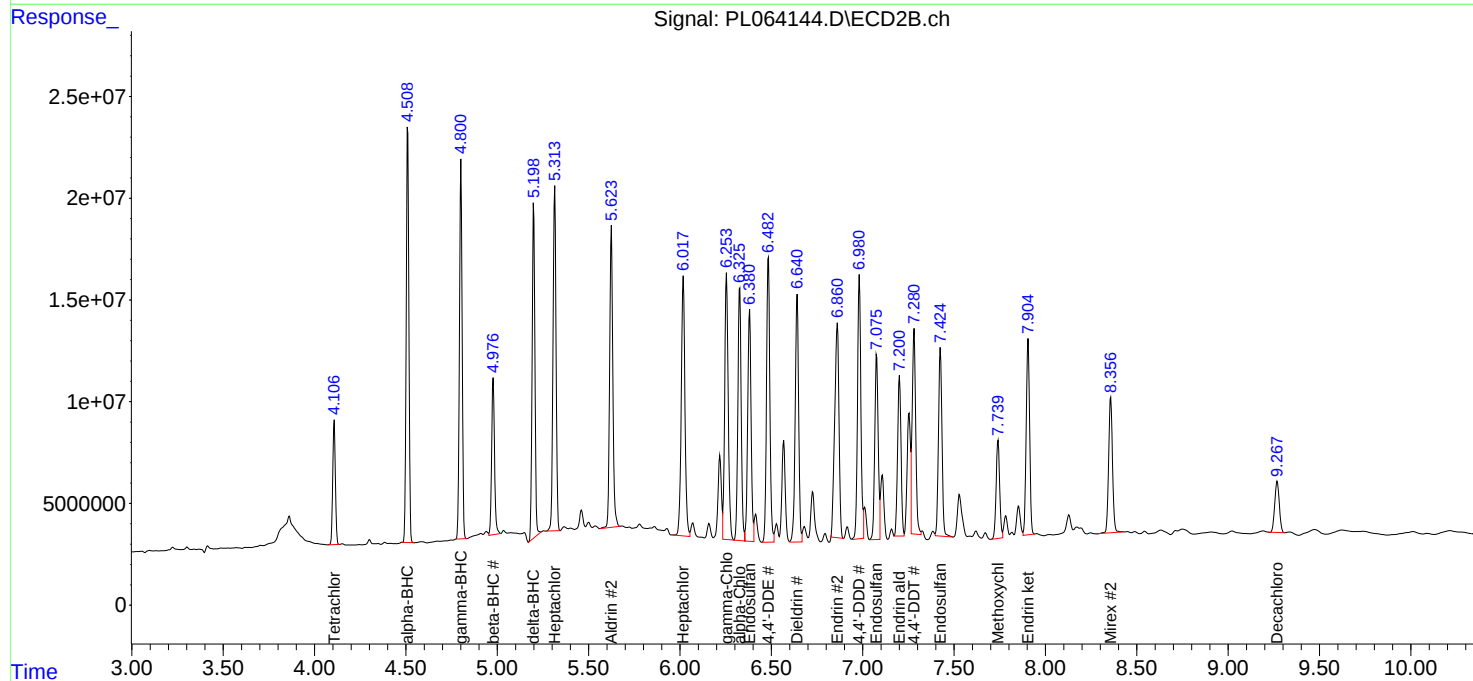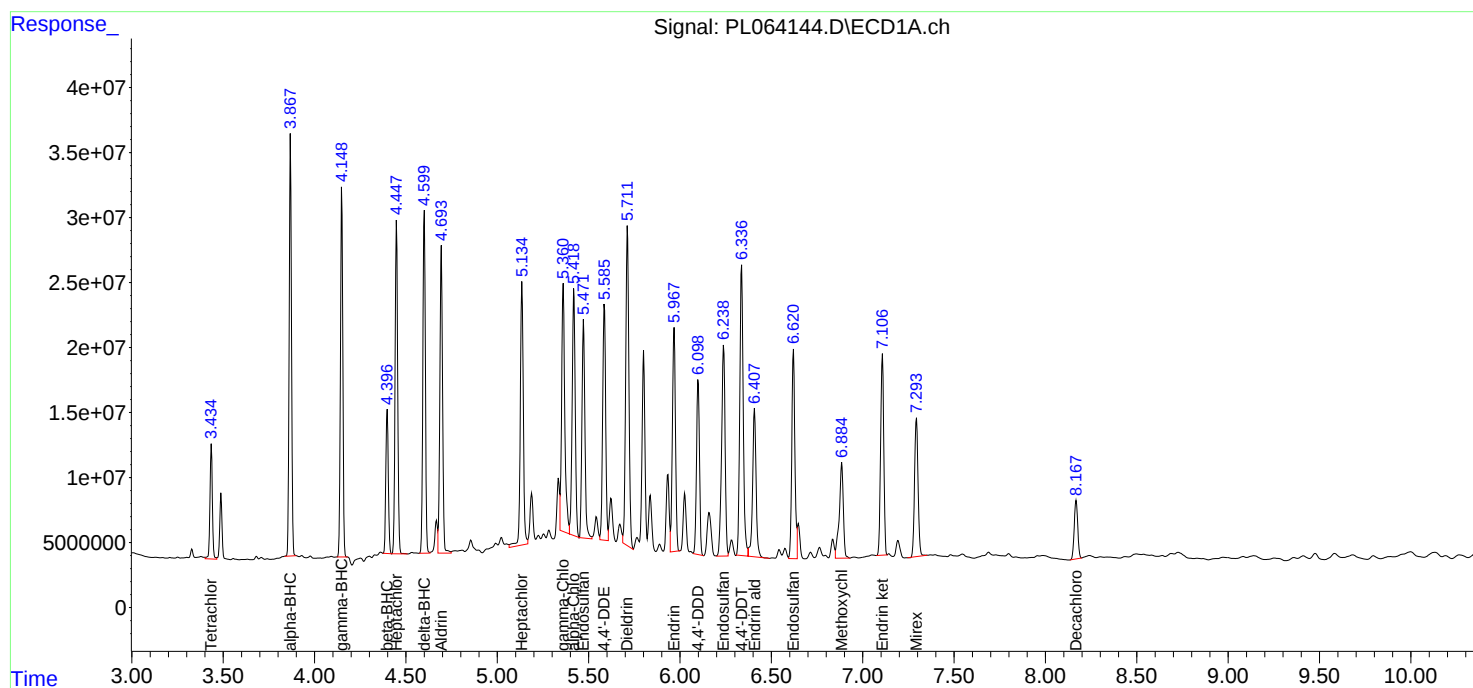

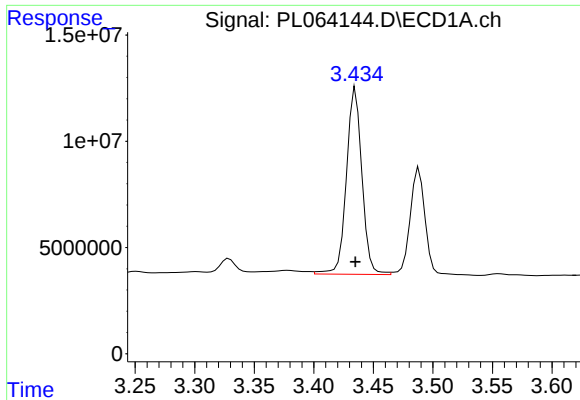


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 79696355
Conc: 26.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

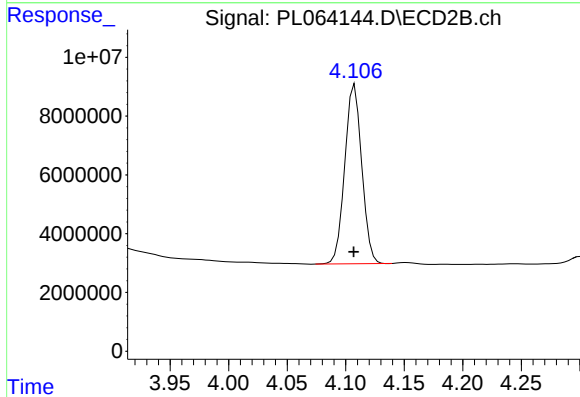


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 61645972
Conc: 24.11 ng/ml

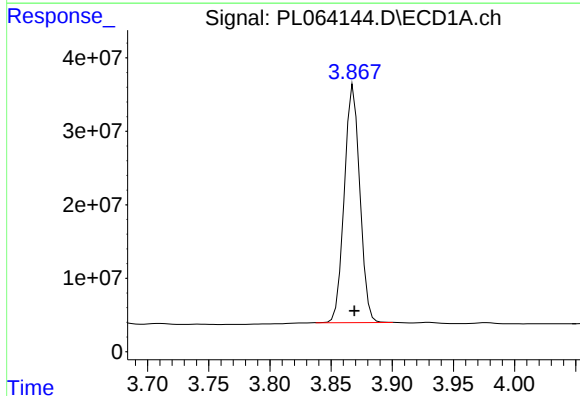


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 285340784
Conc: 57.37 ng/ml

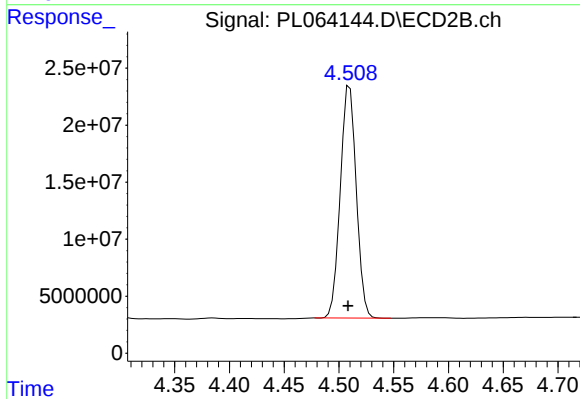

#2 alpha-BHC

R.T.: 4.510 min
Delta R.T.: 0.002 min
Response: 206657086
Conc: 56.55 ng/ml

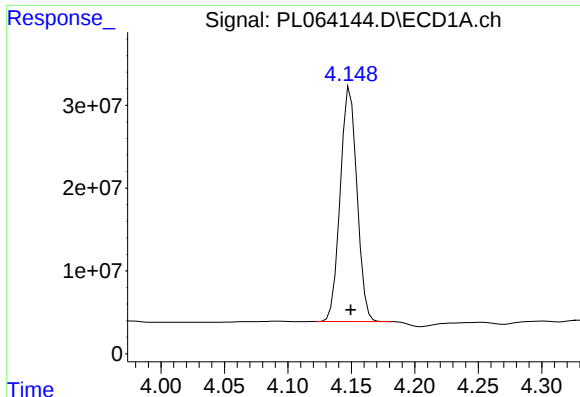


#3 gamma-BHC (Lindane)

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 259915553
Conc: 56.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

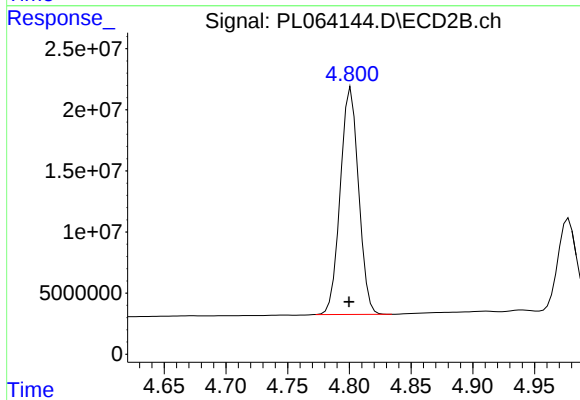


#3 gamma-BHC (Lindane)

R.T.: 4.801 min
Delta R.T.: 0.001 min
Response: 191655154
Conc: 54.41 ng/ml

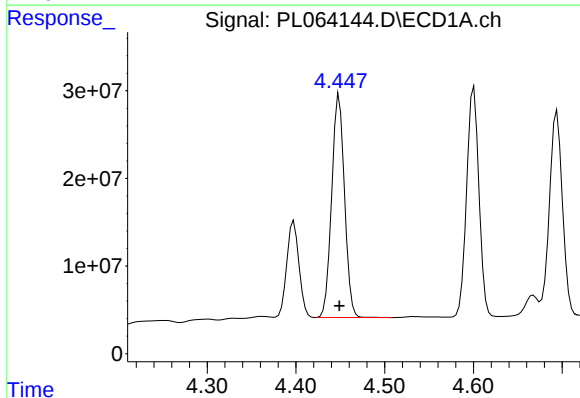


#4 Heptachlor

R.T.: 4.449 min
Delta R.T.: 0.000 min
Response: 255498420
Conc: 58.31 ng/ml

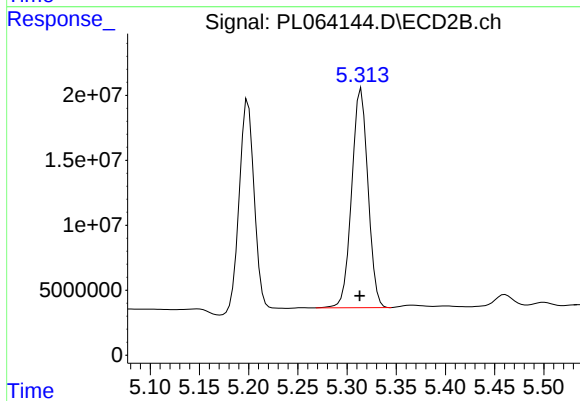

#4 Heptachlor

R.T.: 5.314 min
Delta R.T.: 0.002 min
Response: 193836799
Conc: 53.97 ng/ml

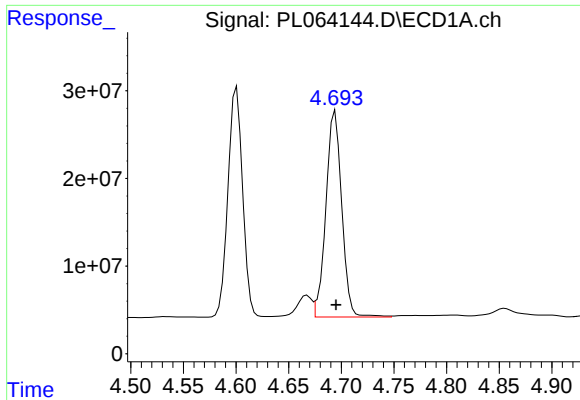


#5 Aldrin

R.T.: 4.694 min
Delta R.T.: 0.000 min
Response: 245620573
Conc: 61.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

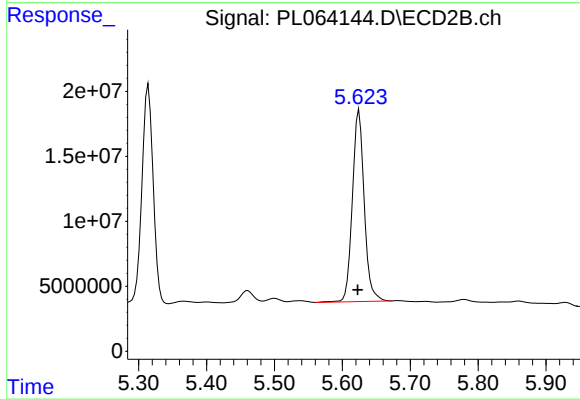


#5 Aldrin

R.T.: 5.625 min
Delta R.T.: 0.002 min
Response: 178661336
Conc: 57.56 ng/ml

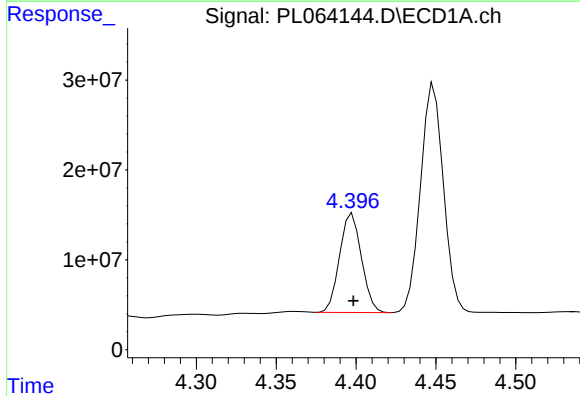


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 105026891
Conc: 56.85 ng/ml

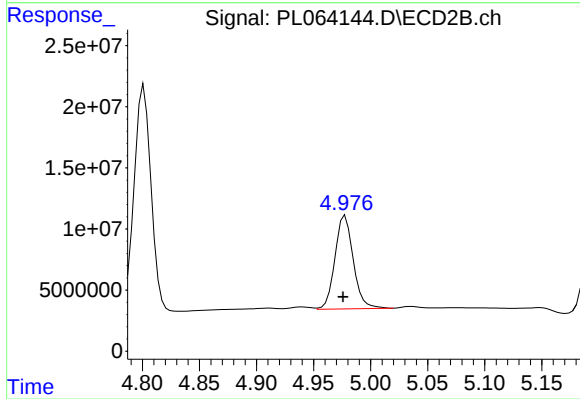

#6 beta-BHC

R.T.: 4.978 min
Delta R.T.: 0.002 min
Response: 85338395
Conc: 53.21 ng/ml

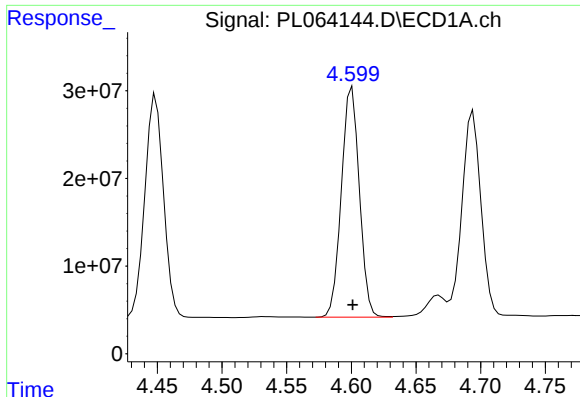


#7 delta-BHC

R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 253465575
Conc: 54.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

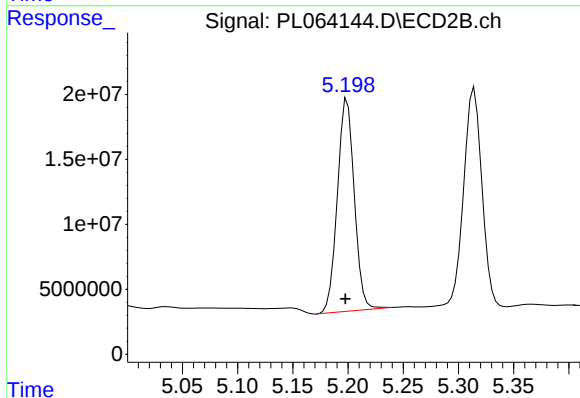


#7 delta-BHC

R.T.: 5.199 min
Delta R.T.: 0.002 min
Response: 174133592
Conc: 54.85 ng/ml

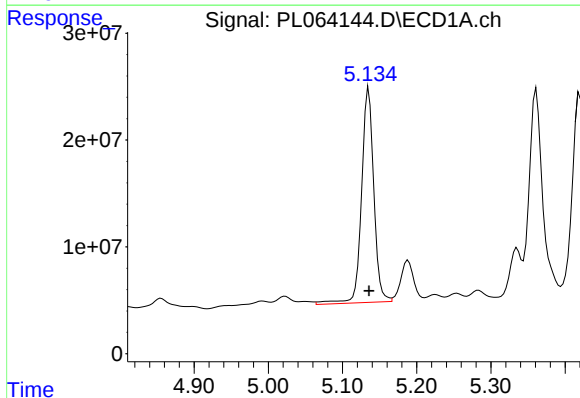


#8 Heptachlor epoxide

R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 230906112
Conc: 60.93 ng/ml

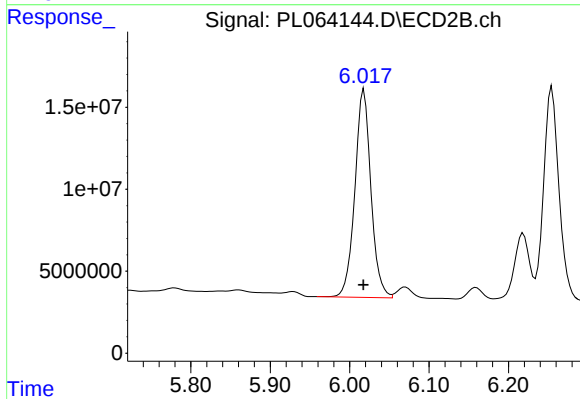

#8 Heptachlor epoxide

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 178031230
Conc: 68.34 ng/ml

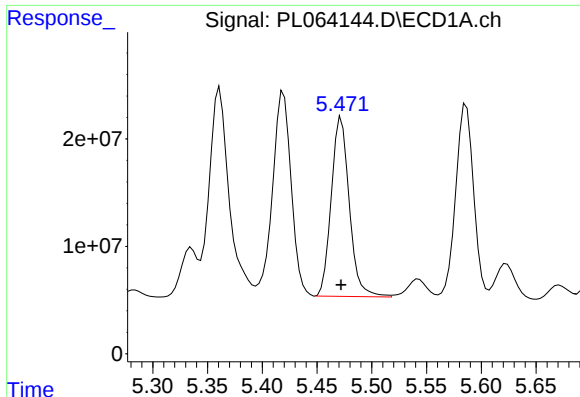


#9 Endosulfan I

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 191233020
Conc: 54.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

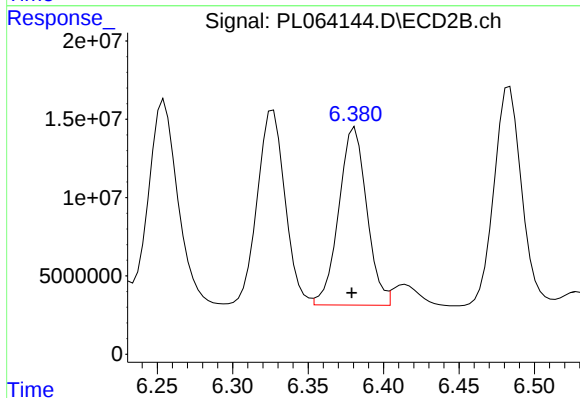


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 146739662
Conc: 53.54 ng/ml

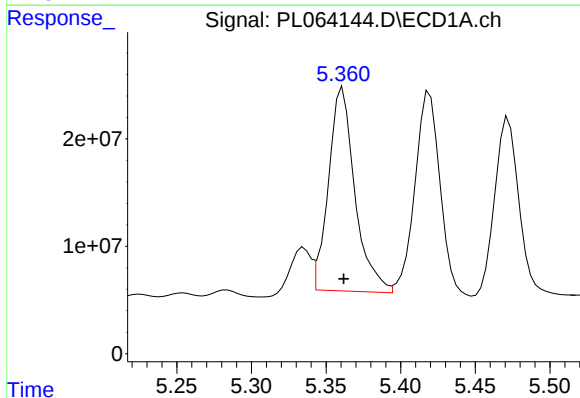


#10 gamma-Chlordane

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 233560299
Conc: 60.29 ng/ml

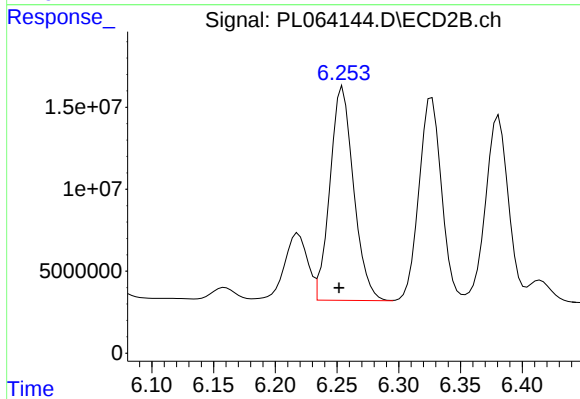

#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: 0.003 min
Response: 174174664
Conc: 57.97 ng/ml

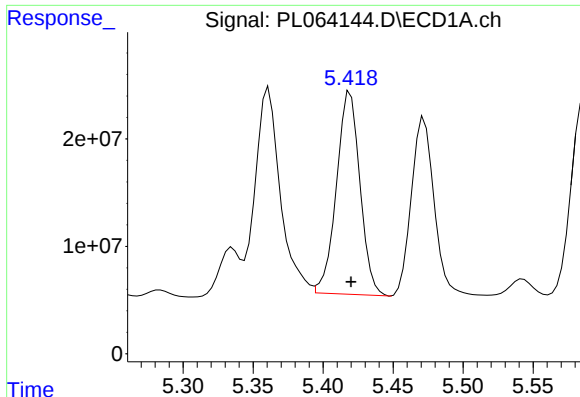


#11 alpha-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.000 min
Response: 220728667
Conc: 57.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

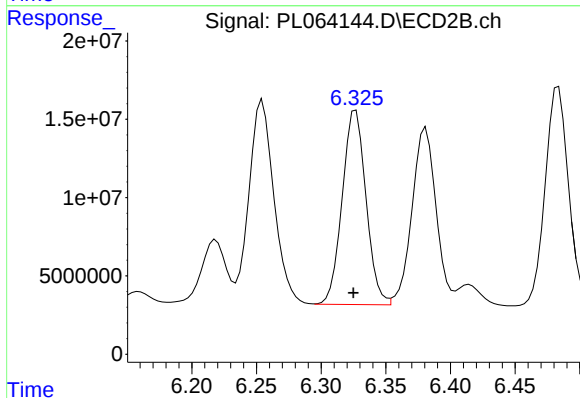


#11 alpha-Chlordane

R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 158557308
Conc: 52.09 ng/ml

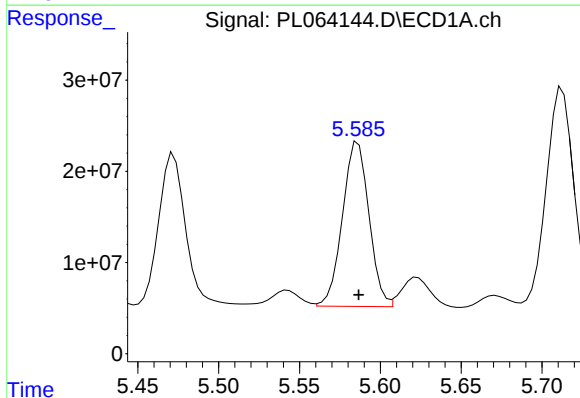


#12 4,4'-DDE

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 205931744
Conc: 58.46 ng/ml

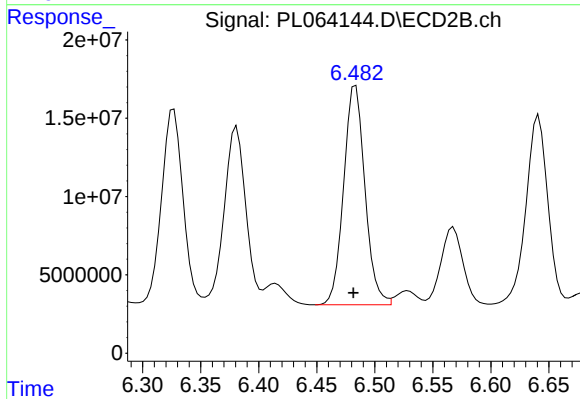

#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 178659304
Conc: 67.07 ng/ml

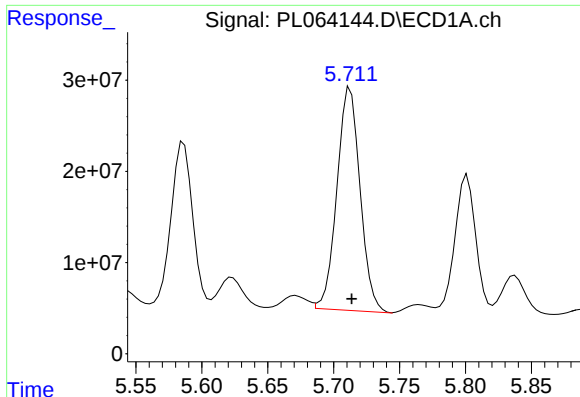


#13 Dieldrin

R.T.: 5.711 min
Delta R.T.: -0.003 min
Response: 298331437
Conc: 80.21 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

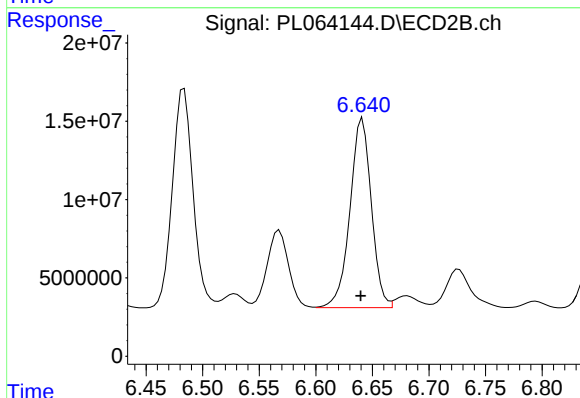


#13 Dieldrin

R.T.: 6.641 min
Delta R.T.: 0.001 min
Response: 158874241
Conc: 56.50 ng/ml

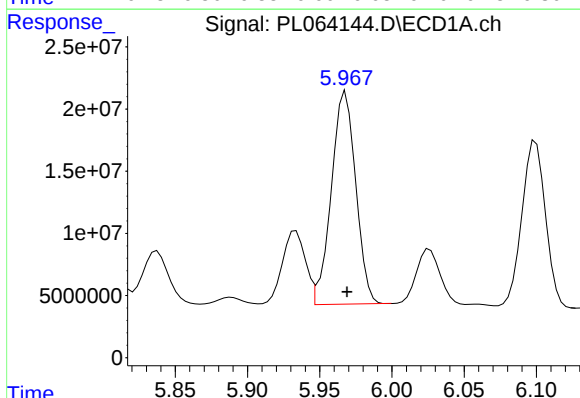


#14 Endrin

R.T.: 5.967 min
Delta R.T.: -0.002 min
Response: 199887516
Conc: 57.56 ng/ml m

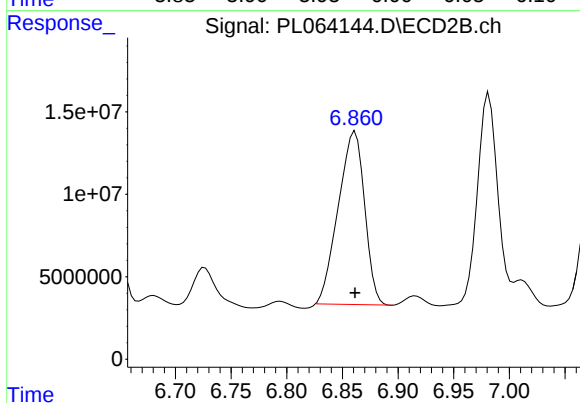

#14 Endrin

R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 173101001
Conc: 75.80 ng/ml

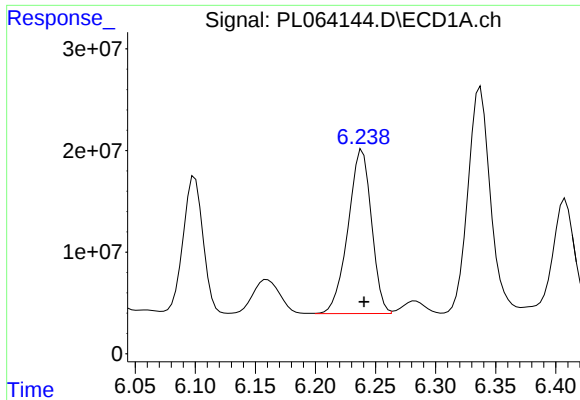


#15 Endosulfan II

R.T.: 6.238 min
Delta R.T.: -0.003 min
Response: 219079309
Conc: 64.63 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

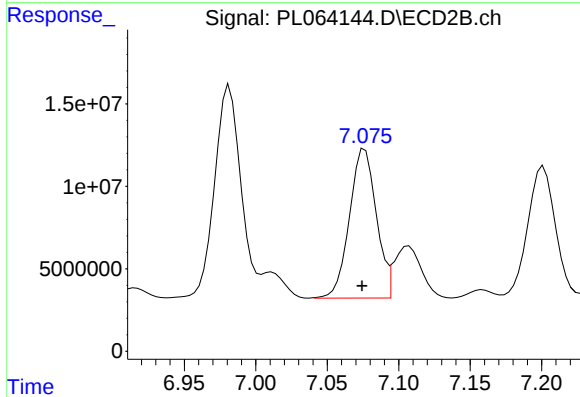


#15 Endosulfan II

R.T.: 7.075 min
Delta R.T.: 0.000 min
Response: 121868782
Conc: 48.24 ng/ml m

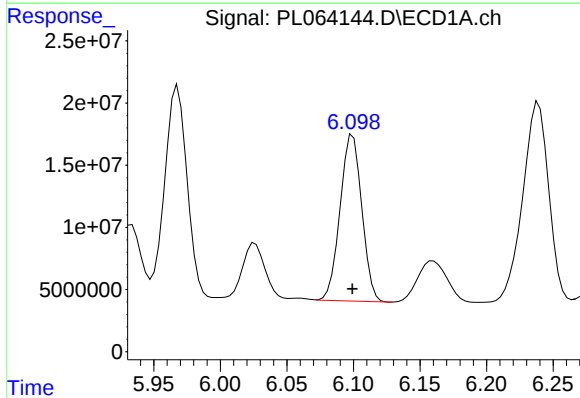


#16 4,4'-DDD

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 152167335
Conc: 52.17 ng/ml

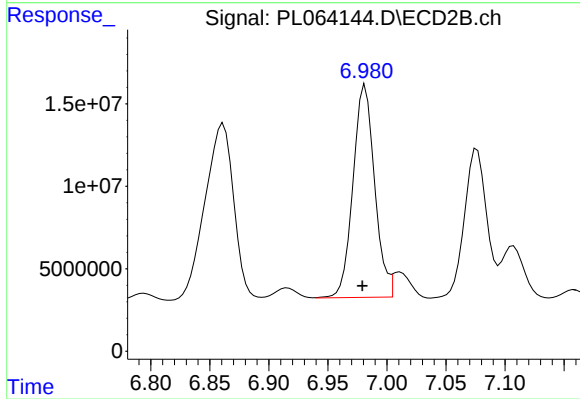

#16 4,4'-DDD

R.T.: 6.980 min
Delta R.T.: 0.001 min
Response: 166513328
Conc: 75.12 ng/ml m

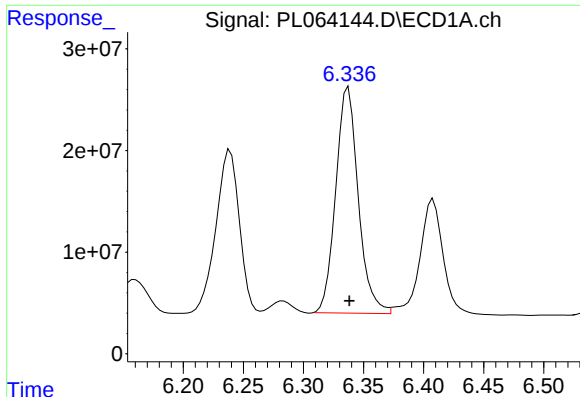


#17 4,4'-DDT

R.T.: 6.337 min
Delta R.T.: 0.000 min
Response: 290484364
Conc: 97.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

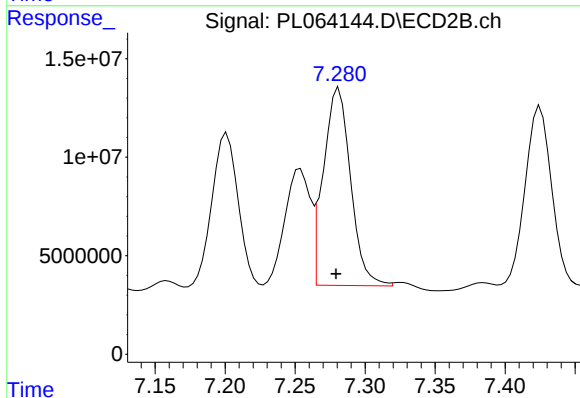


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.002 min
Response: 135530358
Conc: 59.84 ng/ml

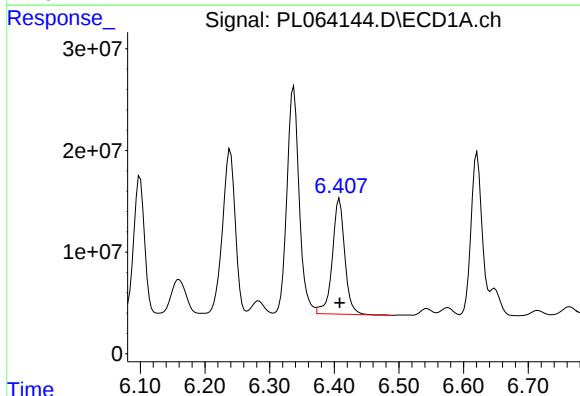


#18 Endrin aldehyde

R.T.: 6.408 min
Delta R.T.: 0.000 min
Response: 152299082
Conc: 53.09 ng/ml

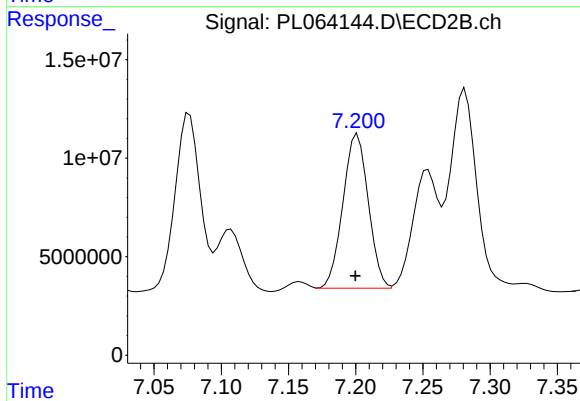

#18 Endrin aldehyde

R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 102422936
Conc: 47.24 ng/ml m

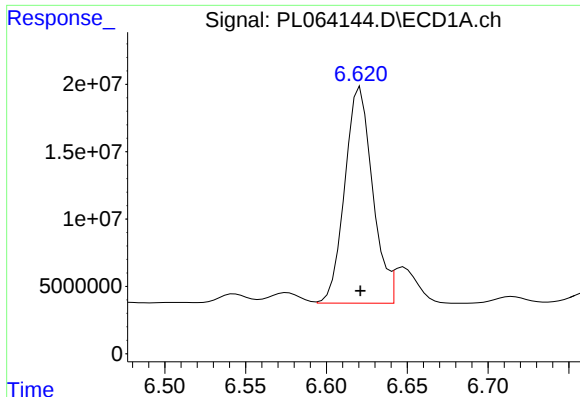


#19 Endosulfan Sulfate

R.T.: 6.621 min
Delta R.T.: 0.000 min
Response: 191326270
Conc: 56.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

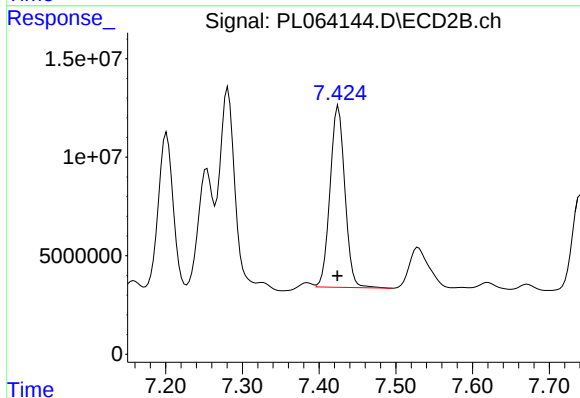


#19 Endosulfan Sulfate

R.T.: 7.425 min
Delta R.T.: 0.002 min
Response: 123500293
Conc: 50.00 ng/ml

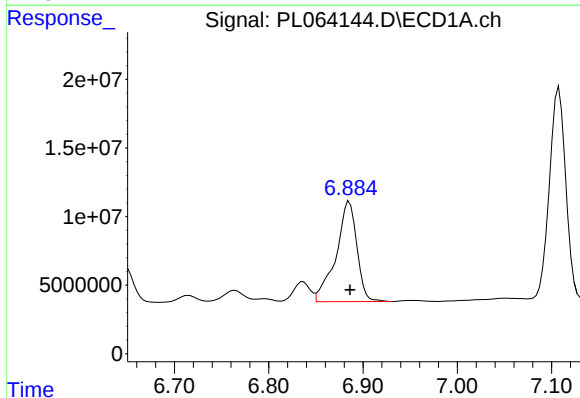


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 112872759
Conc: 67.54 ng/ml

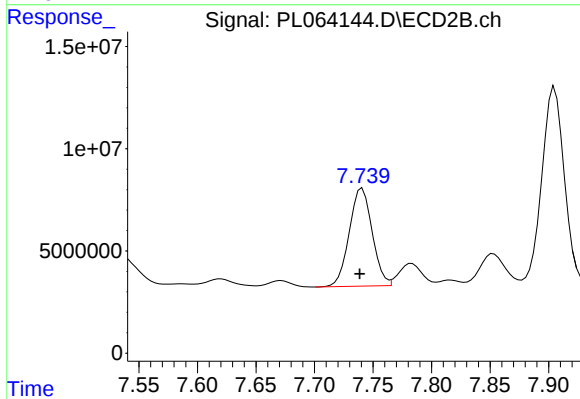

#20 Methoxychlor

R.T.: 7.741 min
Delta R.T.: 0.002 min
Response: 65203288
Conc: 48.26 ng/ml

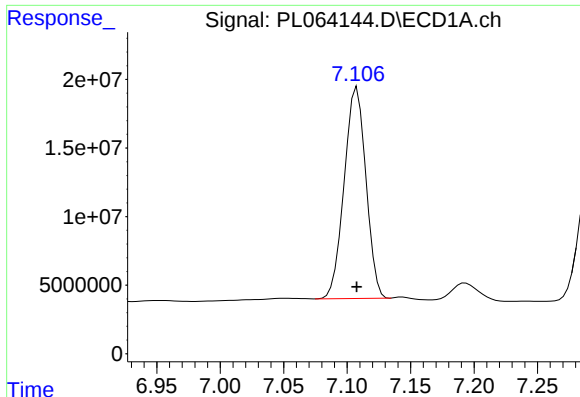


#21 Endrin ketone

R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 183598791
Conc: 51.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD


Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

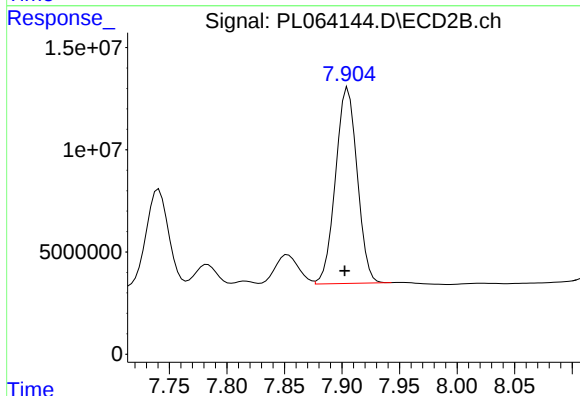


#21 Endrin ketone

R.T.: 7.905 min
Delta R.T.: 0.003 min
Response: 125721016
Conc: 50.41 ng/ml

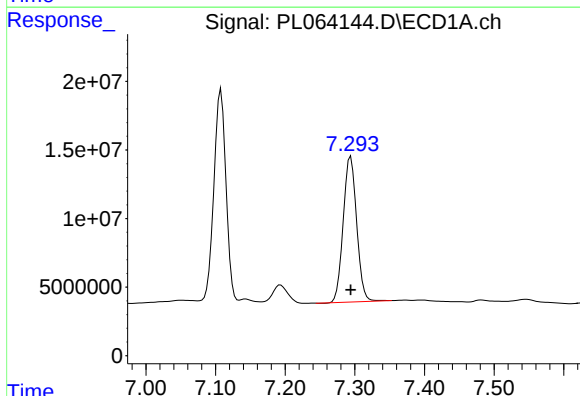


#22 Mirex

R.T.: 7.294 min
Delta R.T.: 0.000 min
Response: 142244309
Conc: 52.28 ng/ml

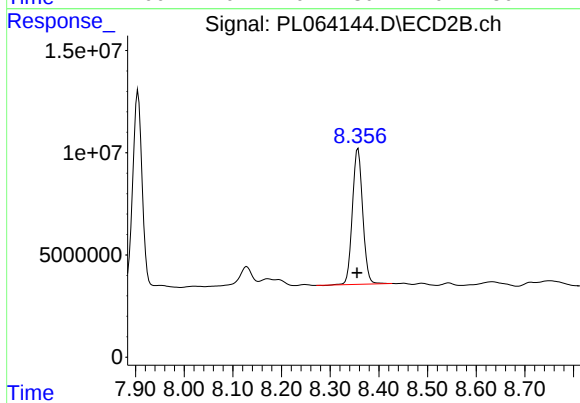

#22 Mirex

R.T.: 8.357 min
Delta R.T.: 0.002 min
Response: 97647162
Conc: 48.13 ng/ml

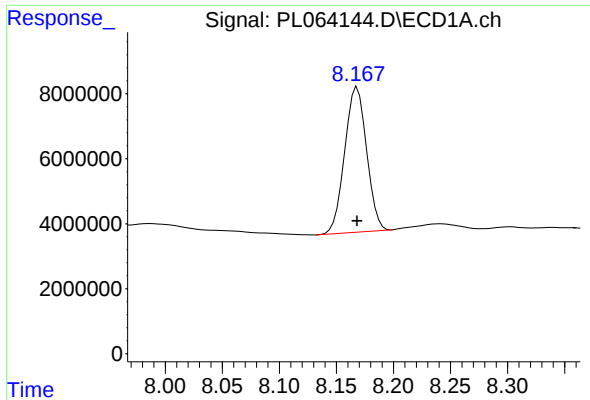


#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 59713382
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORE-3-1FT-7FTMSD

Manual Integrations
APPROVED

Ankita
1/15/2021 10:23:18 AM

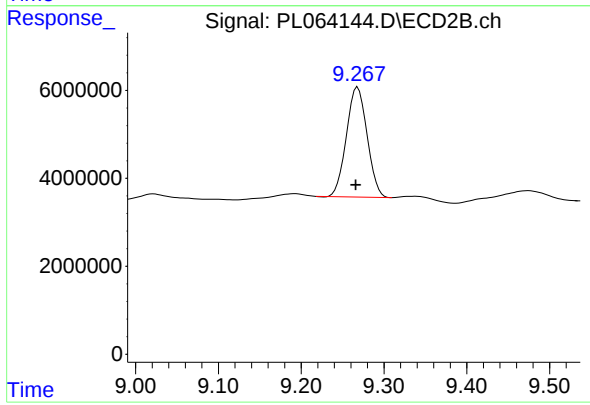

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 43552225
Conc: 18.35 ng/ml