

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
 Data File : PL071994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 13:16
 Operator : AR\AJ
 Sample : PB142029BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:34:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.494	10092947	27356687	21.849	22.266
28)	SA Decachlor...	10.327	11.392	17109883	29370221	23.664	24.785
Target Compounds							
6)	B beta-BHC	6.044f	6.740	226008	1423145	0.835	1.992 #
7)	B delta-BHC	0.000	6.976f	0	284664	N.D.	0.185 #
9)	A Endosulfan I	0.000	8.379f	0	80778	N.D.	0.065 #
10)	B gamma-Chl...	0.000	8.222	0	69783	N.D.	0.051 #
11)	B alpha-Chl...	0.000	8.302	0	28829	N.D.	0.022 #
15)	B Endosulfa...	0.000	9.149f	0	502190	N.D.	0.447 #
21)	B Endrin ke...	0.000	9.993	0	178260	N.D.	0.158 #
25)	Chlordane-3	0.000	8.222	0	69783	N.D.	0.342 #
26)	Chlordane-4	0.000	8.302	0	28829	N.D.	0.118 #
27)	Chlordane-5	0.000	9.192	0	65593	N.D.	1.638 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
Data File : PL071994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 13:16
Operator : AR\AJ
Sample : PB142029BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:34:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

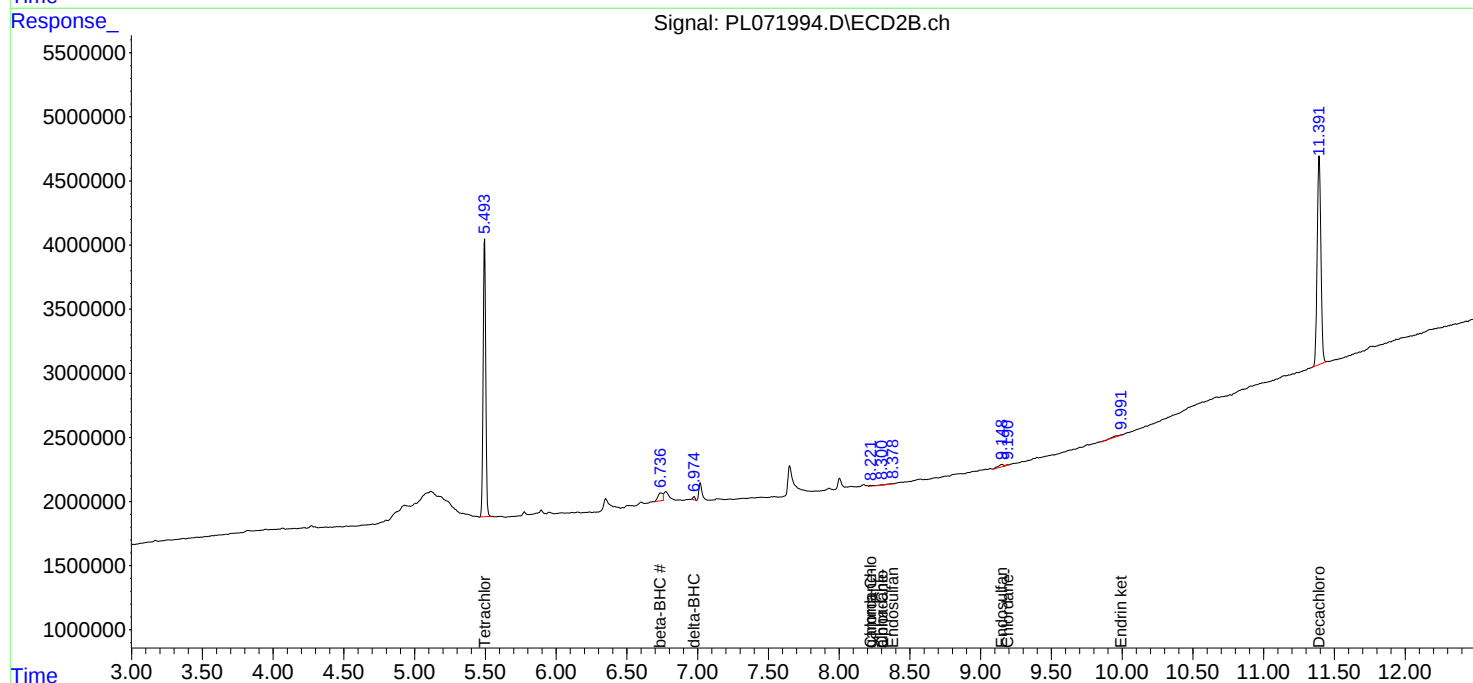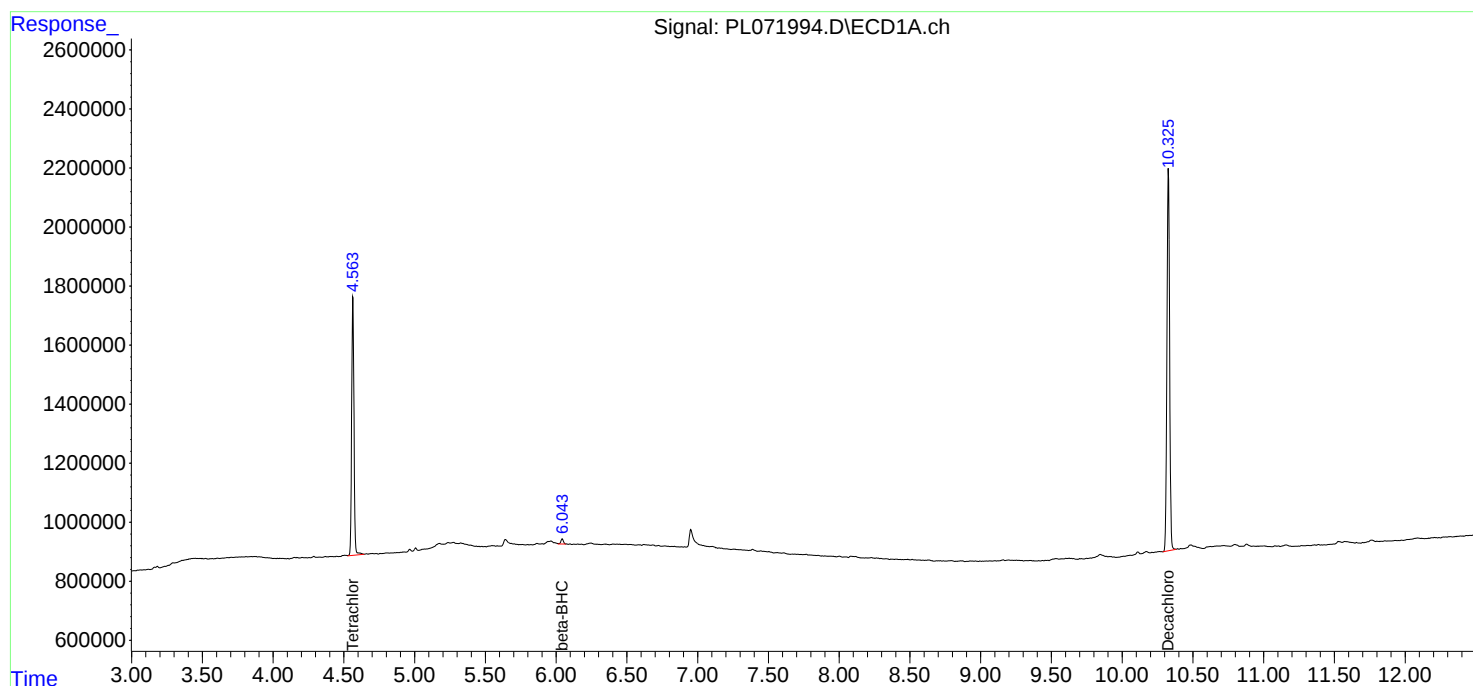


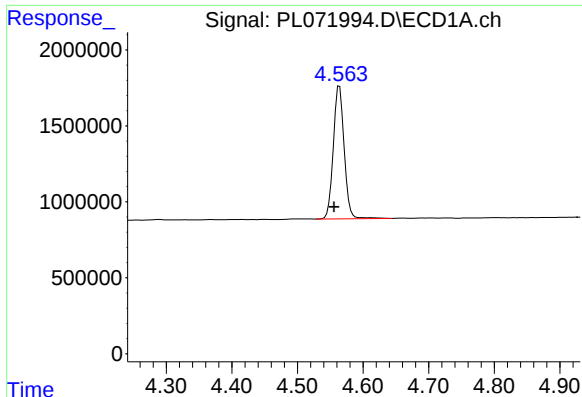

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.008 min
Response: 10092947
Conc: 21.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

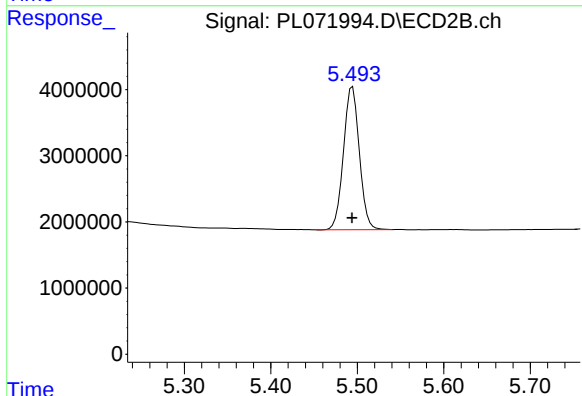


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 27356687
Conc: 22.27 ng/ml

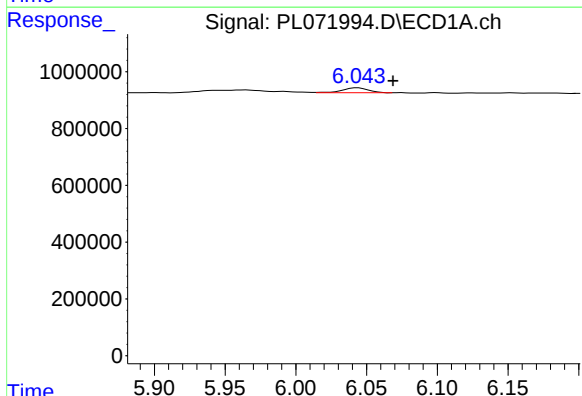


#6 beta-BHC

R.T.: 6.044 min
Delta R.T.: -0.025 min
Response: 226008
Conc: 0.84 ng/ml

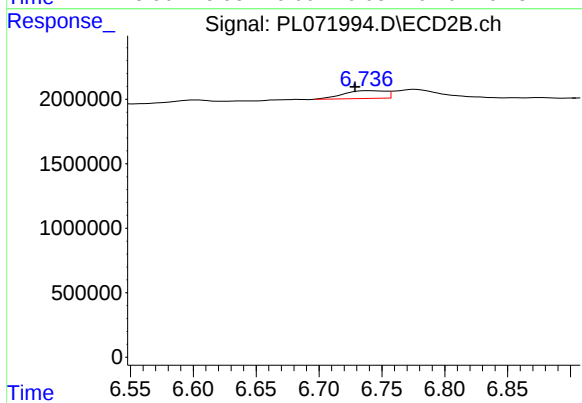

#6 beta-BHC


R.T.: 6.740 min
Delta R.T.: 0.011 min
Response: 1423145
Conc: 1.99 ng/ml

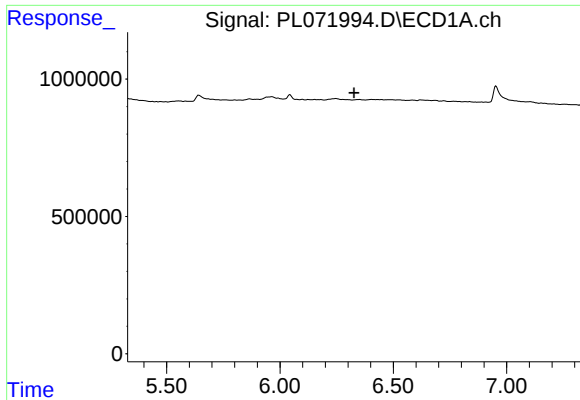

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

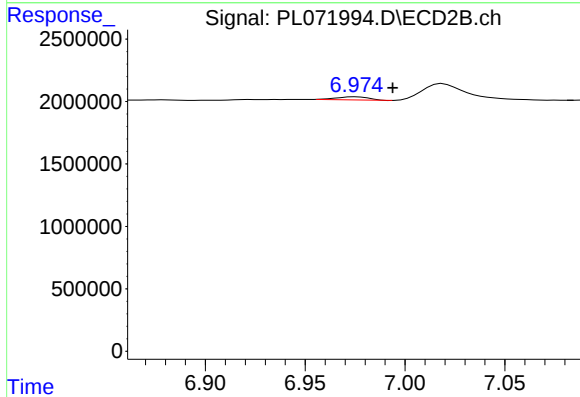


#7 delta-BHC

R.T.: 6.976 min
Delta R.T.: -0.018 min
Response: 284664
Conc: 0.19 ng/ml

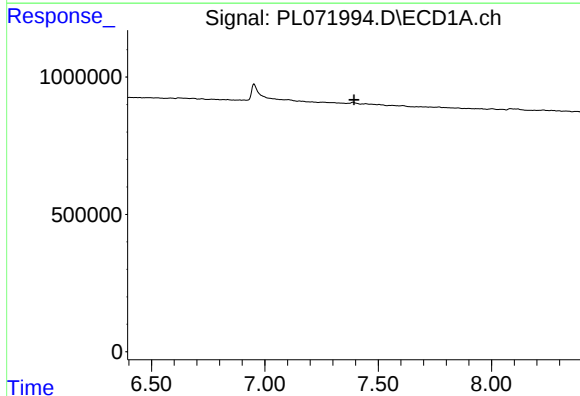


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

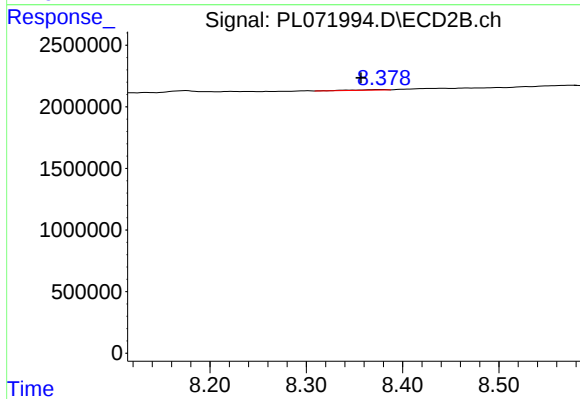

#9 Endosulfan I


R.T.: 8.379 min
Delta R.T.: 0.022 min
Response: 80778
Conc: 0.07 ng/ml

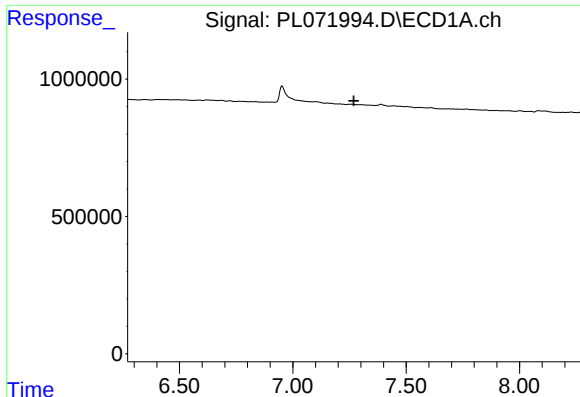

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

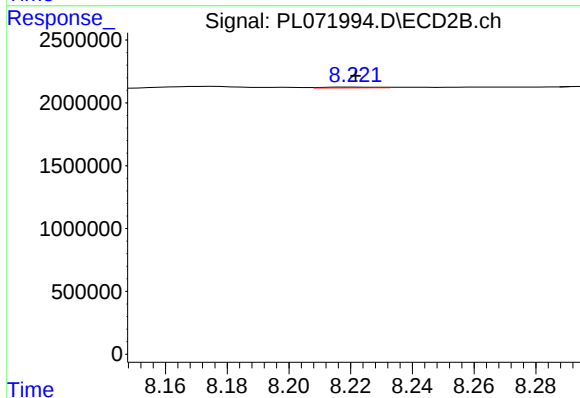


#10 gamma-Chlordane

R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 69783
Conc: 0.05 ng/ml

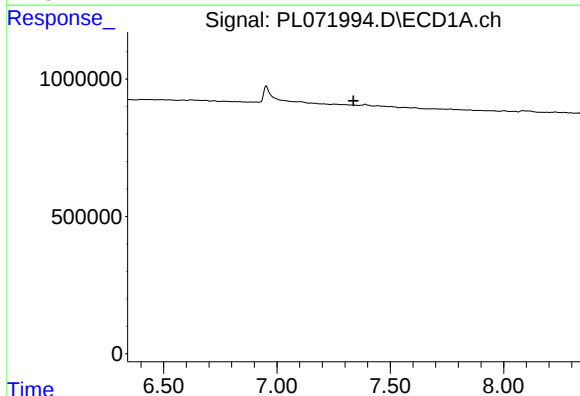


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

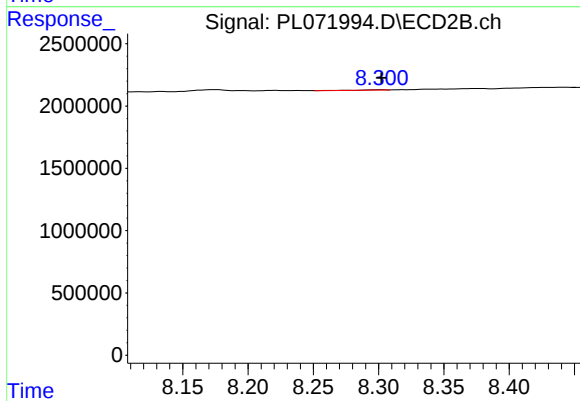

#11 alpha-Chlordane


R.T.: 8.302 min
Delta R.T.: 0.000 min
Response: 28829
Conc: 0.02 ng/ml

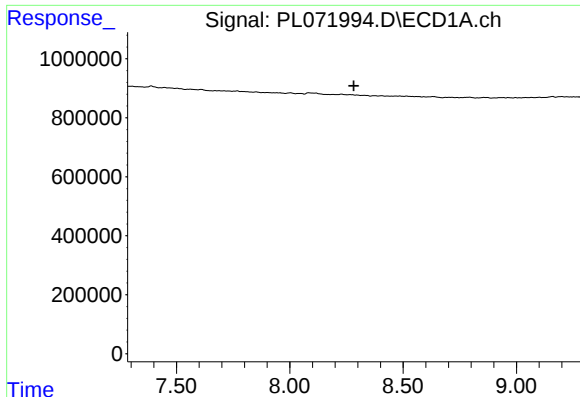

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

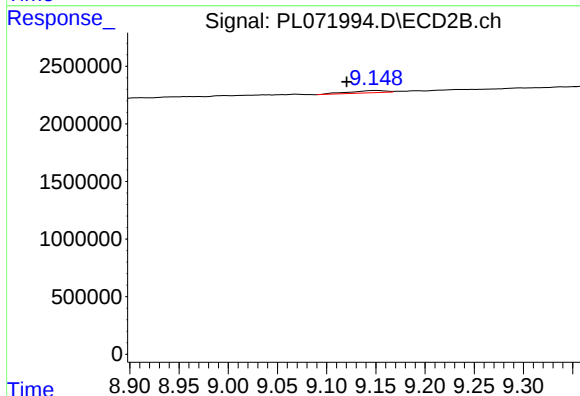


#15 Endosulfan II

R.T.: 9.149 min
Delta R.T.: 0.029 min
Response: 502190
Conc: 0.45 ng/ml

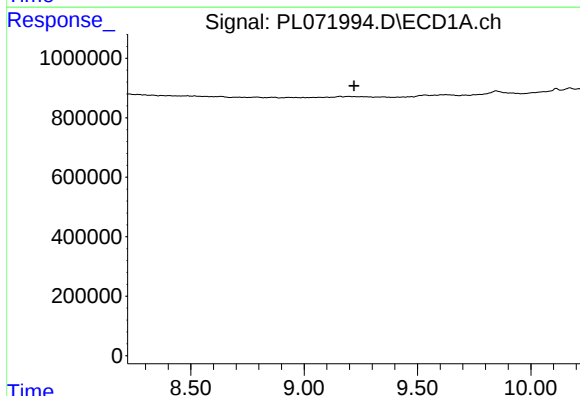


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

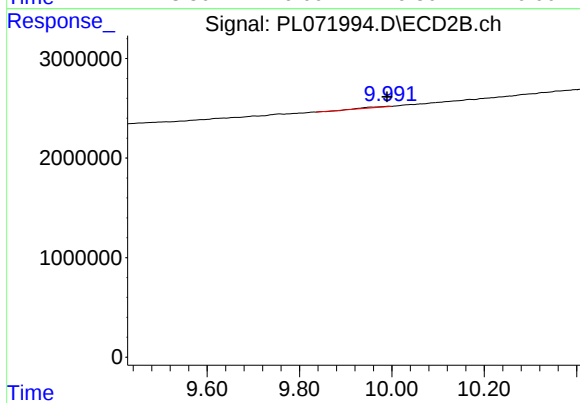

#21 Endrin ketone


R.T.: 9.993 min
Delta R.T.: 0.003 min
Response: 178260
Conc: 0.16 ng/ml

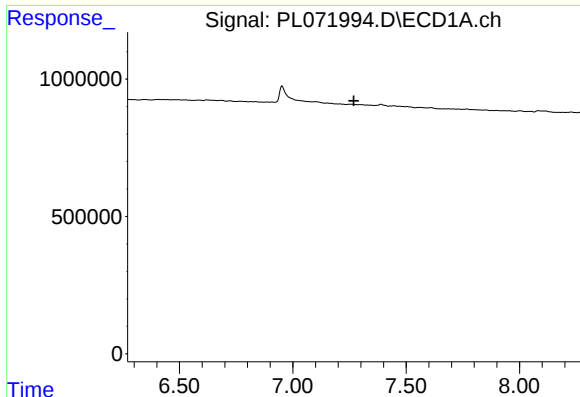

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

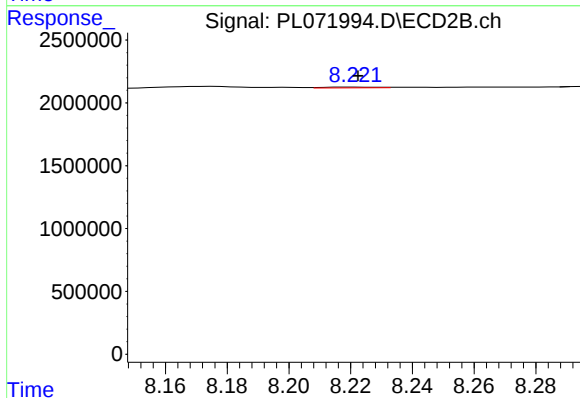


#25 Chlordane-3

R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 69783
Conc: 0.34 ng/ml

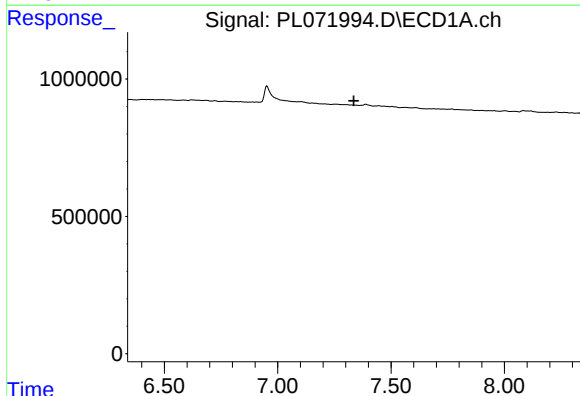


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

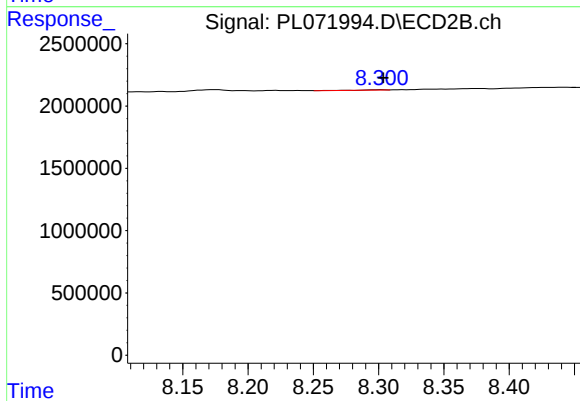

#26 Chlordane-4


R.T.: 8.302 min
Delta R.T.: -0.002 min
Response: 28829
Conc: 0.12 ng/ml

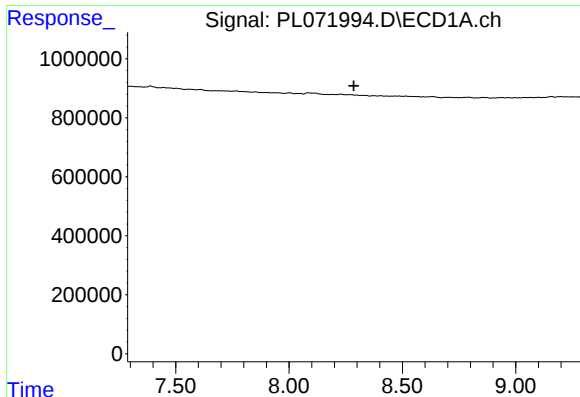

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

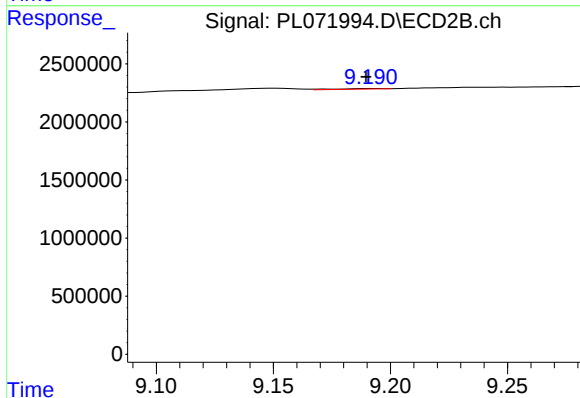


#27 Chlorine-5

R.T.: 9.192 min
Delta R.T.: 0.002 min
Response: 65593
Conc: 1.64 ng/ml

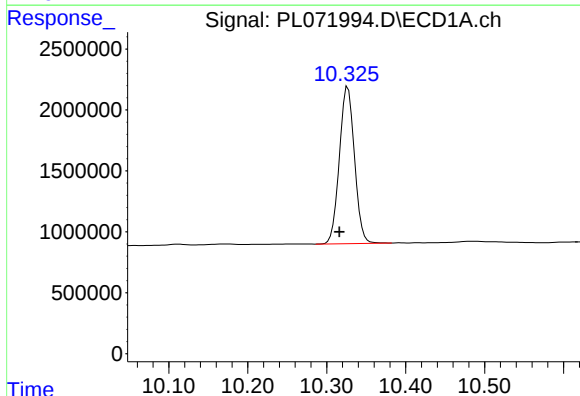

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.011 min
Response: 17109883
Conc: 23.66 ng/ml

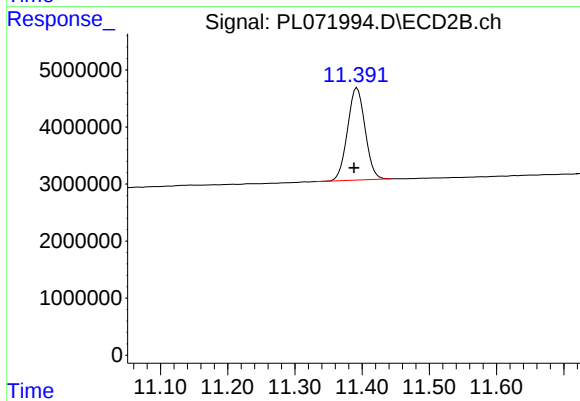

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.004 min
Response: 29370221
Conc: 24.78 ng/ml