

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
 Data File : PL072001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 15:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:36:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	9735963	28130595	21.076	22.896
28)	SA Decachlor...	10.322	11.389	15827353	28654730	21.890	24.181
Target Compounds							
7)	B delta-BHC	0.000	6.971f	0	387769	N.D.	0.253 #
8)	B Heptachlo...	0.000	7.966	0	519578	N.D.	0.372 #
10)	B gamma-Chl...	0.000	8.231	0	322514	N.D.	0.236 #
11)	B alpha-Chl...	0.000	8.317	0	92518	N.D.	0.070 #
15)	B Endosulfa...	0.000	9.104f	0	135203	N.D.	0.120 #
16)	A 4,4'-DDD	0.000	9.035	0	126379	N.D.	0.131 #
19)	B Endosulfa...	0.000	9.511f	0	58577	N.D.	0.056 #
25)	Chlordane-3	0.000	8.231	0	322514	N.D.	1.580 #
26)	Chlordane-4	0.000	8.317	0	92518	N.D.	0.380 #
27)	Chlordane-5	0.000	9.186	0	24442	N.D.	0.610 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
Data File : PL072001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 15:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:36:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

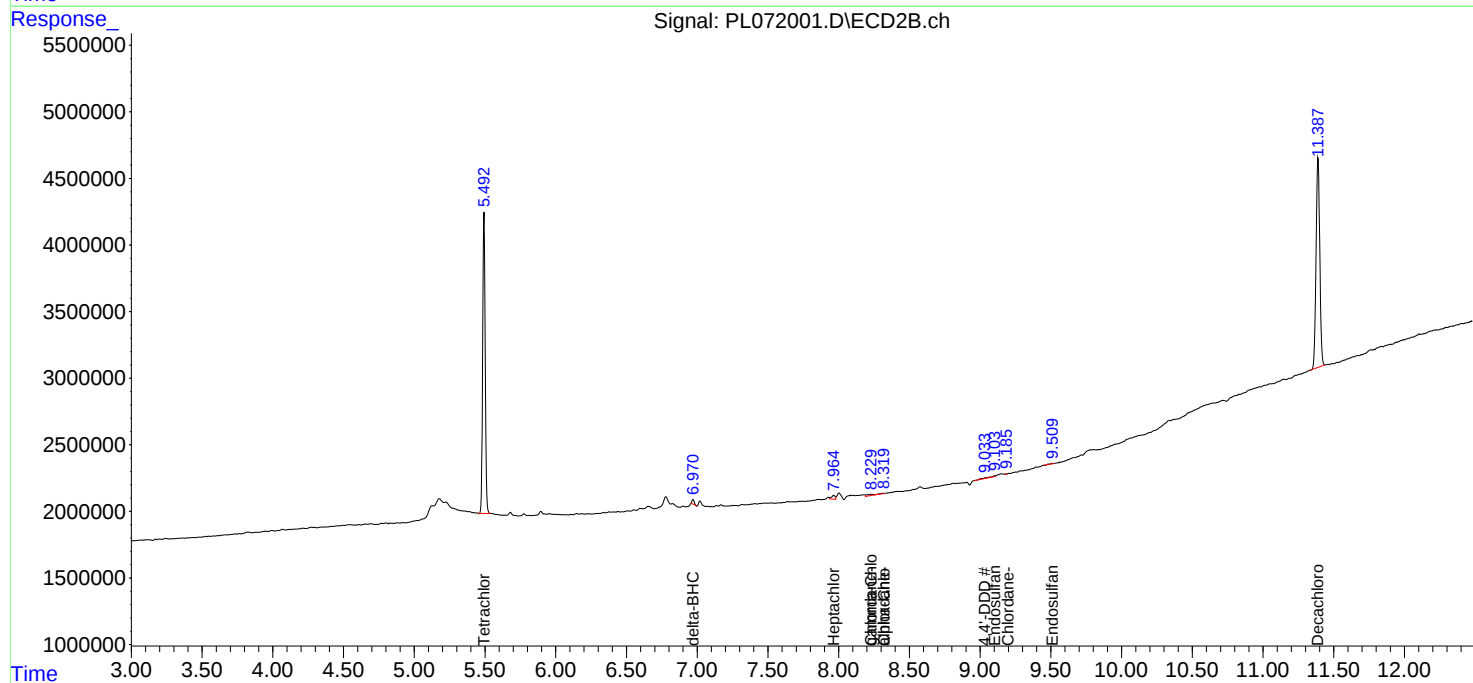


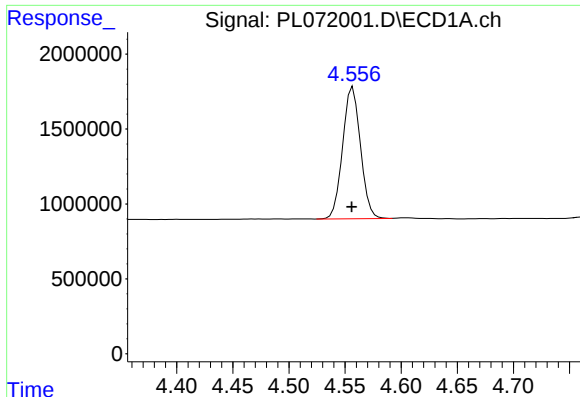

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 9735963
Conc: 21.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

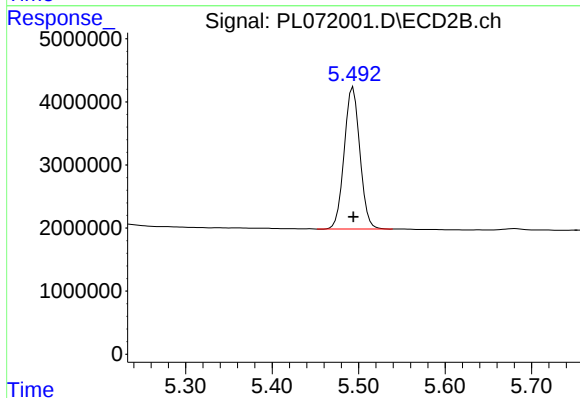


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 28130595
Conc: 22.90 ng/ml

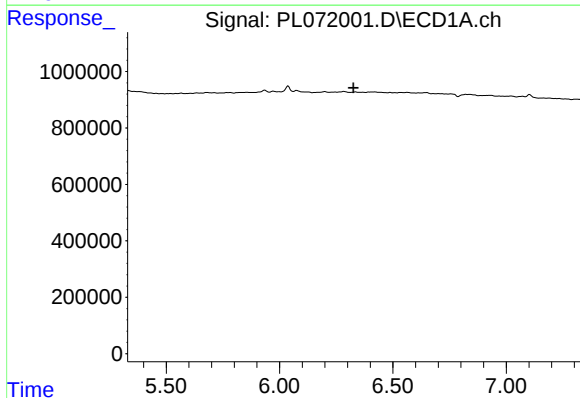


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

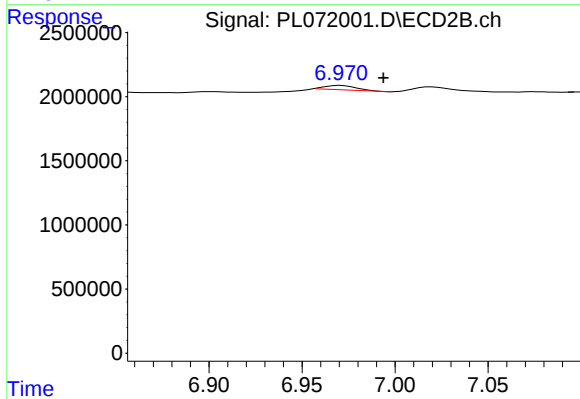

#7 delta-BHC


R.T.: 6.971 min
Delta R.T.: -0.023 min
Response: 387769
Conc: 0.25 ng/ml

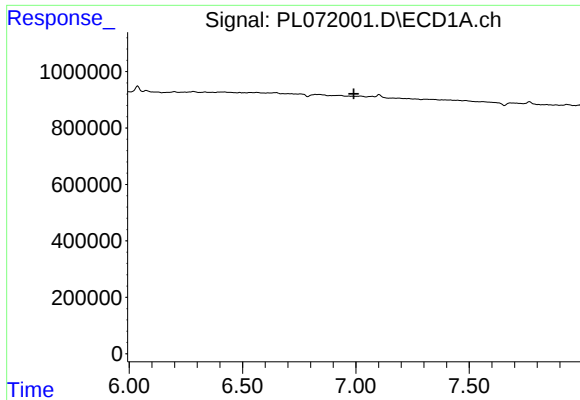

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

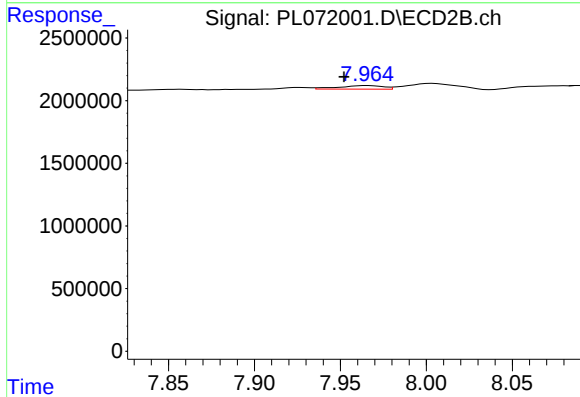


#8 Heptachlor epoxide

R.T.: 7.966 min
Delta R.T.: 0.013 min
Response: 519578
Conc: 0.37 ng/ml

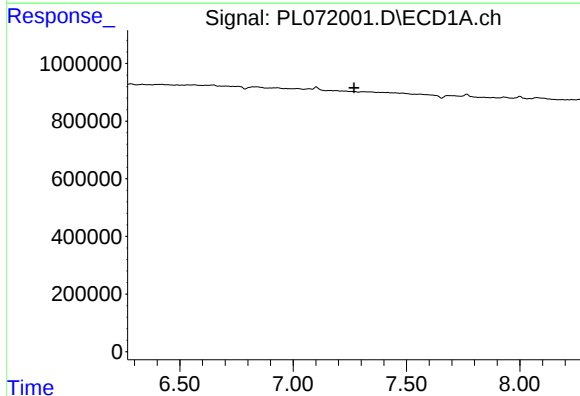


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

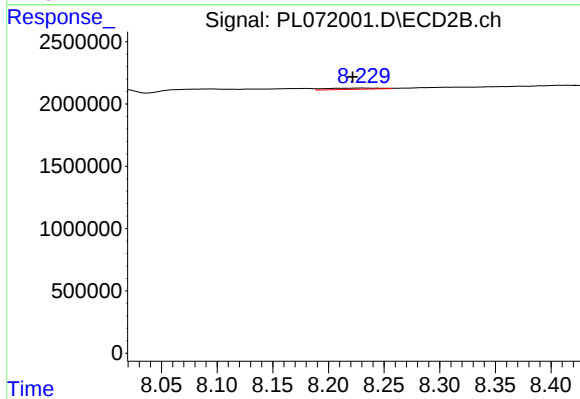

#10 gamma-Chlordane


R.T.: 8.231 min
Delta R.T.: 0.009 min
Response: 322514
Conc: 0.24 ng/ml

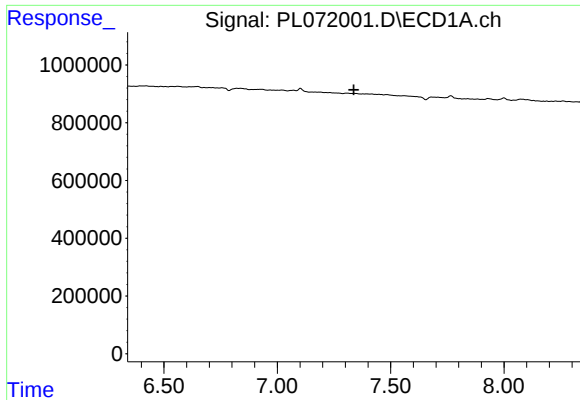

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

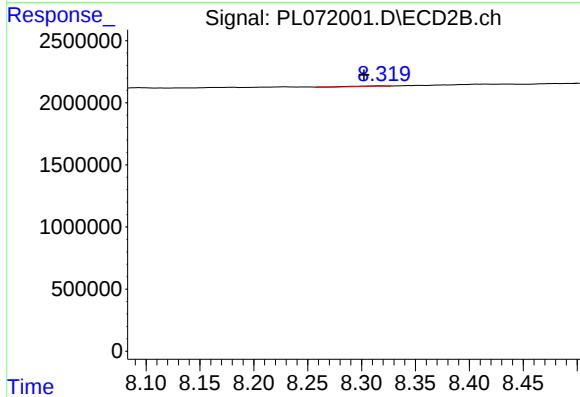


#11 alpha-Chlordane

R.T.: 8.317 min
Delta R.T.: 0.015 min
Response: 92518
Conc: 0.07 ng/ml

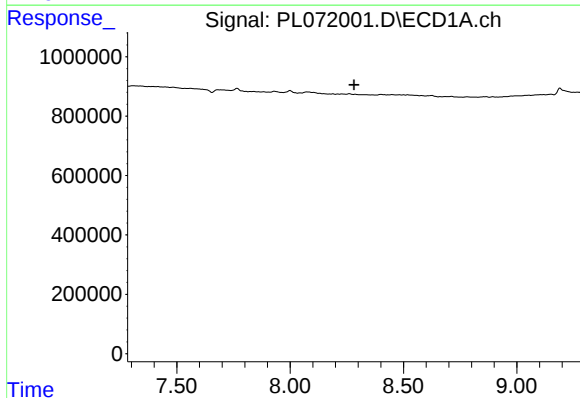


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

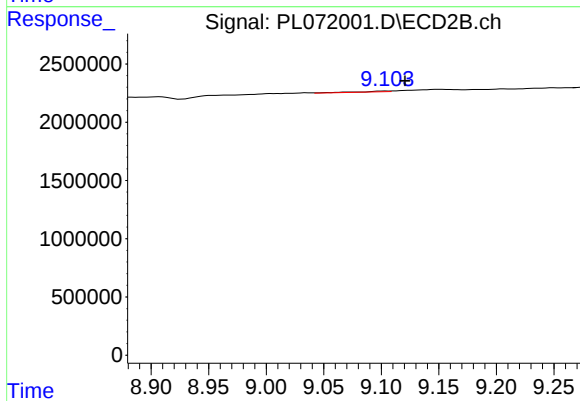

#15 Endosulfan II


R.T.: 9.104 min
Delta R.T.: -0.017 min
Response: 135203
Conc: 0.12 ng/ml

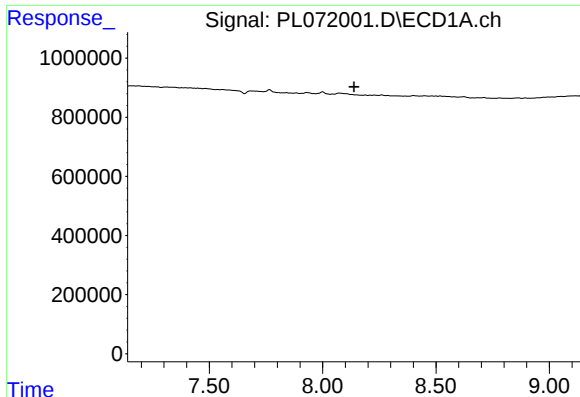

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

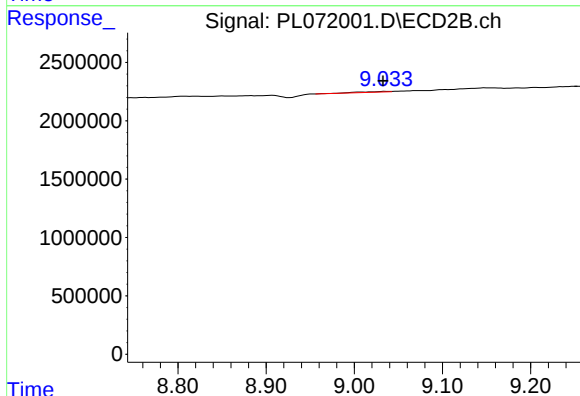


#16 4,4'-DDD

R.T.: 9.035 min
Delta R.T.: 0.003 min
Response: 126379
Conc: 0.13 ng/ml

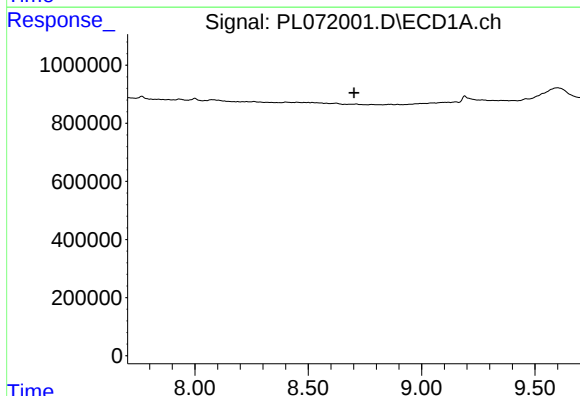


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

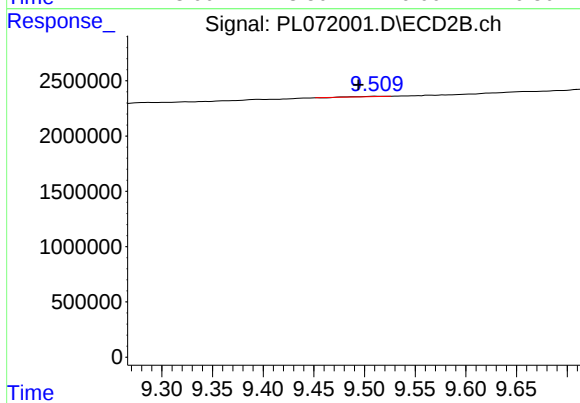

#19 Endosulfan Sulfate


R.T.: 9.511 min
Delta R.T.: 0.017 min
Response: 58577
Conc: 0.06 ng/ml

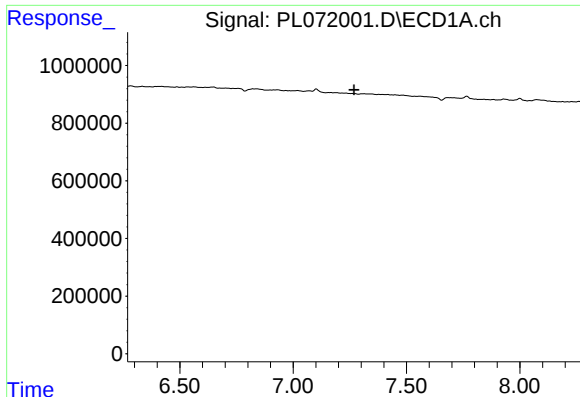

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

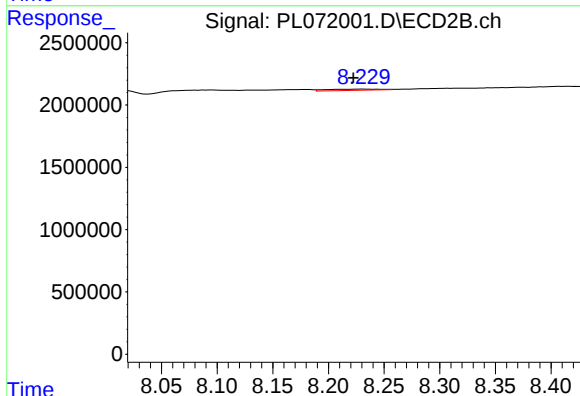


#25 Chlordane-3

R.T.: 8.231 min
Delta R.T.: 0.008 min
Response: 322514
Conc: 1.58 ng/ml

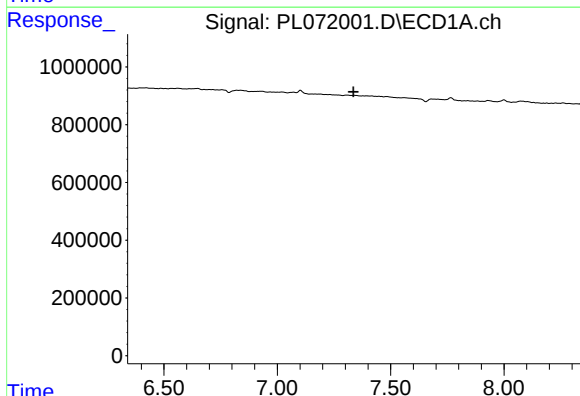


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

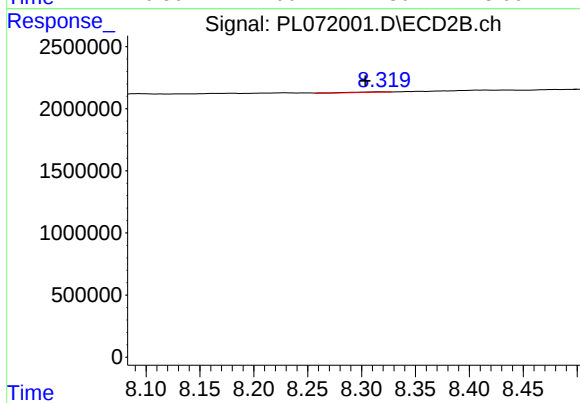

#26 Chlordane-4


R.T.: 8.317 min
Delta R.T.: 0.014 min
Response: 92518
Conc: 0.38 ng/ml

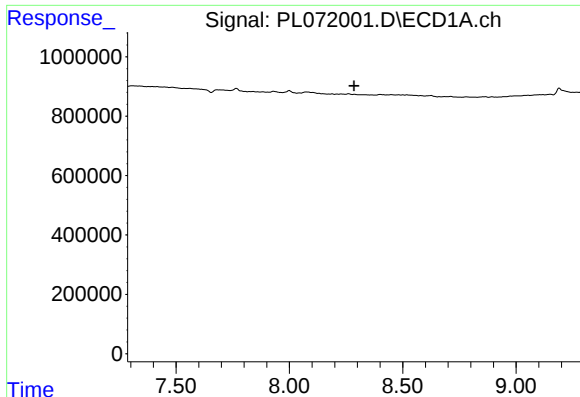

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

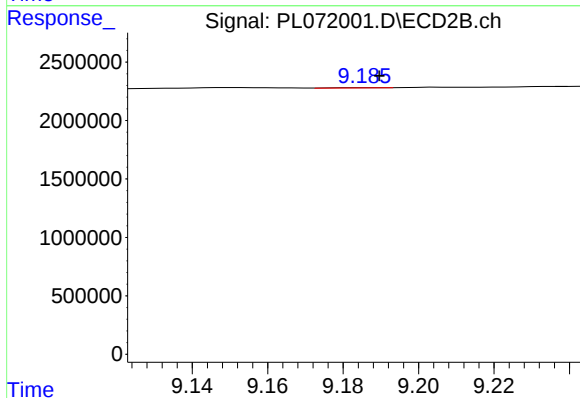


#27 Chlorine-5

R.T.: 9.186 min
Delta R.T.: -0.003 min
Response: 24442
Conc: 0.61 ng/ml

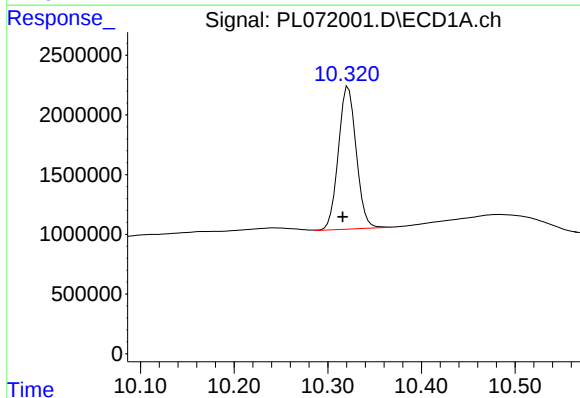

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 15827353
Conc: 21.89 ng/ml

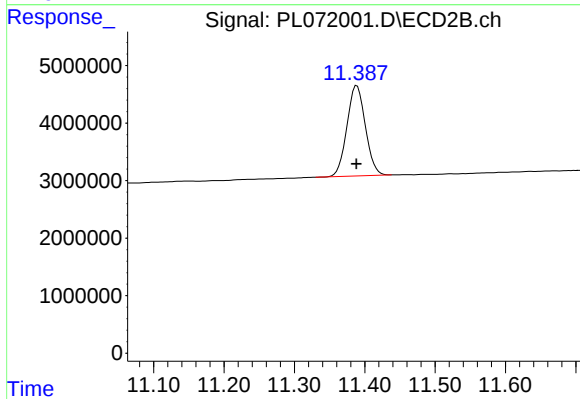

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.000 min
Response: 28654730
Conc: 24.18 ng/ml