

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
 Data File : PL072003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 16:08
 Operator : AR\AJ
 Sample : PB142052BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:37:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9923902	27865740	21.483	22.680
28)	SA Decachlor...	10.322	11.391	17066514	29681685	23.604	25.047
Target Compounds							
7)	B delta-BHC	0.000	6.974f	0	306224	N.D.	0.199 #
8)	B Heptachlo...	0.000	7.968f	0	98280	N.D.	0.070 #
9)	A Endosulfan I	0.000	8.338f	0	7870	N.D.	0.006 #
10)	B gamma-Chl...	0.000	8.224	0	166047	N.D.	0.121 #
11)	B alpha-Chl...	0.000	8.322f	0	126031	N.D.	0.095 #
17)	MA 4,4'-DDT	0.000	9.324f	0	41878	N.D.	0.044 #
25)	Chlordane-3	0.000	8.224	0	166047	N.D.	0.814 #
26)	Chlordane-4	0.000	8.322f	0	126031	N.D.	0.518 #
27)	Chlordane-5	0.000	9.209f	0	295360	N.D.	7.376 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
Data File : PL072003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 16:08
Operator : AR\AJ
Sample : PB142052BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:37:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

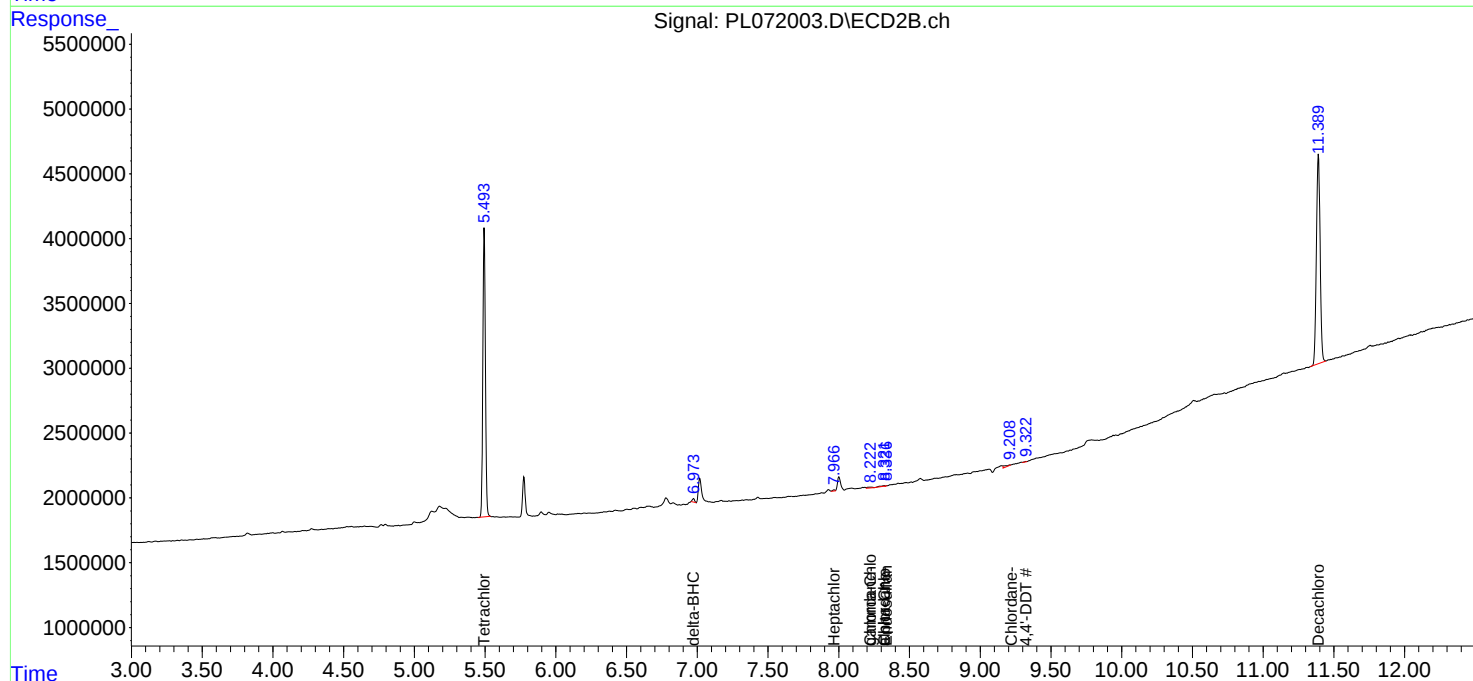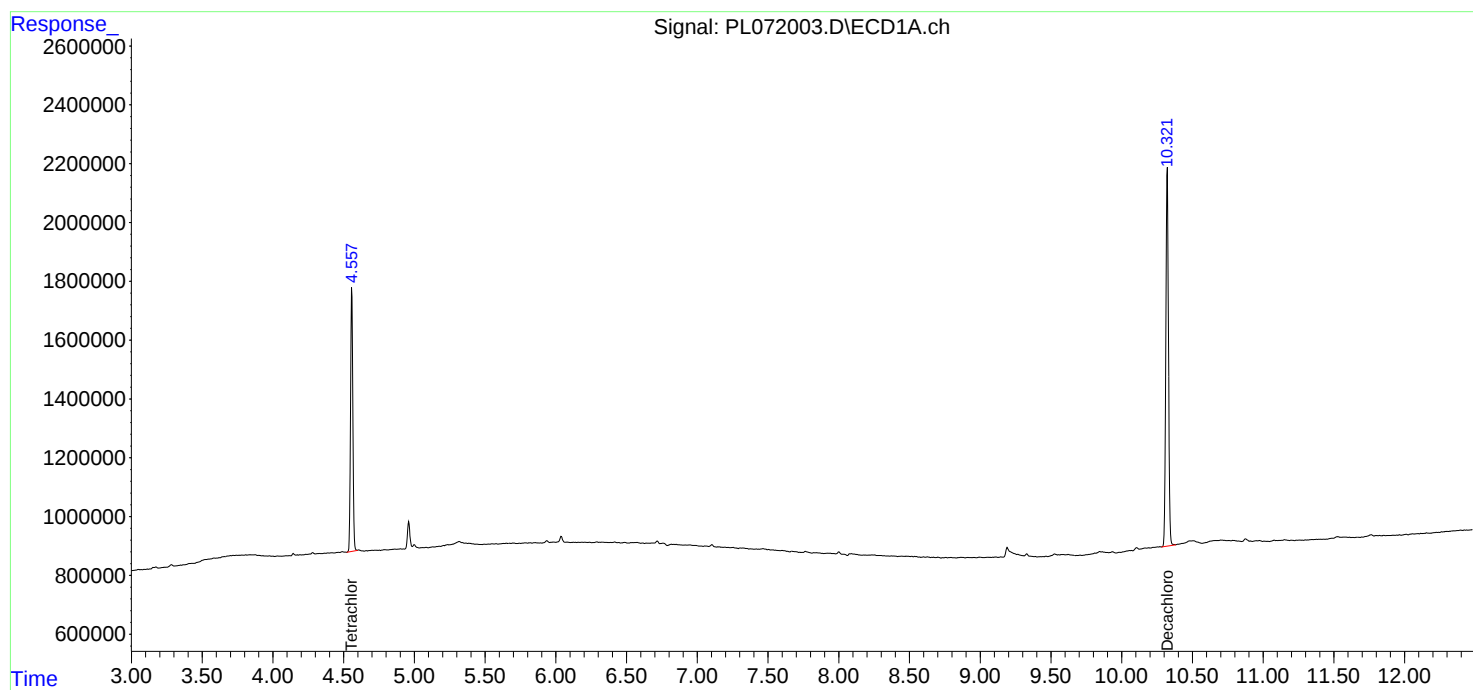


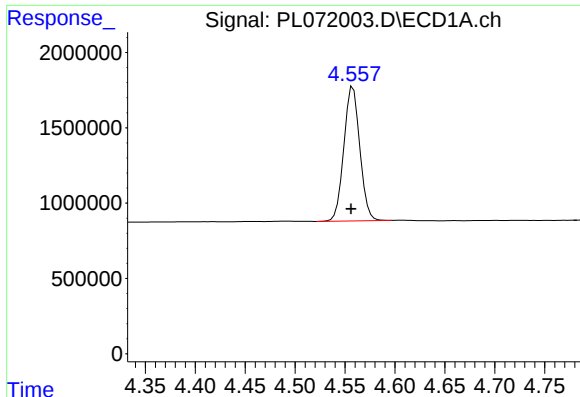

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9923902
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

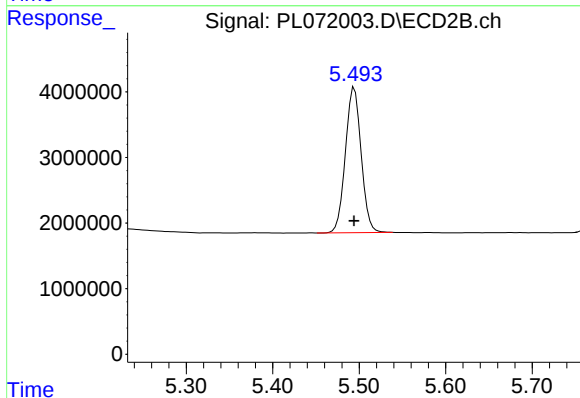


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 27865740
Conc: 22.68 ng/ml

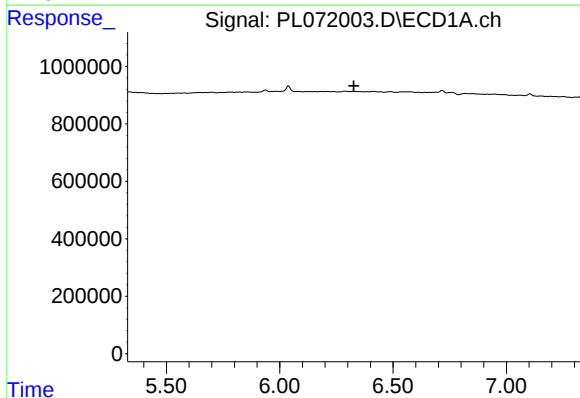


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

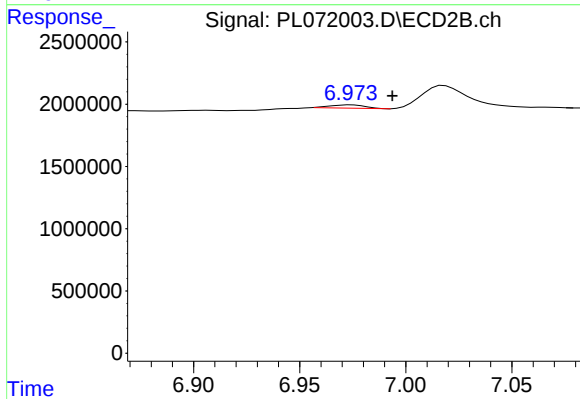

#7 delta-BHC


R.T.: 6.974 min
Delta R.T.: -0.020 min
Response: 306224
Conc: 0.20 ng/ml

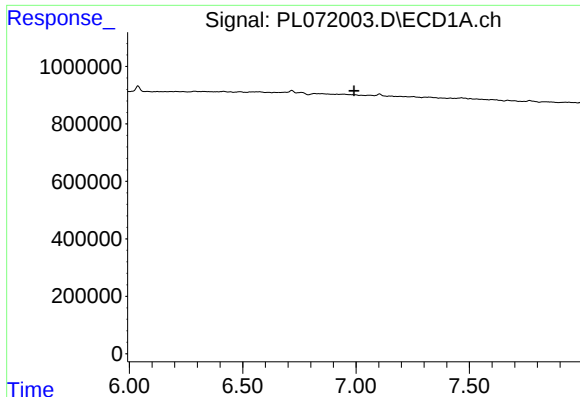

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

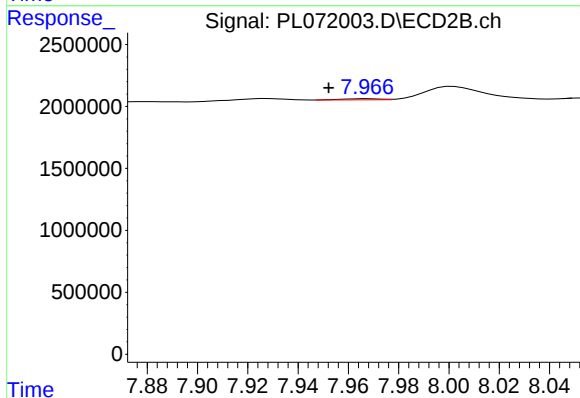


#8 Heptachlor epoxide

R.T.: 7.968 min
Delta R.T.: 0.016 min
Response: 98280
Conc: 0.07 ng/ml

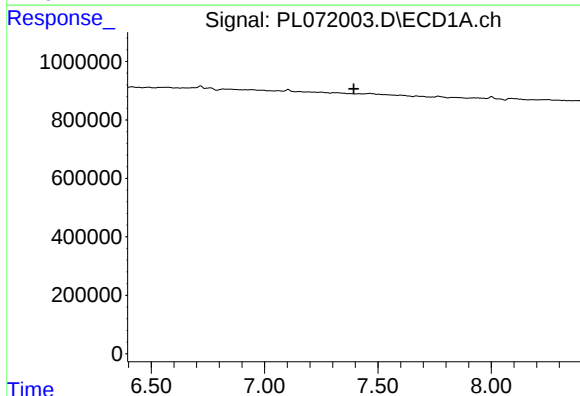


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

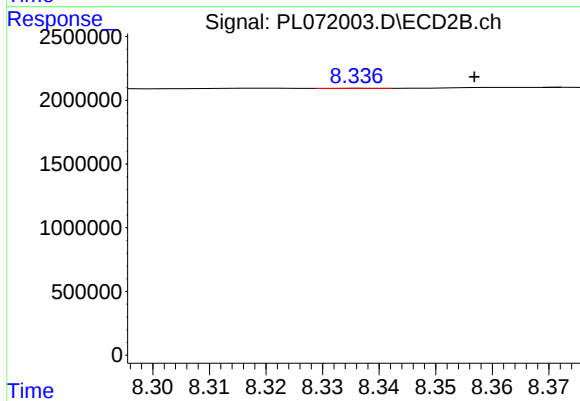

#9 Endosulfan I


R.T.: 8.338 min
Delta R.T.: -0.019 min
Response: 7870
Conc: 0.01 ng/ml

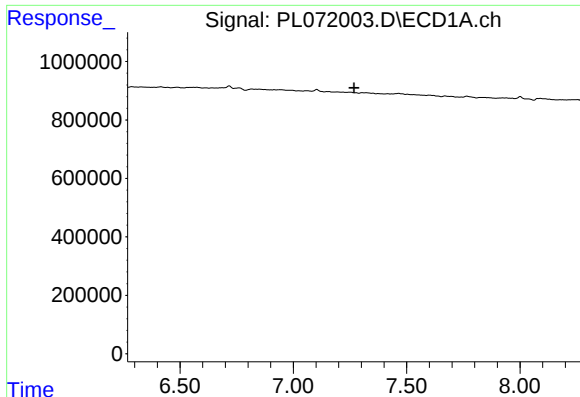

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

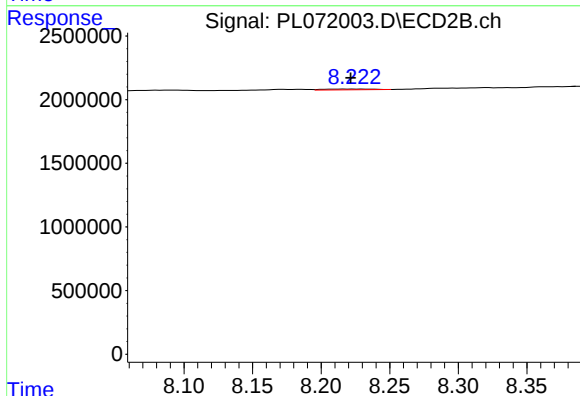


#10 gamma-Chlordane

R.T.: 8.224 min
Delta R.T.: 0.002 min
Response: 166047
Conc: 0.12 ng/ml

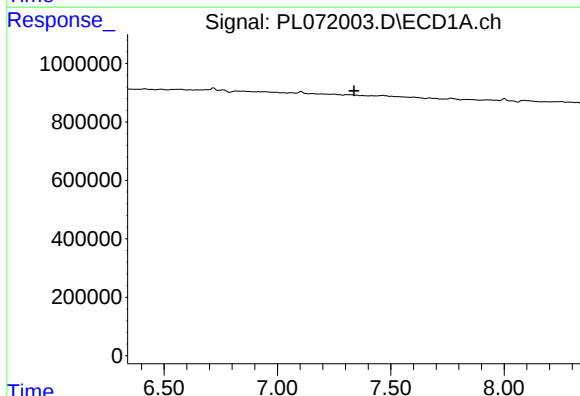


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

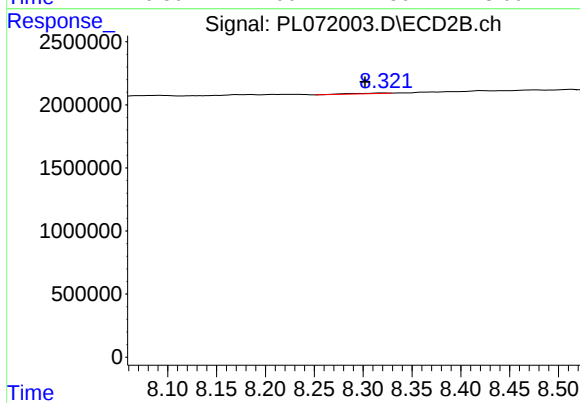

#11 alpha-Chlordane


R.T.: 8.322 min
Delta R.T.: 0.020 min
Response: 126031
Conc: 0.09 ng/ml

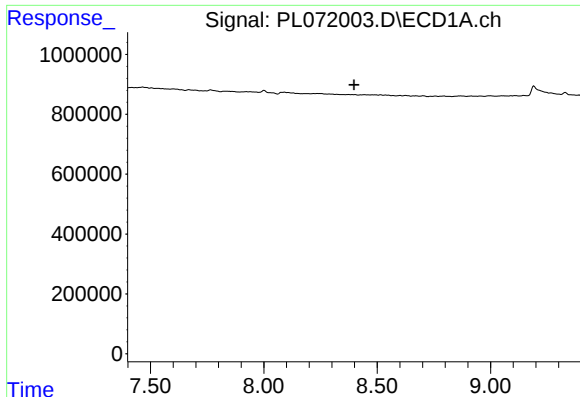

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

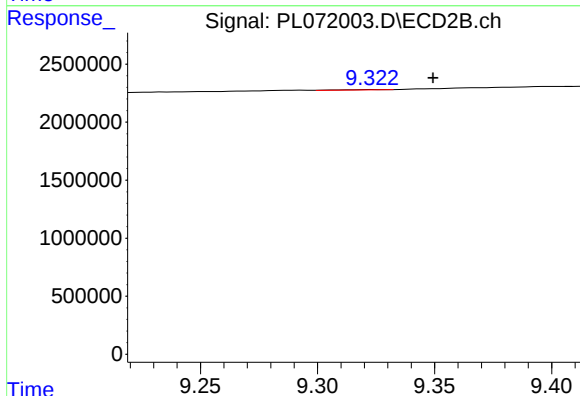


#17 4,4'-DDT

R.T.: 9.324 min
Delta R.T.: -0.026 min
Response: 41878
Conc: 0.04 ng/ml

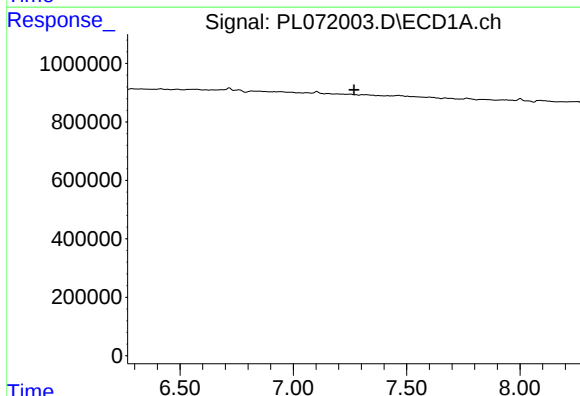


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

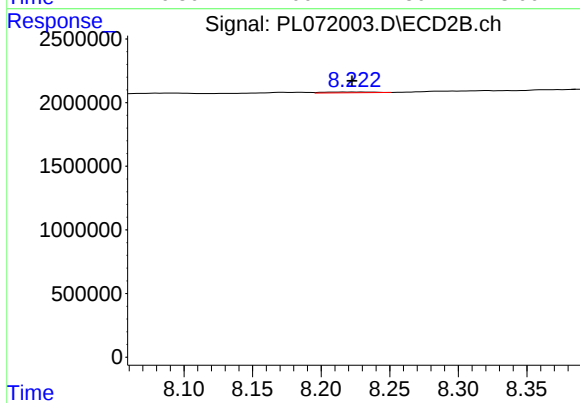

#25 Chlordane-3


R.T.: 8.224 min
Delta R.T.: 0.001 min
Response: 166047
Conc: 0.81 ng/ml

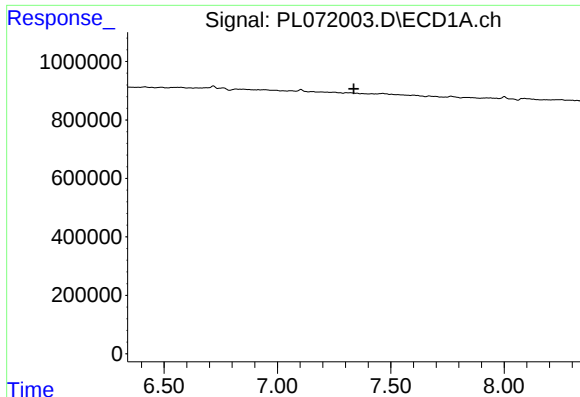

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

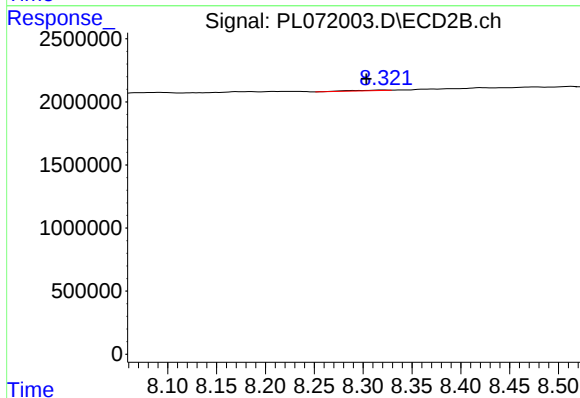


#26 Chlordane-4

R.T.: 8.322 min
Delta R.T.: 0.018 min
Response: 126031
Conc: 0.52 ng/ml

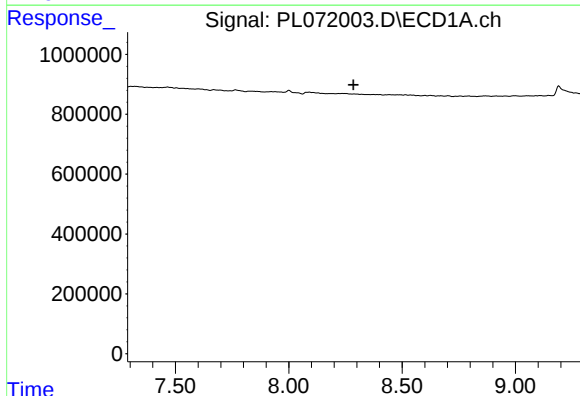


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

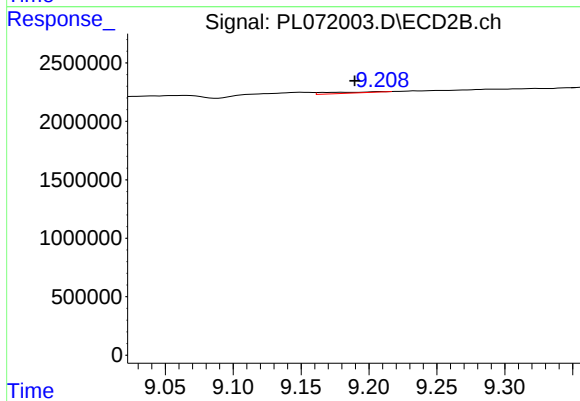

#27 Chlordane-5


R.T.: 9.209 min
Delta R.T.: 0.020 min
Response: 295360
Conc: 7.38 ng/ml

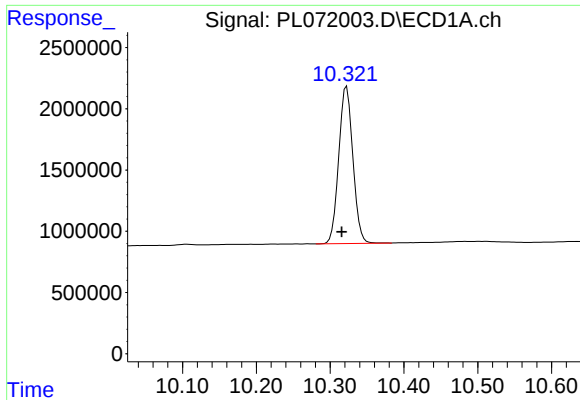

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.007 min
Response: 17066514
Conc: 23.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

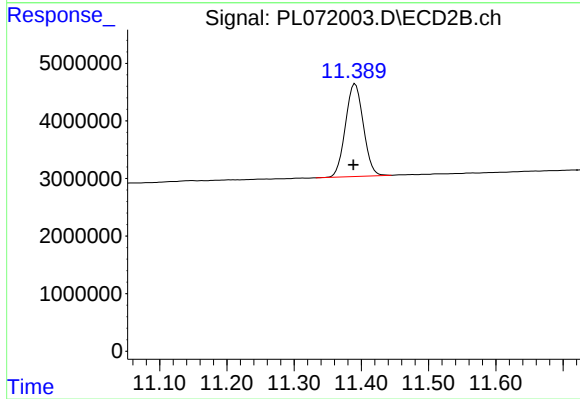

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.003 min
Response: 29681685
Conc: 25.05 ng/ml