

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
 Data File : PL072010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 18:02
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 21:38:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	9672298	27393565	20.938	22.296
28)	SA Decachlor...	10.322	11.389	16402420	28745761	22.686	24.258
Target Compounds							
7)	B delta-BHC	0.000	6.971f	0	418088	N.D.	0.272 #
8)	B Heptachlo...	0.000	7.968f	0	312342	N.D.	0.224 #
9)	A Endosulfan I	0.000	8.347	0	44315	N.D.	0.036 #
10)	B gamma-Chl...	0.000	8.228	0	318838	N.D.	0.233 #
11)	B alpha-Chl...	0.000	8.289	0	67429	N.D.	0.051 #
12)	B 4,4'-DDE	0.000	8.515f	0	49578	N.D.	0.039 #
15)	B Endosulfa...	0.000	9.149f	0	192540	N.D.	0.171 #
19)	B Endosulfa...	0.000	9.507	0	117331	N.D.	0.113 #
21)	B Endrin ke...	0.000	9.998	0	78850	N.D.	0.070 #
25)	Chlordane-3	0.000	8.228	0	318838	N.D.	1.562 #
26)	Chlordane-4	0.000	8.289	0	67429	N.D.	0.277 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011422\
Data File : PL072010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 18:02
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 21:38:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

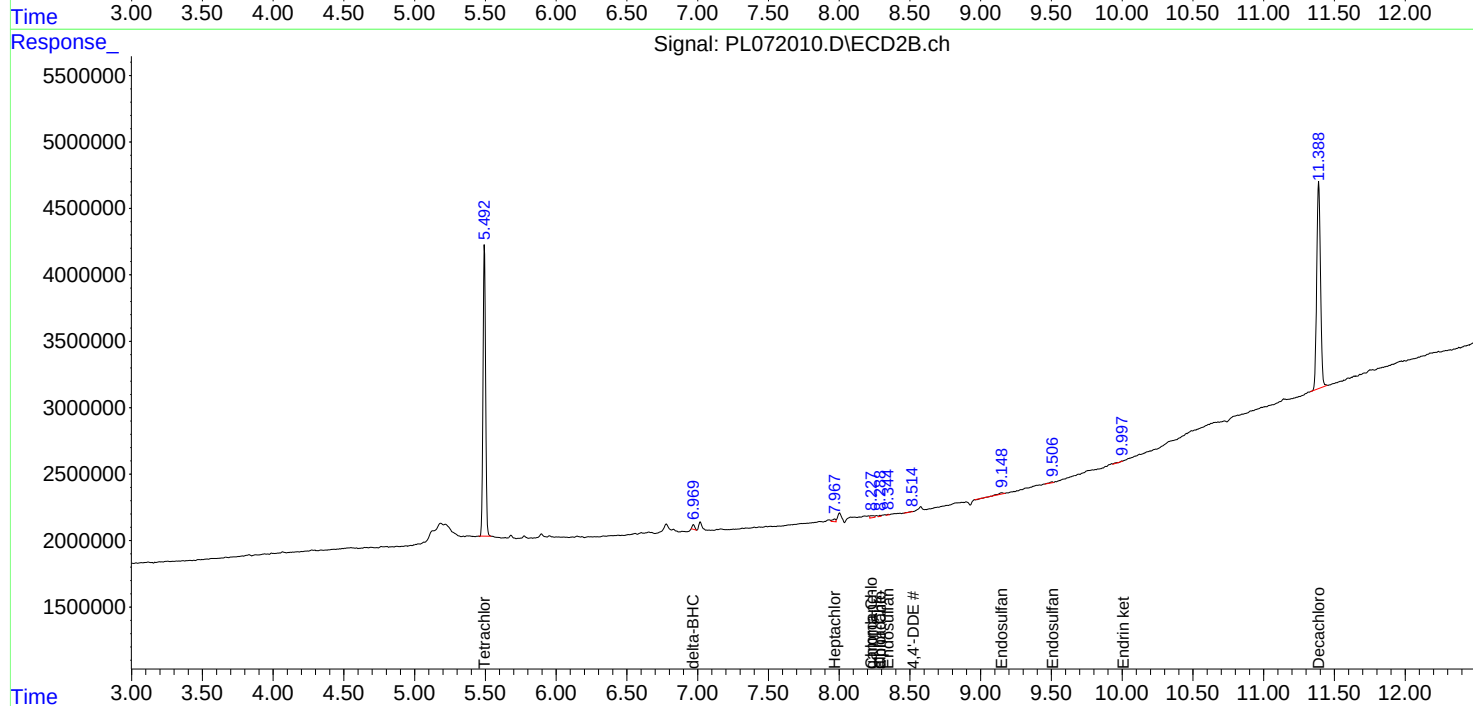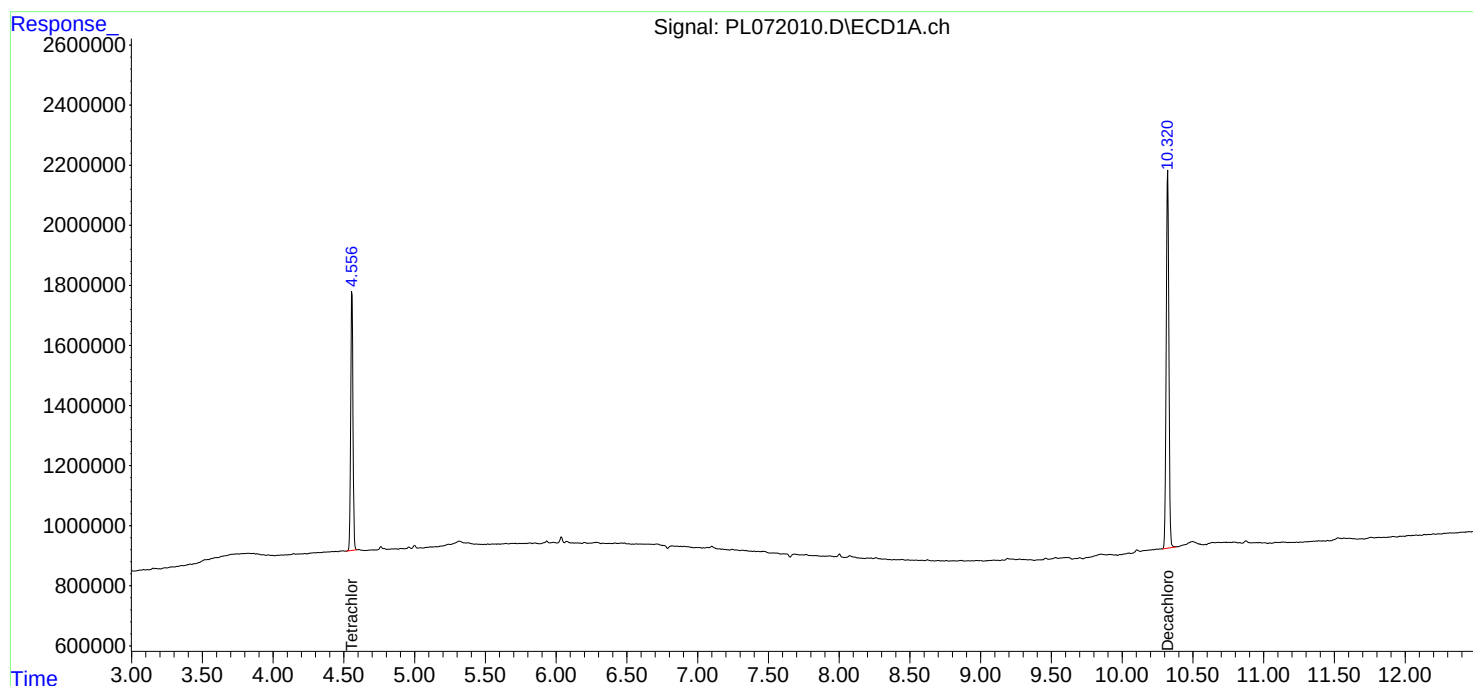


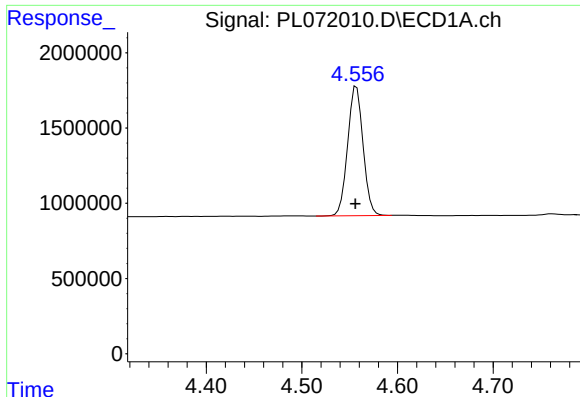

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 9672298
Conc: 20.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

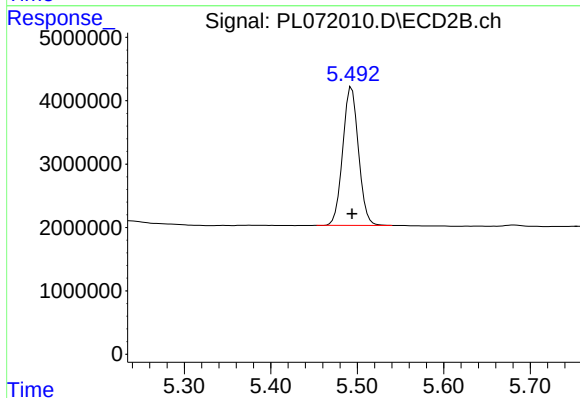


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 27393565
Conc: 22.30 ng/ml

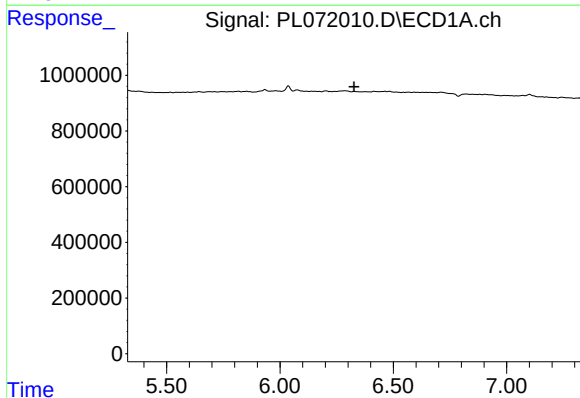


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

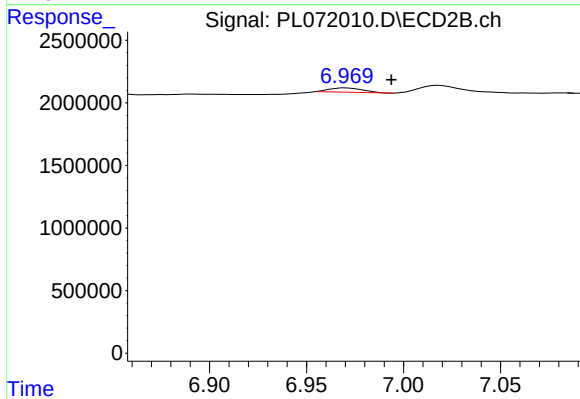

#7 delta-BHC


R.T.: 6.971 min
Delta R.T.: -0.023 min
Response: 418088
Conc: 0.27 ng/ml

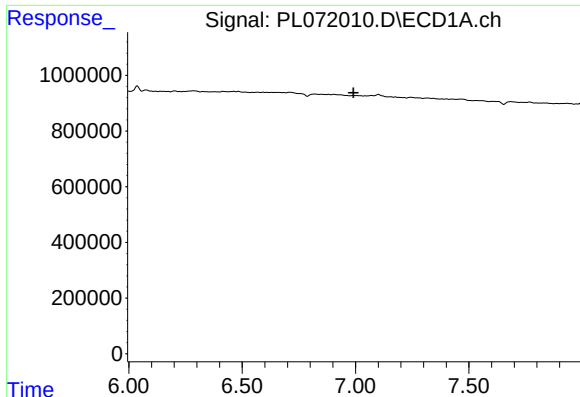

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

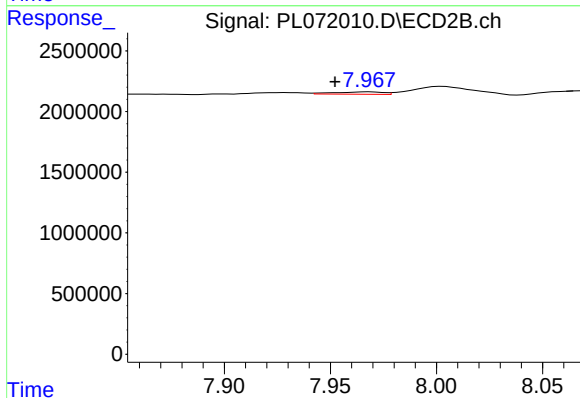


#8 Heptachlor epoxide

R.T.: 7.968 min
Delta R.T.: 0.016 min
Response: 312342
Conc: 0.22 ng/ml

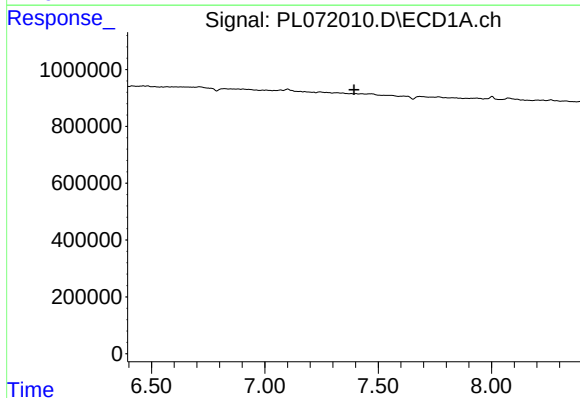


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

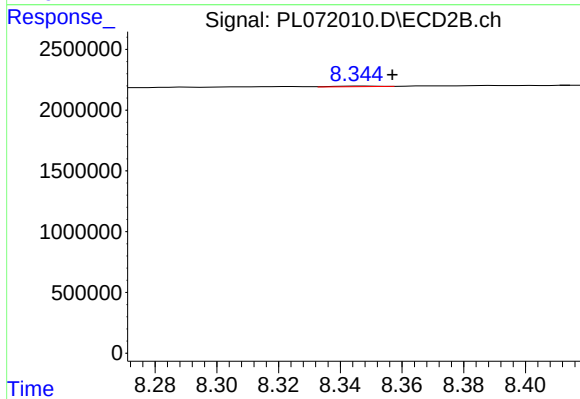

#9 Endosulfan I


R.T.: 8.347 min
Delta R.T.: -0.009 min
Response: 44315
Conc: 0.04 ng/ml

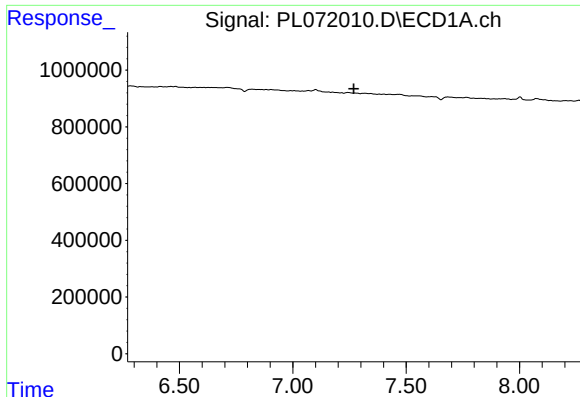

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

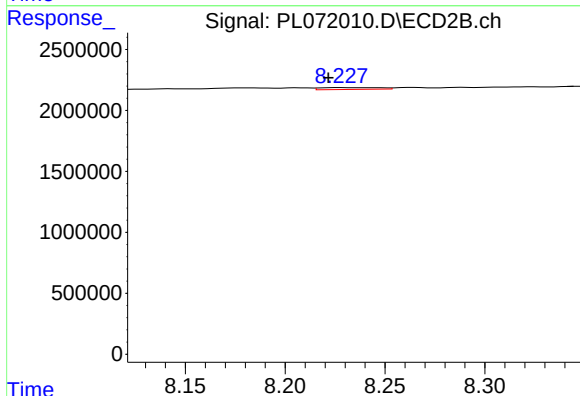


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: 0.007 min
Response: 318838
Conc: 0.23 ng/ml

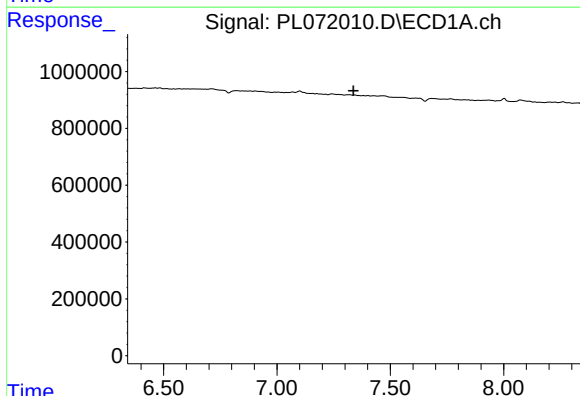


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

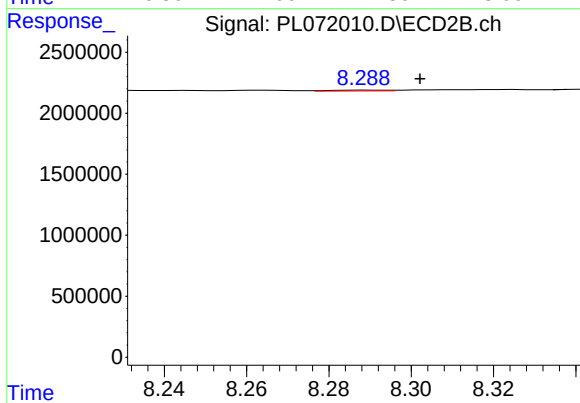

#11 alpha-Chlordane


R.T.: 8.289 min
Delta R.T.: -0.013 min
Response: 67429
Conc: 0.05 ng/ml

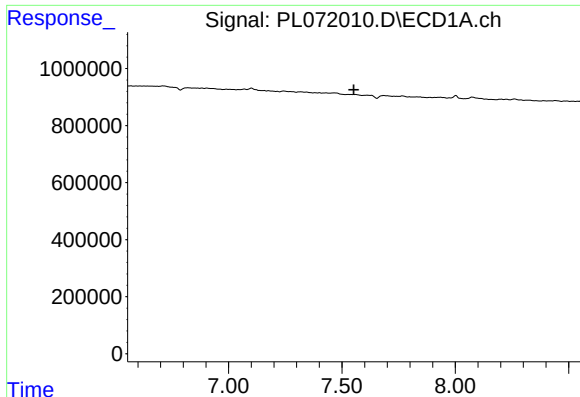

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

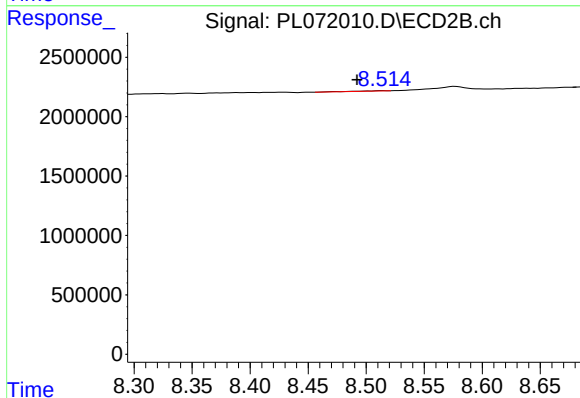


#12 4,4'-DDE

R.T.: 8.515 min
Delta R.T.: 0.023 min
Response: 49578
Conc: 0.04 ng/ml

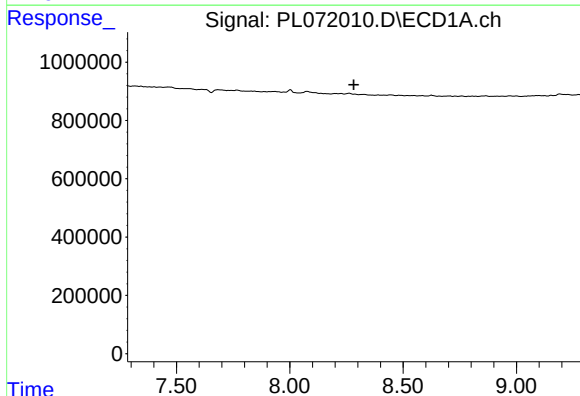


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

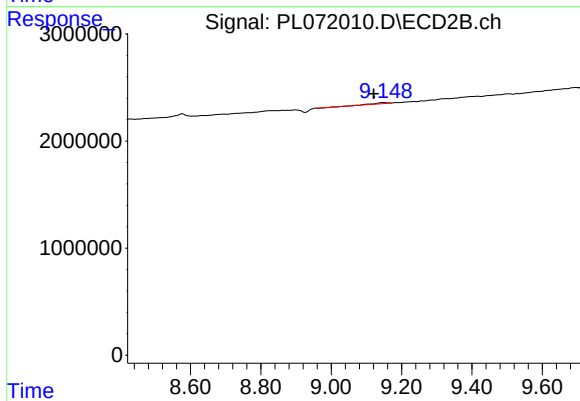

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.029 min
Response: 192540
Conc: 0.17 ng/ml

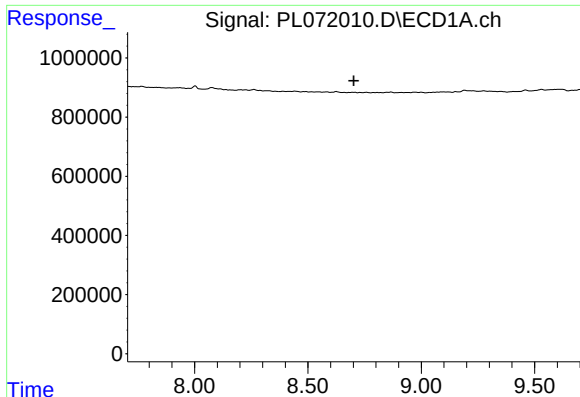

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

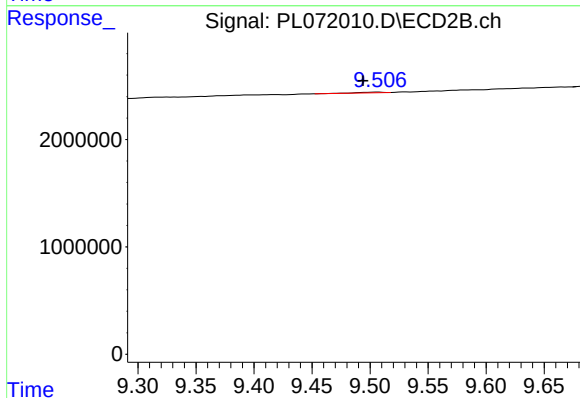


#19 Endosulfan Sulfate

R.T.: 9.507 min
Delta R.T.: 0.013 min
Response: 117331
Conc: 0.11 ng/ml

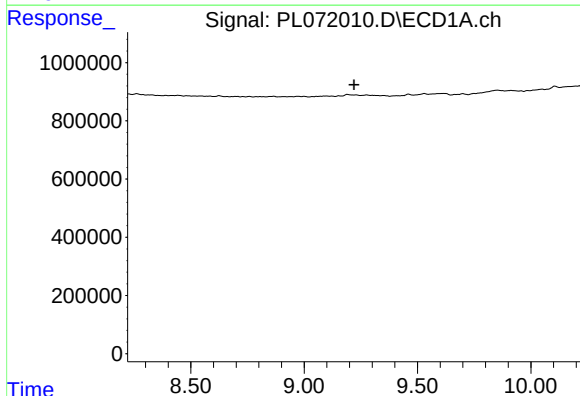


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.220 min
Response: 0
Conc: N.D.

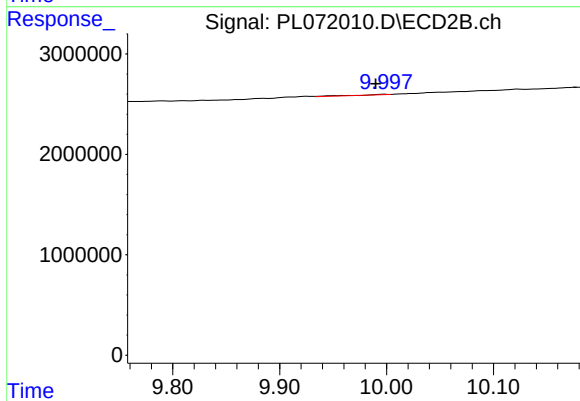

#21 Endrin ketone


R.T.: 9.998 min
Delta R.T.: 0.009 min
Response: 78850
Conc: 0.07 ng/ml

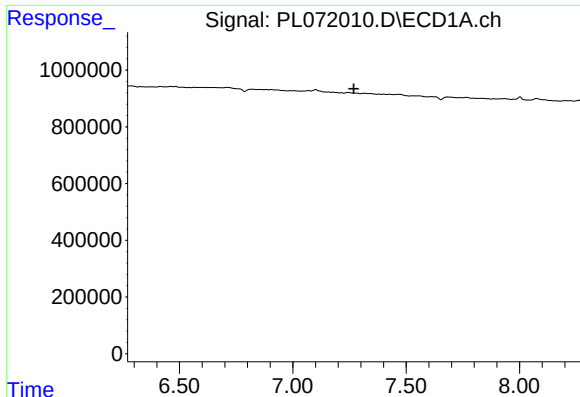

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

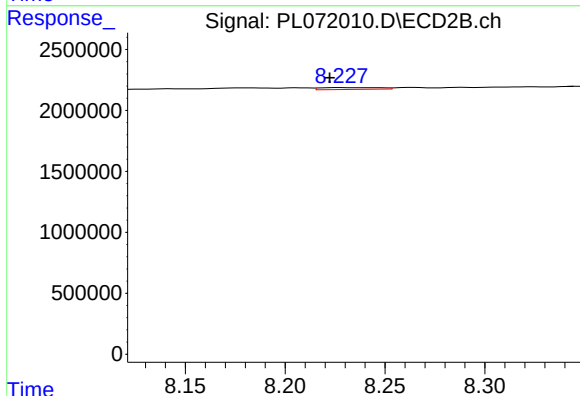


#25 Chlordane-3

R.T.: 8.228 min
Delta R.T.: 0.006 min
Response: 318838
Conc: 1.56 ng/ml

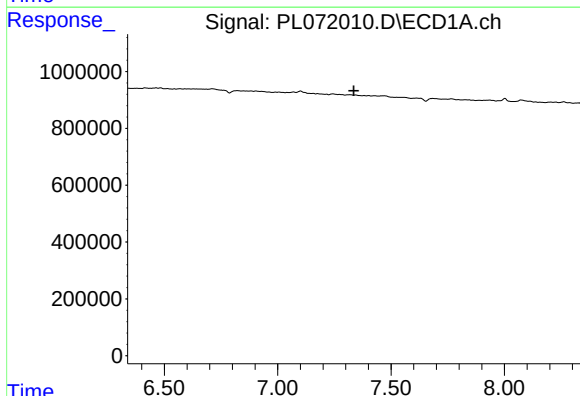


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

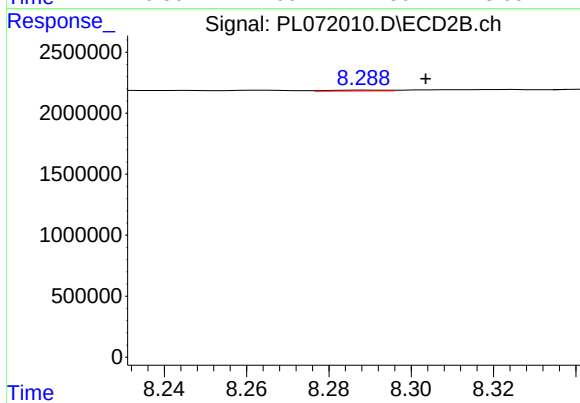

#26 Chlordane-4


R.T.: 8.289 min
Delta R.T.: -0.014 min
Response: 67429
Conc: 0.28 ng/ml

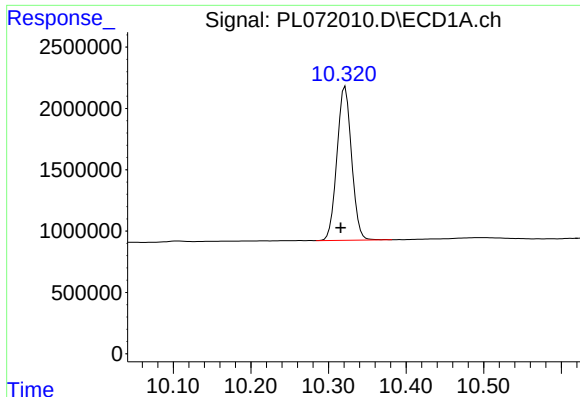

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 16402420
Conc: 22.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

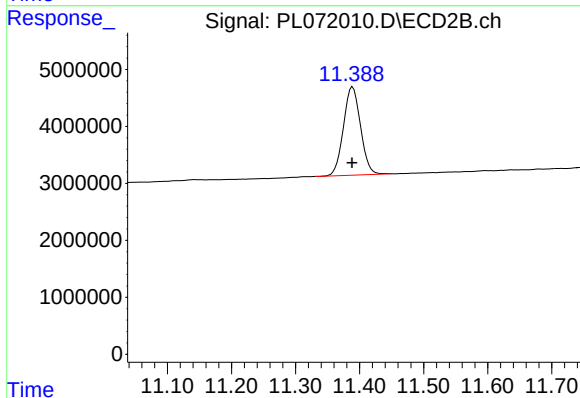

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.001 min
Response: 28745761
Conc: 24.26 ng/ml