

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011423\
 Data File : PL080314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 14:14
 Operator : AR\AJ
 Sample : 01133-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/16/2023
 Supervised By :Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:29:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.691	8534477	8632476	4.272m	3.860
28) SA Decachlor...	8.791	7.842	8189550	11138150	5.551	4.955

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011423\
Data File : PL080314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 14:14
Operator : AR\AJ
Sample : 01133-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSITE-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/16/2023
Supervised By : Ankita Jodhani 01/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:29:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

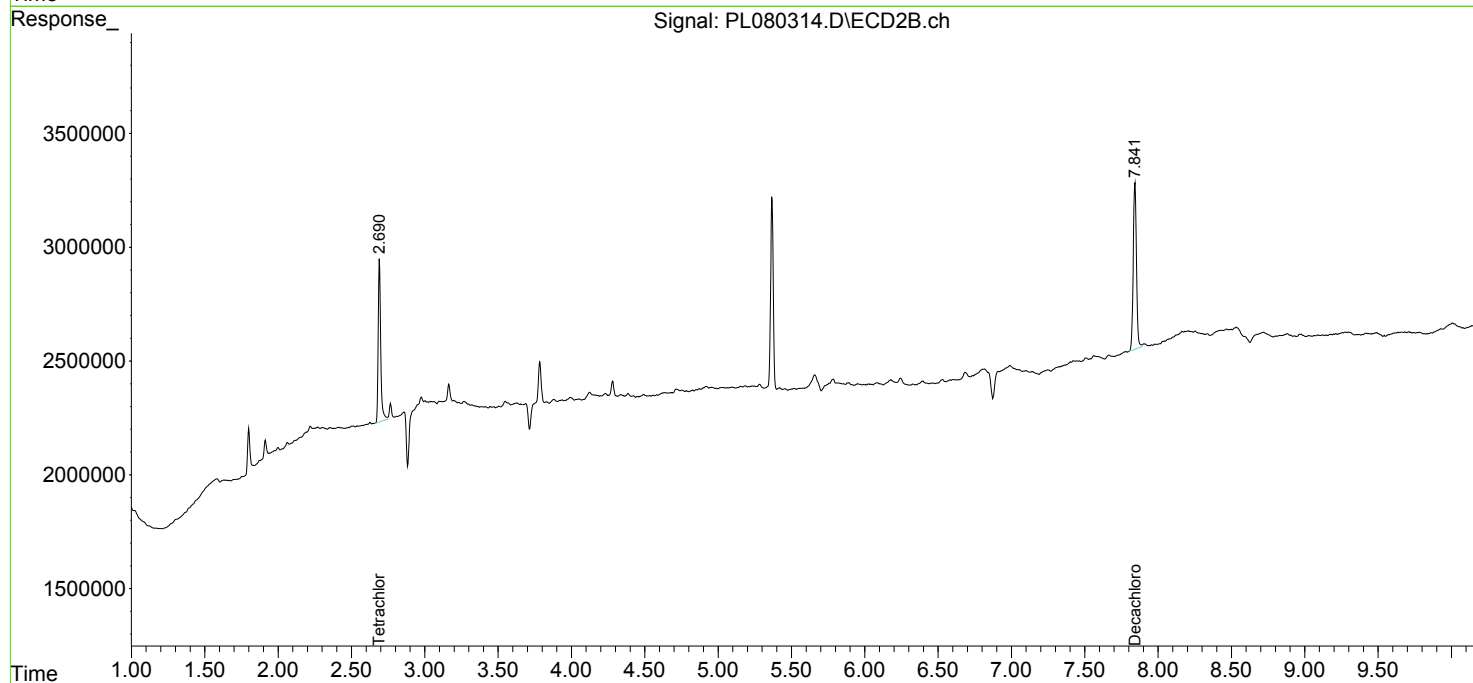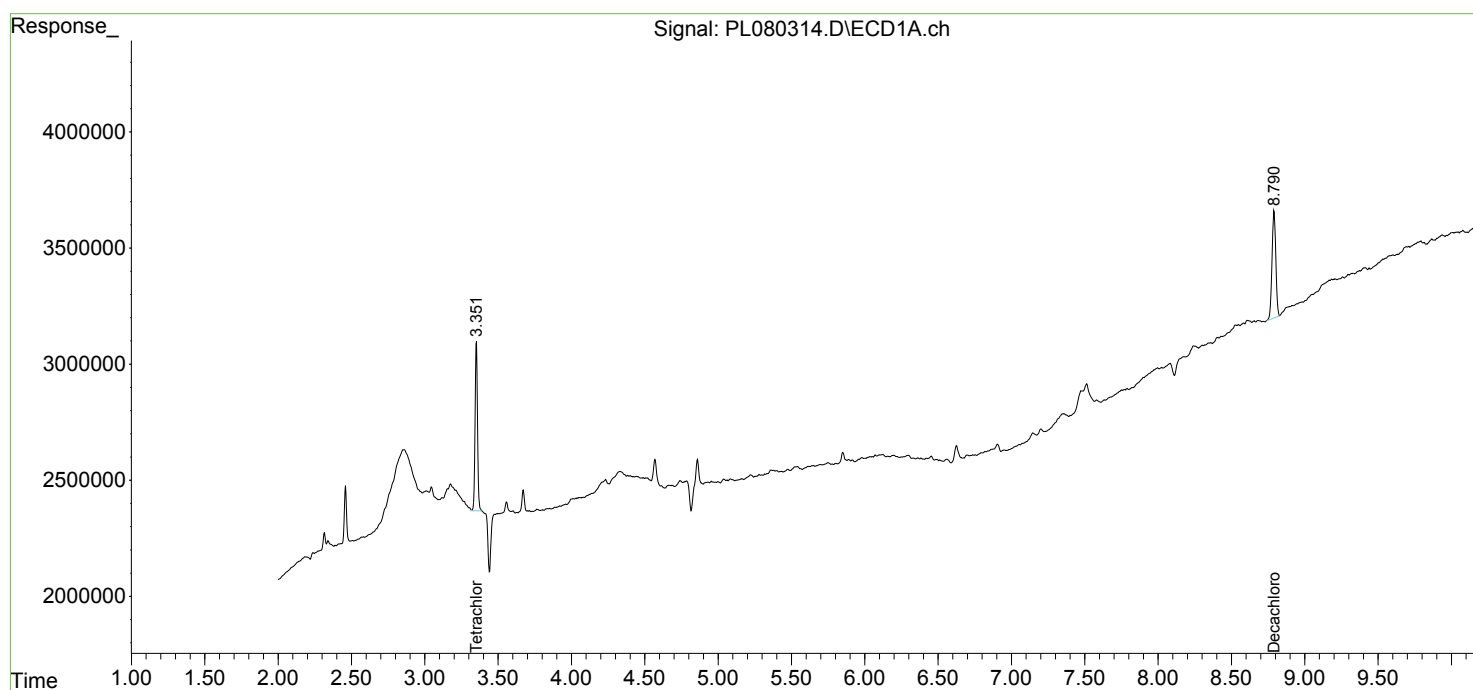

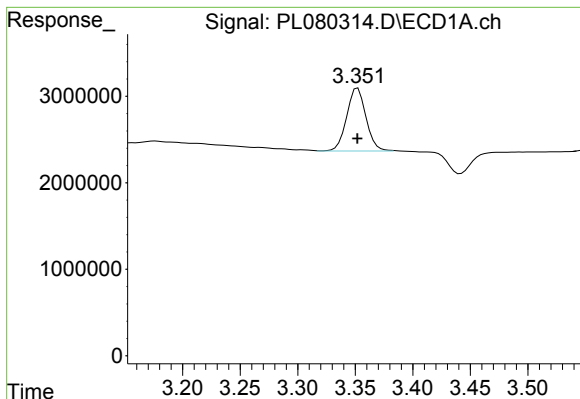


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: -0.001 min
Response: 8534477
Conc: 4.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/16/2023
Supervised By :Ankita Jodhani 01/16/2023

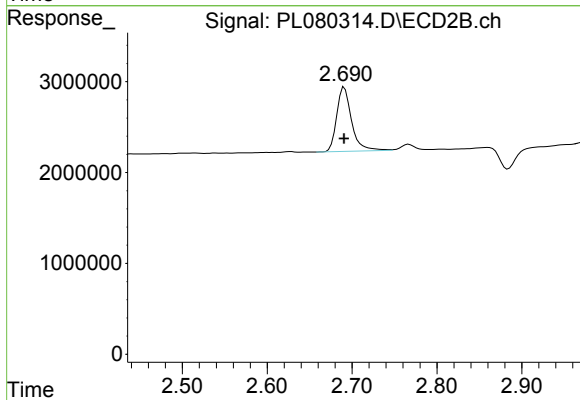


#1 Tetrachloro-m-xylene

R.T.: 2.691 min
Delta R.T.: 0.000 min
Response: 8632476
Conc: 3.86 ng/ml

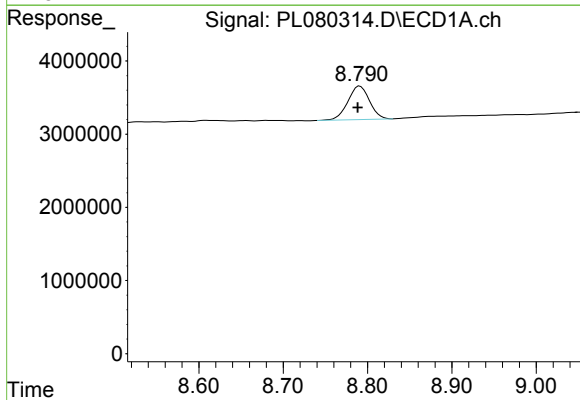

#28 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.002 min
Response: 8189550
Conc: 5.55 ng/ml

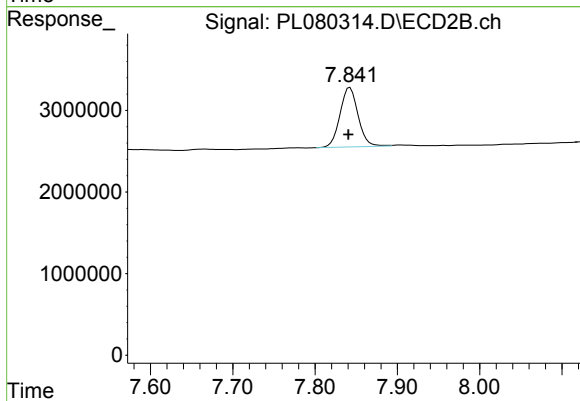

#28 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.002 min
Response: 11138150
Conc: 4.96 ng/ml