

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011425\
 Data File : PL093649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2025 11:51
 Operator : AR\AJ
 Sample : PB166044BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB166044BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 02:08:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.775	49755341	54919515	20.098	18.865
28)	SA Decachlor...	9.068	7.916	43460522	66685669	23.505	22.333
Target Compounds							
2)	A alpha-BHC	0.000	3.269	0	245565	N.D.	0.056 #
5)	MB Aldrin	0.000	4.251f	0	171533	N.D.	0.042 #
6)	B beta-BHC	0.000	3.909	0	132495	N.D.	0.074 #
7)	B delta-BHC	0.000	4.160f	0	73704	N.D.	0.017 #
9)	A Endosulfan I	0.000	5.095	0	64576	N.D.	0.018 #
10)	B gamma-Chl...	0.000	4.992	0	373238	N.D.	0.097 #
11)	B alpha-Chl...	0.000	5.055	0	525195	N.D.	0.138 #
12)	B 4,4'-DDE	0.000	5.254f	0	84451	N.D.	0.023 #
13)	MA Dieldrin	0.000	5.350	0	69695	N.D.	0.018 #
14)	MA Endrin	0.000	5.658f	0	379408	N.D.	0.115 #
15)	B Endosulfa...	0.000	5.922	0	26237	N.D.	0.008 #
20)	A Methoxychlor	0.000	6.625	0	391195	N.D.	0.243 #
24)	Chlordane-2	0.000	4.360	0	20642	N.D.	0.149 #
25)	Chlordane-3	0.000	4.992	0	373238	N.D.	0.880 #
26)	Chlordane-4	0.000	5.055	0	525195	N.D.	1.277 #
27)	Chlordane-5	0.000	5.922	0	26237	N.D.	0.197 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011425\
Data File : PL093649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2025 11:51
Operator : AR\AJ
Sample : PB166044BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB166044BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 02:08:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

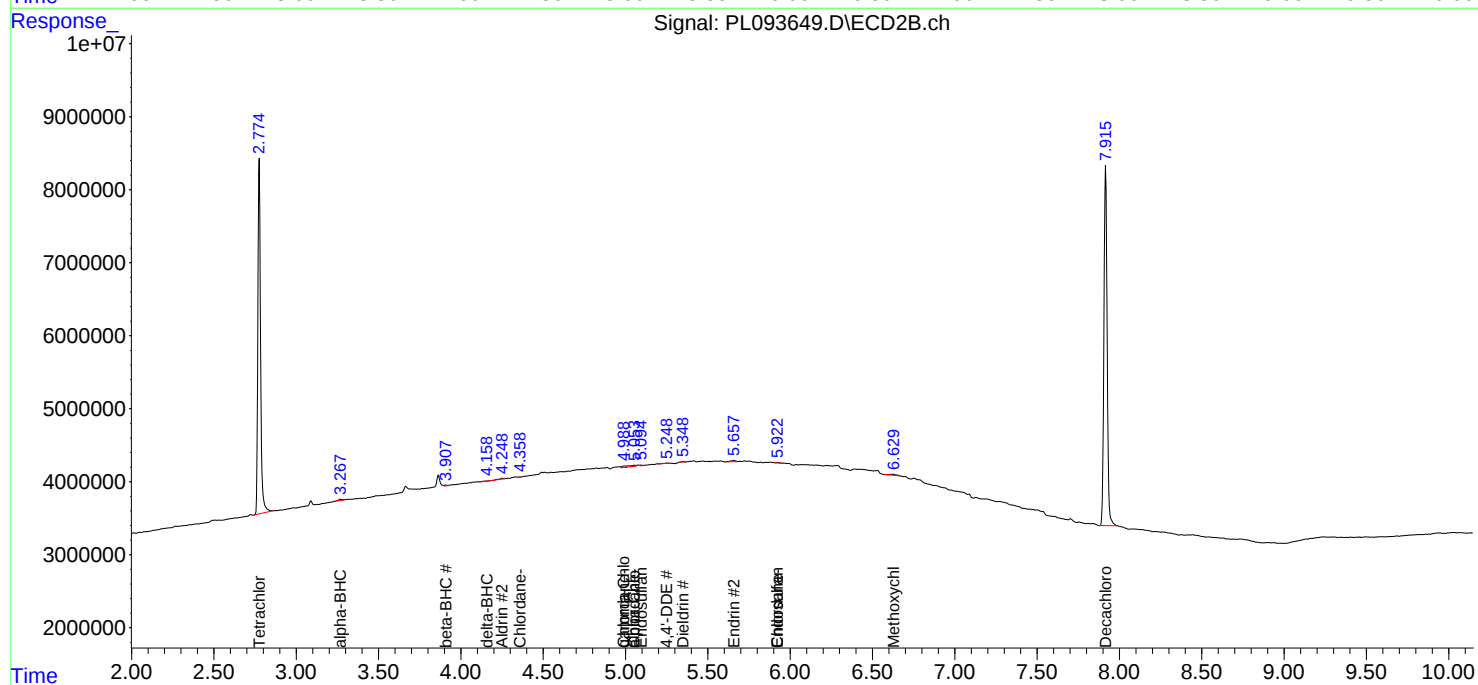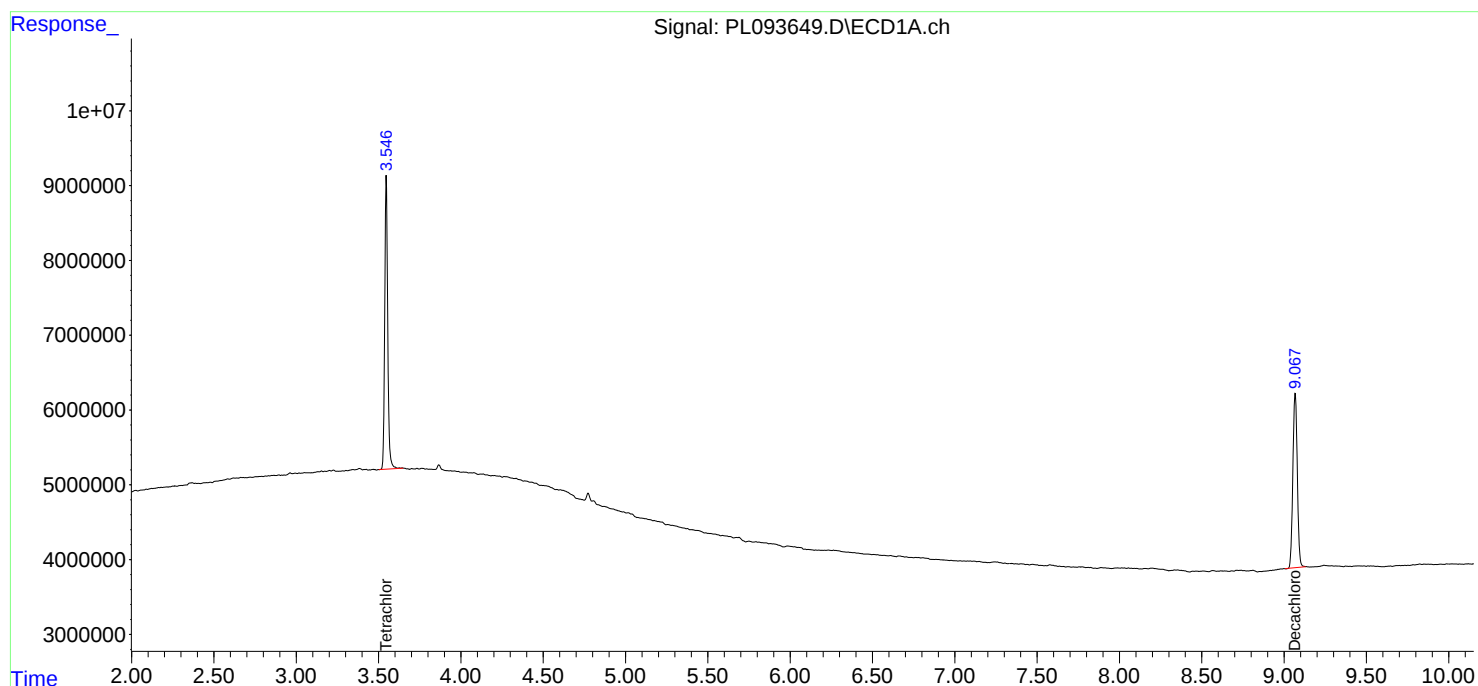


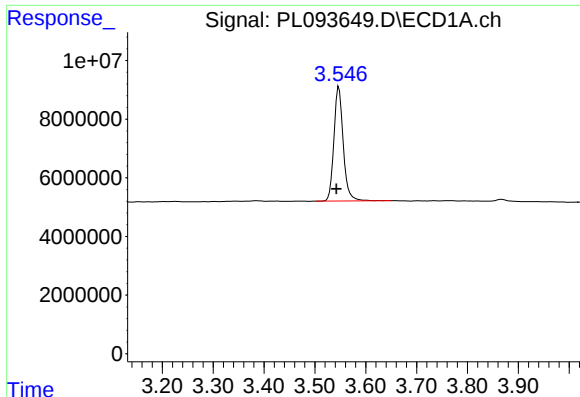

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.005 min
Response: 49755341
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB166044BL

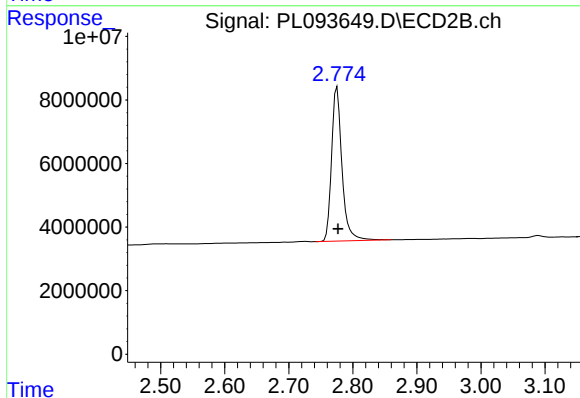


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.002 min
Response: 54919515
Conc: 18.86 ng/ml

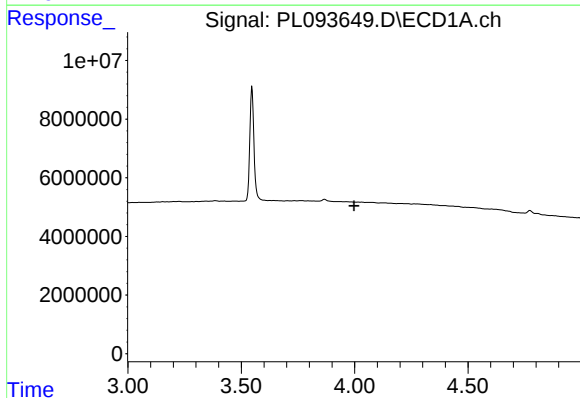


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.997 min
Response: 0
Conc: N.D.

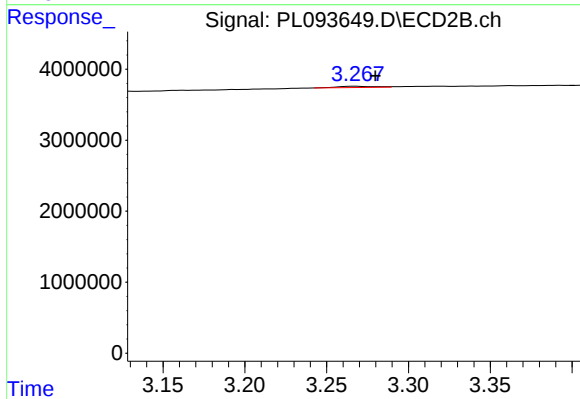

#2 alpha-BHC


R.T.: 3.269 min
Delta R.T.: -0.011 min
Response: 245565
Conc: 0.06 ng/ml

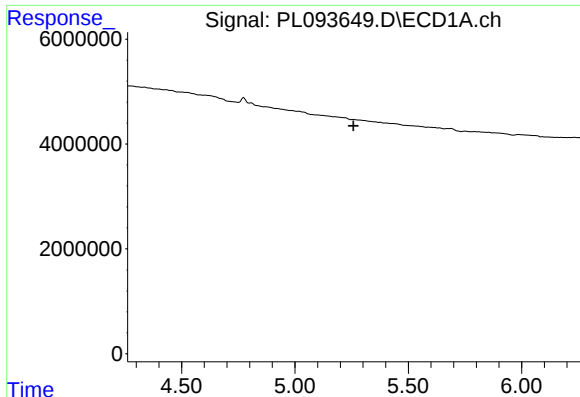

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

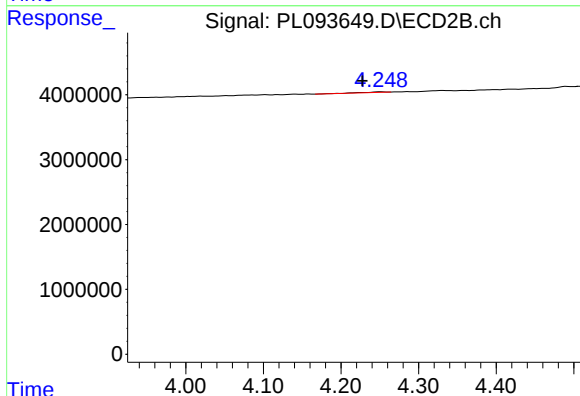


#5 Aldrin

R.T.: 4.251 min
Delta R.T.: 0.023 min
Response: 171533
Conc: 0.04 ng/ml

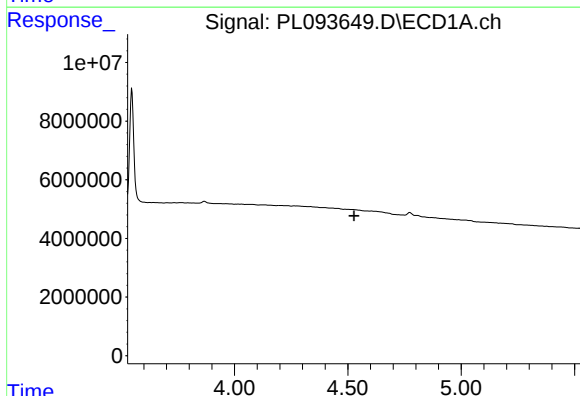


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

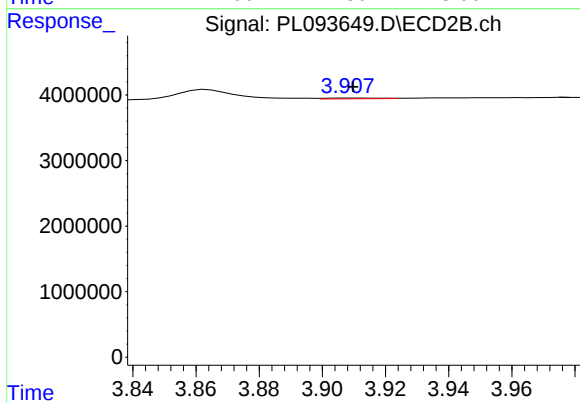

#6 beta-BHC


R.T.: 3.909 min
Delta R.T.: 0.000 min
Response: 132495
Conc: 0.07 ng/ml

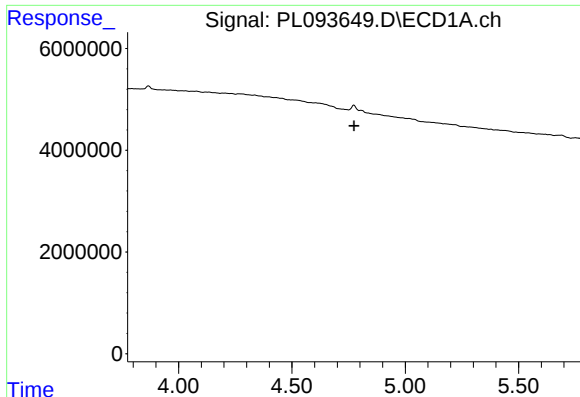

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

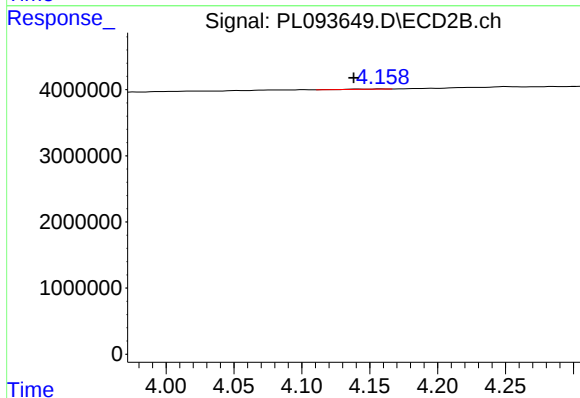


#7 delta-BHC

R.T.: 4.160 min
Delta R.T.: 0.021 min
Response: 73704
Conc: 0.02 ng/ml

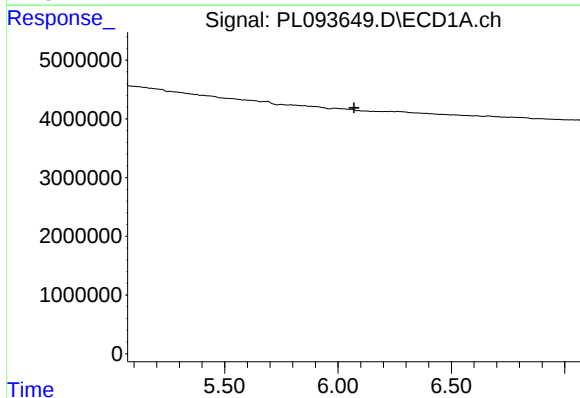


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.071 min
Response: 0
Conc: N.D.

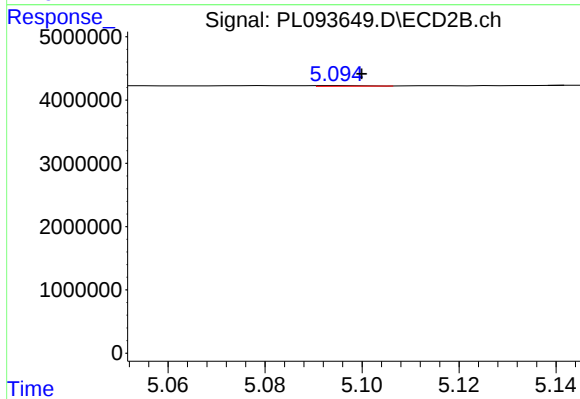

#9 Endosulfan I


R.T.: 5.095 min
Delta R.T.: -0.005 min
Response: 64576
Conc: 0.02 ng/ml

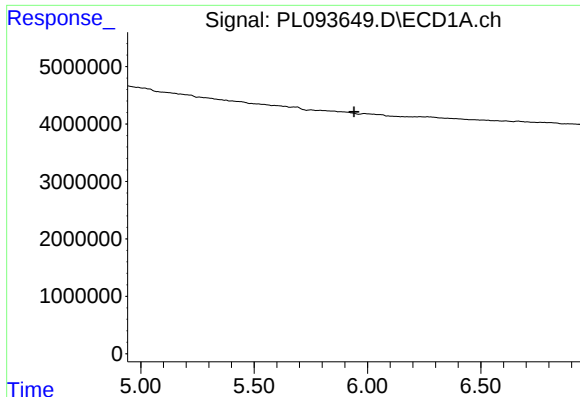

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

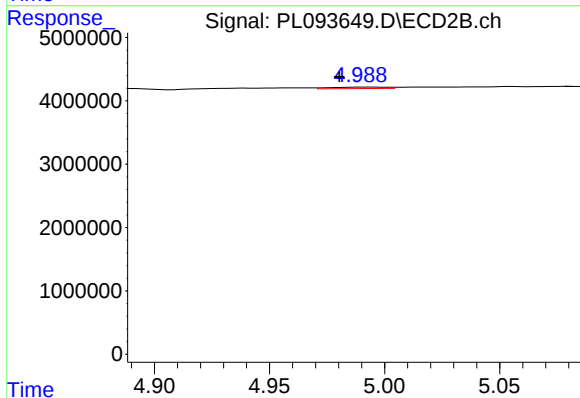


#10 gamma-Chlordane

R.T.: 4.992 min
Delta R.T.: 0.012 min
Response: 373238
Conc: 0.10 ng/ml

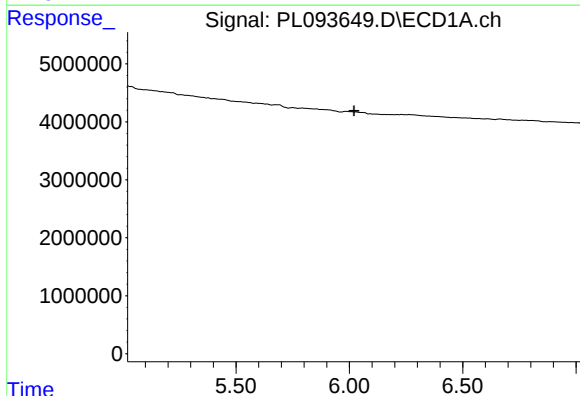


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.020 min
Response: 0
Conc: N.D.

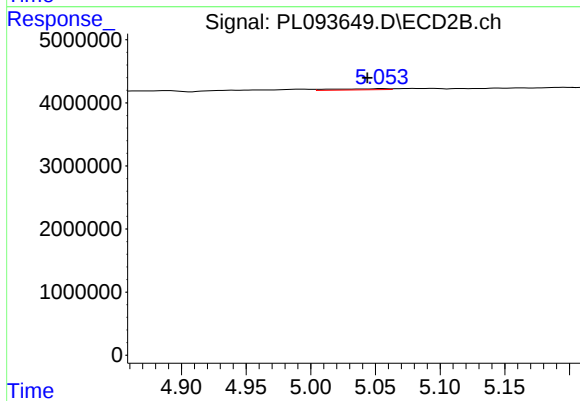

#11 alpha-Chlordane


R.T.: 5.055 min
Delta R.T.: 0.011 min
Response: 525195
Conc: 0.14 ng/ml

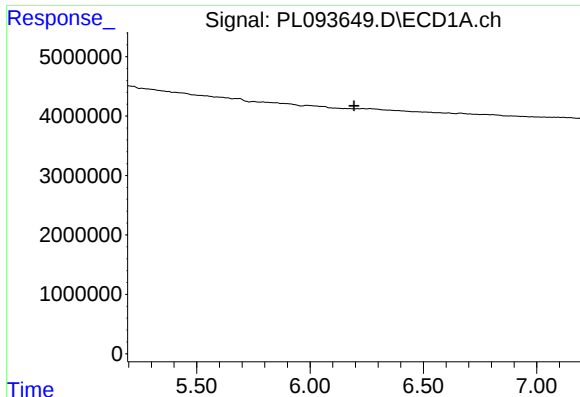

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.194 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

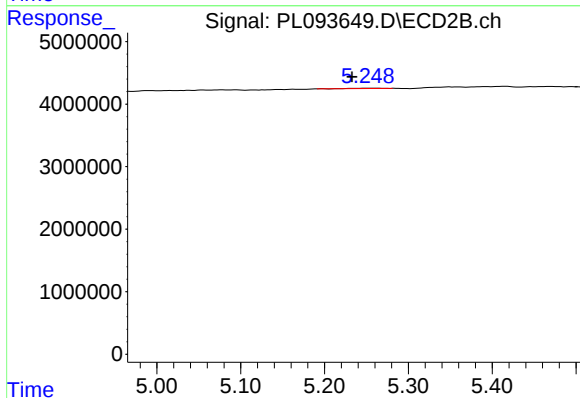


#12 4,4'-DDE

R.T.: 5.254 min
Delta R.T.: 0.021 min
Response: 84451
Conc: 0.02 ng/ml

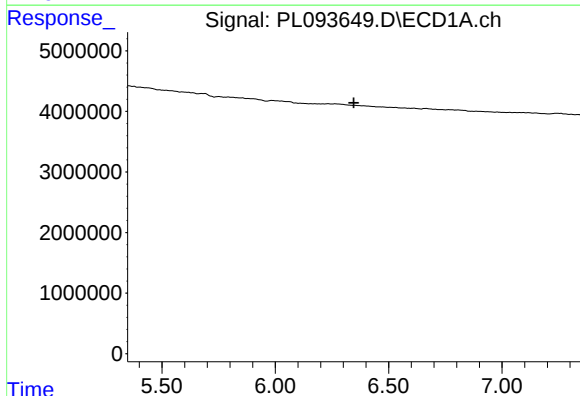


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.346 min
Response: 0
Conc: N.D.

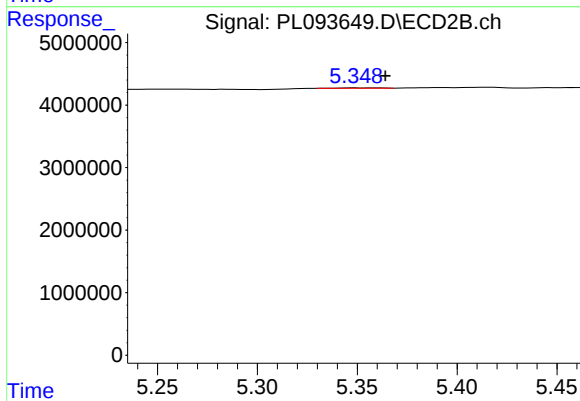

#13 Dieldrin


R.T.: 5.350 min
Delta R.T.: -0.014 min
Response: 69695
Conc: 0.02 ng/ml

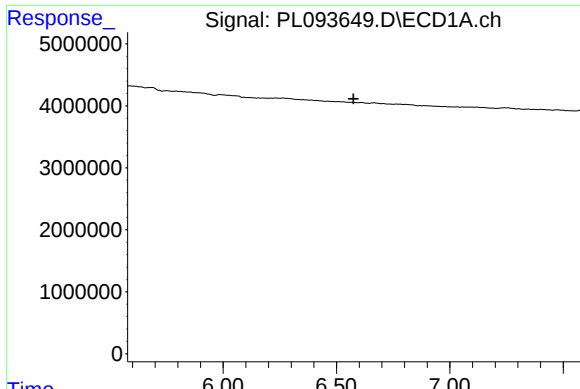

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

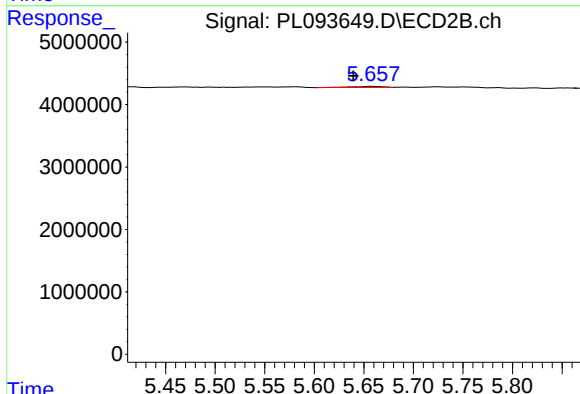


#14 Endrin

R.T.: 5.658 min
Delta R.T.: 0.019 min
Response: 379408
Conc: 0.11 ng/ml

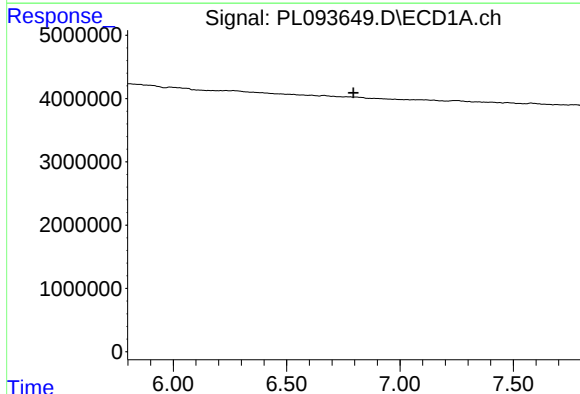


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.795 min
Response: 0
Conc: N.D.

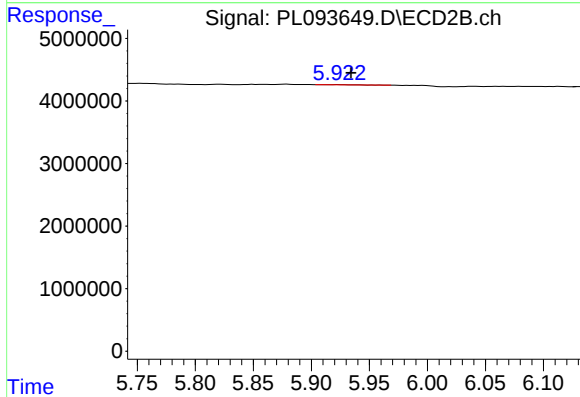

#15 Endosulfan II


R.T.: 5.922 min
Delta R.T.: -0.012 min
Response: 26237
Conc: 0.01 ng/ml

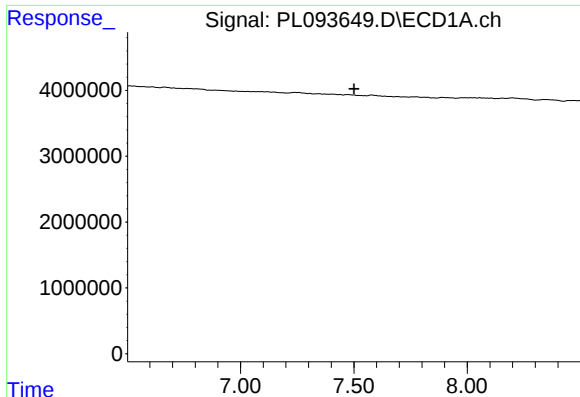

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

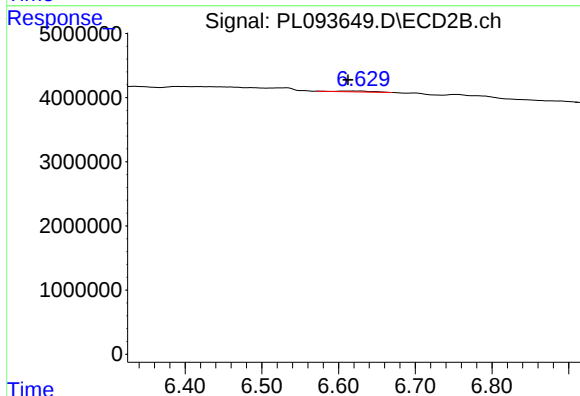


#20 Methoxychlor

R.T.: 6.625 min
Delta R.T.: 0.013 min
Response: 391195
Conc: 0.24 ng/ml

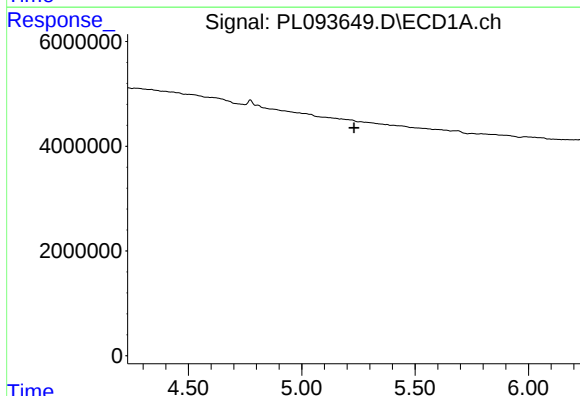


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

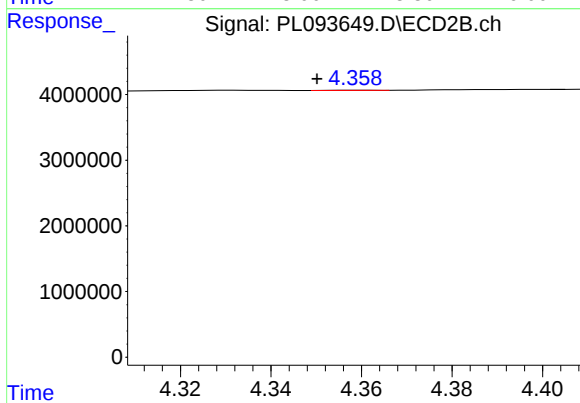

#24 Chlordane-2


R.T.: 4.360 min
Delta R.T.: 0.010 min
Response: 20642
Conc: 0.15 ng/ml

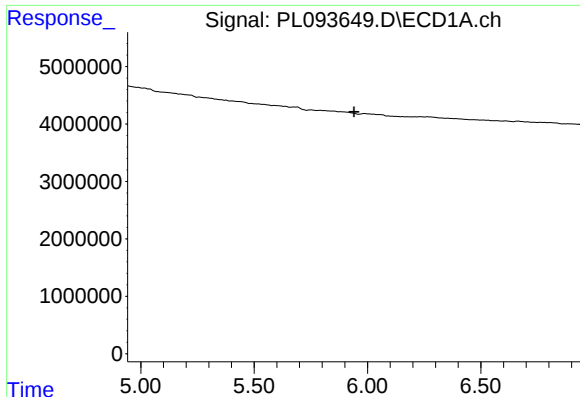

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

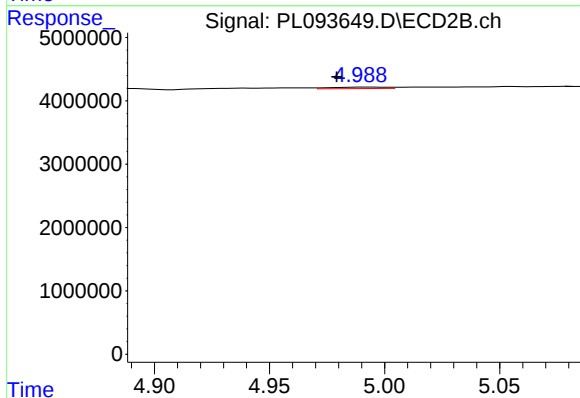


#25 Chlordane-3

R.T.: 4.992 min
Delta R.T.: 0.013 min
Response: 373238
Conc: 0.88 ng/ml

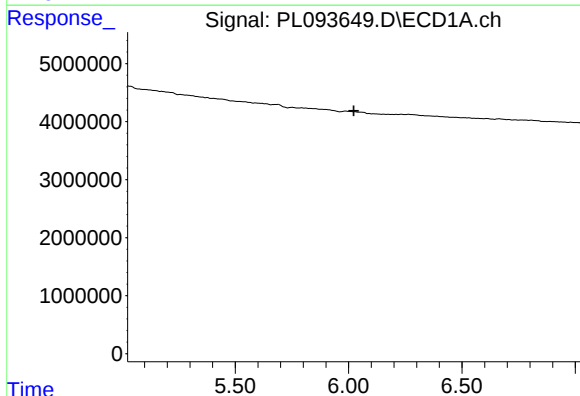


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

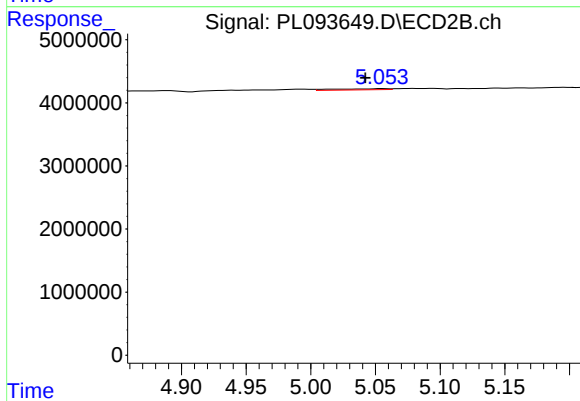

#26 Chlordane-4


R.T.: 5.055 min
Delta R.T.: 0.013 min
Response: 525195
Conc: 1.28 ng/ml

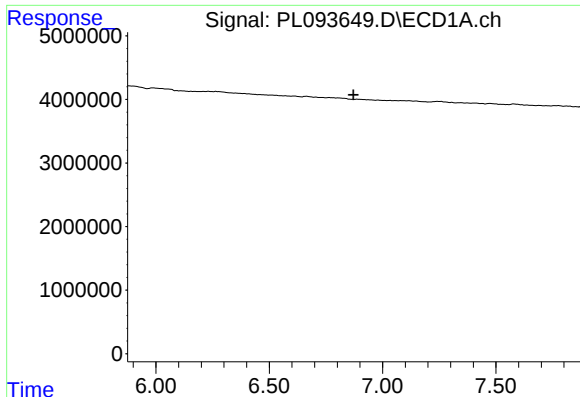

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB166044BL

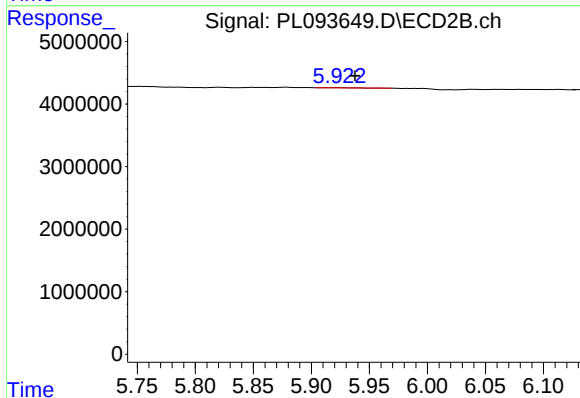


#27 Chlordane-5

R.T.: 5.922 min
Delta R.T.: -0.016 min
Response: 26237
Conc: 0.20 ng/ml

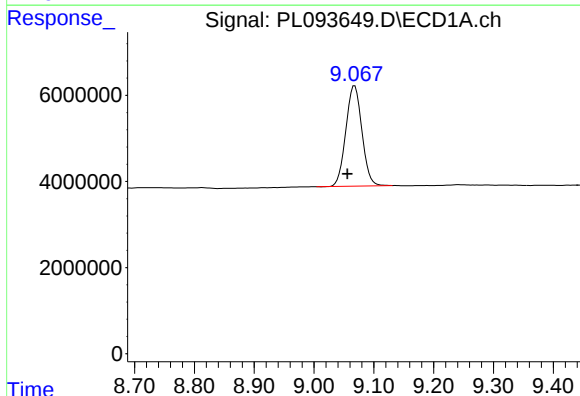

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.012 min
Response: 43460522
Conc: 23.50 ng/ml

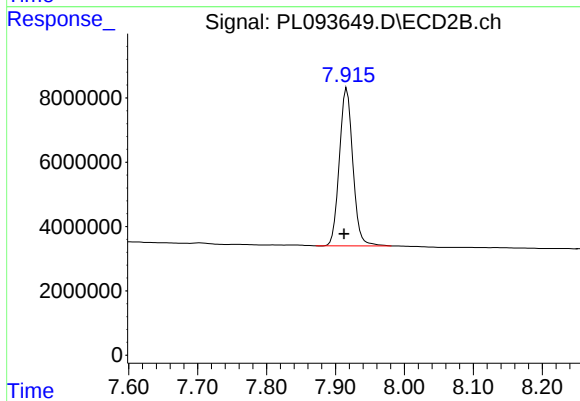

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.004 min
Response: 66685669
Conc: 22.33 ng/ml