

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 14:15
 Operator : AJ\SJ
 Sample : K1139-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:02:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.008	35459473	14009111	7.224	7.188
28)	SA Decachlor...	8.254	9.079	33618174	11270687	5.949	7.095
Target Compounds							
15)	B Endosulfa...	6.278f	0.000	13560014	0	2.606	N.D. #
27)	Chlordane-5	6.278	0.000	13560014	0	68.053	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL0111519\
Data File : PL043892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 14:15
Operator : AJ\SJ
Sample : K1139-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:02:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

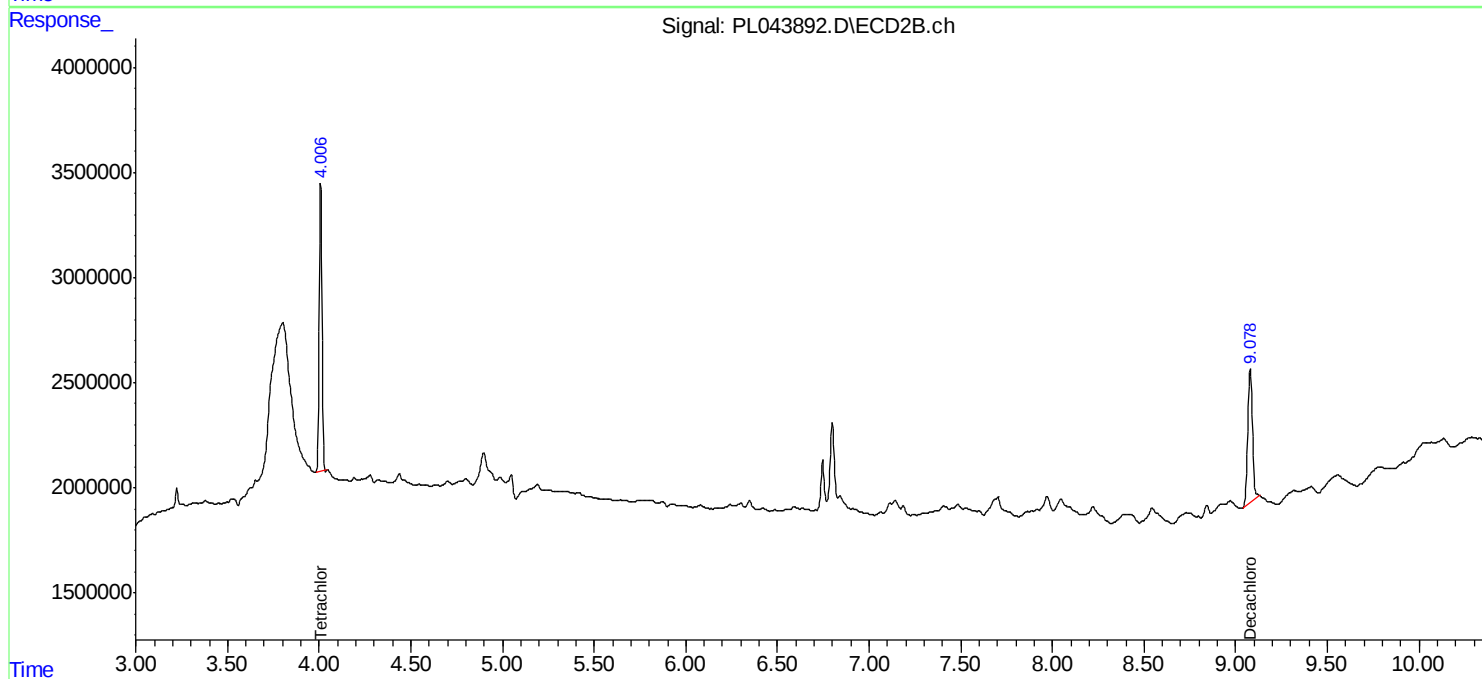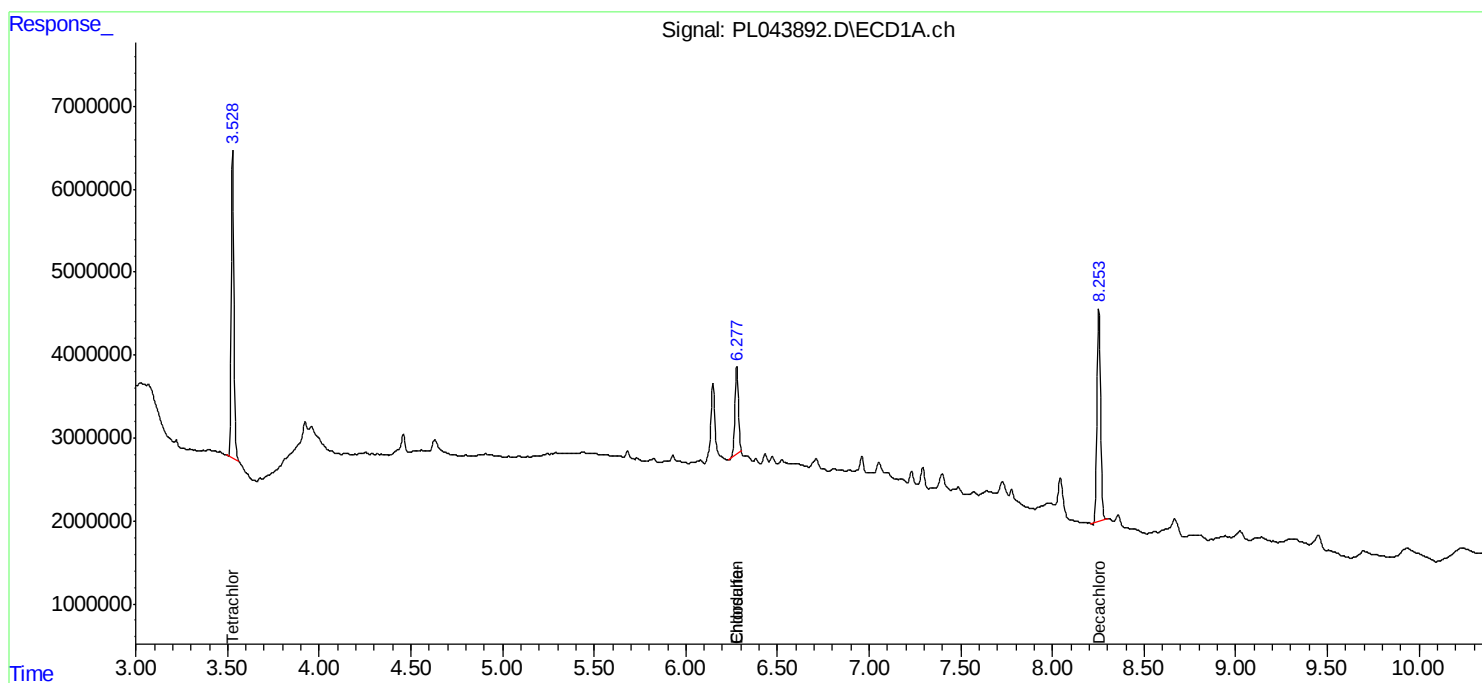


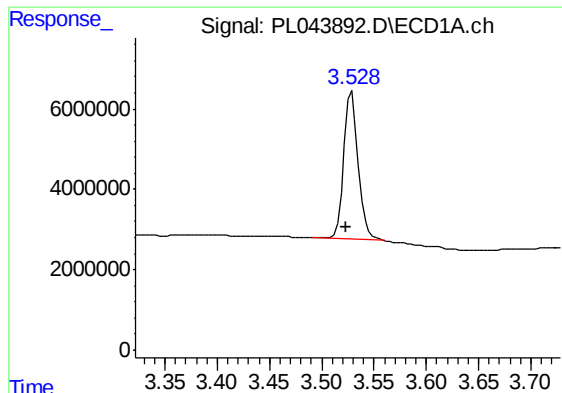

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.006 min
Response: 35459473
Conc: 7.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

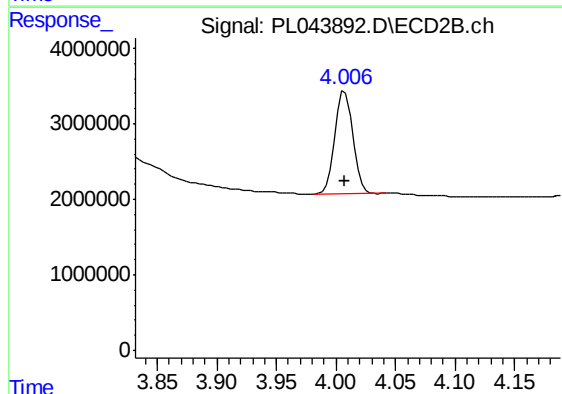


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 14009111
Conc: 7.19 ng/ml

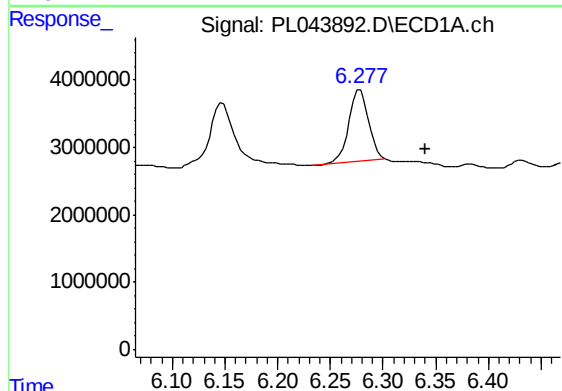


#15 Endosulfan II

R.T.: 6.278 min
Delta R.T.: -0.062 min
Response: 13560014
Conc: 2.61 ng/ml

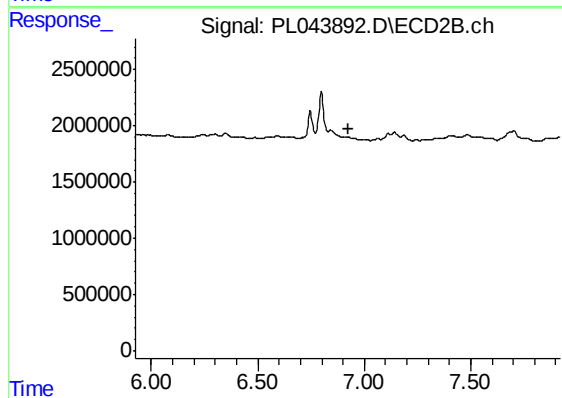

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

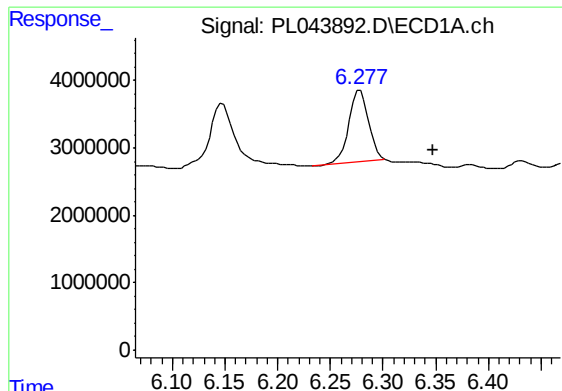

#27 Chlordane-5


R.T.: 6.278 min
Delta R.T.: -0.070 min
Response: 13560014
Conc: 68.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

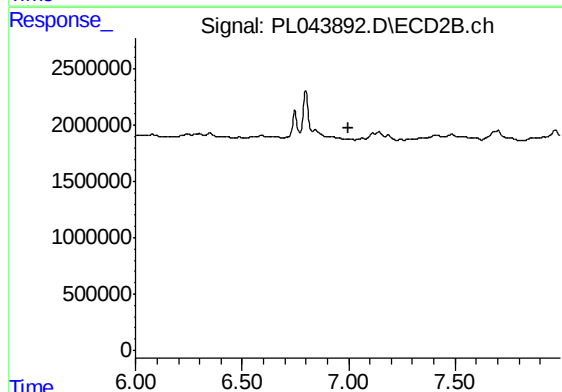


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

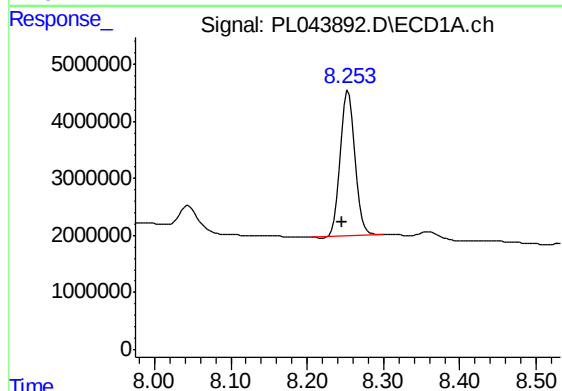

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.008 min
Response: 33618174
Conc: 5.95 ng/ml

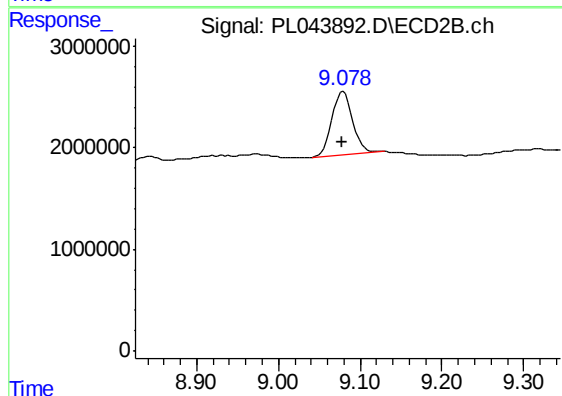

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.001 min
Response: 11270687
Conc: 7.09 ng/ml