

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 14:43
 Operator : AJ\SJ
 Sample : K1139-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:02:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.008	49058528	20009231	9.994	10.267
28)	SA Decachlor...	8.255	9.079	52389667	16479634	9.270	10.374
Target Compounds							
6)	B beta-BHC	4.459f	0.000	6956226	0	2.337	N.D. #
12)	B 4,4'-DDE	5.683	0.000	11073538	0	2.044	N.D. #
15)	B Endosulfa...	6.279f	0.000	14986022	0	2.880	N.D. #
17)	MA 4,4'-DDT	6.435	0.000	8606504	0	1.887	N.D. #
23)	Chlordane-1	4.459	0.000	6956226	0	31.098	N.D. #
27)	Chlordane-5	6.279	0.000	14986022	0	75.209	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 14:43
Operator : AJ\SJ
Sample : K1139-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:02:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

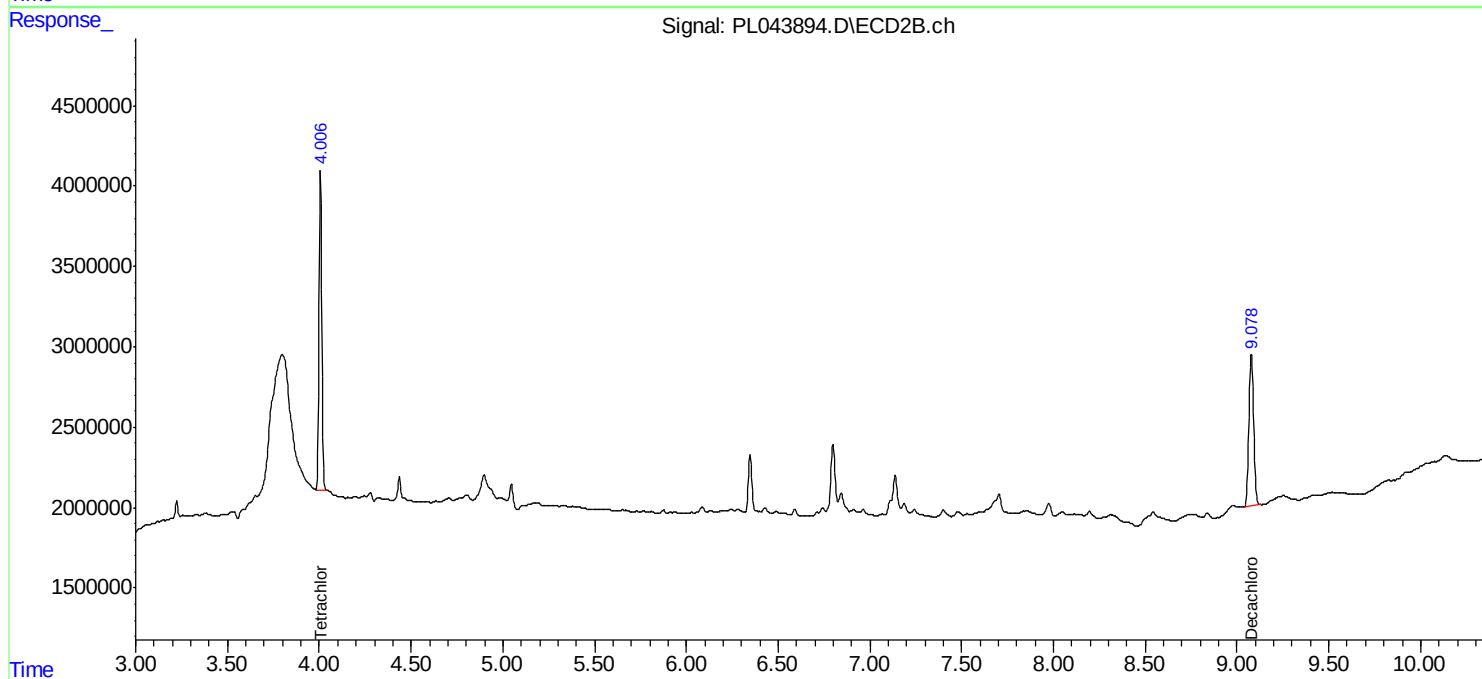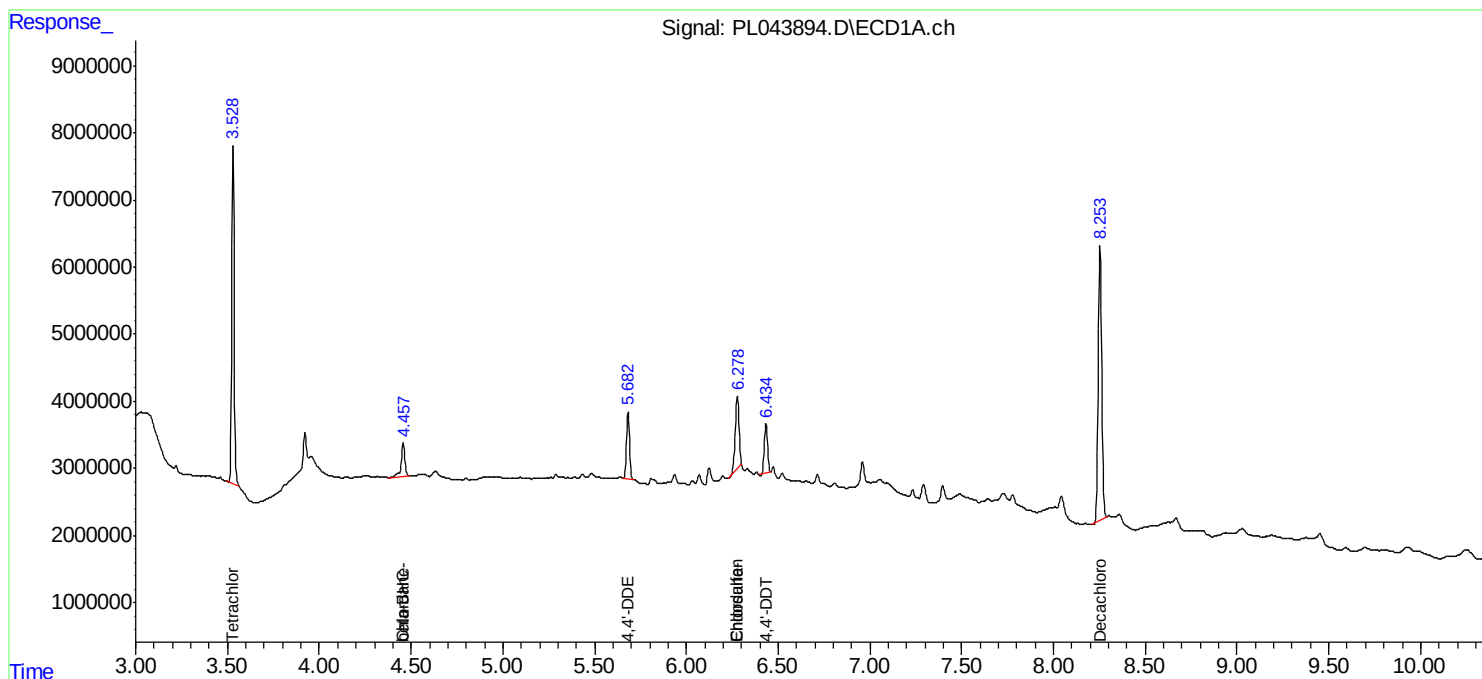


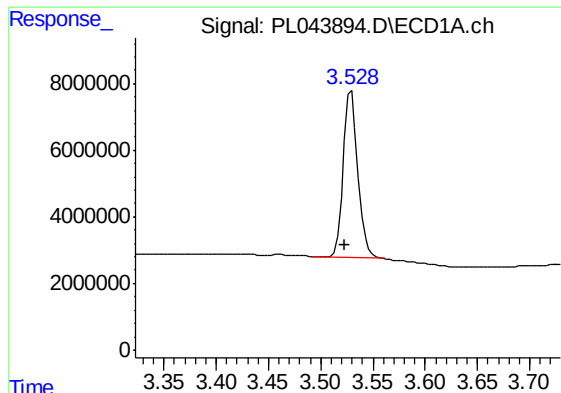

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.006 min
Response: 49058528
Conc: 9.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

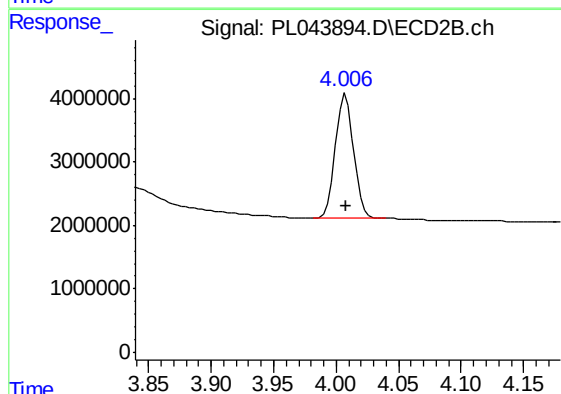


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 20009231
Conc: 10.27 ng/ml

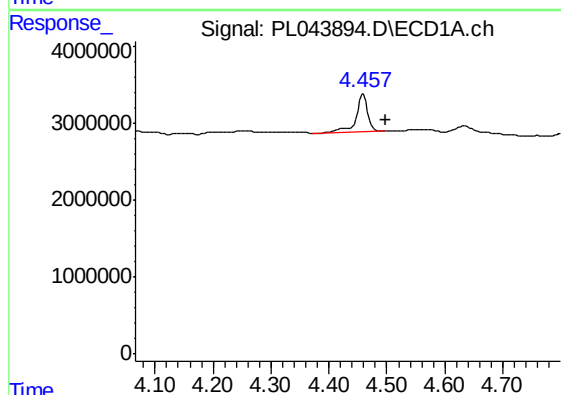


#6 beta-BHC

R.T.: 4.459 min
Delta R.T.: -0.039 min
Response: 6956226
Conc: 2.34 ng/ml

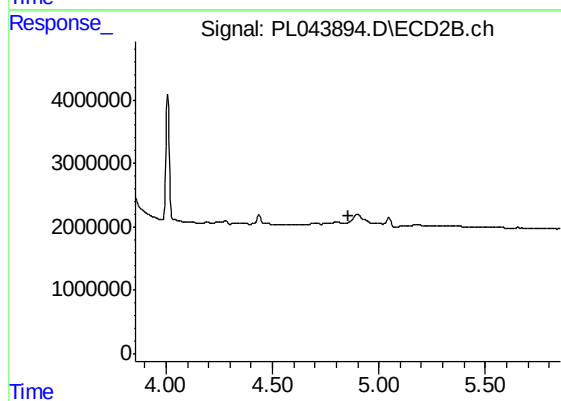

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

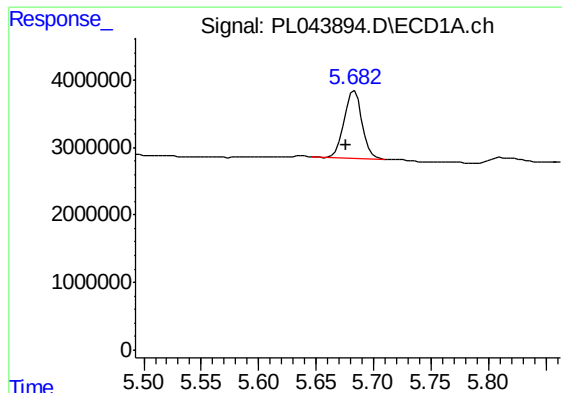

#12 4,4'-DDE


R.T.: 5.683 min
Delta R.T.: 0.007 min
Response: 11073538
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

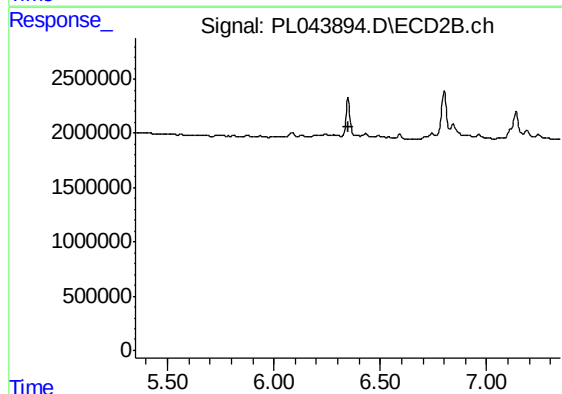


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.348 min
Response: 0
Conc: N.D.

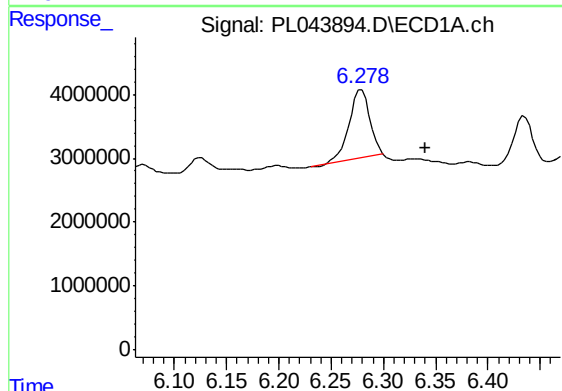


#15 Endosulfan II

R.T.: 6.279 min
Delta R.T.: -0.061 min
Response: 14986022
Conc: 2.88 ng/ml

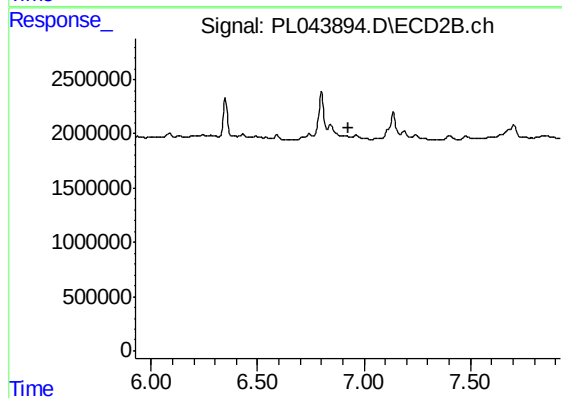

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

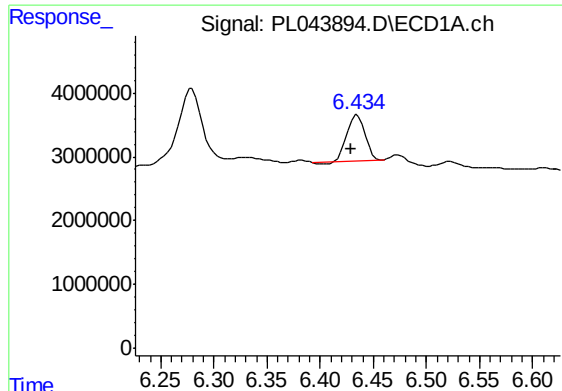

#17 4,4'-DDT


R.T.: 6.435 min
Delta R.T.: 0.006 min
Response: 8606504
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

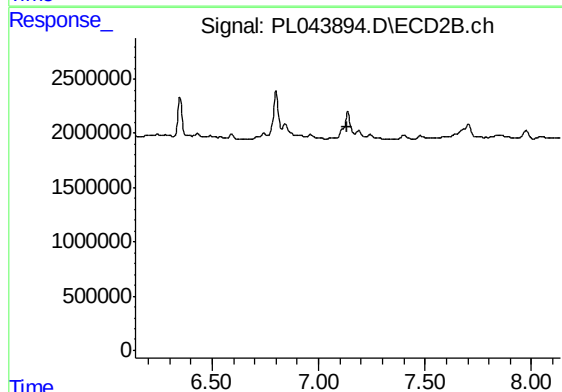


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

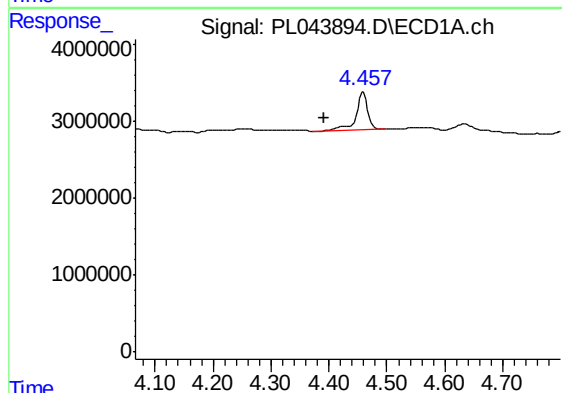


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.068 min
Response: 6956226
Conc: 31.10 ng/ml

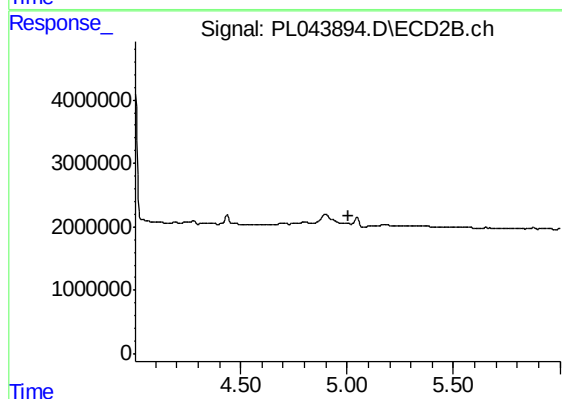

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

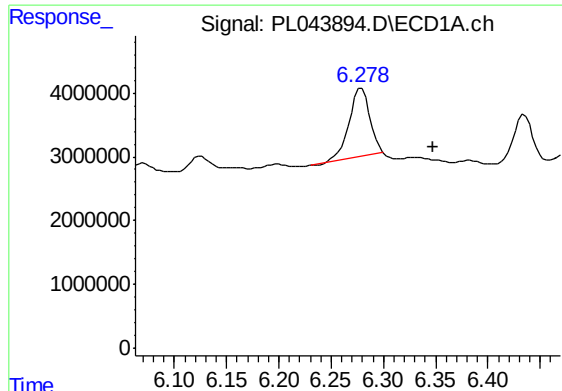

#27 Chlordane-5


R.T.: 6.279 min
Delta R.T.: -0.069 min
Response: 14986022
Conc: 75.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

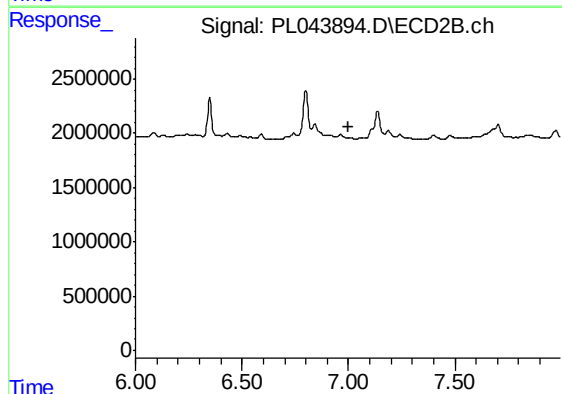


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

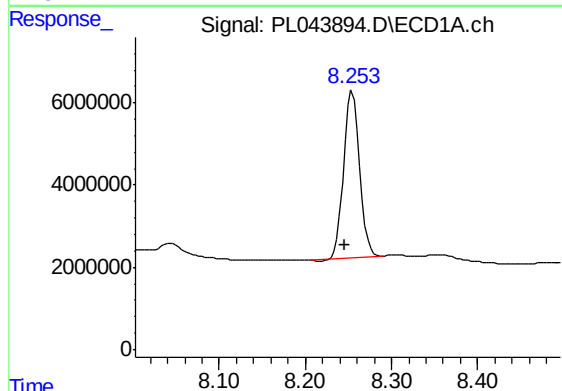

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.008 min
Response: 52389667
Conc: 9.27 ng/ml

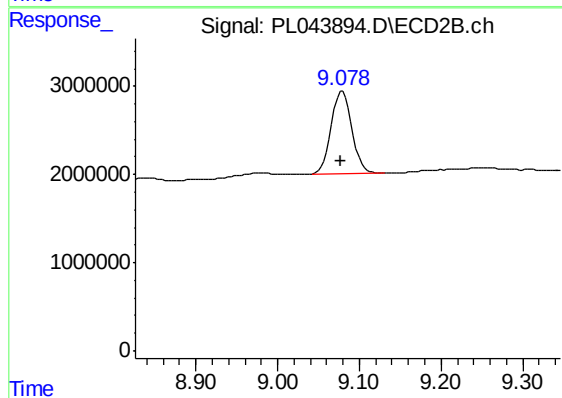

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.001 min
Response: 16479634
Conc: 10.37 ng/ml