

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 18:07
 Operator : AJ\SJ
 Sample : K1127-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:06:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
2) A	alpha-BHC	3.948	0.000	7983001	0	1.038	N.D. #
6) B	beta-BHC	4.459f	0.000	11471099	0	3.853	N.D. #
8) B	Heptachlo...	5.236	0.000	5936510	0	0.934	N.D. #
9) A	Endosulfan I	5.518f	0.000	15063520	0	2.581	N.D. #
10) B	gamma-Chl...	5.518f	0.000	15063520	0	2.347	N.D. #
11) B	alpha-Chl...	5.518	0.000	15063520	0	2.384	N.D. #
15) B	Endosulfa...	6.279f	0.000	13365209	0	2.569	N.D. #
16) A	4,4'-DDD	0.000	6.799f	0	8801722	N.D.	5.825 #
23)	Chlordane-1	4.459	0.000	11471099	0	51.282	N.D. #
25)	Chlordane-3	5.518	0.000	15063520	0	20.744	N.D. #
26)	Chlordane-4	5.518	0.000	15063520	0	23.637	N.D. #
27)	Chlordane-5	6.279	0.000	13365209	0	67.075	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 18:07
Operator : AJ\SJ
Sample : K1127-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:06:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

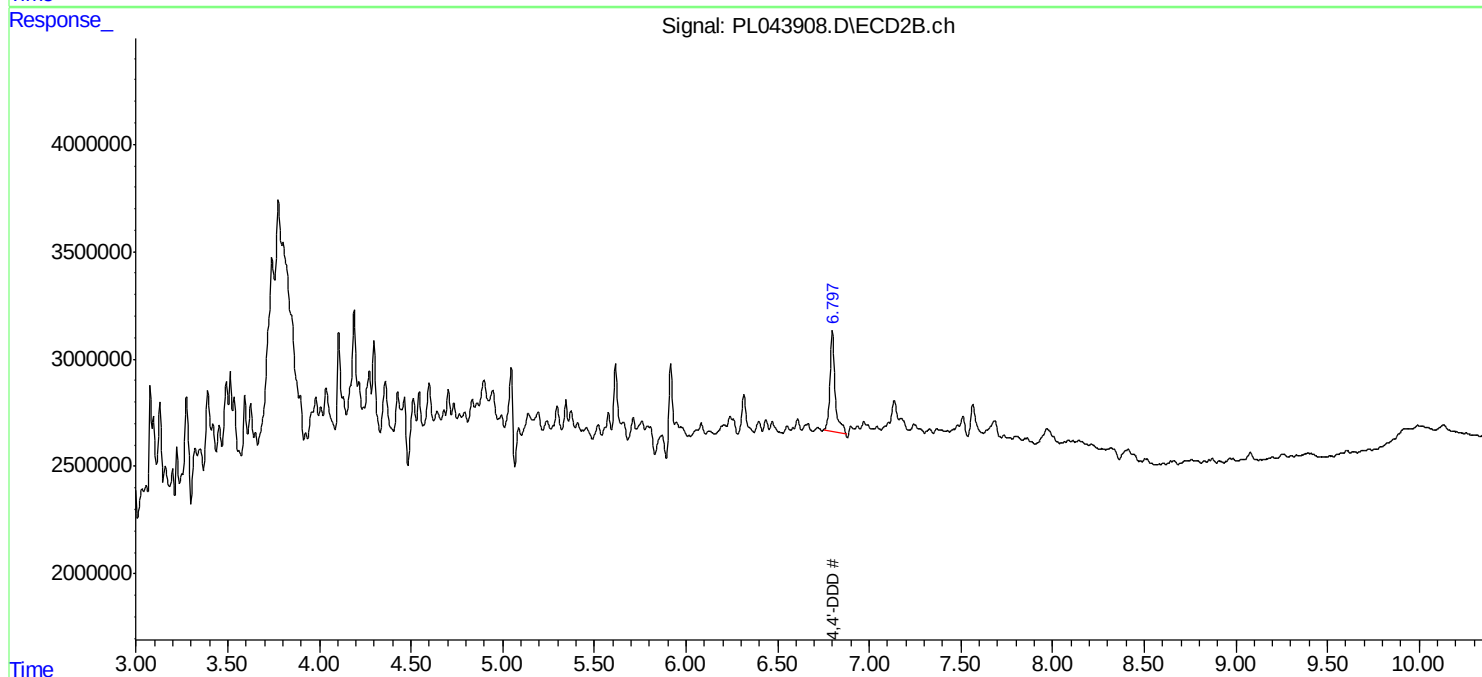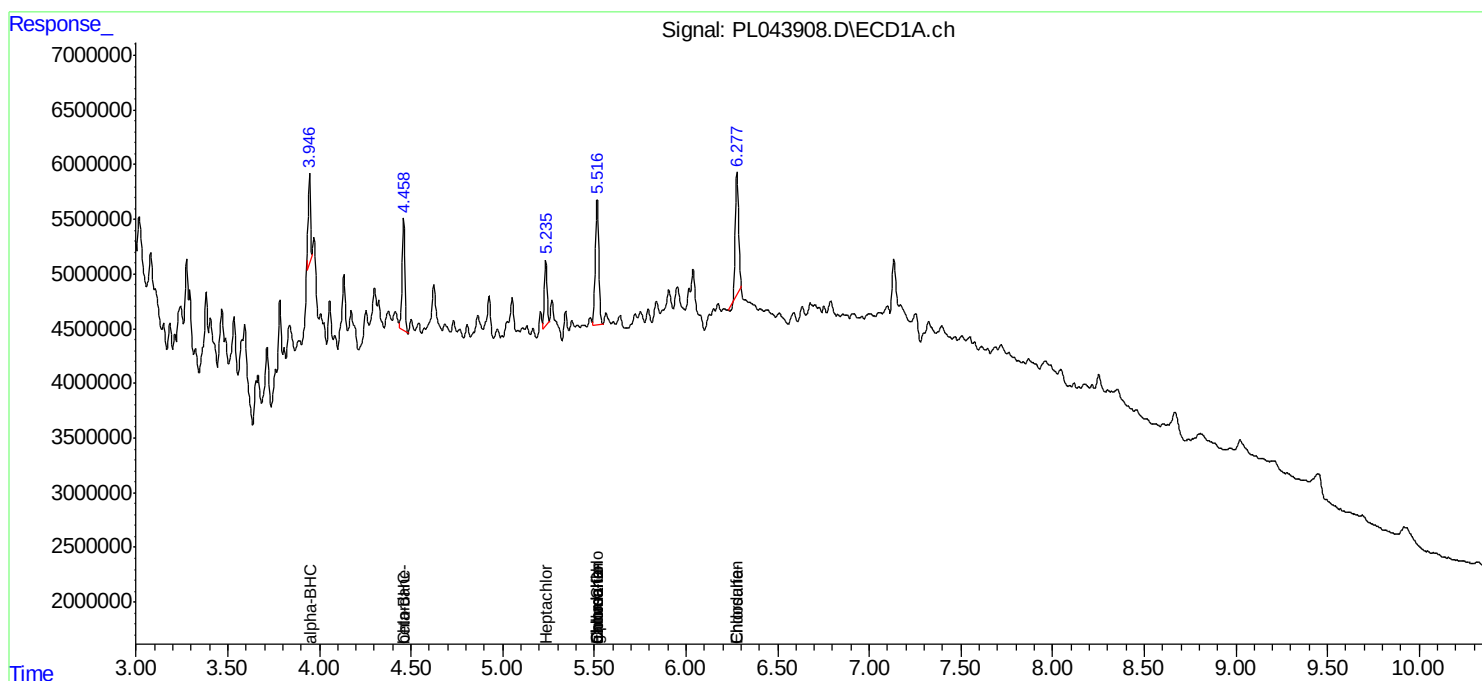


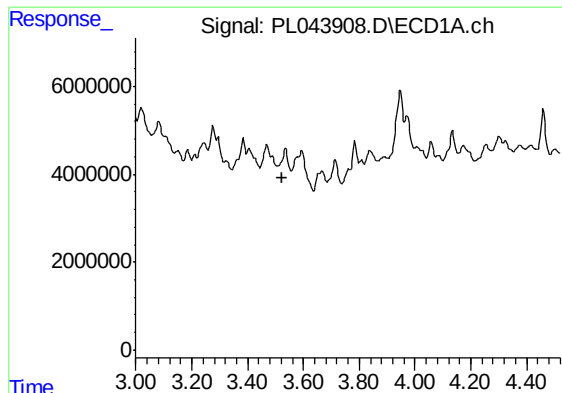

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

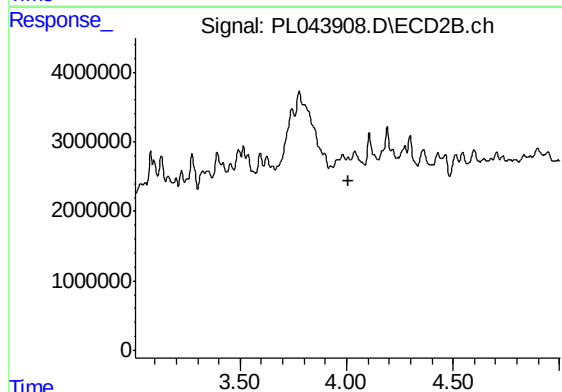


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

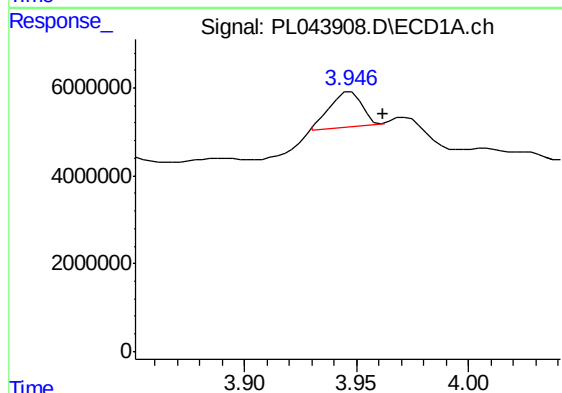


#2 alpha-BHC

R.T.: 3.948 min
Delta R.T.: -0.014 min
Response: 7983001
Conc: 1.04 ng/ml

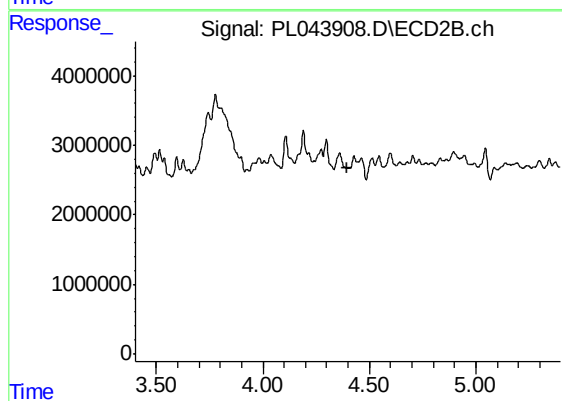

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.398 min
Response: 0
Conc: N.D.

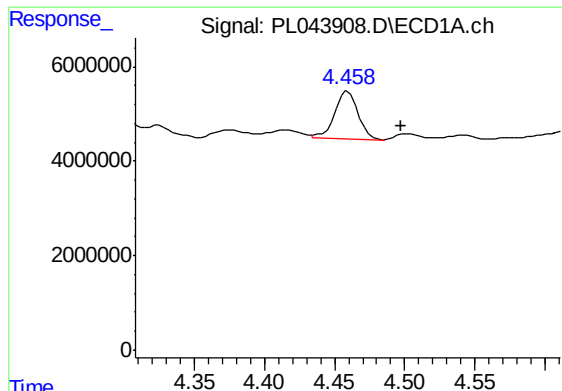

#6 beta-BHC


R.T.: 4.459 min
Delta R.T.: -0.038 min
Response: 11471099
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

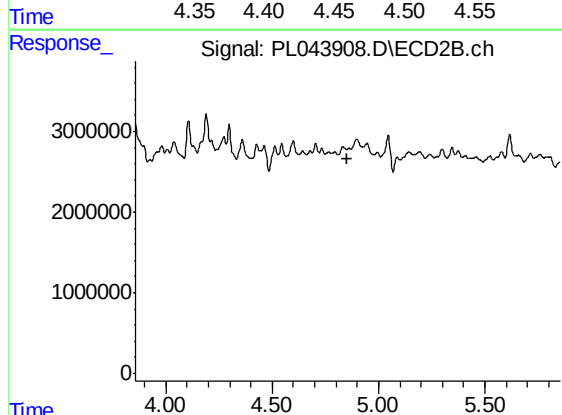


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

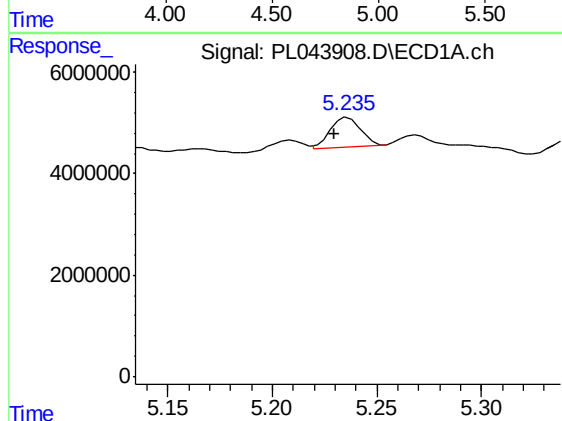


#8 Heptachlor epoxide

R.T.: 5.236 min
Delta R.T.: 0.006 min
Response: 5936510
Conc: 0.93 ng/ml

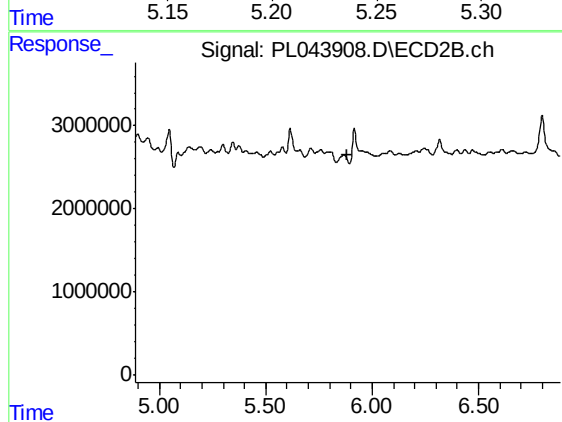

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.885 min
Response: 0
Conc: N.D.

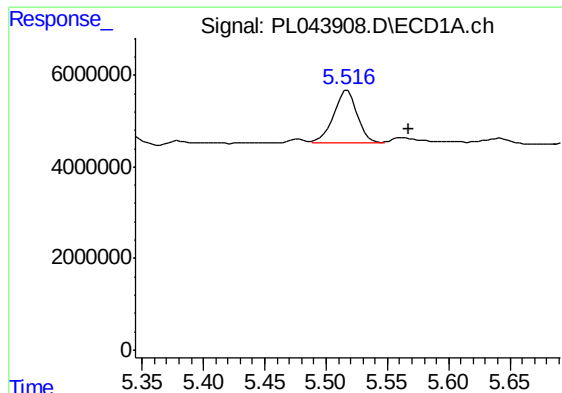

#9 Endosulfan I


R.T.: 5.518 min
Delta R.T.: -0.050 min
Response: 15063520
Conc: 2.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

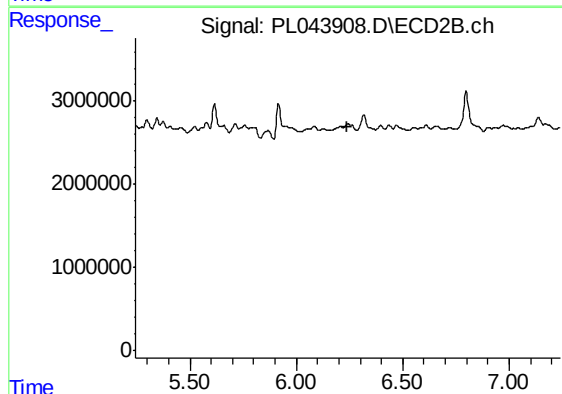


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

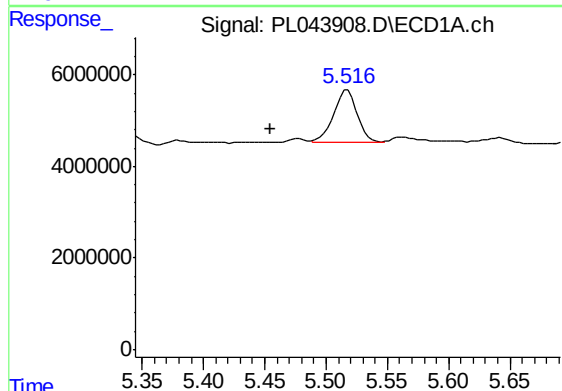


#10 gamma-Chlordane

R.T.: 5.518 min
Delta R.T.: 0.063 min
Response: 15063520
Conc: 2.35 ng/ml

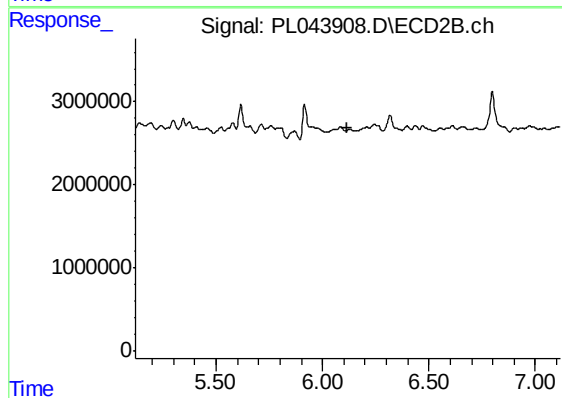

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

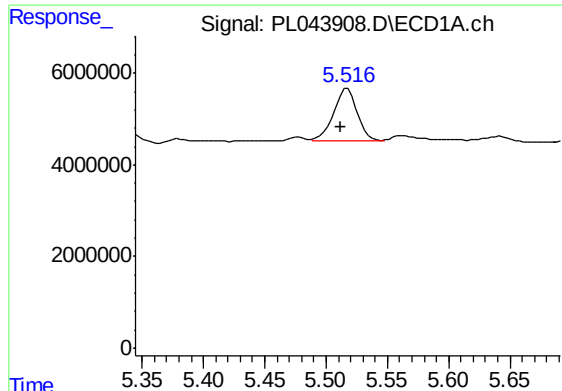

#11 alpha-Chlordane


R.T.: 5.518 min
Delta R.T.: 0.005 min
Response: 15063520
Conc: 2.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

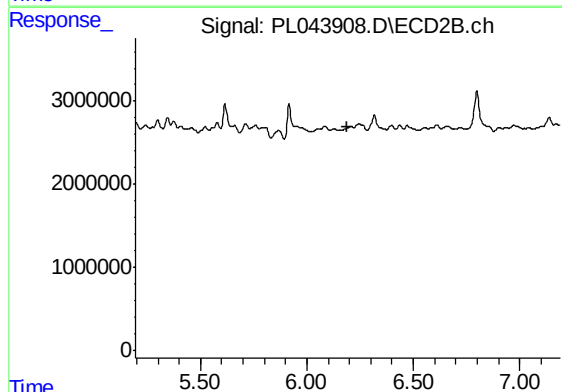


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

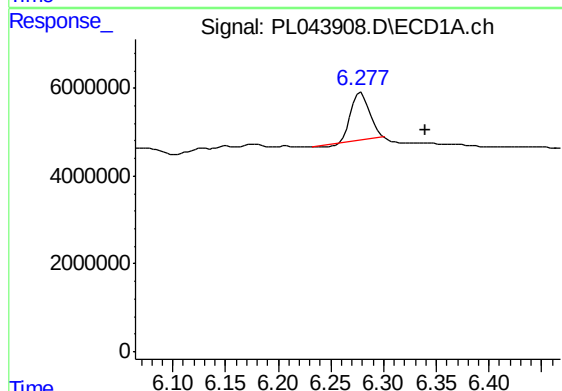


#15 Endosulfan II

R.T.: 6.279 min
Delta R.T.: -0.061 min
Response: 13365209
Conc: 2.57 ng/ml

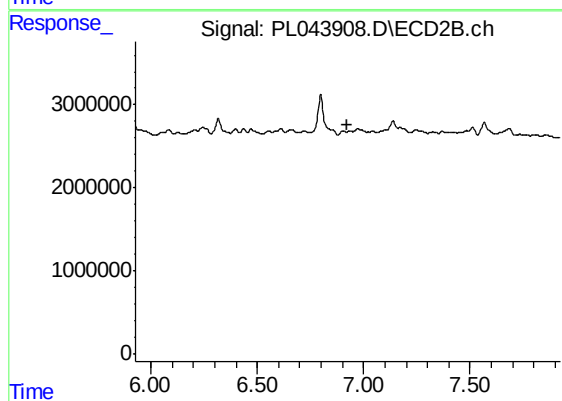

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

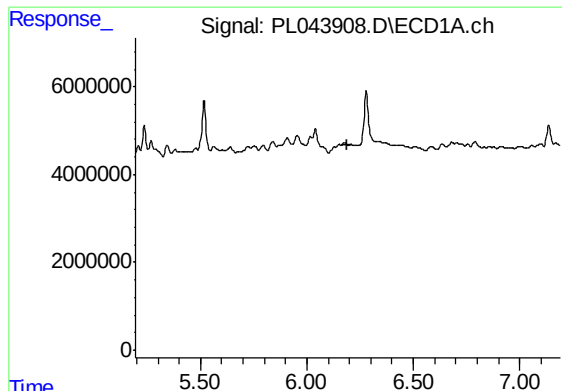

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

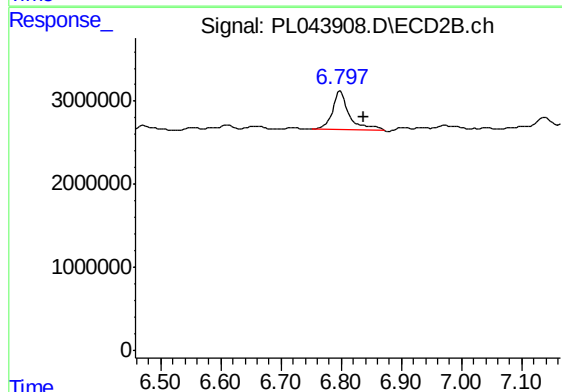


#16 4,4'-DDD

R.T.: 6.799 min
Delta R.T.: -0.039 min
Response: 8801722
Conc: 5.82 ng/ml

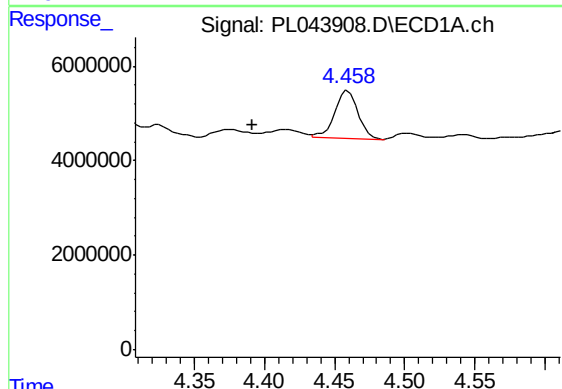


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.068 min
Response: 11471099
Conc: 51.28 ng/ml

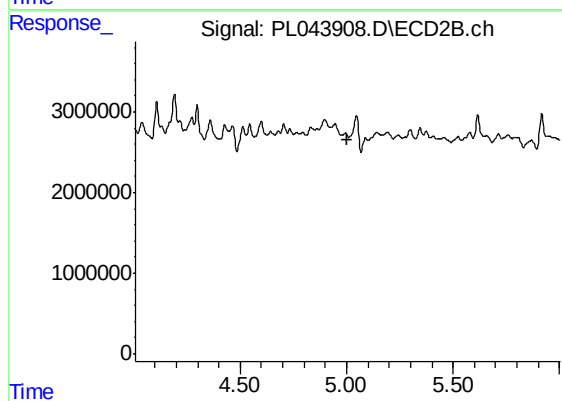

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

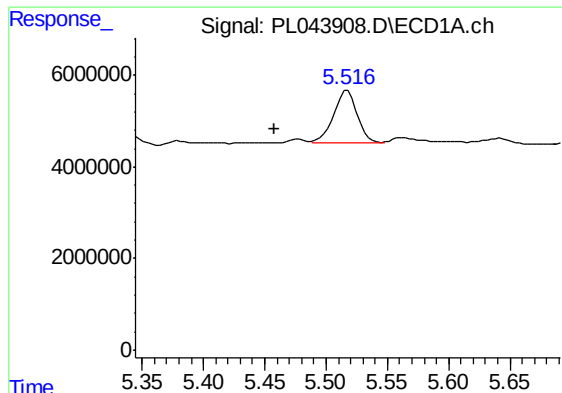

#25 Chlordane-3


R.T.: 5.518 min
Delta R.T.: 0.060 min
Response: 15063520
Conc: 20.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

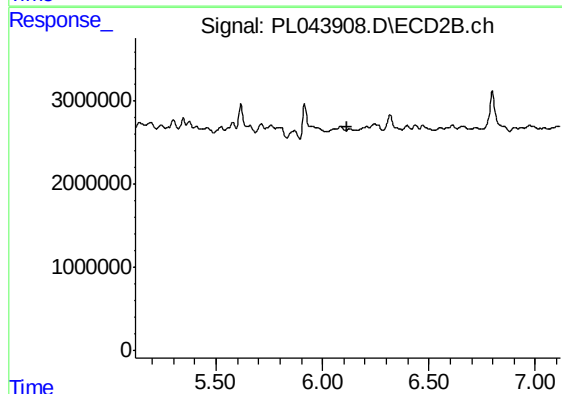


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

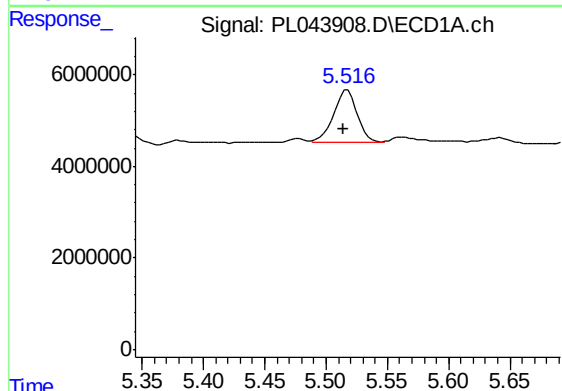


#26 Chlordane-4

R.T.: 5.518 min
Delta R.T.: 0.003 min
Response: 15063520
Conc: 23.64 ng/ml

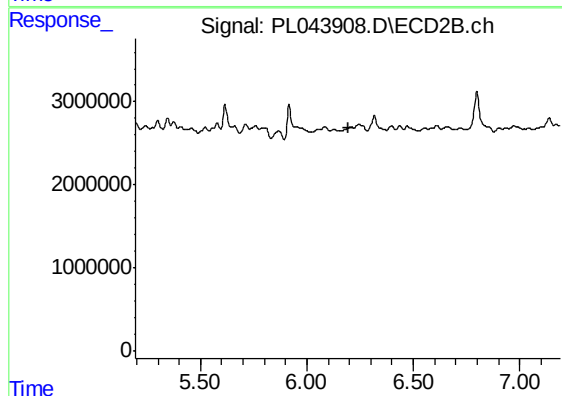

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.194 min
Response: 0
Conc: N.D.

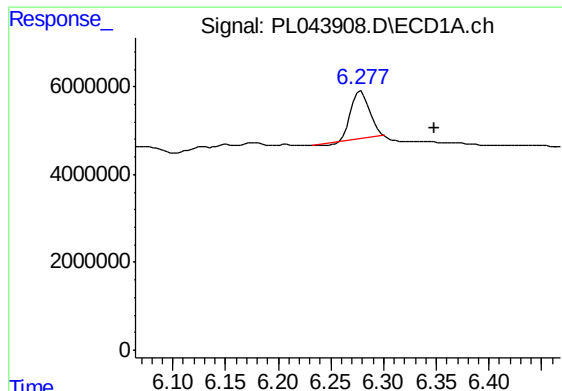

#27 Chlordane-5


R.T.: 6.279 min
Delta R.T.: -0.069 min
Response: 13365209
Conc: 67.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

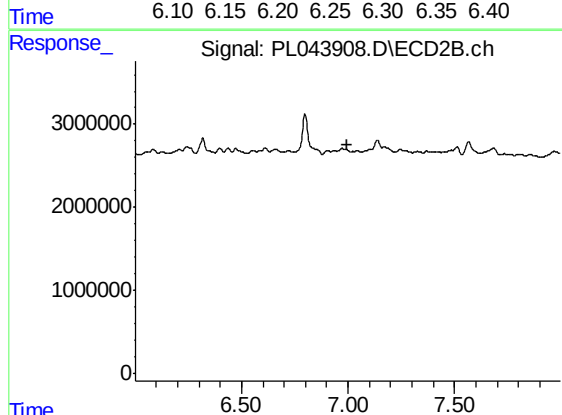


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

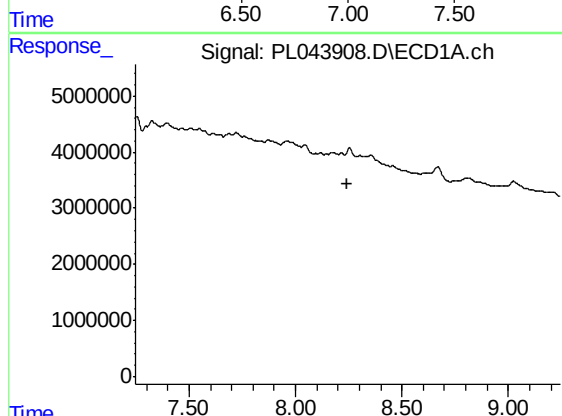

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.246 min
Response: 0
Conc: N.D.

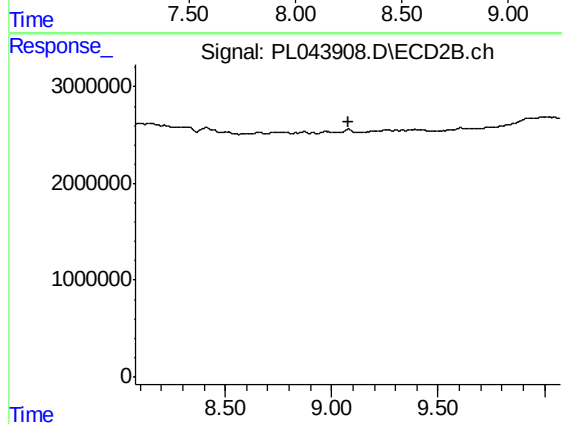

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.