

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 18:21
 Operator : AJ\SJ
 Sample : K1139-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T-CONTAINMENT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:07:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.007	78078542	29002237	15.906	14.882
28)	SA Decachlor...	8.254	9.079	57643283	17508391	10.200	11.022
Target Compounds							
2)	A alpha-BHC	3.922f	0.000	1099802	0	0.143	N.D. #
6)	B beta-BHC	4.460f	0.000	12007497	0	4.034	N.D. #
15)	B Endosulfa...	6.279f	0.000	15154668	0	2.913	N.D. #
16)	A 4,4'-DDD	0.000	6.798f	0	10315662	N.D.	6.827 #
17)	MA 4,4'-DDT	6.448	0.000	16303110	0	3.574	N.D. #
18)	B Endrin al...	6.448f	0.000	16303110	0	3.655	N.D. #
23)	Chlordane-1	4.460	0.000	12007497	0	53.680	N.D. #
27)	Chlordane-5	6.279	0.000	15154668	0	76.056	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 18:21
Operator : AJ\SJ
Sample : K1139-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:07:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

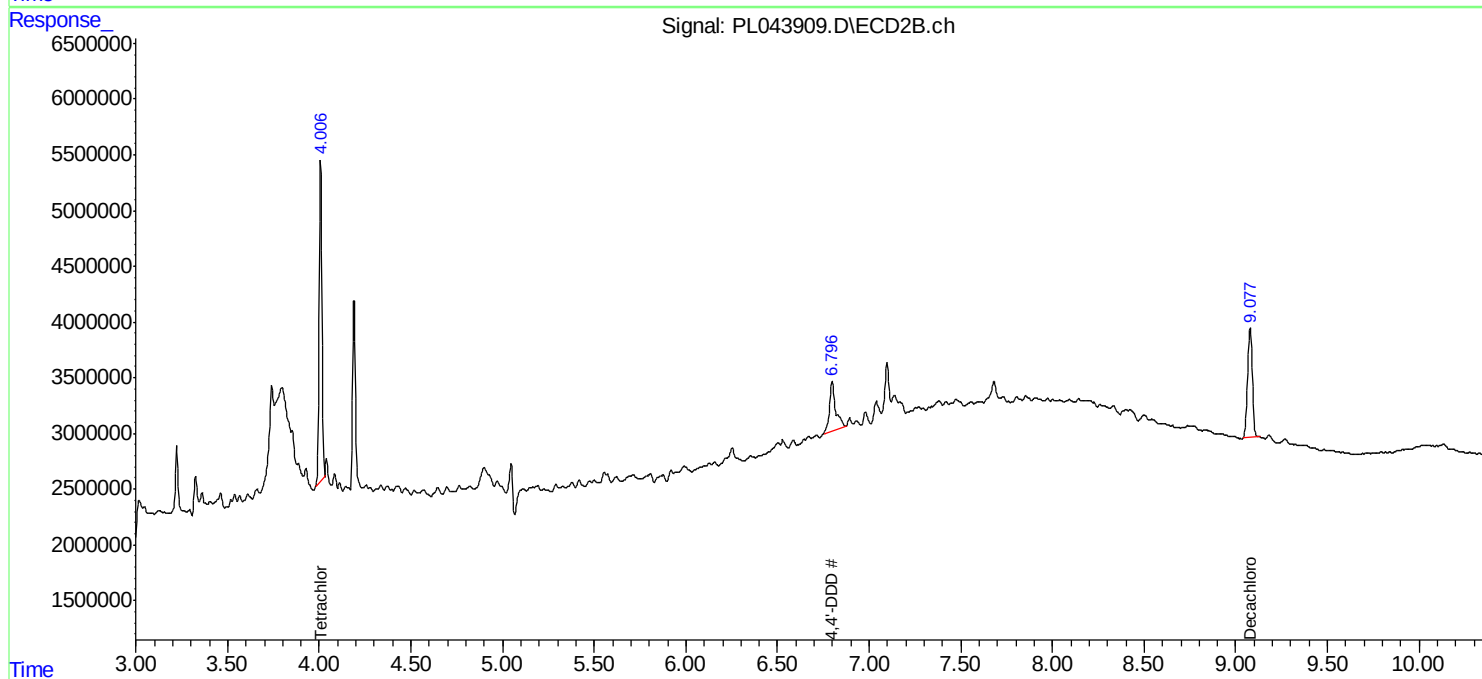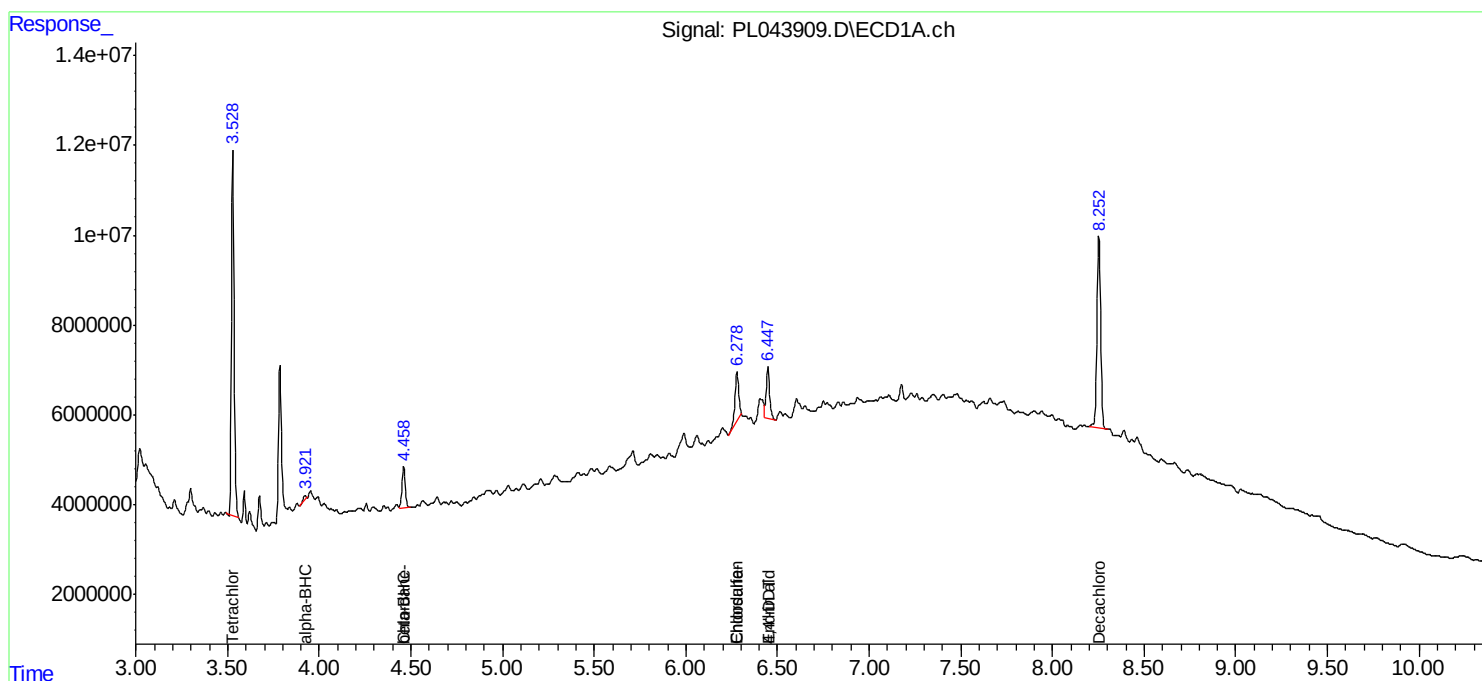


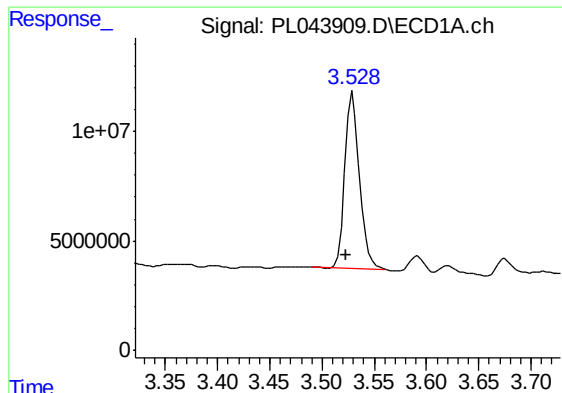

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.007 min
Response: 78078542
Conc: 15.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

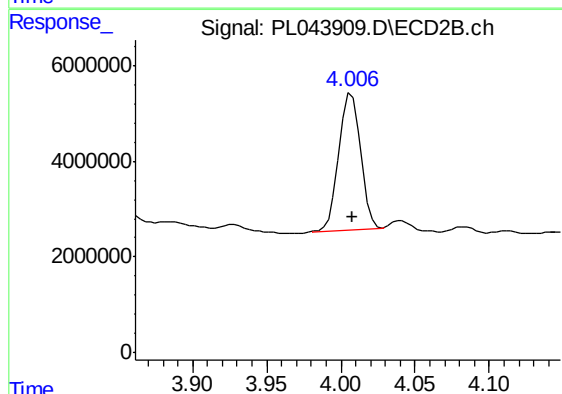


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 29002237
Conc: 14.88 ng/ml

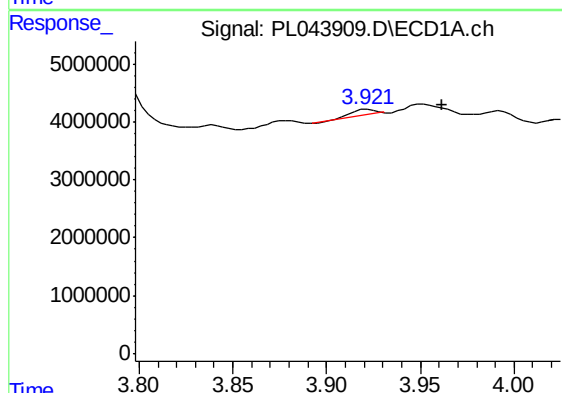


#2 alpha-BHC

R.T.: 3.922 min
Delta R.T.: -0.040 min
Response: 1099802
Conc: 0.14 ng/ml

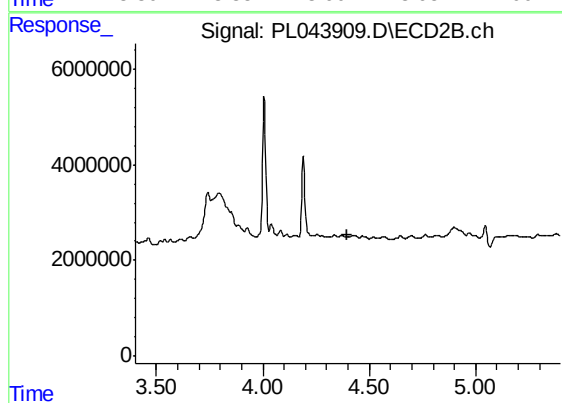

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.398 min
Response: 0
Conc: N.D.

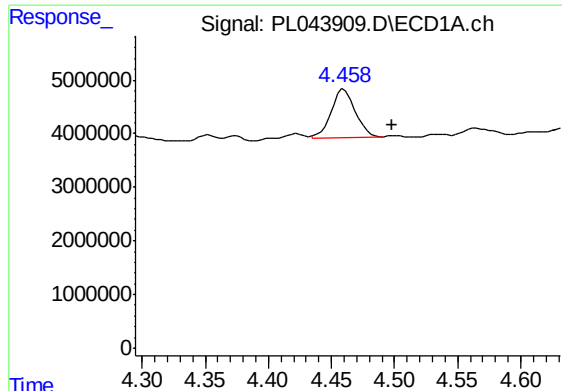

#6 beta-BHC


R.T.: 4.460 min
Delta R.T.: -0.038 min
Response: 12007497
Conc: 4.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

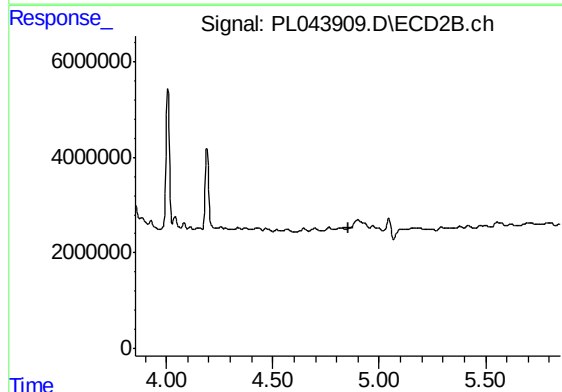


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

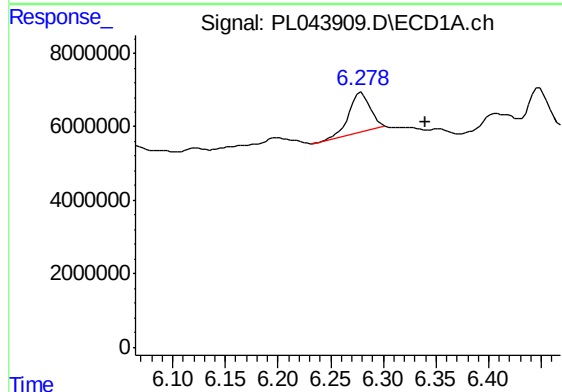


#15 Endosulfan II

R.T.: 6.279 min
Delta R.T.: -0.061 min
Response: 15154668
Conc: 2.91 ng/ml

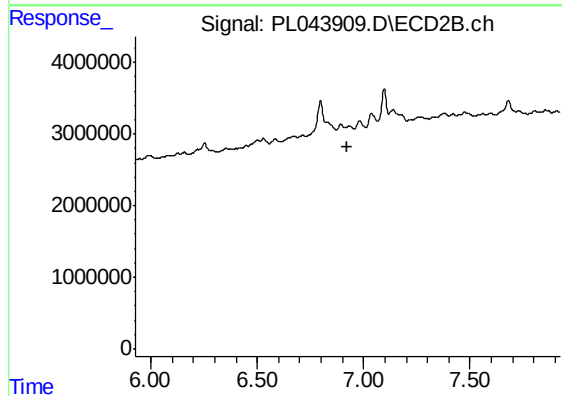

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

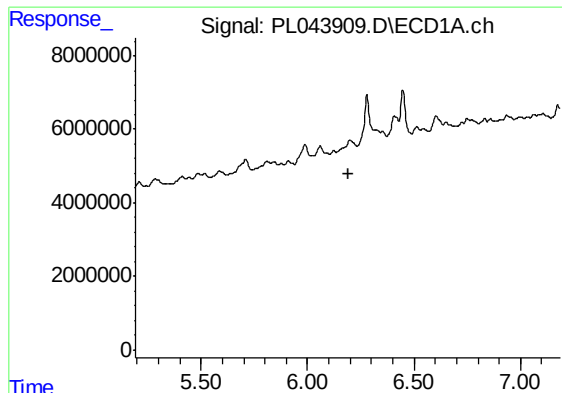

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

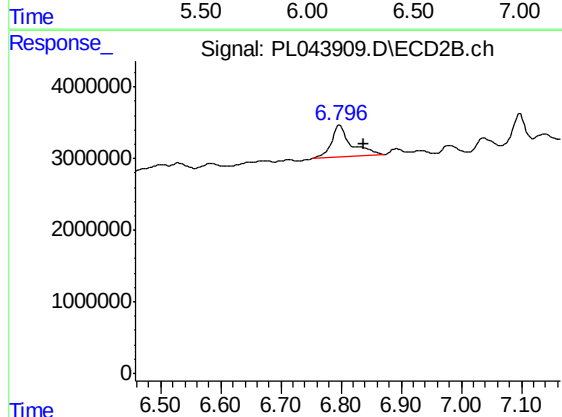


#16 4,4'-DDD

R.T.: 6.798 min
Delta R.T.: -0.040 min
Response: 10315662
Conc: 6.83 ng/ml

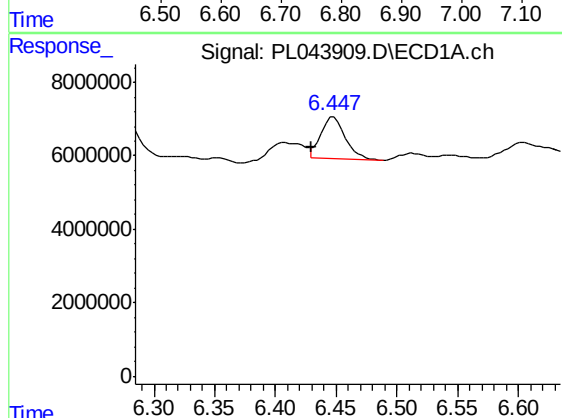


#17 4,4'-DDT

R.T.: 6.448 min
Delta R.T.: 0.019 min
Response: 16303110
Conc: 3.57 ng/ml

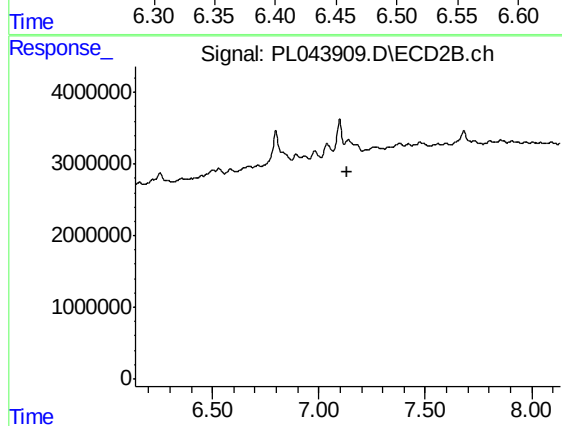

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.136 min
Response: 0
Conc: N.D.

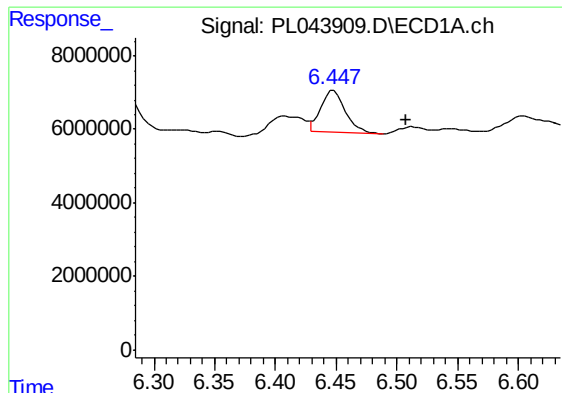

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: -0.059 min
Response: 16303110
Conc: 3.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

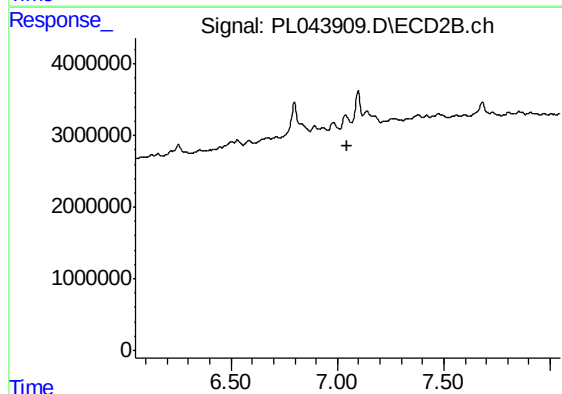


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.049 min
Response: 0
Conc: N.D.

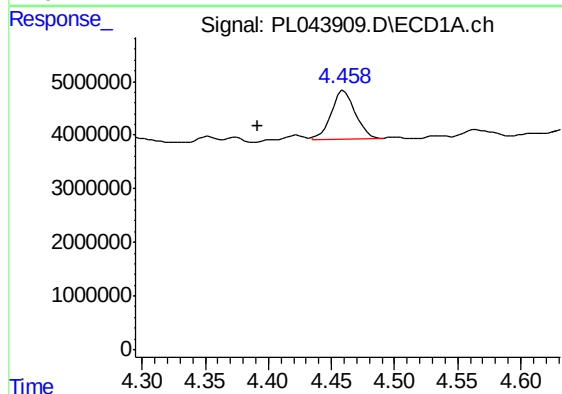


#23 Chlordane-1

R.T.: 4.460 min
Delta R.T.: 0.069 min
Response: 12007497
Conc: 53.68 ng/ml

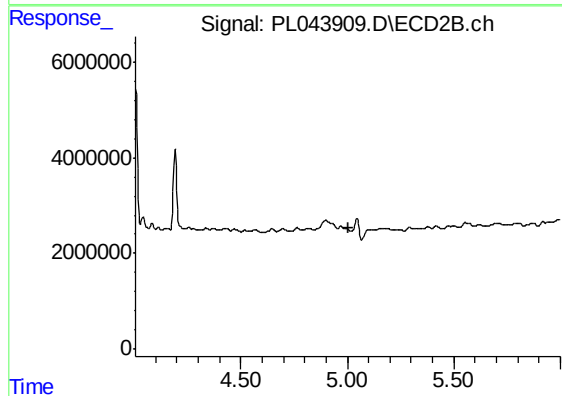

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

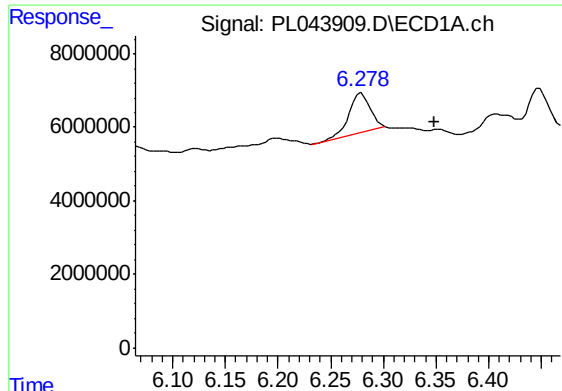

#27 Chlordane-5


R.T.: 6.279 min
Delta R.T.: -0.068 min
Response: 15154668
Conc: 76.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
T-CONTAINMENT

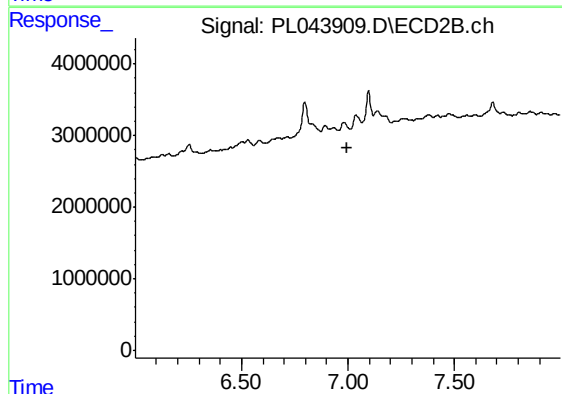


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

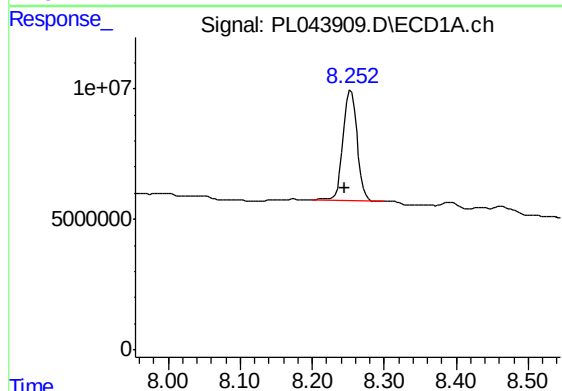

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.008 min
Response: 57643283
Conc: 10.20 ng/ml

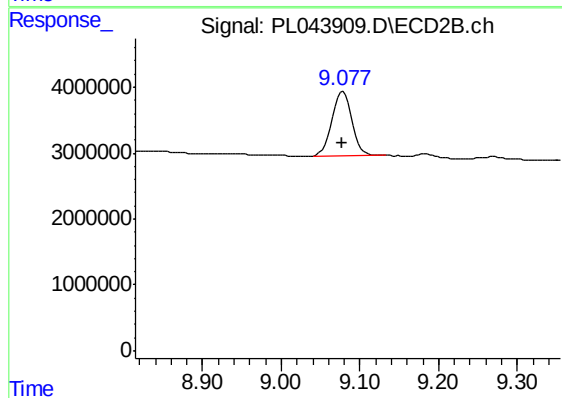

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.001 min
Response: 17508391
Conc: 11.02 ng/ml