

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 22:06
 Operator : AJ\SJ
 Sample : K1139-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:11:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.008	97747606	37707564	19.912	19.349
28)	SA Decachlor...	8.255	9.079	129.6E6	37183587	22.940	23.407
Target Compounds							
6)	B beta-BHC	4.460f	0.000	18253849	0	6.132	N.D. #
15)	B Endosulfa...	6.279f	0.000	13805855	0	2.654	N.D. #
16)	A 4,4'-DDD	0.000	6.799f	0	6469011	N.D.	4.281 #
23)	Chlordane-1	4.460	0.000	18253849	0	81.605	N.D. #
27)	Chlordane-5	6.279	0.000	13805855	0	69.287	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 22:06
Operator : AJ\SJ
Sample : K1139-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:11:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

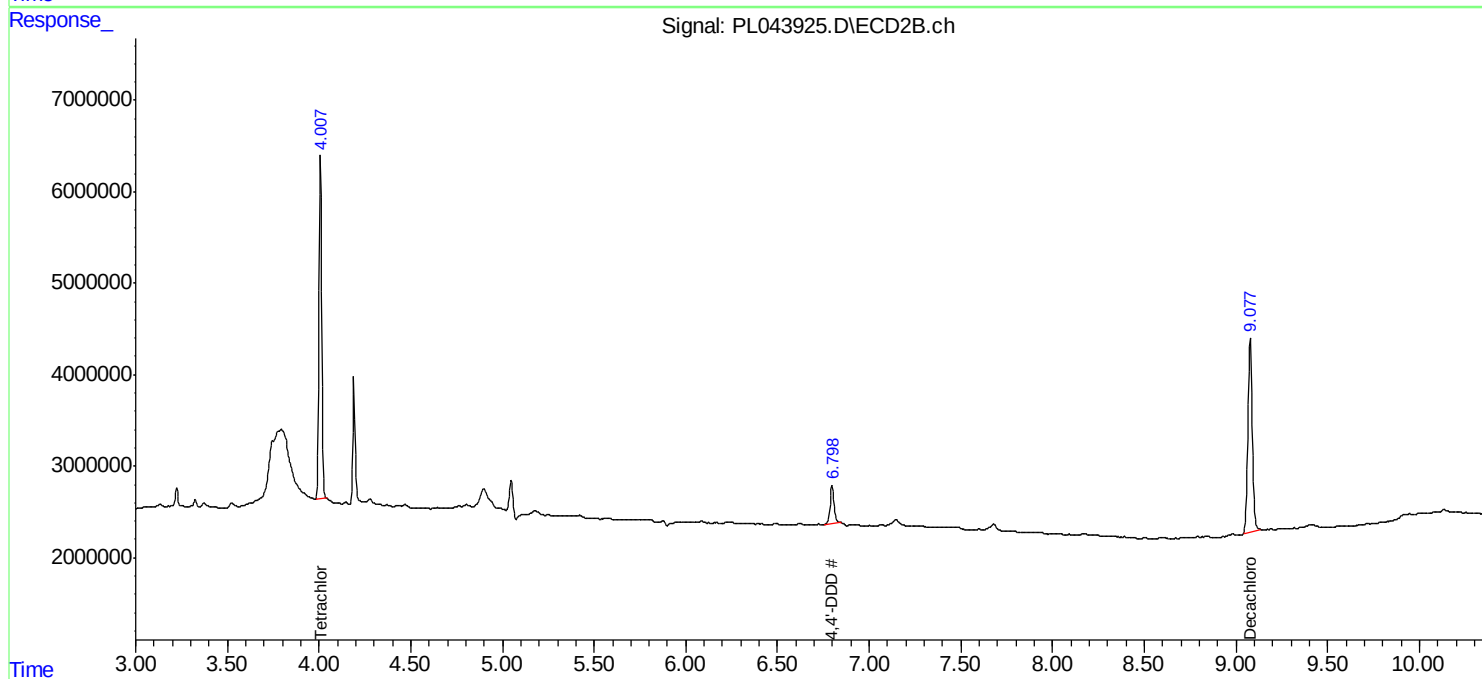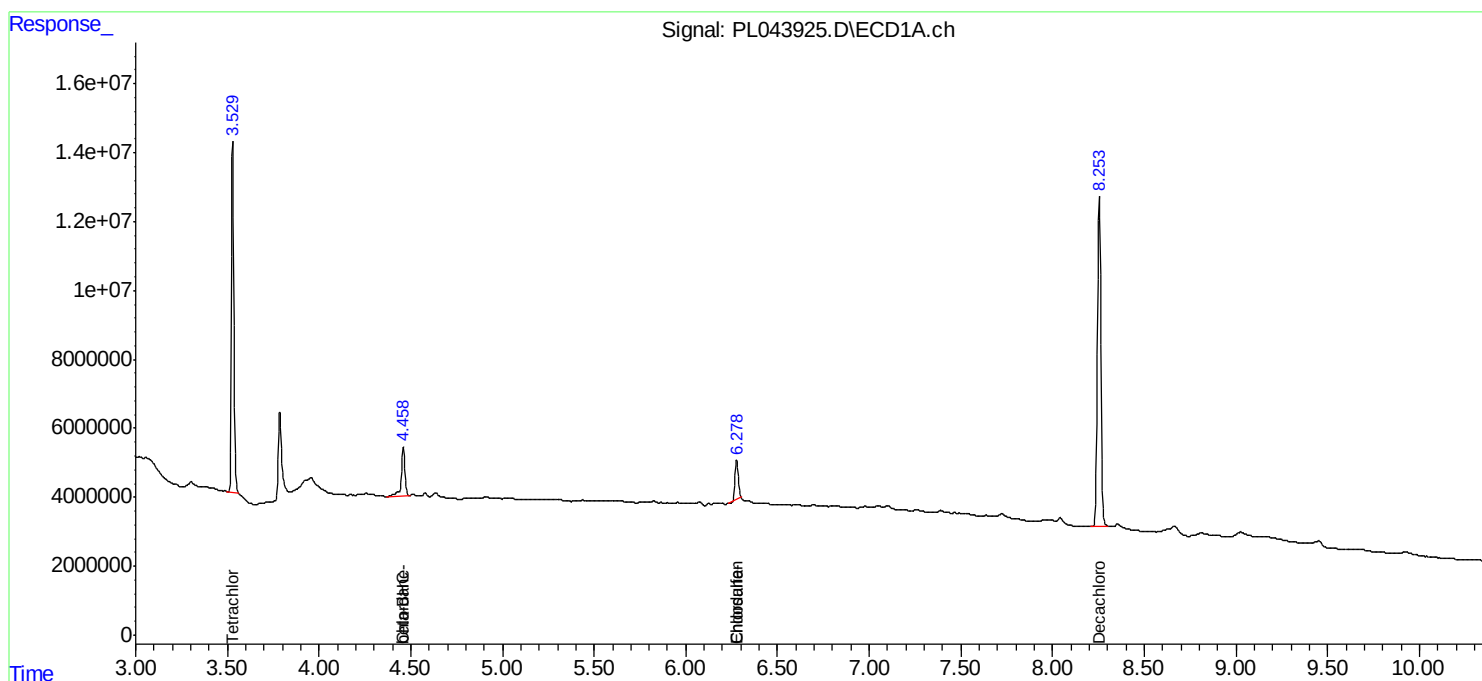


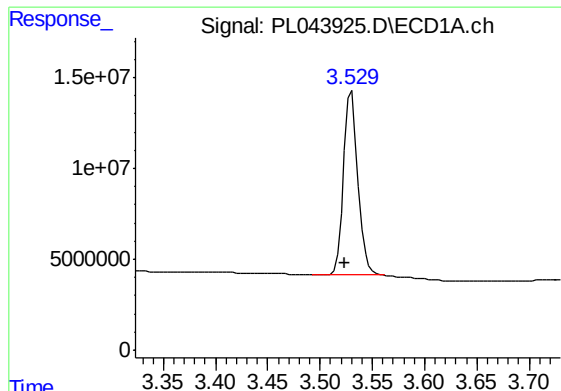

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.007 min
Response: 97747606
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

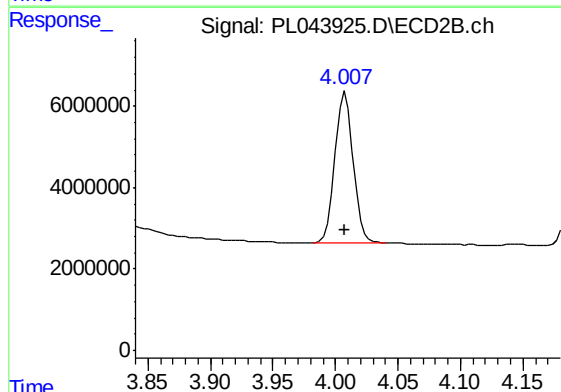


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 37707564
Conc: 19.35 ng/ml

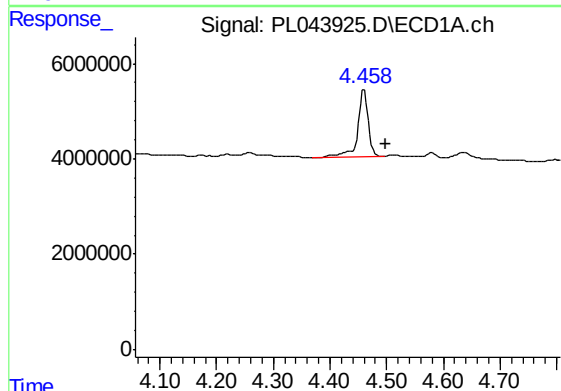


#6 beta-BHC

R.T.: 4.460 min
Delta R.T.: -0.038 min
Response: 18253849
Conc: 6.13 ng/ml

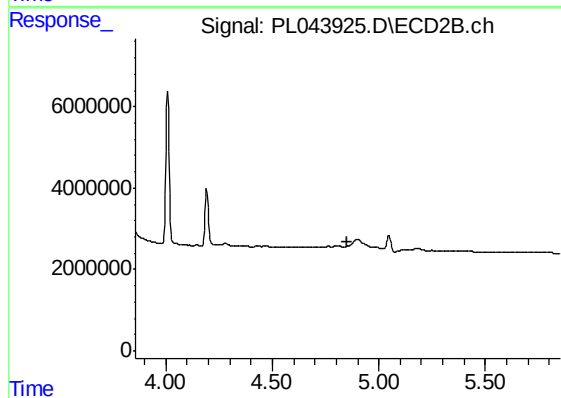

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

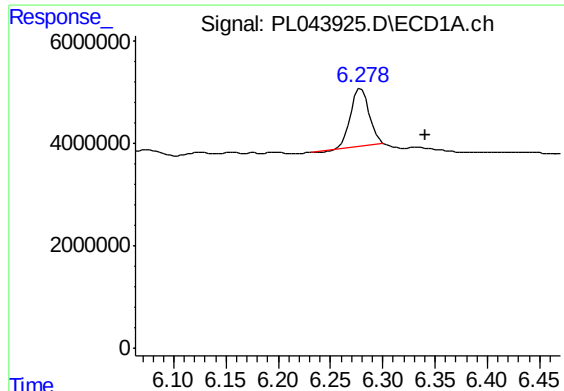

#15 Endosulfan II


R.T.: 6.279 min
Delta R.T.: -0.061 min
Response: 13805855
Conc: 2.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

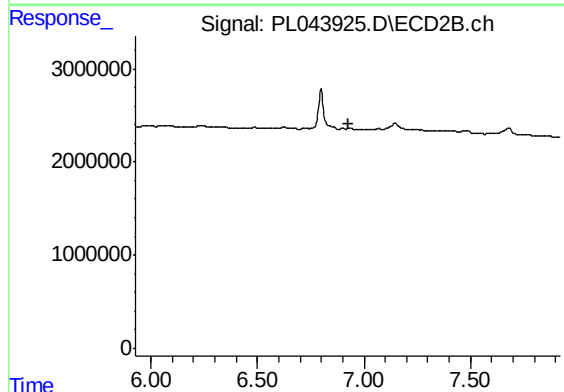


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

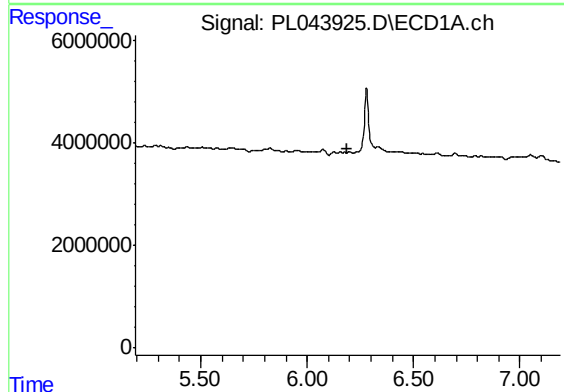


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

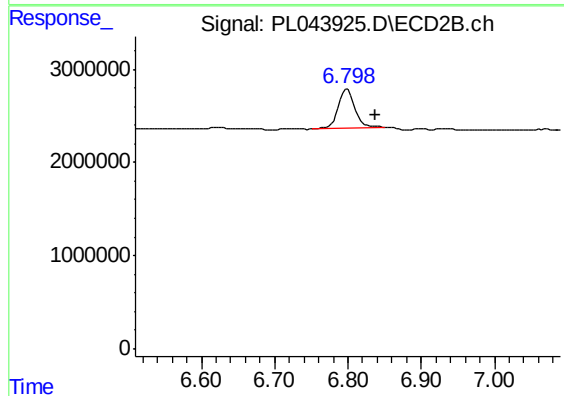

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: -0.039 min
Response: 6469011
Conc: 4.28 ng/ml

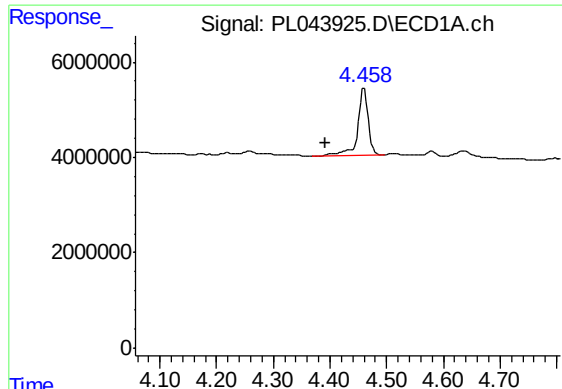

#23 Chlordane-1


R.T.: 4.460 min
Delta R.T.: 0.068 min
Response: 18253849
Conc: 81.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

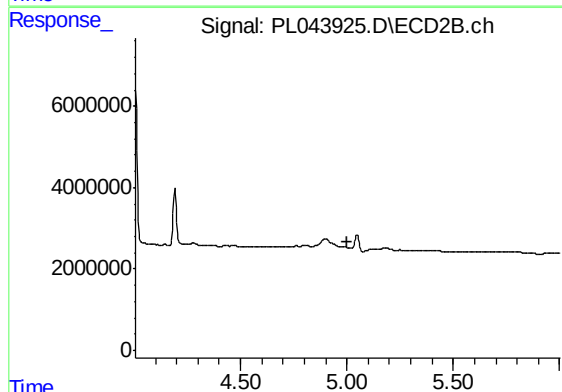


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

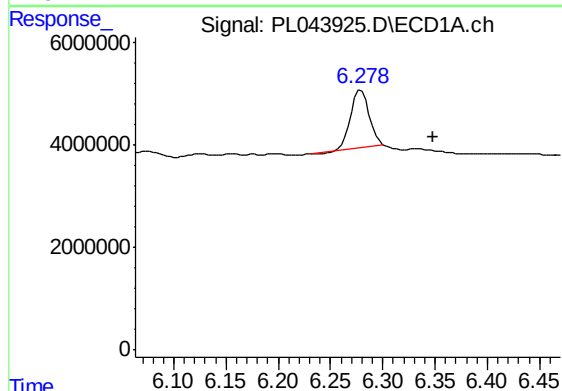


#27 Chlordane-5

R.T.: 6.279 min
Delta R.T.: -0.069 min
Response: 13805855
Conc: 69.29 ng/ml

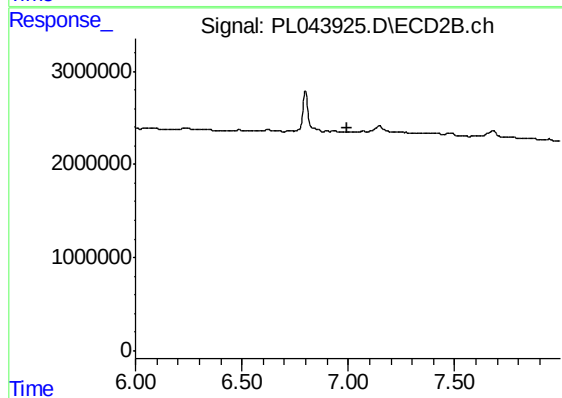

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

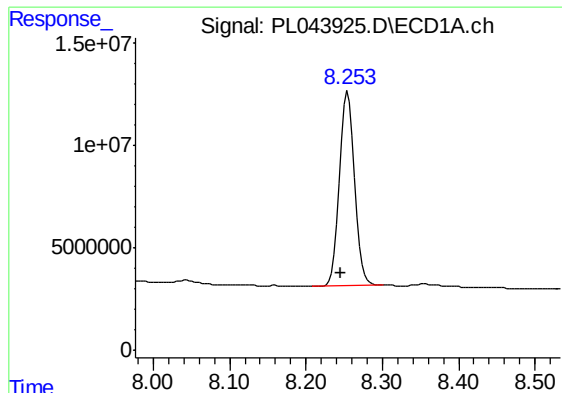

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.009 min
Response: 129641015
Conc: 22.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

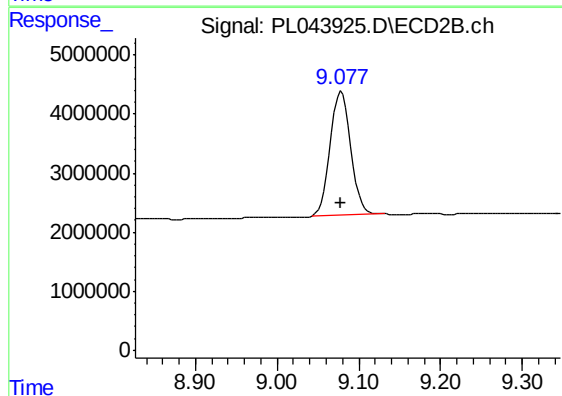

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.000 min
Response: 37183587
Conc: 23.41 ng/ml