

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 23:17
 Operator : AJ\SJ
 Sample : K1139-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:12:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.008	99190871	38213211	20.206	19.608
28)	SA Decachlor...	8.255	9.079	137.6E6	38776240	24.343	24.410
Target Compounds							
6)	B beta-BHC	4.460f	0.000	18822858	0	6.323	N.D. #
15)	B Endosulfa...	6.279f	0.000	12912516	0	2.482	N.D. #
23)	Chlordane-1	4.460	0.000	18822858	0	84.149	N.D. #
27)	Chlordane-5	6.279	0.000	12912516	0	64.803	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 23:17
Operator : AJ\SJ
Sample : K1139-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:12:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

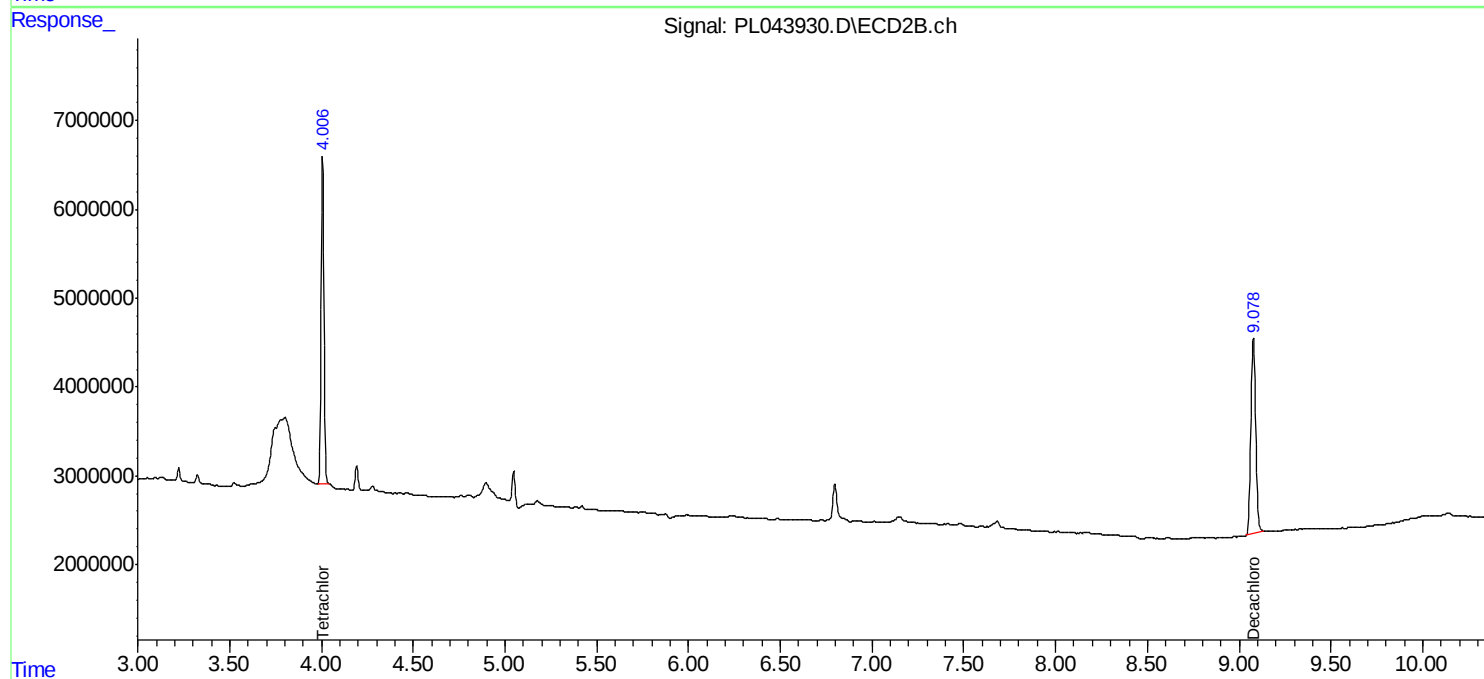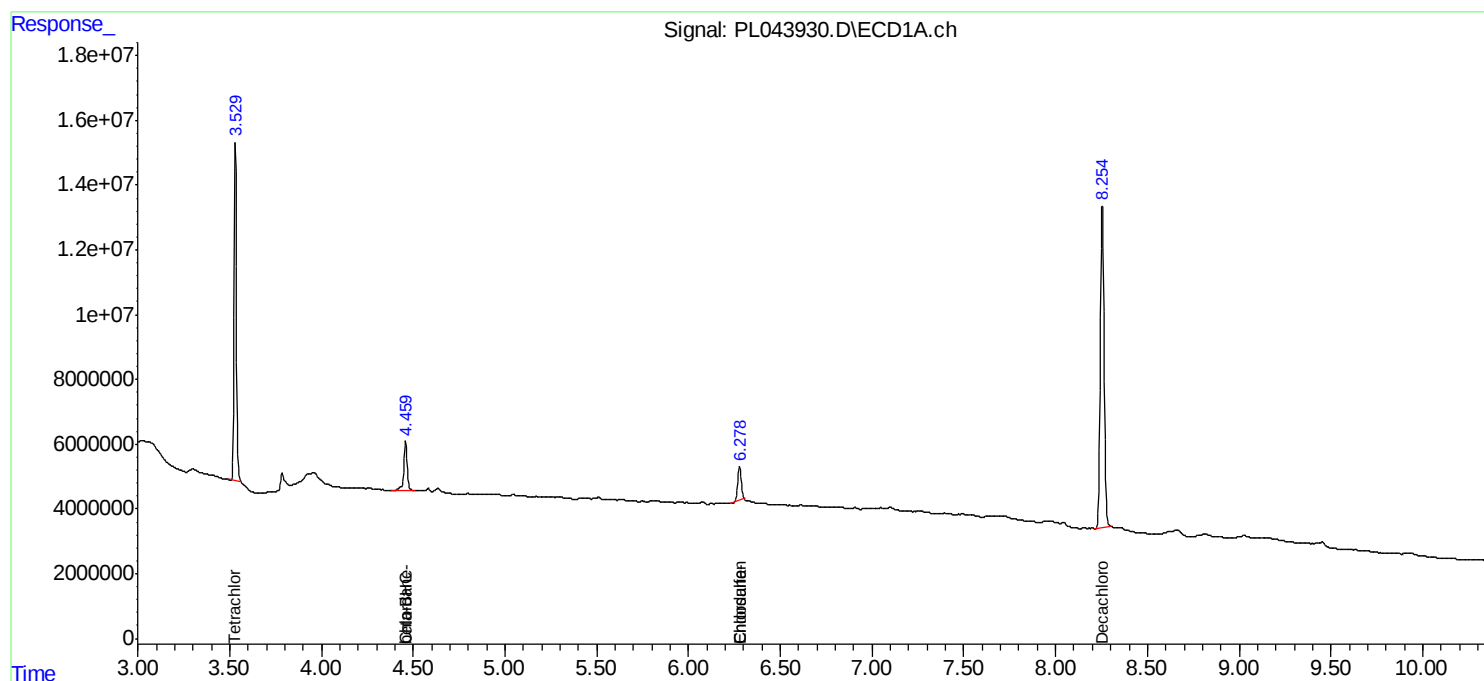


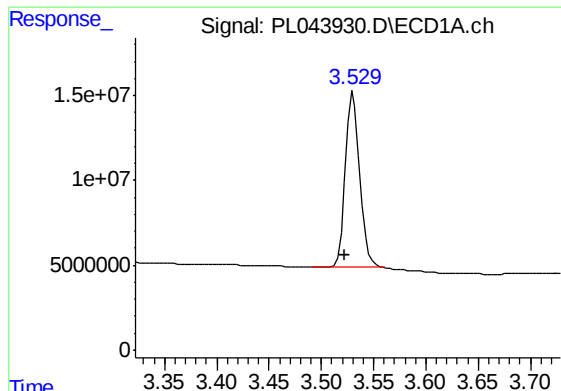

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.008 min
Response: 99190871
Conc: 20.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-7

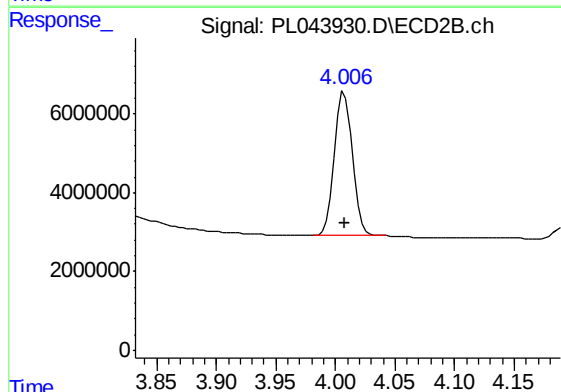


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 38213211
Conc: 19.61 ng/ml

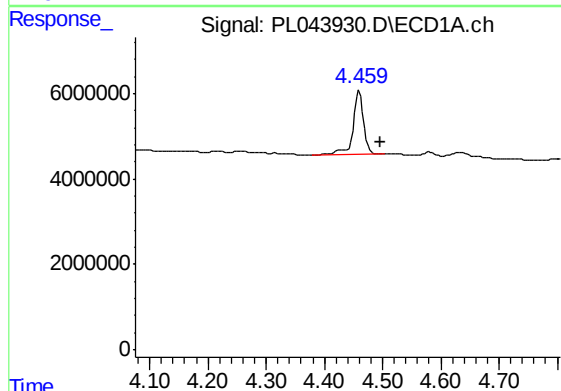


#6 beta-BHC

R.T.: 4.460 min
Delta R.T.: -0.038 min
Response: 18822858
Conc: 6.32 ng/ml

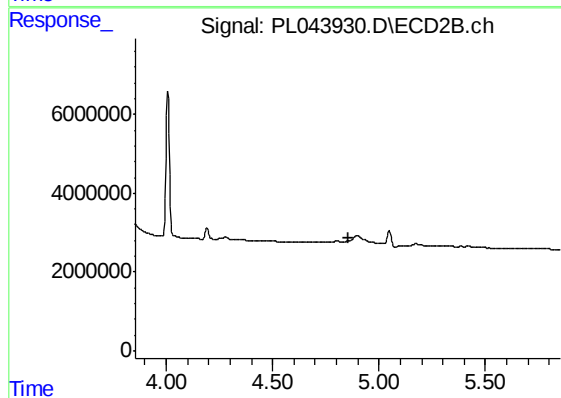

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

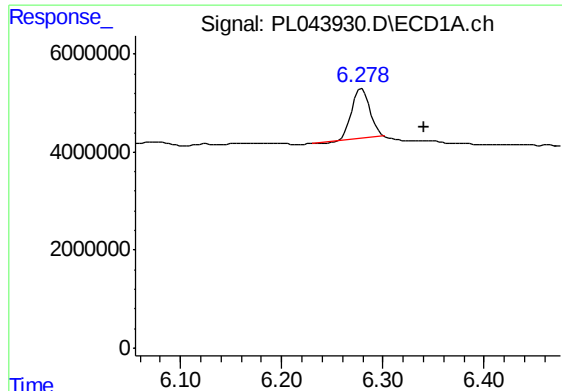

#15 Endosulfan II


R.T.: 6.279 min
Delta R.T.: -0.061 min
Response: 12912516
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-7

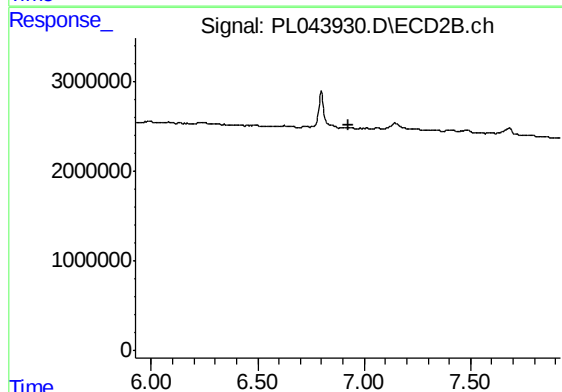


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

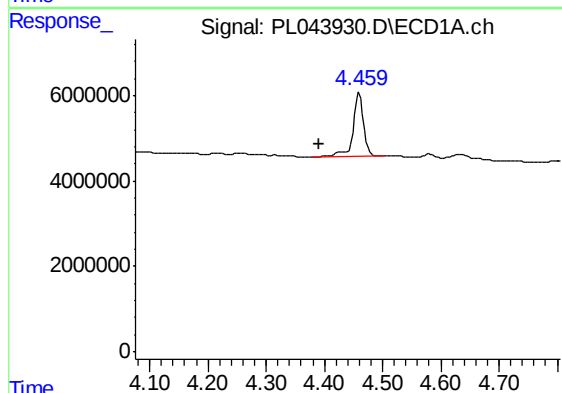


#23 Chlordane-1

R.T.: 4.460 min
Delta R.T.: 0.069 min
Response: 18822858
Conc: 84.15 ng/ml

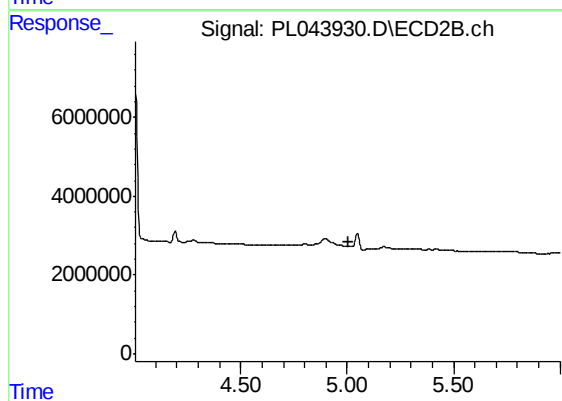

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

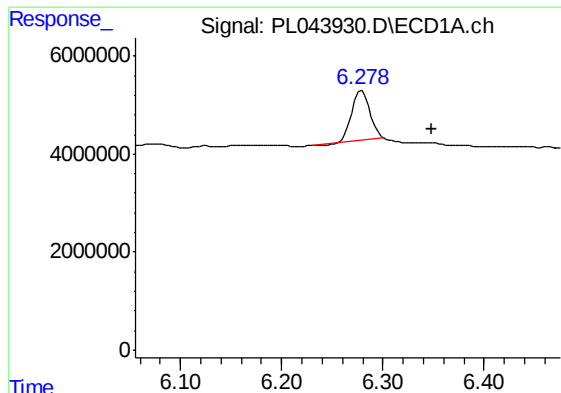

#27 Chlordane-5


R.T.: 6.279 min
Delta R.T.: -0.069 min
Response: 12912516
Conc: 64.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-7

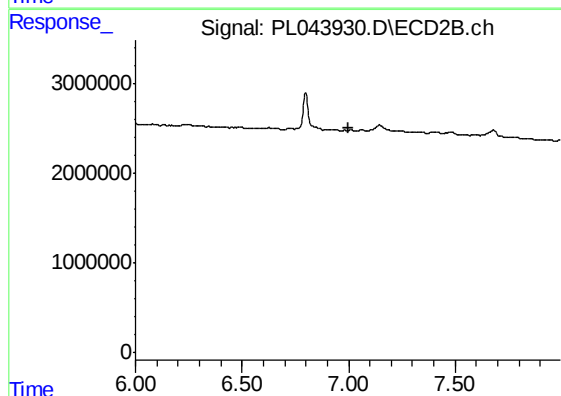


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

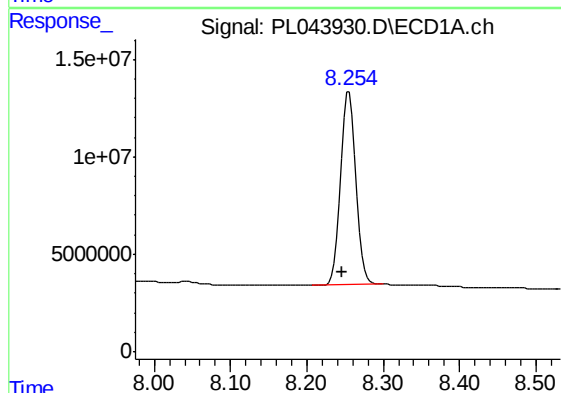

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.009 min
Response: 137570450
Conc: 24.34 ng/ml

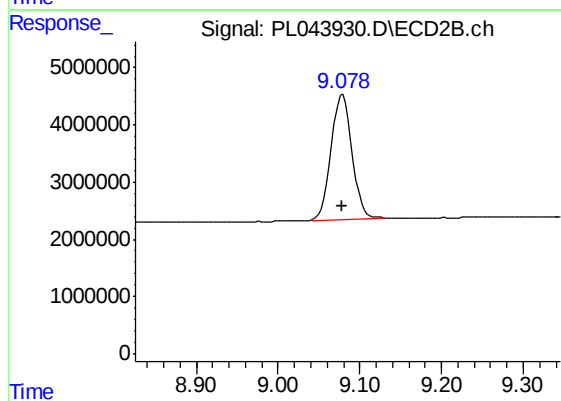

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.001 min
Response: 38776240
Conc: 24.41 ng/ml