

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
 Data File : PL043932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2019 23:45
 Operator : AJ\SJ
 Sample : K1139-18
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 02:12:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.008	98754564	37890741	20.118	19.443
28)	SA Decachlor...	8.255	9.079	134.4E6	38393059	23.785	24.168
Target Compounds							
6)	B beta-BHC	4.460f	0.000	9628707	0	3.234	N.D. #
15)	B Endosulfa...	6.280f	0.000	12351657	0	2.374	N.D. #
16)	A 4,4'-DDD	0.000	6.799f	0	6830274	N.D.	4.520 #
23)	Chlordane-1	4.460	0.000	9628707	0	43.046	N.D. #
27)	Chlordane-5	6.280	0.000	12351657	0	61.988	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011519\
Data File : PL043932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2019 23:45
Operator : AJ\SJ
Sample : K1139-18
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 02:12:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

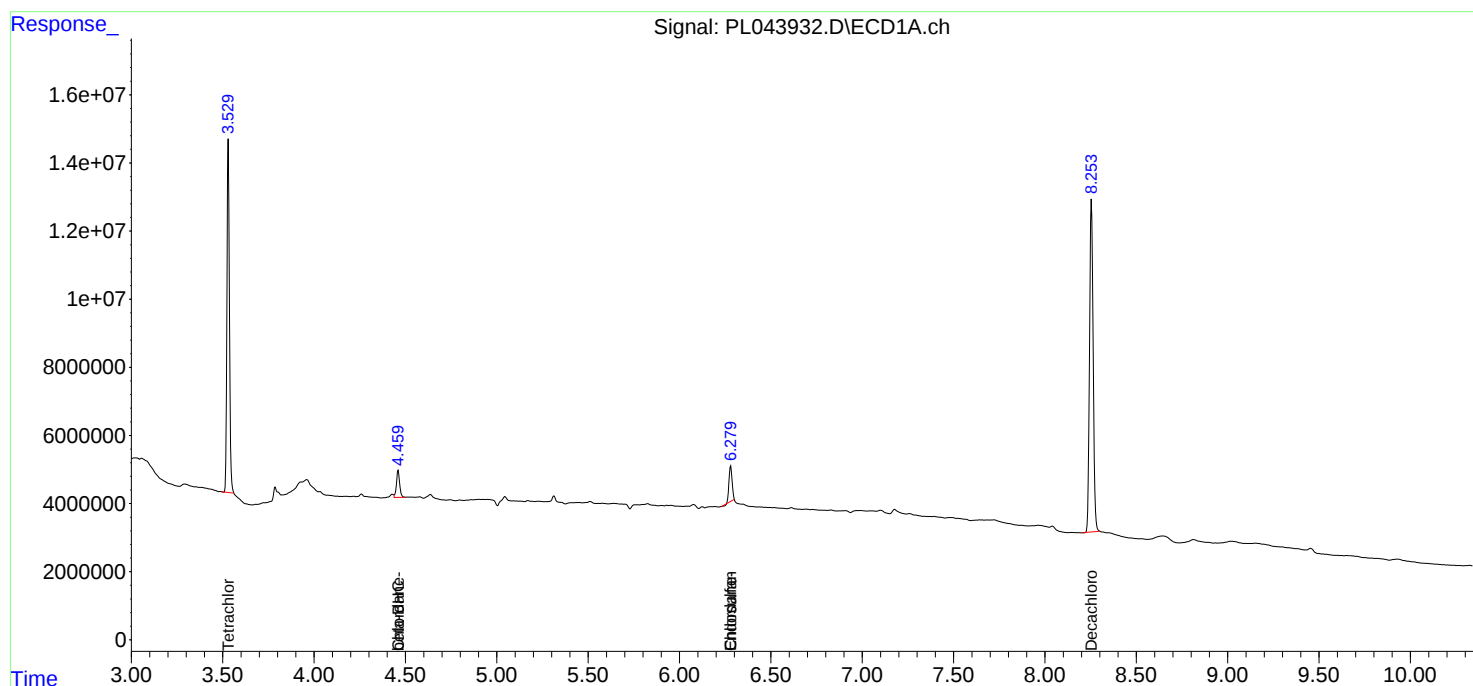


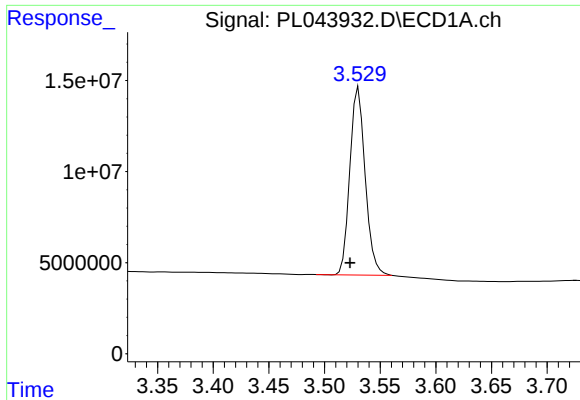

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.008 min
Response: 98754564
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

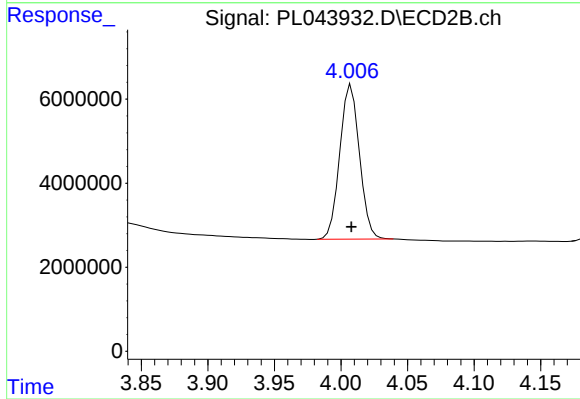


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 37890741
Conc: 19.44 ng/ml

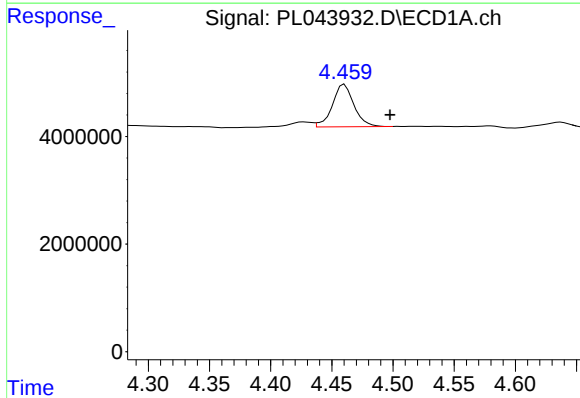


#6 beta-BHC

R.T.: 4.460 min
Delta R.T.: -0.037 min
Response: 9628707
Conc: 3.23 ng/ml

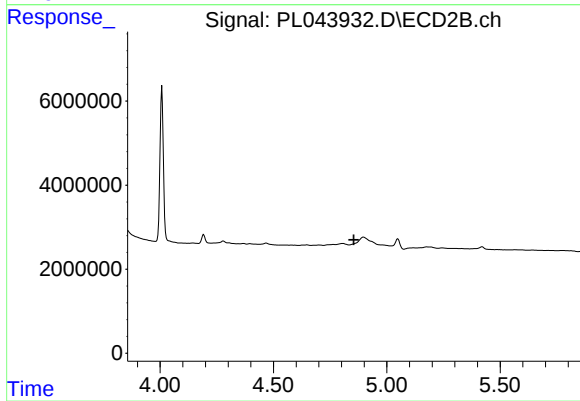

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.855 min
Response: 0
Conc: N.D.

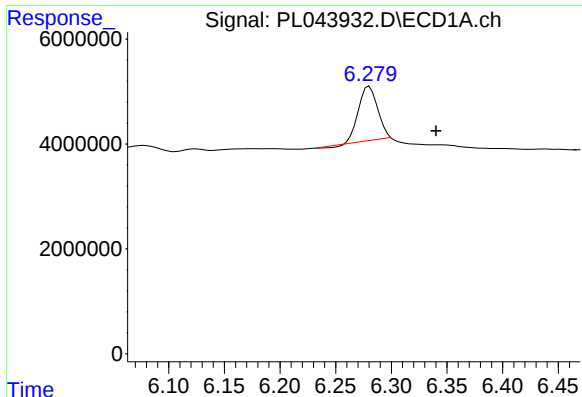

#15 Endosulfan II


R.T.: 6.280 min
Delta R.T.: -0.060 min
Response: 12351657
Conc: 2.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

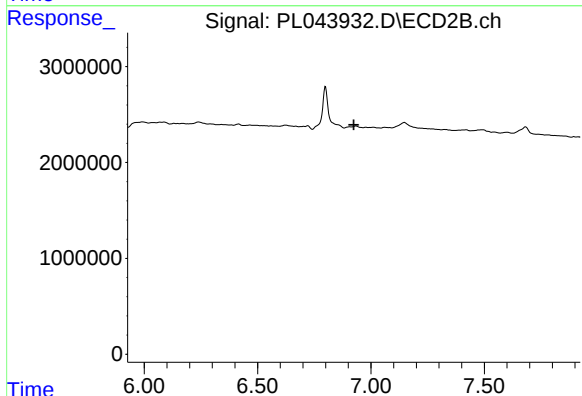


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

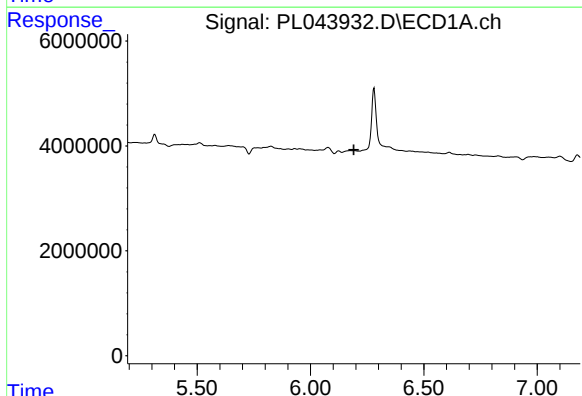


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

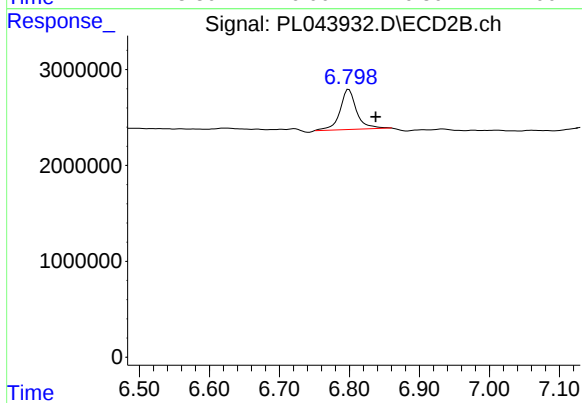

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: -0.038 min
Response: 6830274
Conc: 4.52 ng/ml

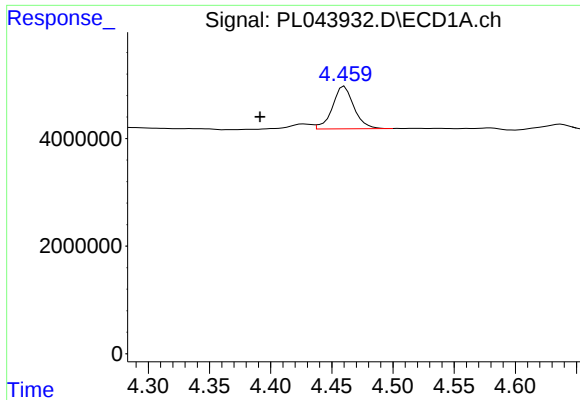

#23 Chlordane-1


R.T.: 4.460 min
Delta R.T.: 0.069 min
Response: 9628707
Conc: 43.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

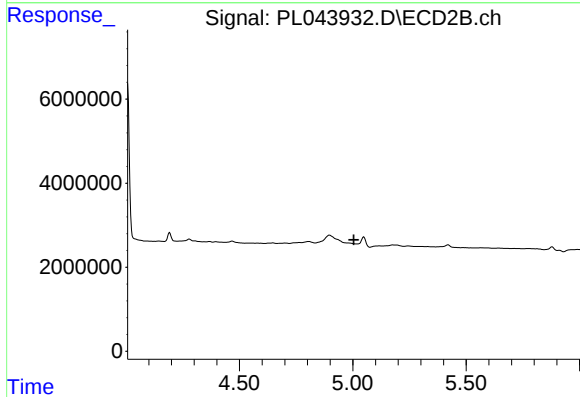


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

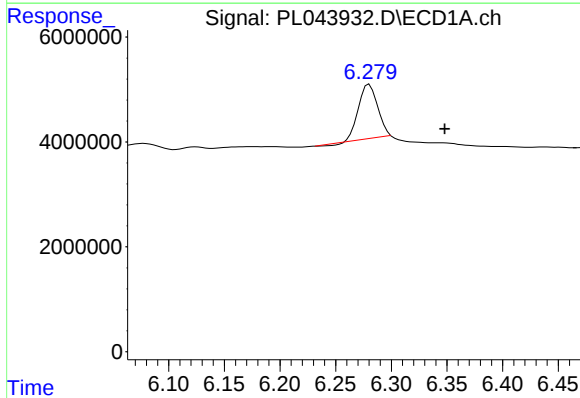


#27 Chlordane-5

R.T.: 6.280 min
Delta R.T.: -0.068 min
Response: 12351657
Conc: 61.99 ng/ml

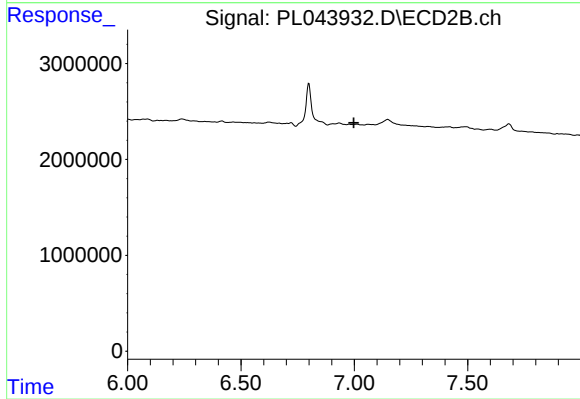

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

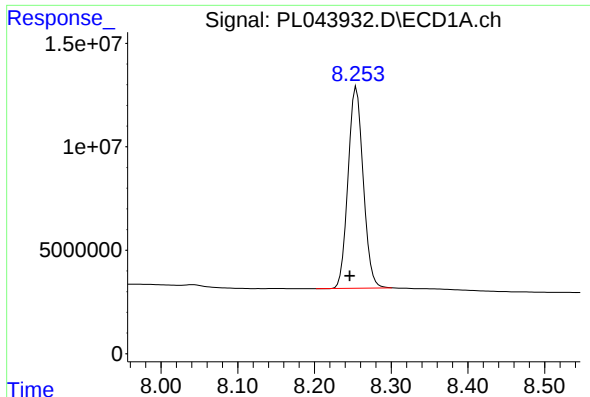

#28 Decachlorobiphenyl


R.T.: 8.255 min

Delta R.T.: 0.008 min

Response: 134413229

Conc: 23.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

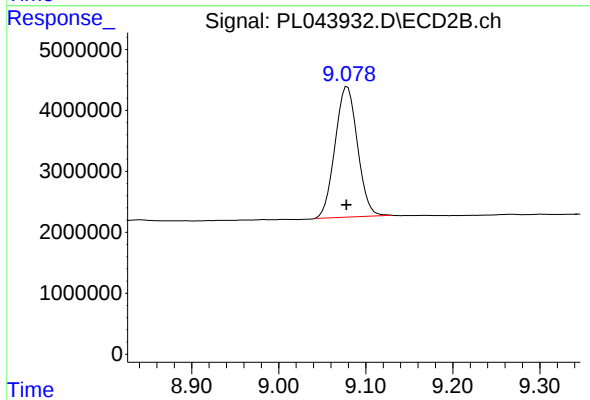

#28 Decachlorobiphenyl

R.T.: 9.079 min

Delta R.T.: 0.001 min

Response: 38393059

Conc: 24.17 ng/ml