

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011520\
 Data File : PL055763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2020 15:30
 Operator : AJ\MA
 Sample : L1125-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FESB-34-(4.5-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 00:36:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.968	212.2E6	65260213	22.964	24.635
28)	SA Decachlor...	8.238	8.959	175.4E6	42501883	19.975	20.443
Target Compounds							
9)	A Endosulfan I	5.566f	0.000	66238962	0	5.361	N.D. #
10)	B gamma-Chl...	0.000	6.035	0	9995961	N.D.	3.551 #
13)	MA Dieldrin	5.786	0.000	37053210	0	2.827	N.D. #
15)	B Endosulfa...	6.316	0.000	13189021	0	1.223	N.D. #
18)	B Endrin al...	0.000	6.939f	0	12256623	N.D.	6.036 #
21)	B Endrin ke...	0.000	7.675f	0	6345137	N.D.	2.665 #
25)	Chlordane-3	0.000	6.035	0	9995961	N.D.	29.269 #
27)	Chlordane-5	6.316	6.939f	13189021	12256623	36.638	174.623 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011520\
Data File : PL055763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2020 15:30
Operator : AJ\MA
Sample : L1125-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 00:36:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

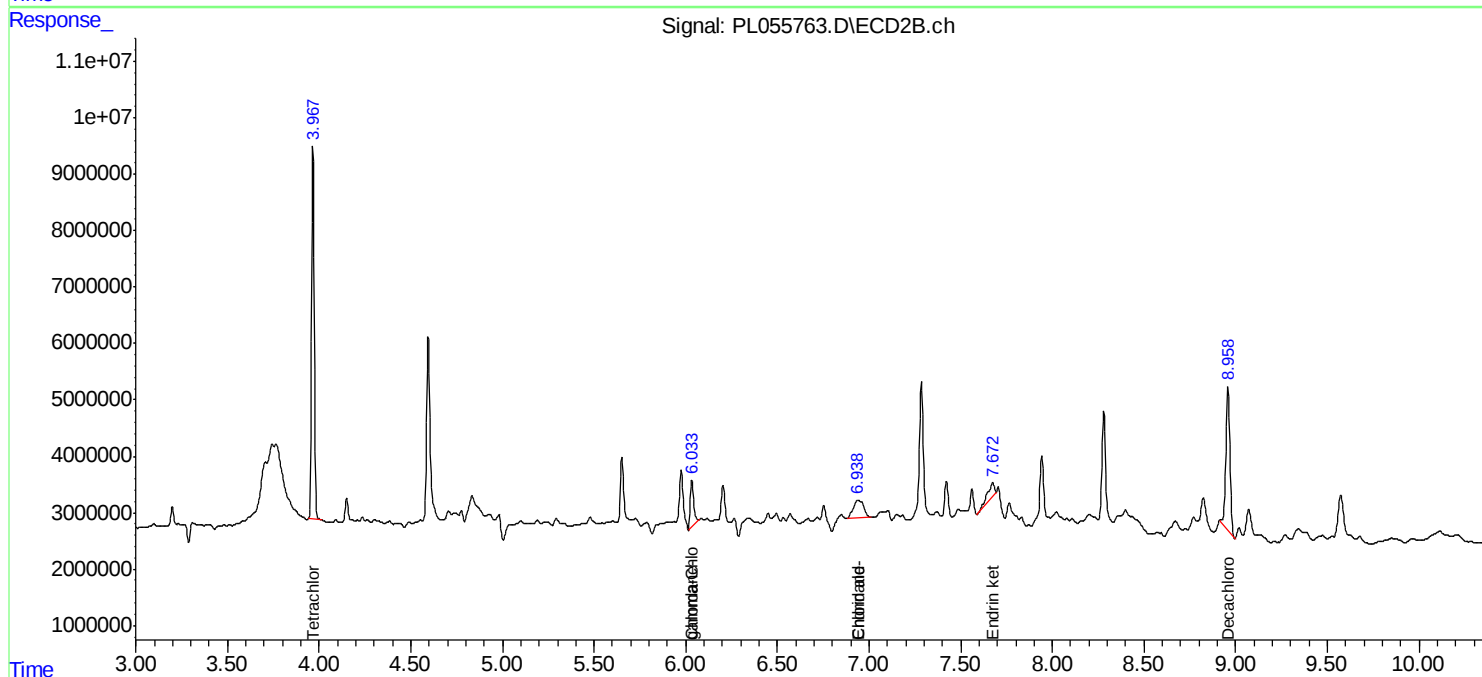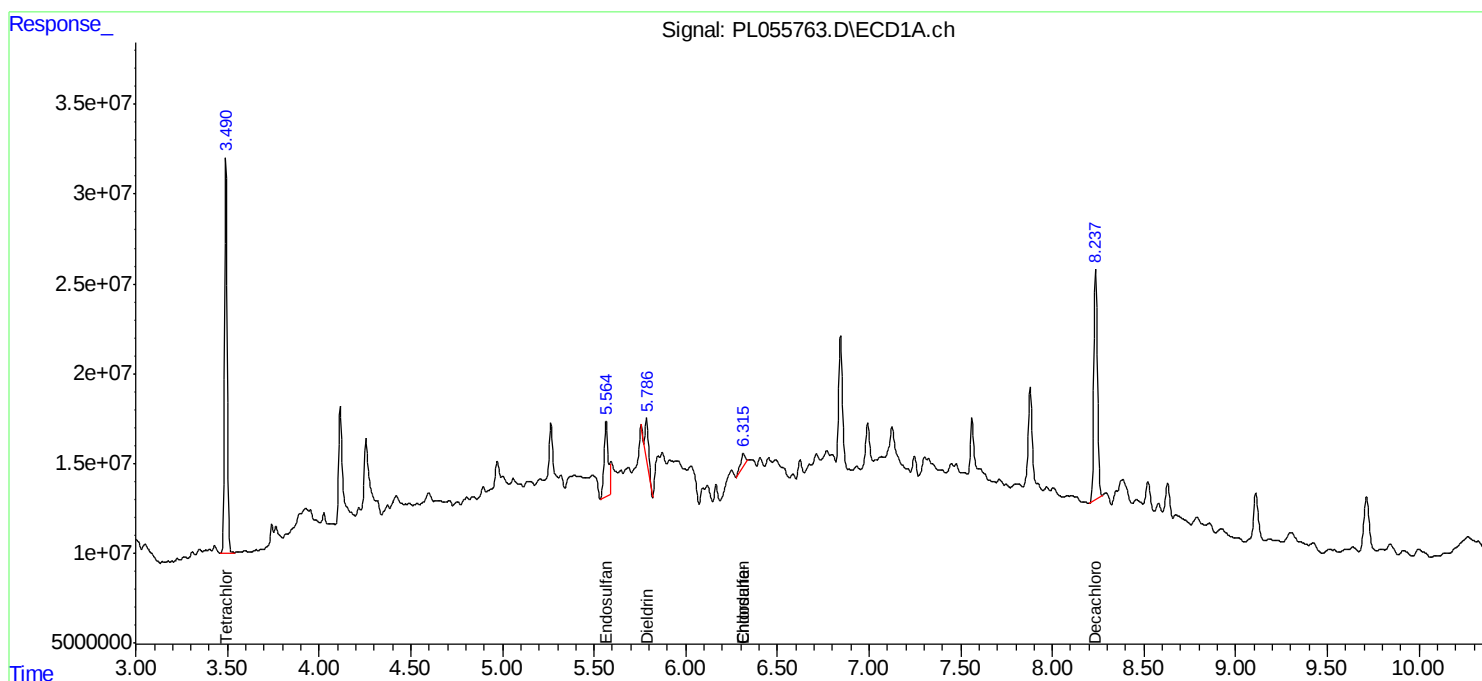


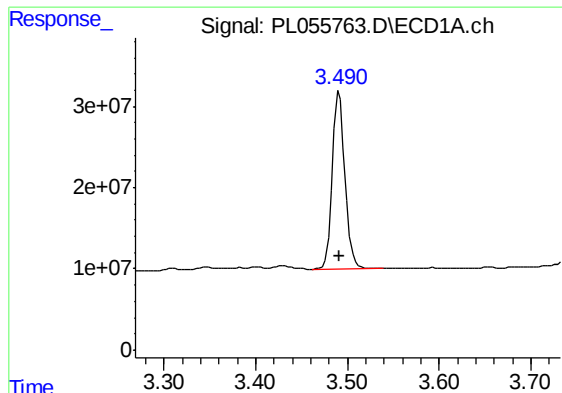

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 212200302
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

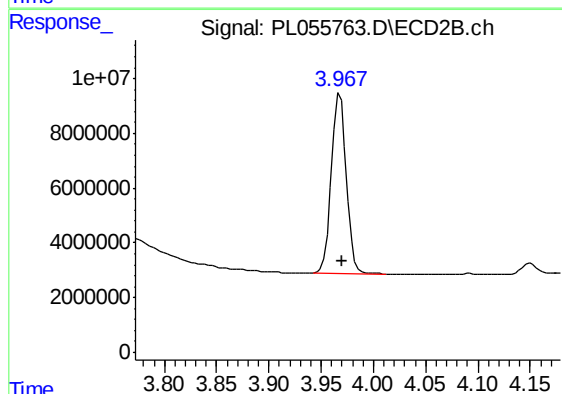


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 65260213
Conc: 24.63 ng/ml

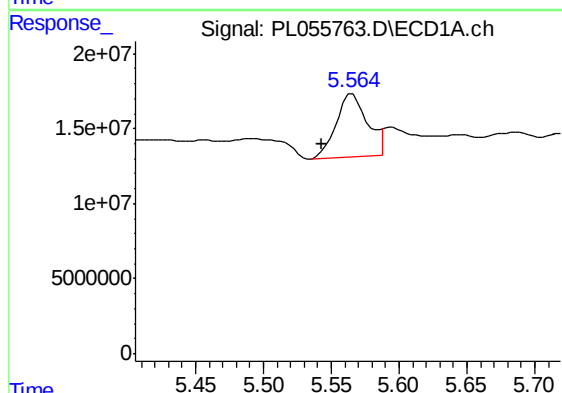


#9 Endosulfan I

R.T.: 5.566 min
Delta R.T.: 0.022 min
Response: 66238962
Conc: 5.36 ng/ml

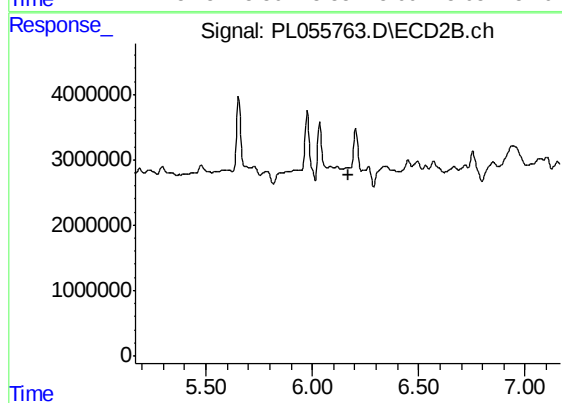

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

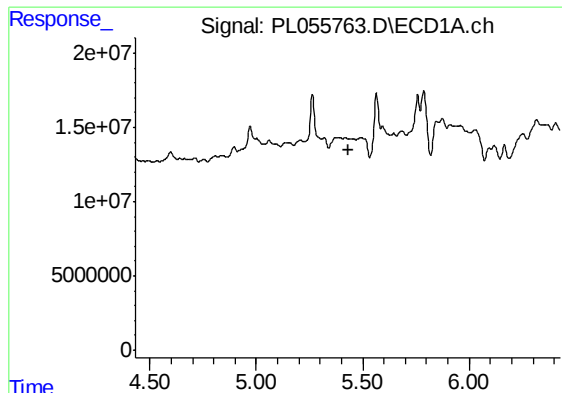

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

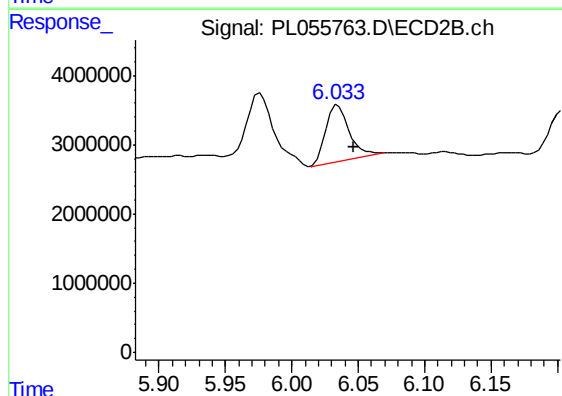


#10 gamma-Chlordane

R.T.: 6.035 min
Delta R.T.: -0.012 min
Response: 9995961
Conc: 3.55 ng/ml

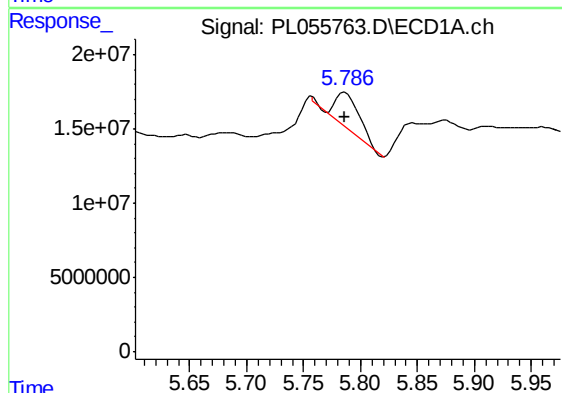


#13 Dieldrin

R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 37053210
Conc: 2.83 ng/ml

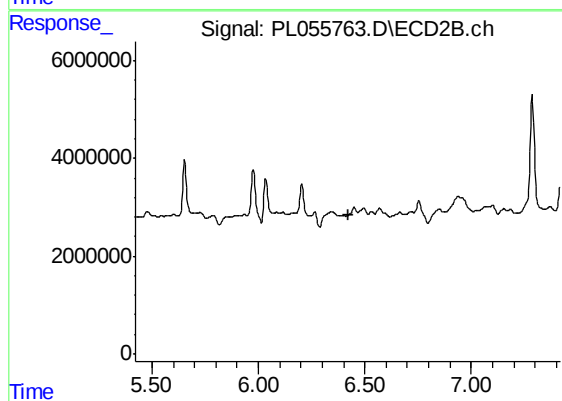

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.422 min
Response: 0
Conc: N.D.

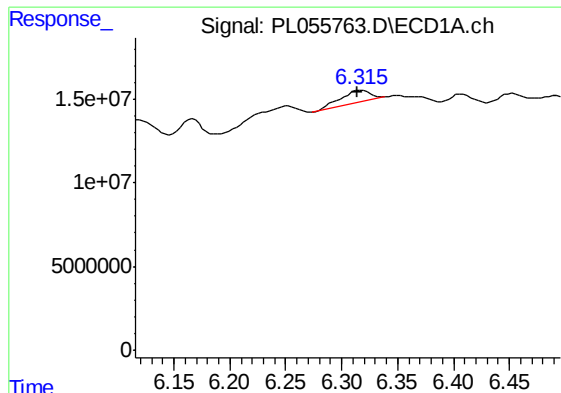

#15 Endosulfan II


R.T.: 6.316 min
Delta R.T.: 0.002 min
Response: 13189021
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

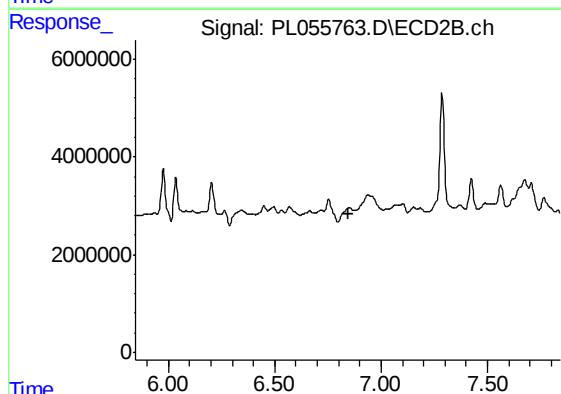


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.845 min
Response: 0
Conc: N.D.

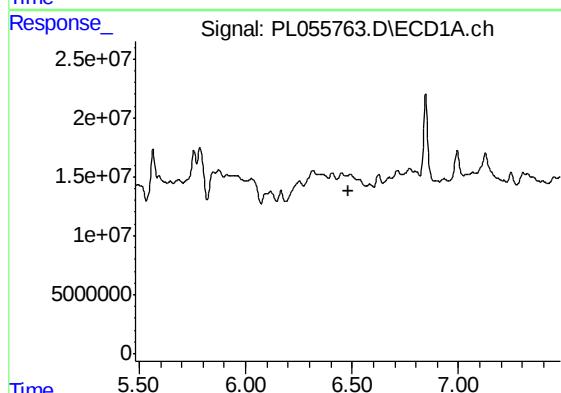


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.482 min
Response: 0
Conc: N.D.

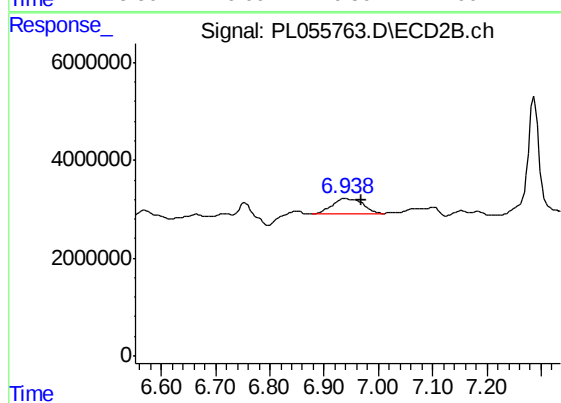

#18 Endrin aldehyde


R.T.: 6.939 min
Delta R.T.: -0.029 min
Response: 12256623
Conc: 6.04 ng/ml

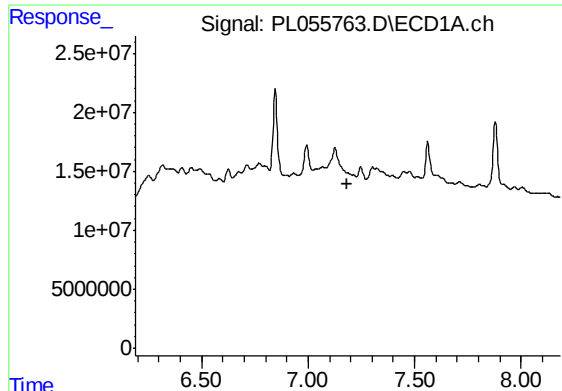

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

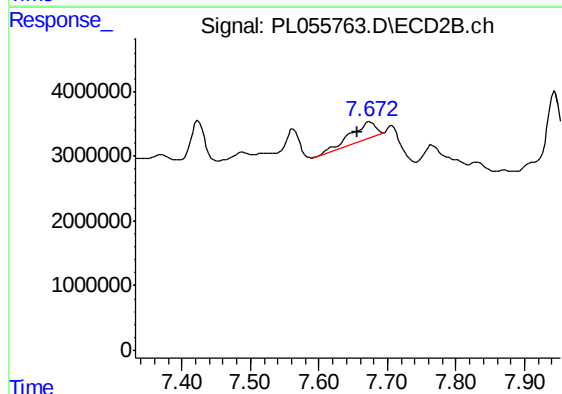


#21 Endrin ketone

R.T.: 7.675 min
Delta R.T.: 0.018 min
Response: 6345137
Conc: 2.66 ng/ml

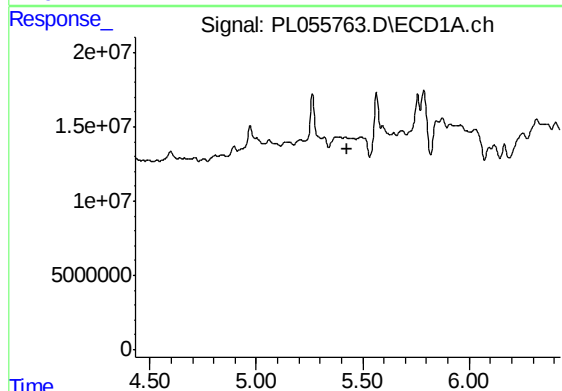


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.430 min
Response: 0
Conc: N.D.

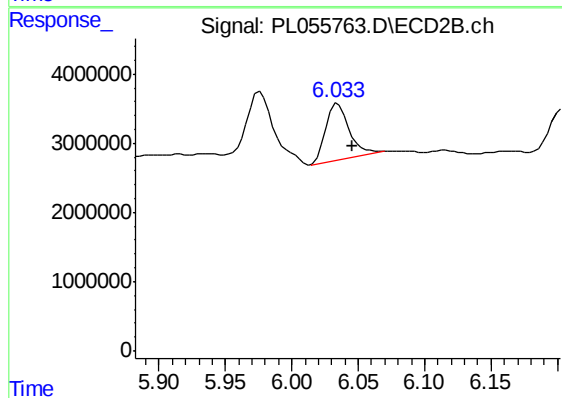

#25 Chlordane-3


R.T.: 6.035 min
Delta R.T.: -0.011 min
Response: 9995961
Conc: 29.27 ng/ml

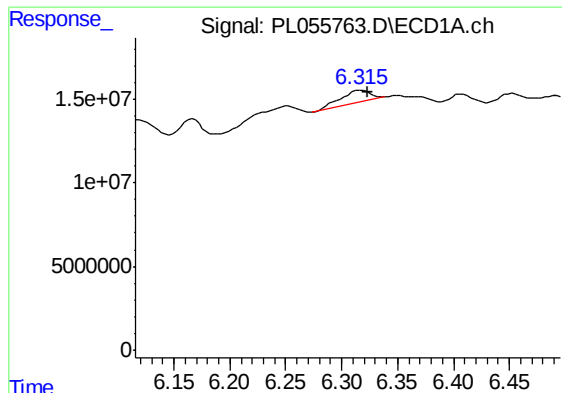

#27 Chlordane-5


R.T.: 6.316 min
Delta R.T.: -0.007 min
Response: 13189021
Conc: 36.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
FESB-34-(4.5-5)

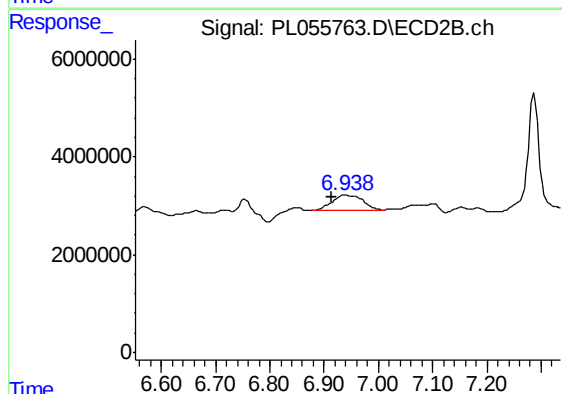


#27 Chlordane-5

R.T.: 6.939 min
Delta R.T.: 0.024 min
Response: 12256623
Conc: 174.62 ng/ml

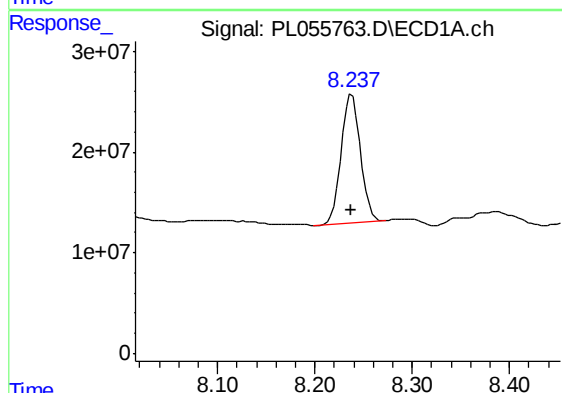

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 175415544
Conc: 19.98 ng/ml

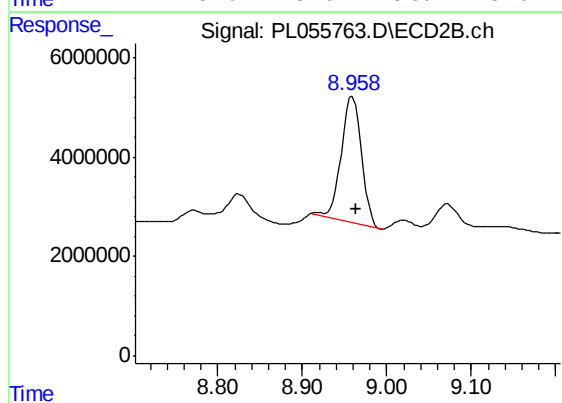

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.004 min
Response: 42501883
Conc: 20.44 ng/ml