

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011619\
 Data File : PL043936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2019 12:22
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 00:13:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.008	117.6E6	45012439	23.962	23.097
28)	SA Decachlor...	8.256	9.079	140.1E6	39249593	24.784	24.708
Target Compounds							
6)	B beta-BHC	4.460f	0.000	9286488	0	3.120	N.D. #
8)	B Heptachlo...	5.161f	0.000	3325580	0	0.523	N.D. #
15)	B Endosulfa...	6.282f	0.000	21435876	0	4.120	N.D. #
16)	A 4,4'-DDD	0.000	6.799f	0	10331291	N.D.	6.837 #
23)	Chlordane-1	4.460	0.000	9286488	0	41.516	N.D. #
27)	Chlordane-5	6.282	0.000	21435876	0	107.579	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011619\
Data File : PL043936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2019 12:22
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 00:13:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

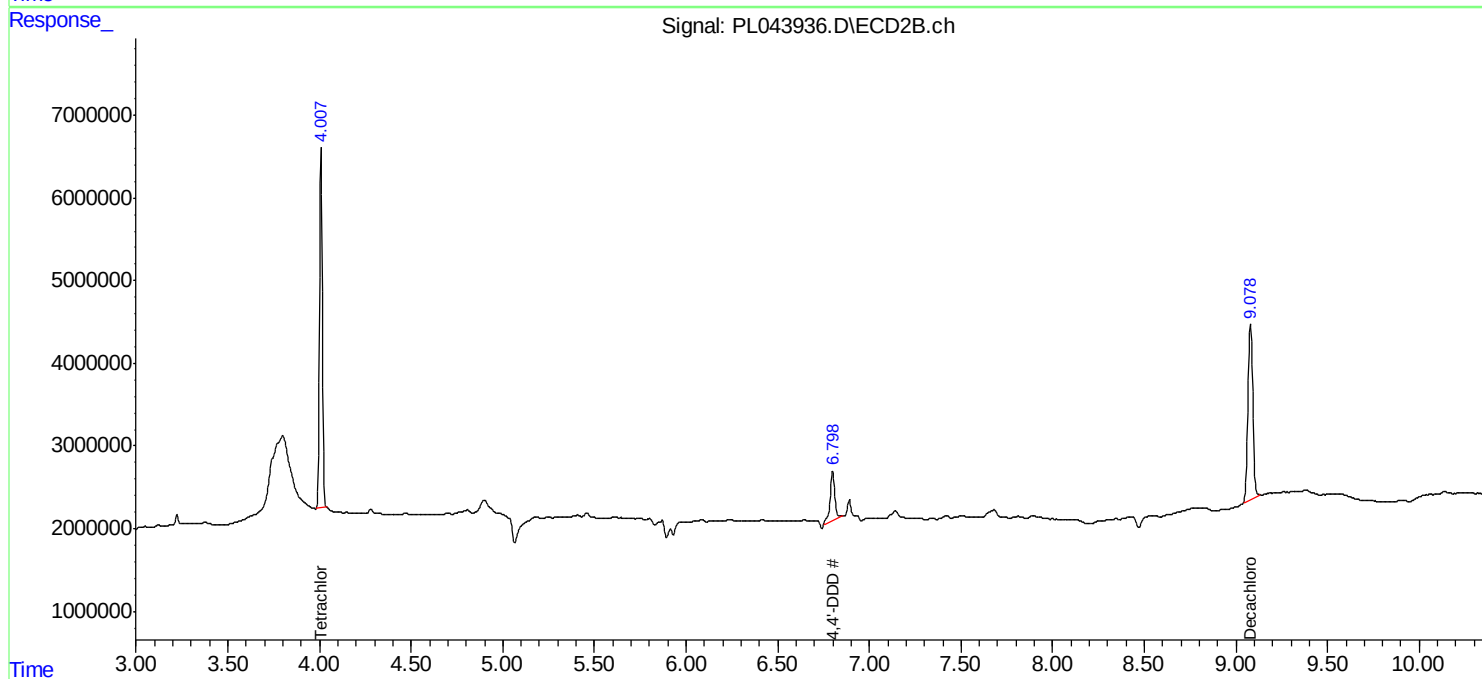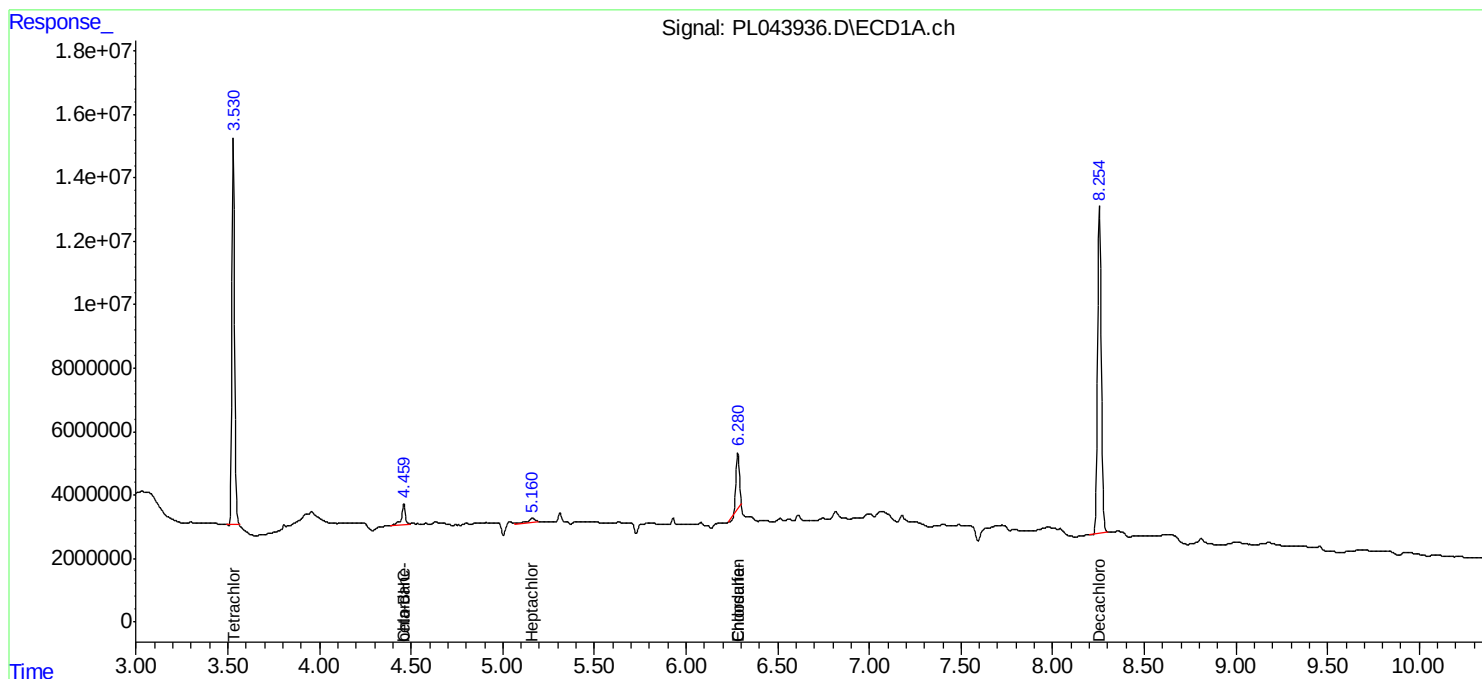


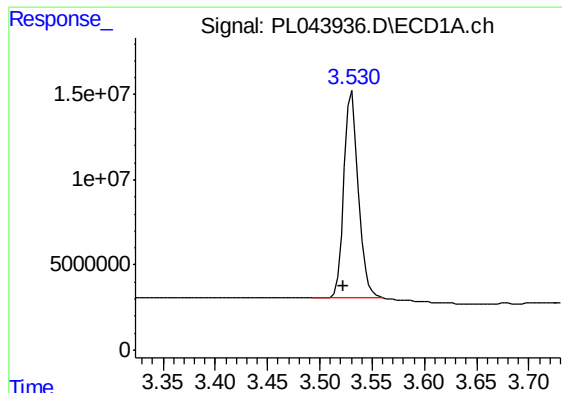

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.008 min
Response: 117627913
Conc: 23.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

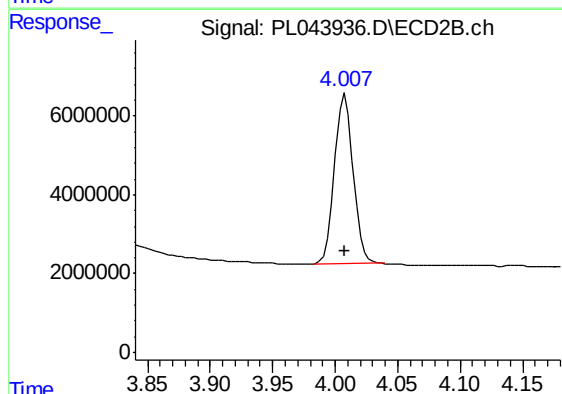


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 45012439
Conc: 23.10 ng/ml

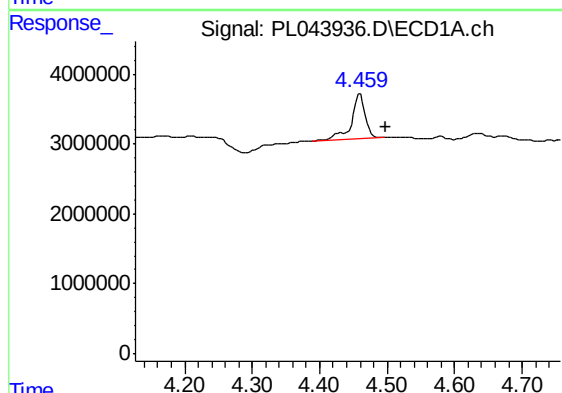


#6 beta-BHC

R.T.: 4.460 min
Delta R.T.: -0.037 min
Response: 9286488
Conc: 3.12 ng/ml

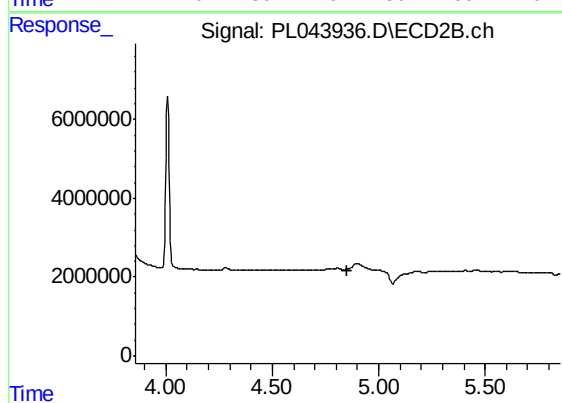

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

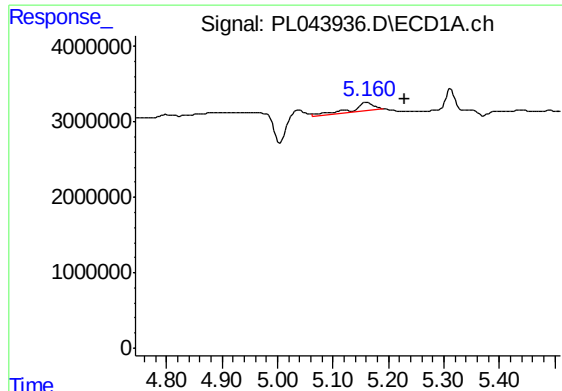

#8 Heptachlor epoxide


R.T.: 5.161 min
Delta R.T.: -0.069 min
Response: 3325580
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

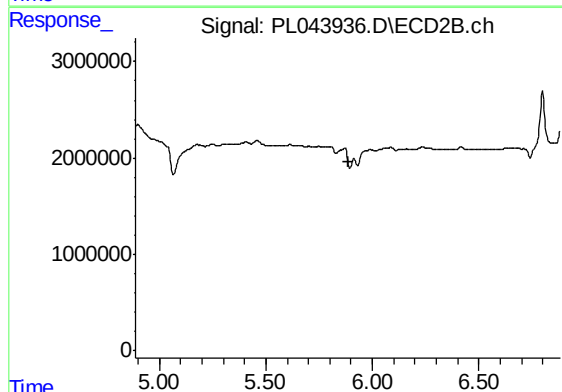


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.885 min
Response: 0
Conc: N.D.

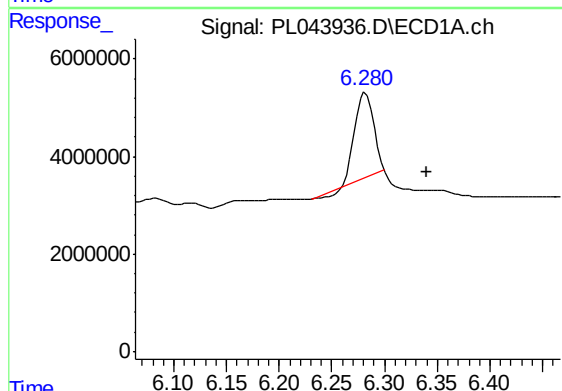


#15 Endosulfan II

R.T.: 6.282 min
Delta R.T.: -0.058 min
Response: 21435876
Conc: 4.12 ng/ml

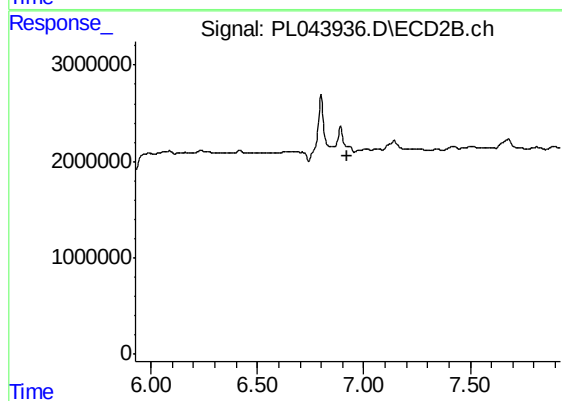

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

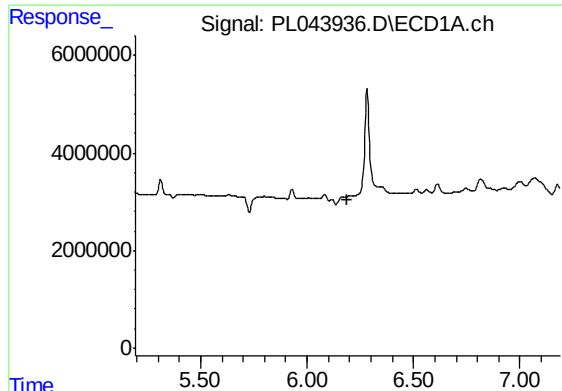

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

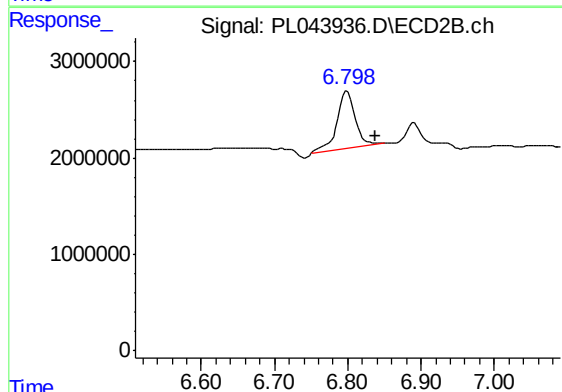


#16 4,4'-DDD

R.T.: 6.799 min
Delta R.T.: -0.039 min
Response: 10331291
Conc: 6.84 ng/ml

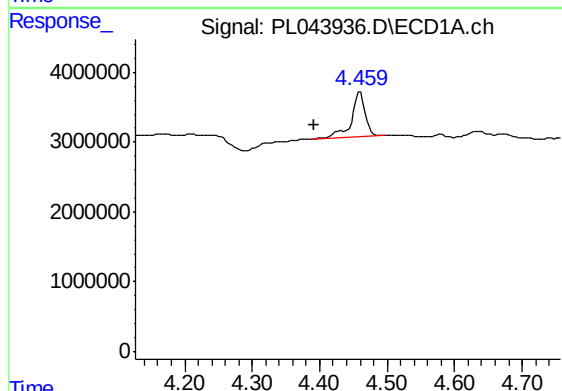


#23 Chlordane-1

R.T.: 4.460 min
Delta R.T.: 0.069 min
Response: 9286488
Conc: 41.52 ng/ml

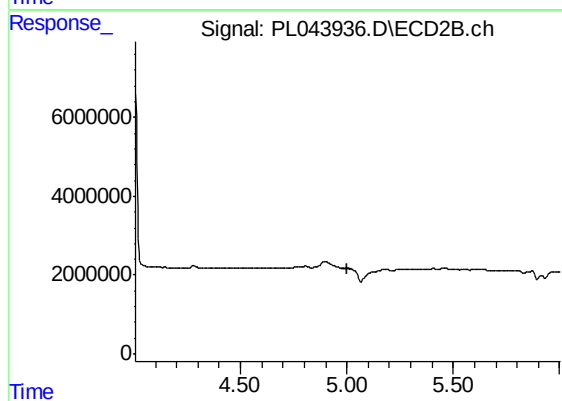

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

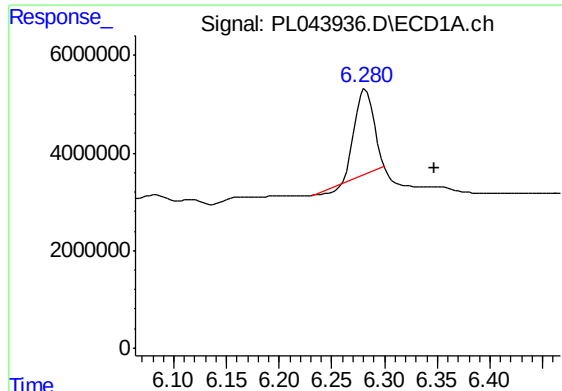

#27 Chlordane-5


R.T.: 6.282 min
Delta R.T.: -0.066 min
Response: 21435876
Conc: 107.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

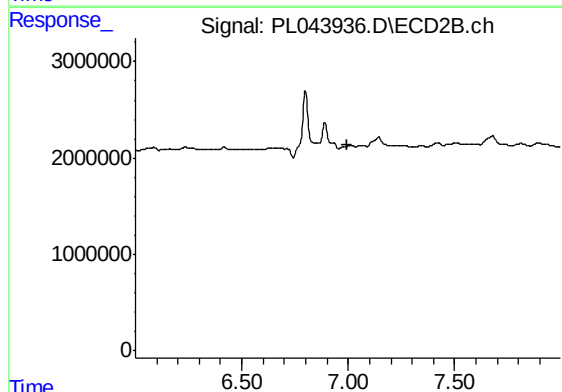


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

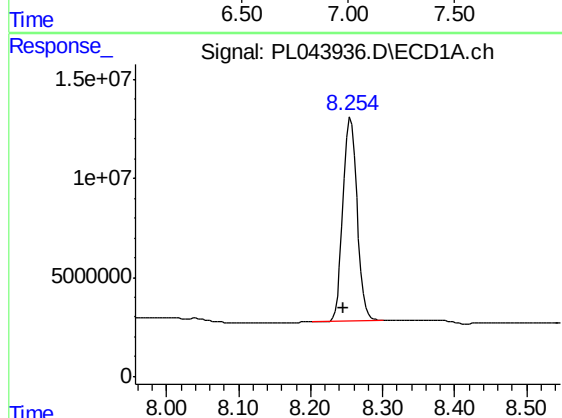

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.010 min
Response: 140059767
Conc: 24.78 ng/ml

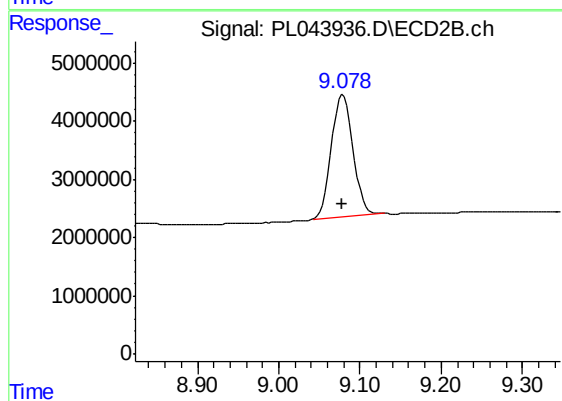

#28 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: 0.001 min
Response: 39249593
Conc: 24.71 ng/ml