

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011619\
 Data File : PL043959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2019 19:09
 Operator : AJ\SJ
 Sample : K1147-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 00:20:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	4.008	42488779	20689256	8.656	10.616
28) SA Decachlor...	8.273	9.080	69455473	25458518	12.290	16.026 #
Target Compounds						
16) A 4,4'-DDD	0.000	6.800f	0	7767752	N.D.	5.141 #
20) A Methoxychlor	6.980	0.000	9672278	0	3.783	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011619\
Data File : PL043959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2019 19:09
Operator : AJ\SJ
Sample : K1147-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 00:20:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

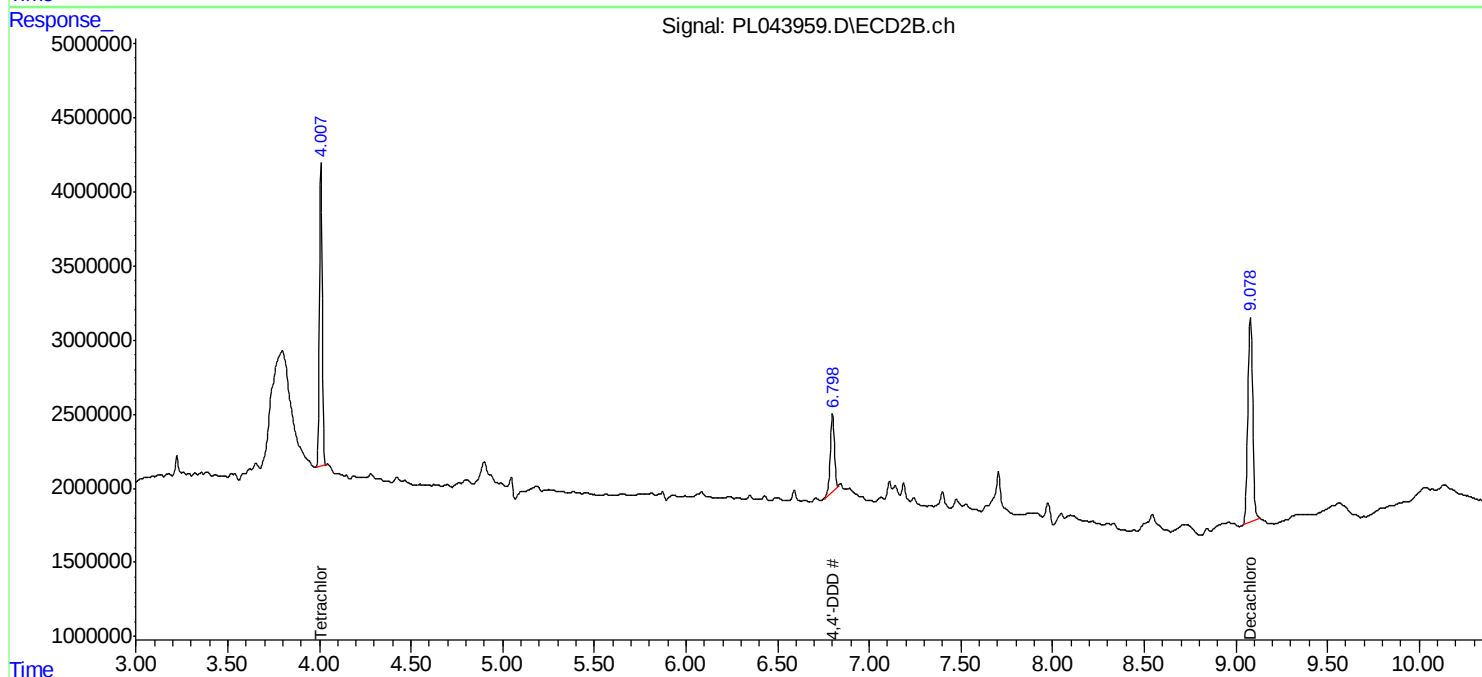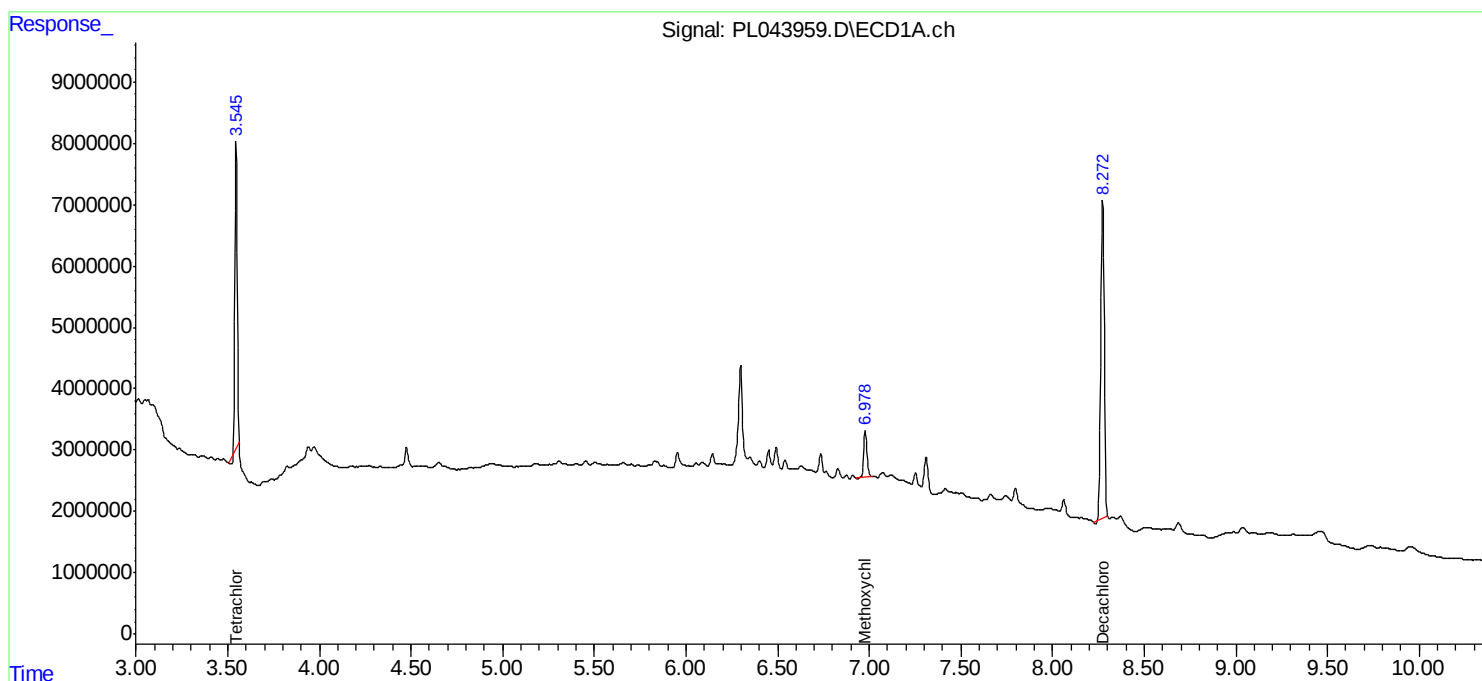


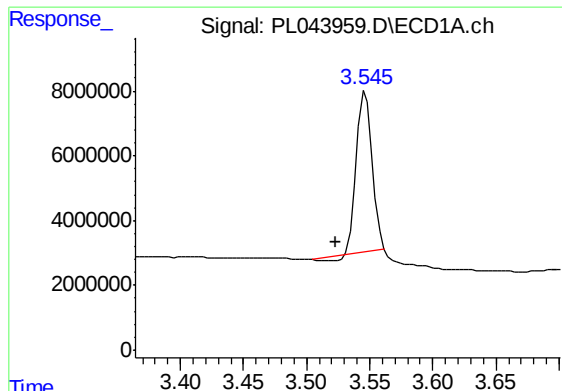

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.024 min
Response: 42488779
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

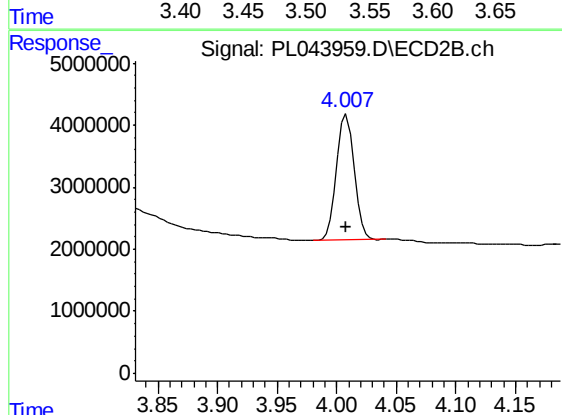


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 20689256
Conc: 10.62 ng/ml

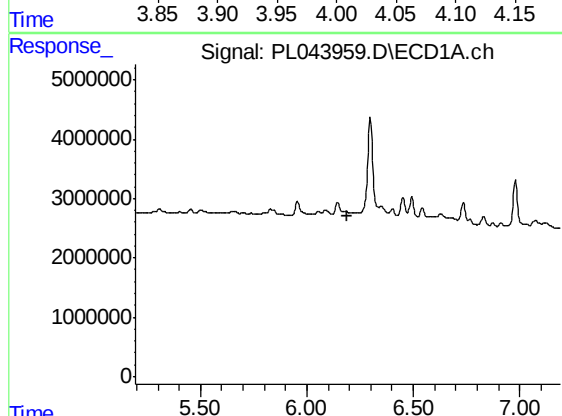


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

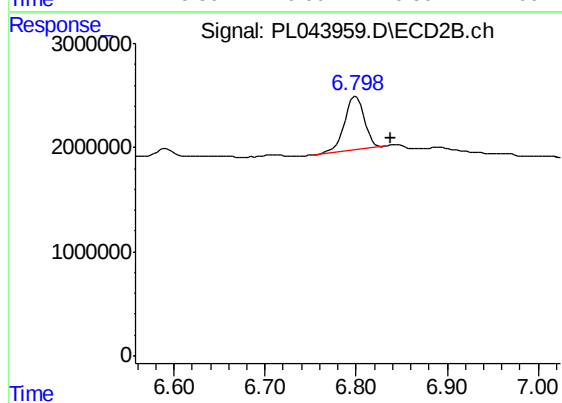

#16 4,4'-DDD


R.T.: 6.800 min
Delta R.T.: -0.038 min
Response: 7767752
Conc: 5.14 ng/ml

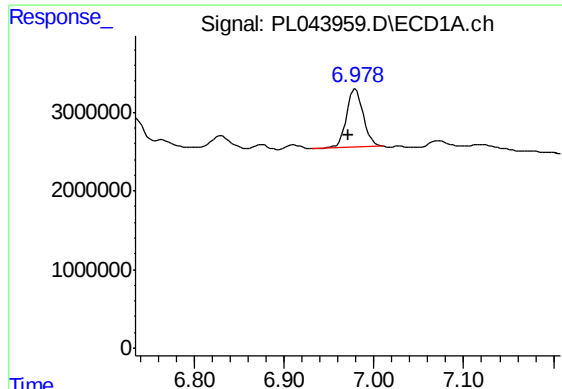

#20 Methoxychlor


R.T.: 6.980 min
Delta R.T.: 0.008 min
Response: 9672278
Conc: 3.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

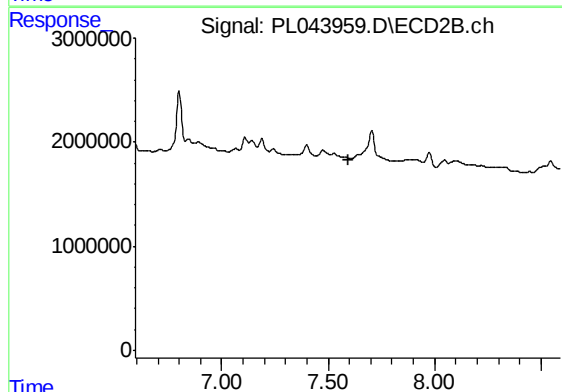


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.594 min
Response: 0
Conc: N.D.

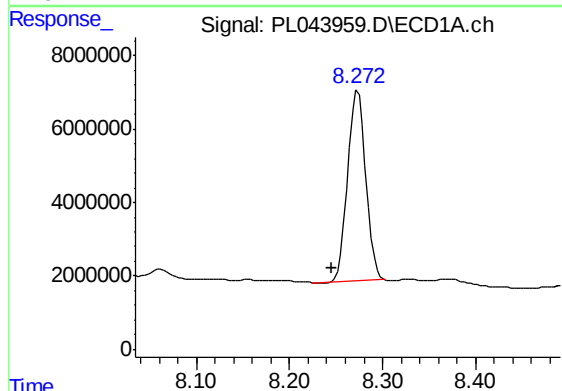

#28 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: 0.027 min
Response: 69455473
Conc: 12.29 ng/ml

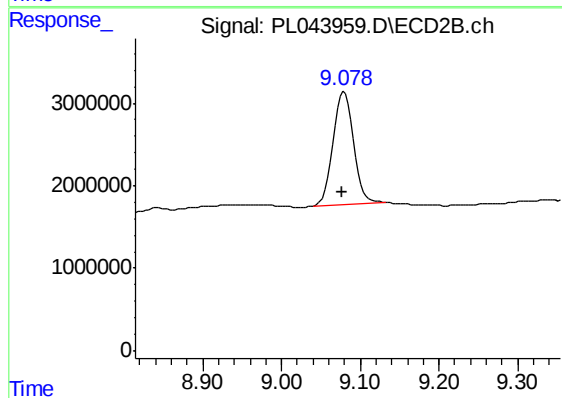

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.002 min
Response: 25458518
Conc: 16.03 ng/ml