

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011620\
 Data File : PL055782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2020 09:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 00:37:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.492	3.968	225.9E6	63461036	24.444	23.955
28) SA Decachlor...	8.240	8.959	180.8E6	42727154	20.593	20.551
Target Compounds						
9) A Endosulfan I	5.552	0.000	12123443	0	0.981	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011620\
Data File : PL055782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2020 09:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 00:37:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

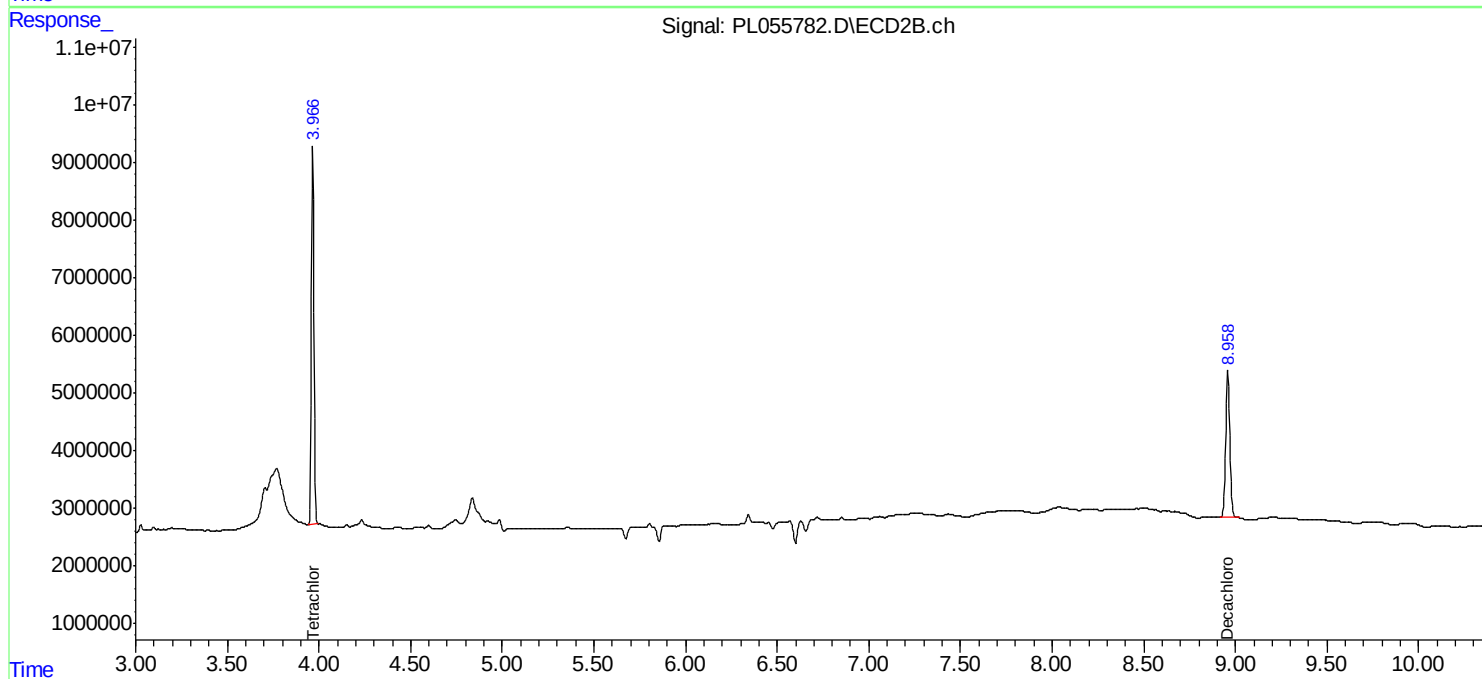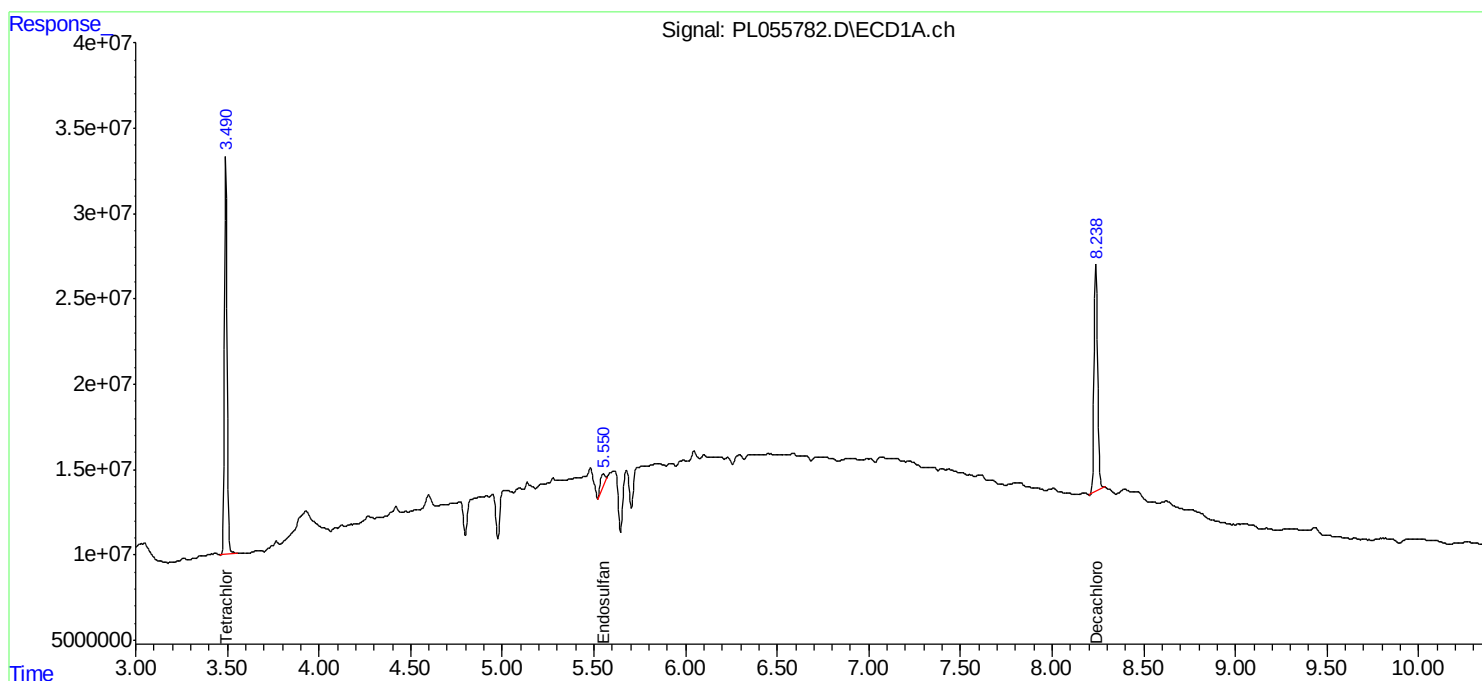


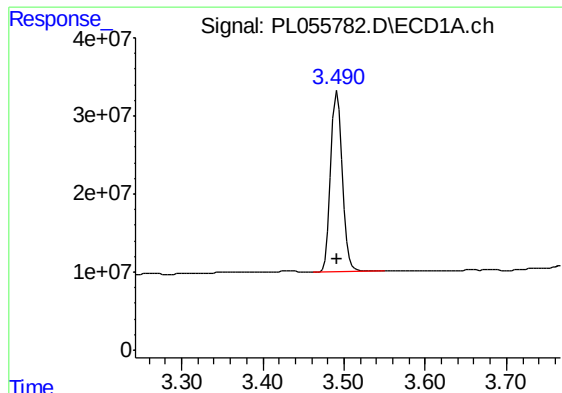

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 225882874
Conc: 24.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

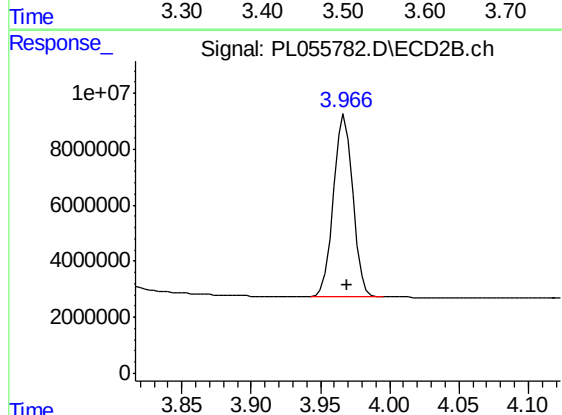


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 63461036
Conc: 23.96 ng/ml

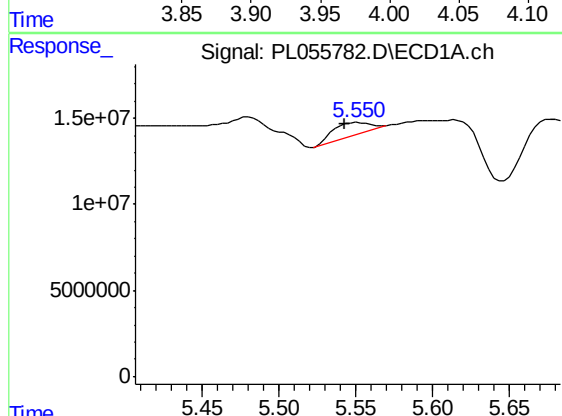


#9 Endosulfan I

R.T.: 5.552 min
Delta R.T.: 0.009 min
Response: 12123443
Conc: 0.98 ng/ml

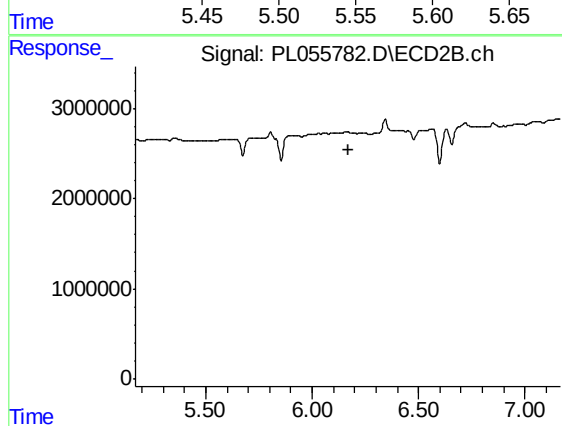

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

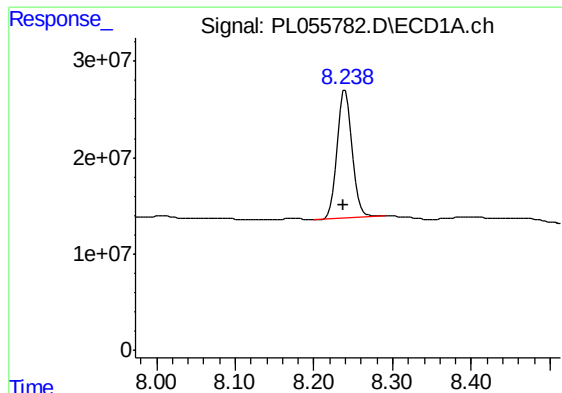

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.002 min
Response: 180839396
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

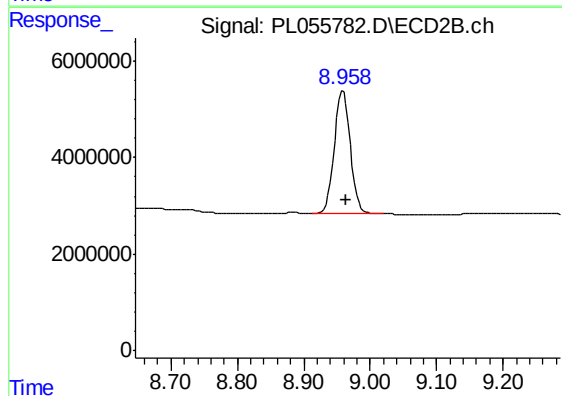

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.004 min
Response: 42727154
Conc: 20.55 ng/ml