

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011620\
 Data File : PL055795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2020 15:23
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 00:41:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.968	189.9E6	57196383	20.550	21.591
28)	SA Decachlor...	8.238	8.958	164.8E6	40330619	18.771	19.398
Target Compounds							
9)	A Endosulfan I	5.550	0.000	10242463	0	0.829	N.D. #
10)	B gamma-Chl...	5.415f	0.000	65415869	0	4.886	N.D. #
11)	B alpha-Chl...	5.480	0.000	40328662	0	3.071	N.D. #
18)	B Endrin al...	6.481	0.000	24708660	0	2.618	N.D. #
25)	Chlordane-3	5.415	0.000	65415869	0	55.574	N.D. #
26)	Chlordane-4	5.480	0.000	40328662	0	41.304	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011620\
Data File : PL055795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2020 15:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 00:41:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

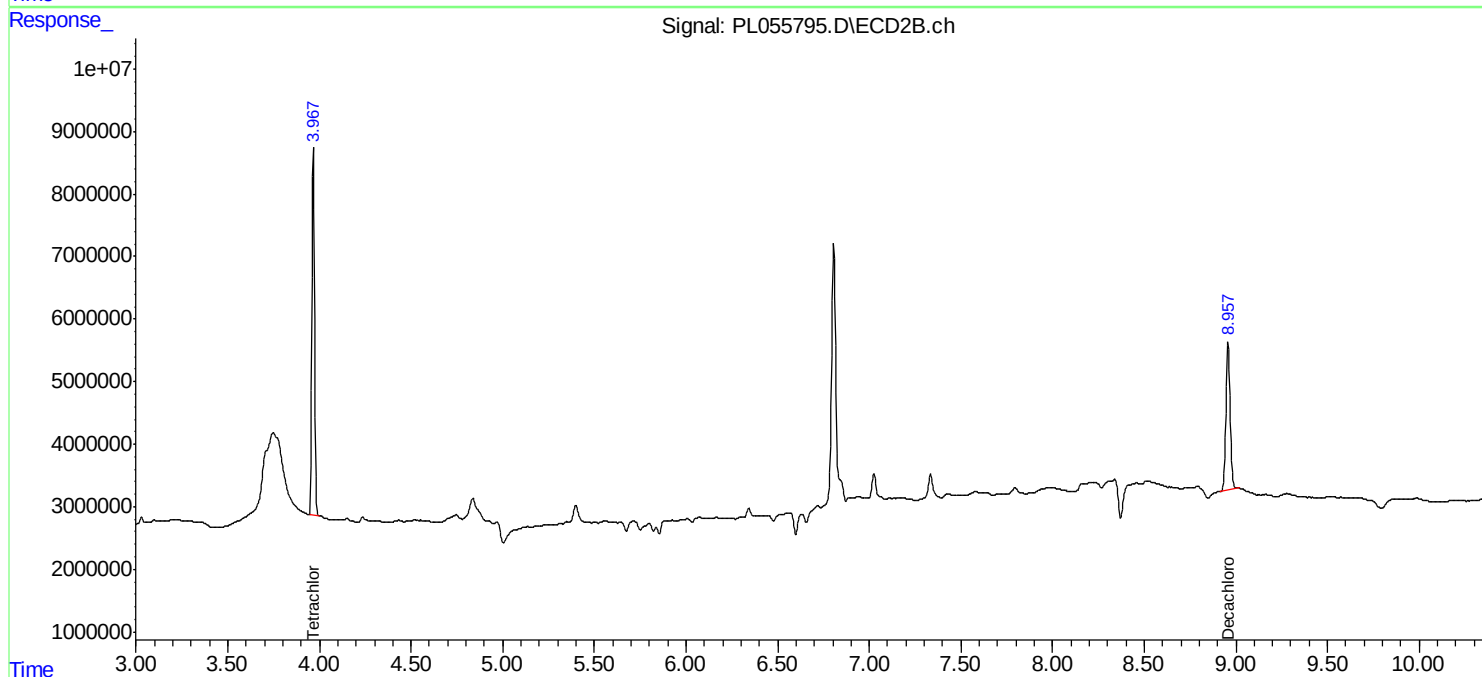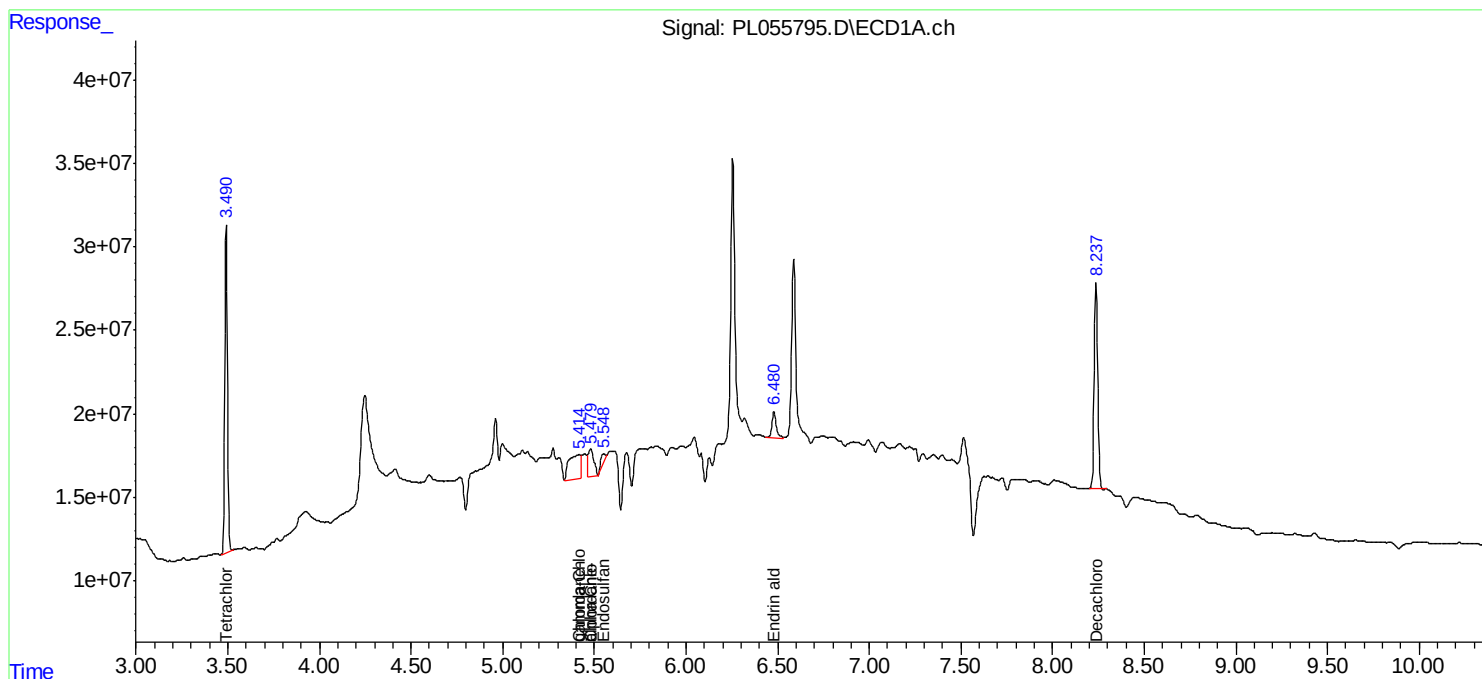


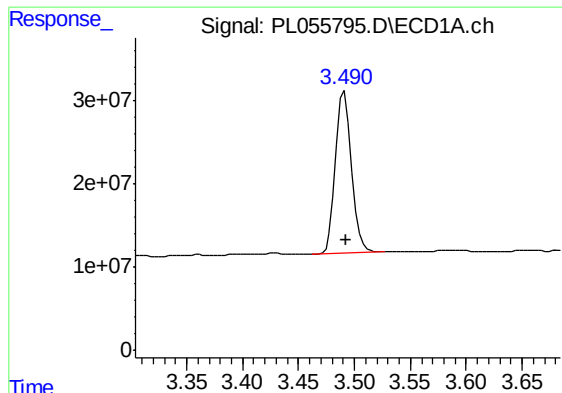

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 189892392
Conc: 20.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

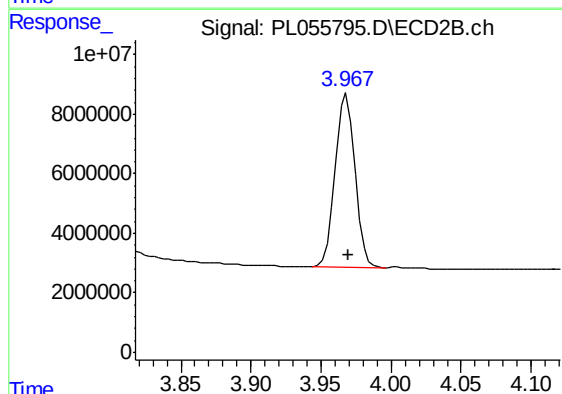


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.001 min
Response: 57196383
Conc: 21.59 ng/ml

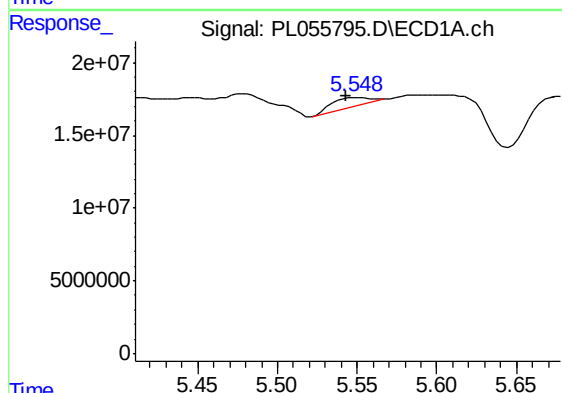


#9 Endosulfan I

R.T.: 5.550 min
Delta R.T.: 0.007 min
Response: 10242463
Conc: 0.83 ng/ml

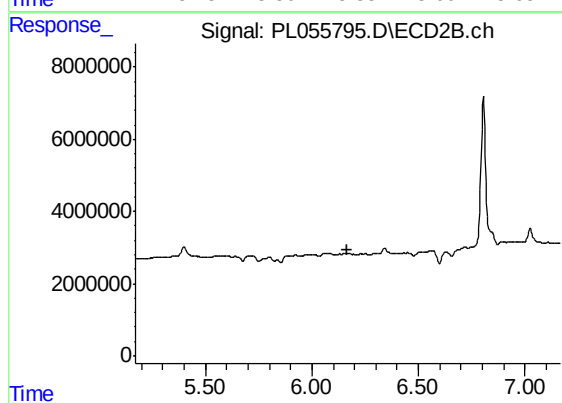

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

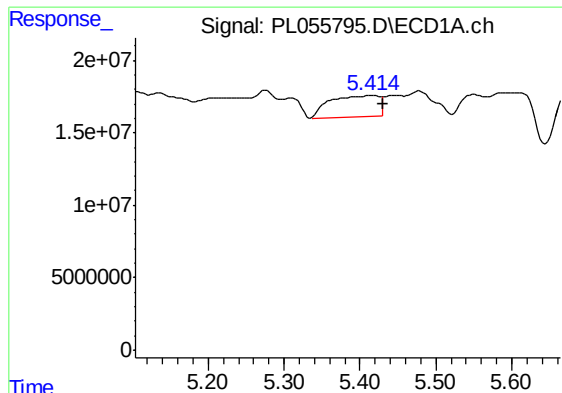

#10 gamma-Chlordane


R.T.: 5.415 min
Delta R.T.: -0.015 min
Response: 65415869
Conc: 4.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

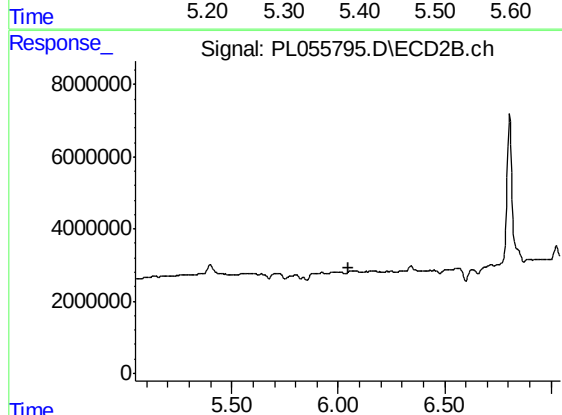


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.047 min
Response: 0
Conc: N.D.

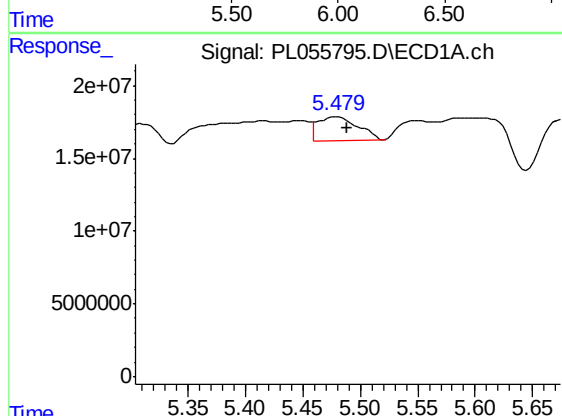


#11 alpha-Chlordane

R.T.: 5.480 min
Delta R.T.: -0.009 min
Response: 40328662
Conc: 3.07 ng/ml

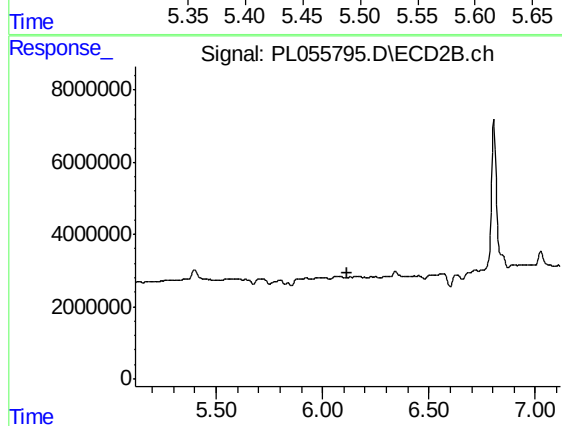

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

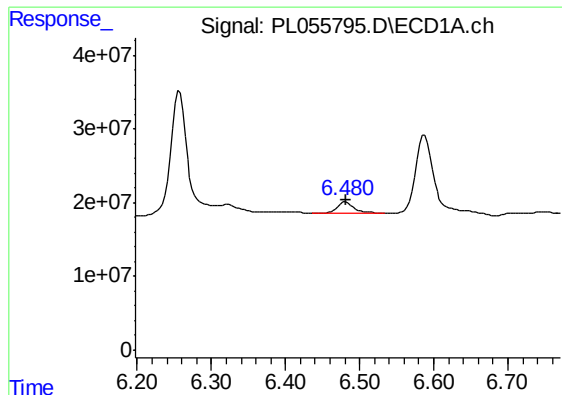

#18 Endrin aldehyde


R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 24708660
Conc: 2.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

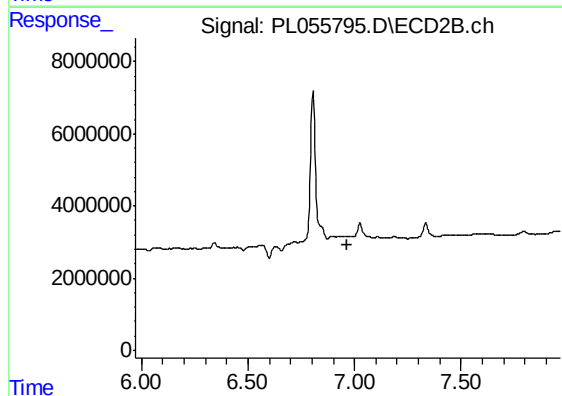


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.968 min
Response: 0
Conc: N.D.

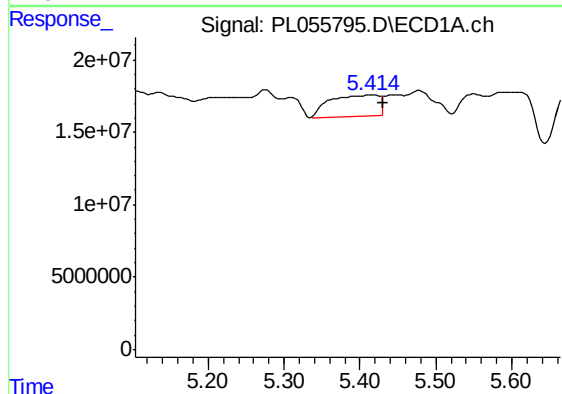


#25 Chlordane-3

R.T.: 5.415 min
Delta R.T.: -0.015 min
Response: 65415869
Conc: 55.57 ng/ml

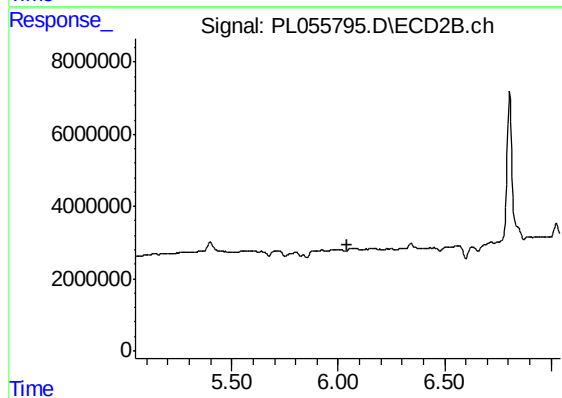

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

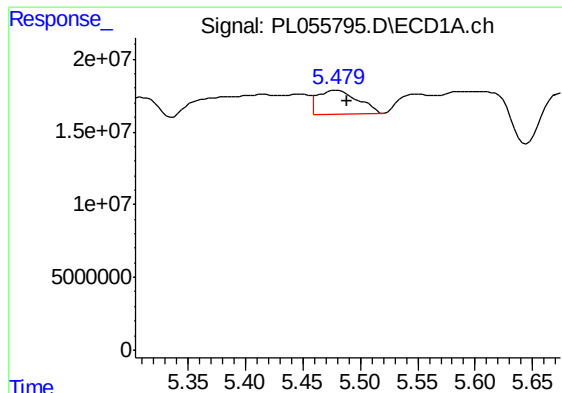

#26 Chlordane-4


R.T.: 5.480 min
Delta R.T.: -0.008 min
Response: 40328662
Conc: 41.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

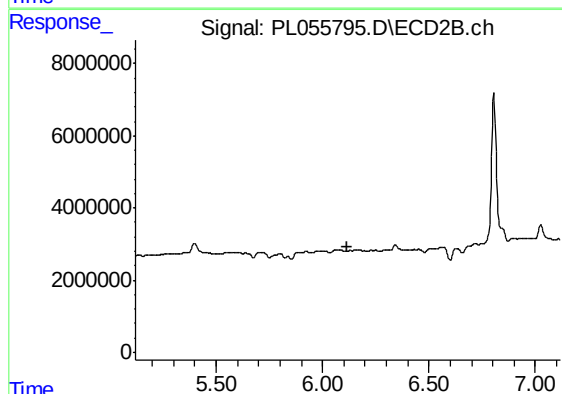


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

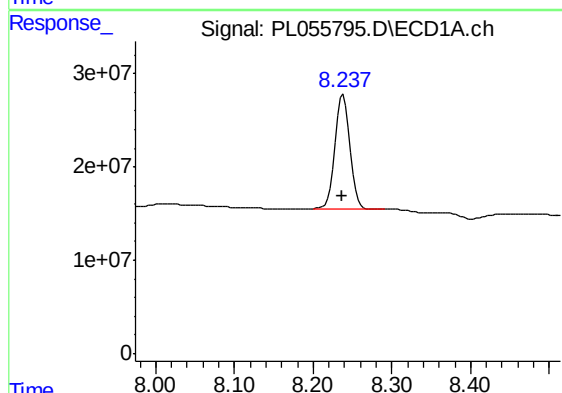

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 164841000
Conc: 18.77 ng/ml

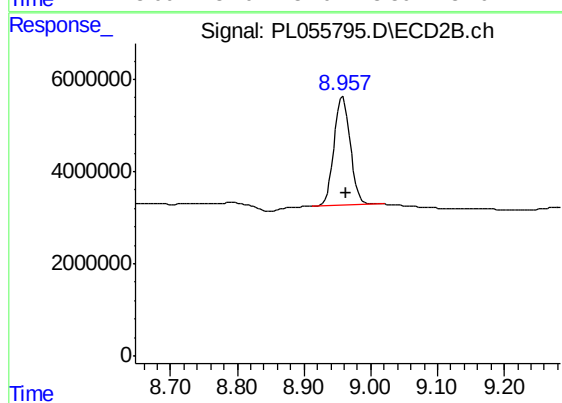

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.005 min
Response: 40330619
Conc: 19.40 ng/ml