

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011623\
 Data File : PL080350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2023 18:19
 Operator : AR\AJ
 Sample : 01159-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/17/2023
 Supervised By : Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 20:42:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.690	44702903	46515266	22.378m	20.798
2) SA Decachlor...	8.790	7.840	32469035	43158396	22.007	19.200

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011623\
Data File : PL080350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2023 18:19
Operator : AR\AJ
Sample : 01159-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MH-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/17/2023
Supervised By : Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 20:42:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

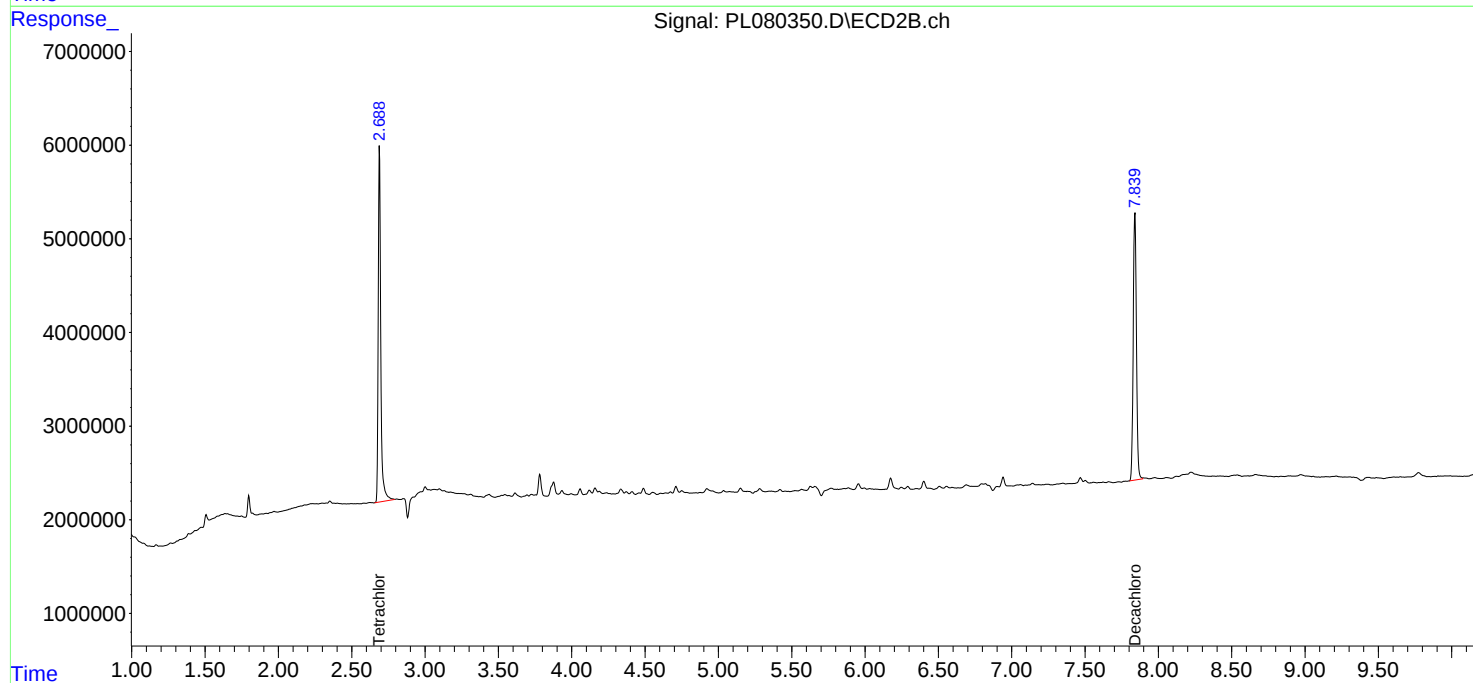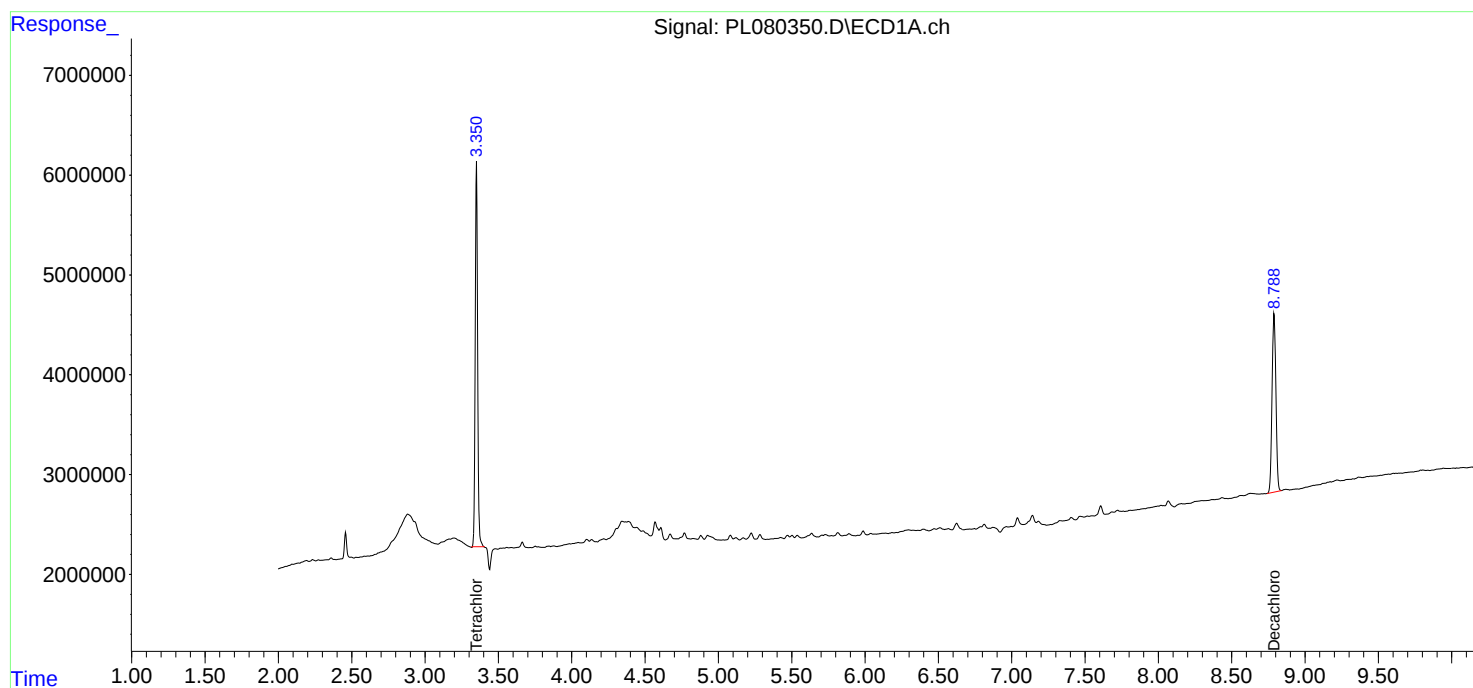

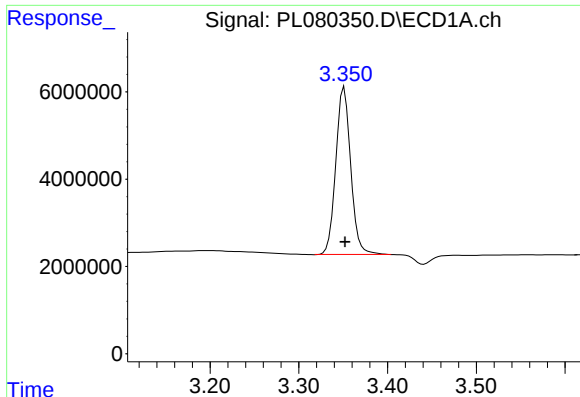


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 44702903
Conc: 22.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

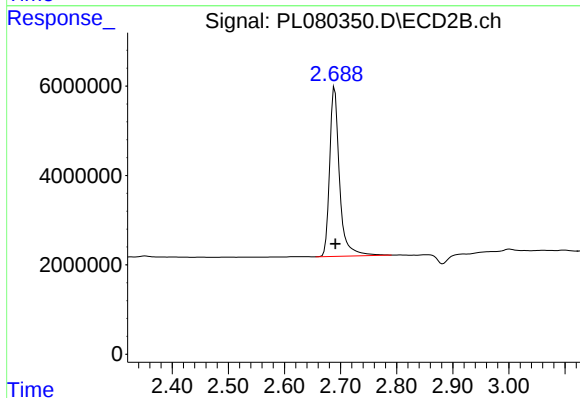


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: -0.001 min
Response: 46515266
Conc: 20.80 ng/ml

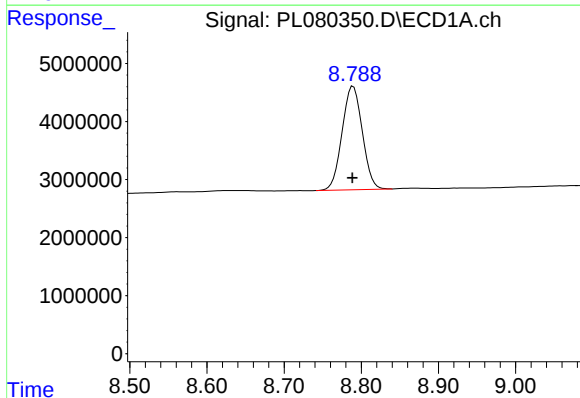

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 32469035
Conc: 22.01 ng/ml

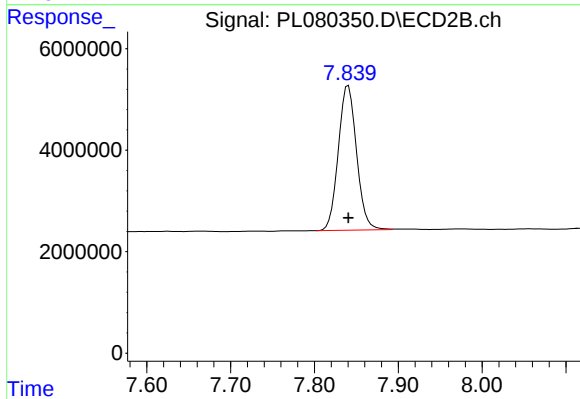

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 43158396
Conc: 19.20 ng/ml