

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
 Data File : PL044002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2019 11:47
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 06:08:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 18 06:08:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	4.007	307.5E6	108.9E6	50.000	50.000
28)	SA Decachlor...	8.288	9.075	326.4E6	103.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.432	5.003	131.8E6	52590501	500.000	500.000
24)	Chlordane-2	4.933	5.471	149.1E6	51647460	500.000	500.000
25)	Chlordane-3	5.501	6.117	465.7E6	178.4E6	500.000	500.000
26)	Chlordane-4	5.557	6.191	395.0E6	215.3E6	500.000	500.000
27)	Chlordane-5	6.392	6.995	131.8E6	41315692	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
Data File : PL044002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2019 11:47
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 06:08:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
Quant Title : GC Extractables
QLast Update : Fri Jan 18 06:08:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

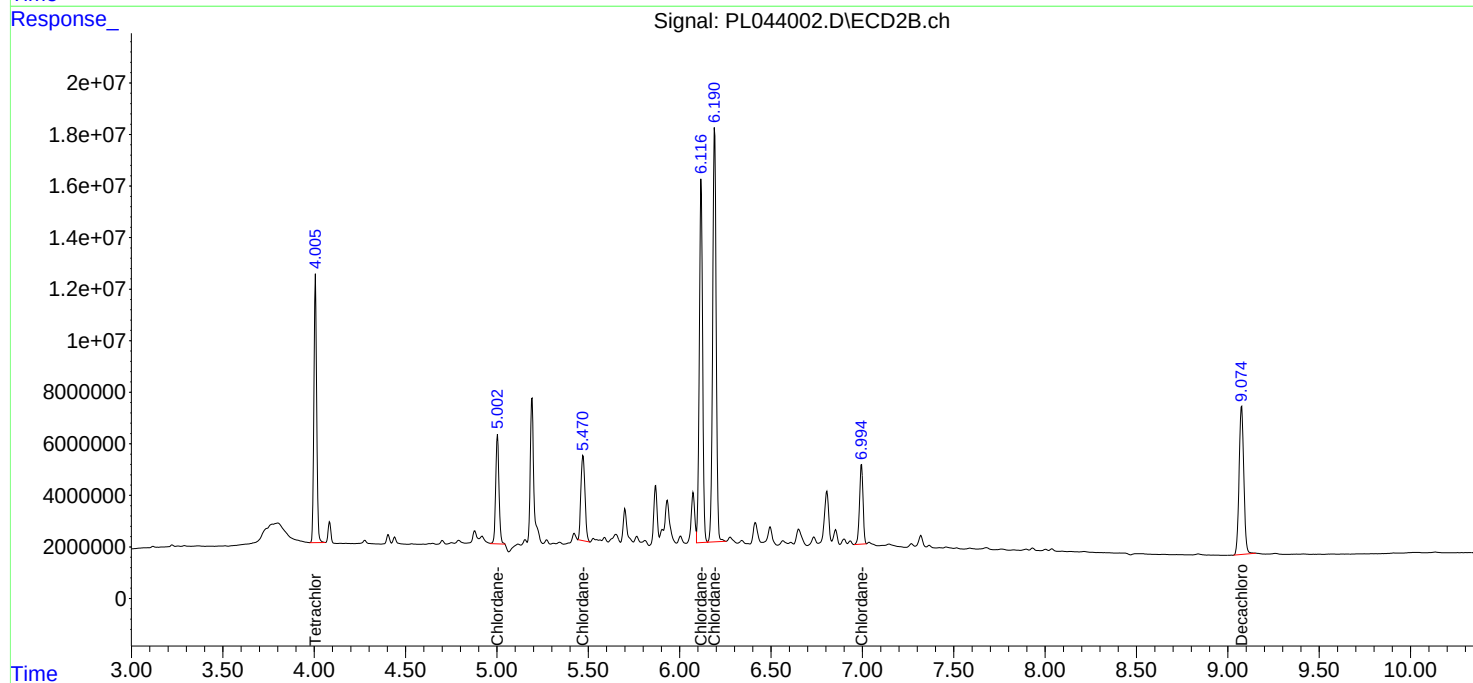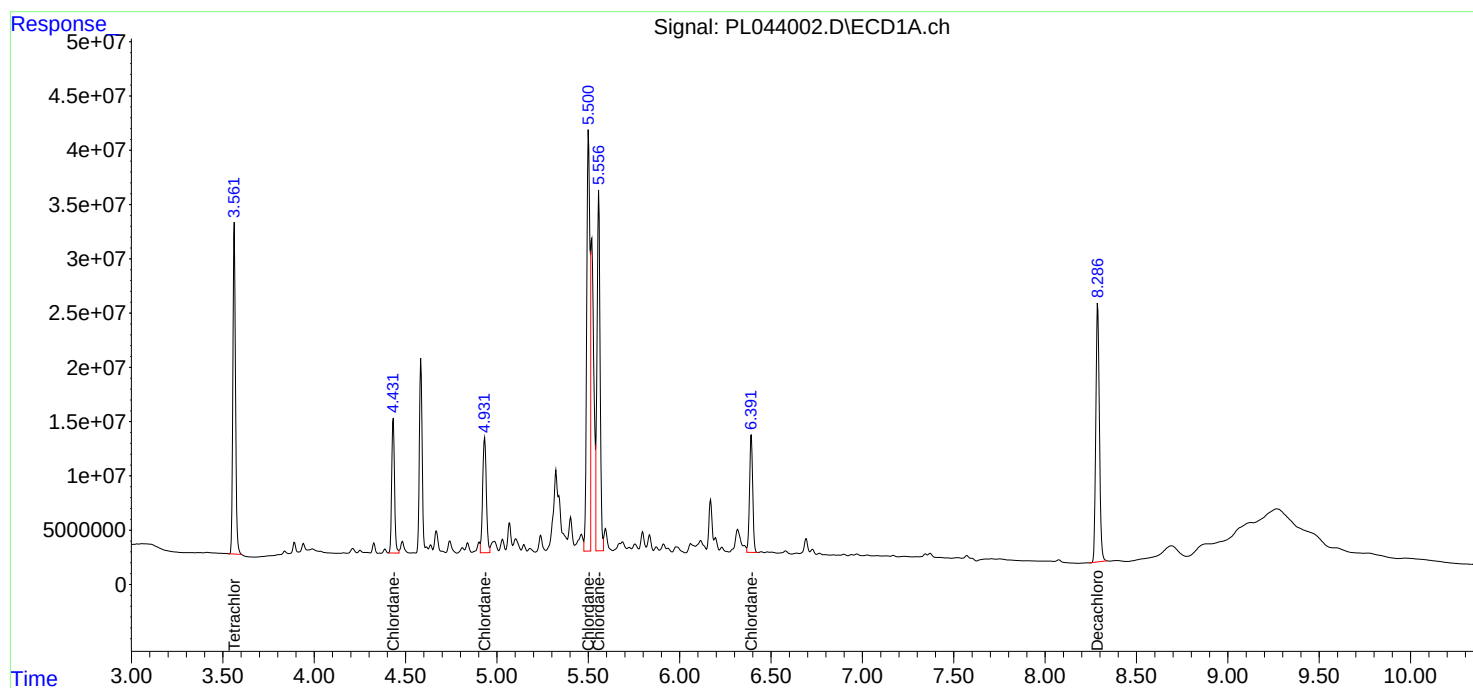


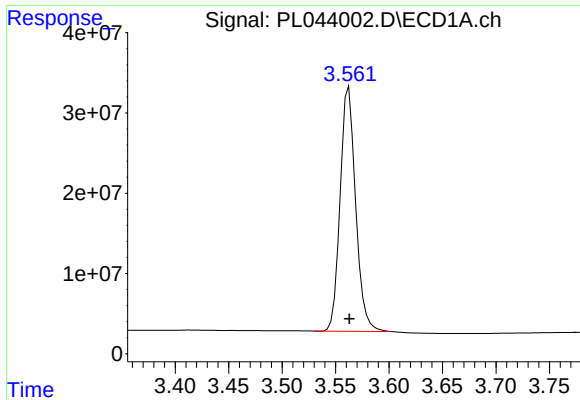

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 307521031
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

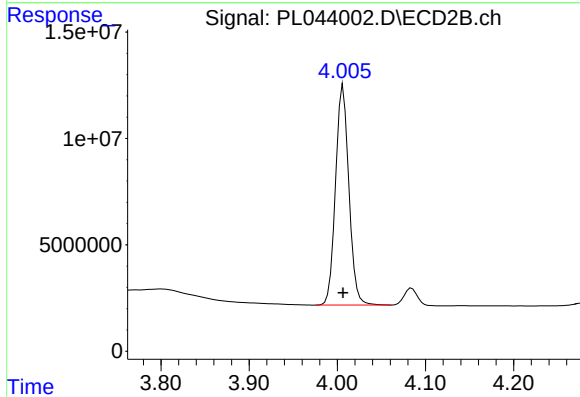


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 108947210
Conc: 50.00 ng/ml

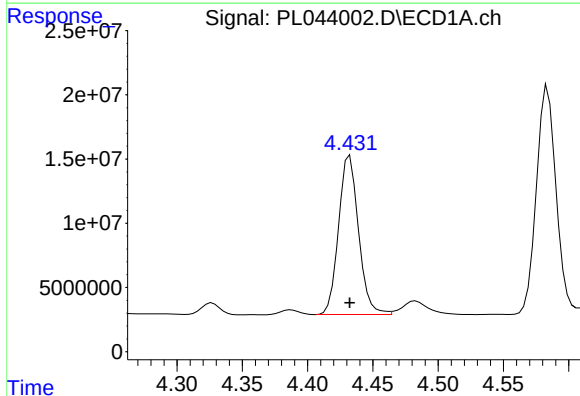


#23 Chlordane-1

R.T.: 4.432 min
Delta R.T.: 0.000 min
Response: 131769153
Conc: 500.00 ng/ml

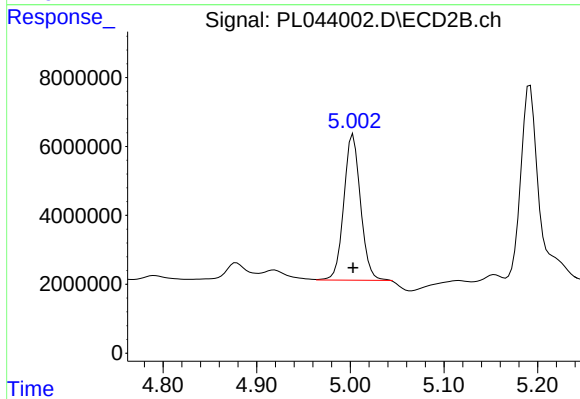

#23 Chlordane-1


R.T.: 5.003 min
Delta R.T.: 0.000 min
Response: 52590501
Conc: 500.00 ng/ml

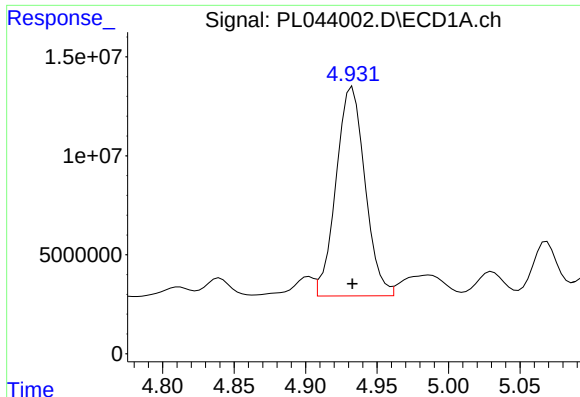

#24 Chlordane-2


R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 149076644
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

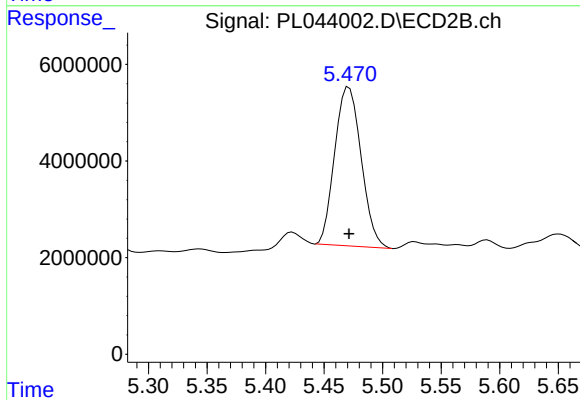


#24 Chlordane-2

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 51647460
Conc: 500.00 ng/ml

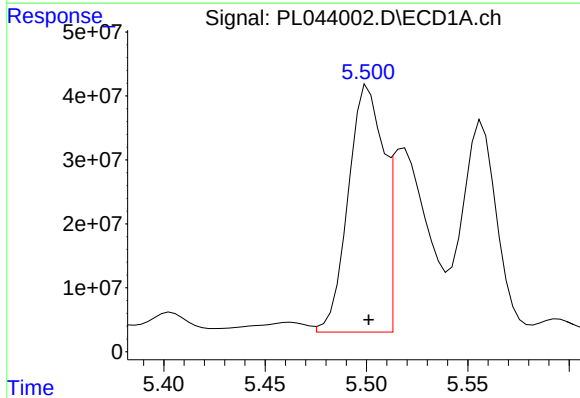


#25 Chlordane-3

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 465658891
Conc: 500.00 ng/ml

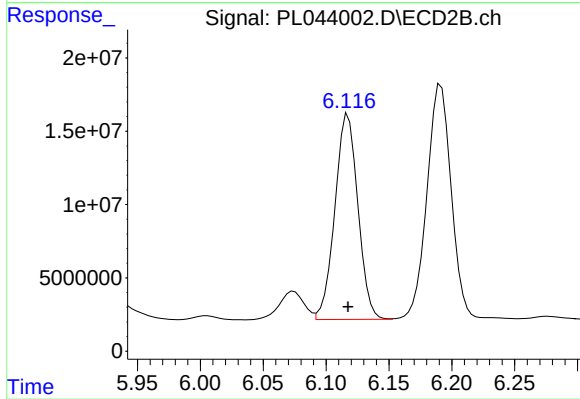

#25 Chlordane-3


R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 178359593
Conc: 500.00 ng/ml

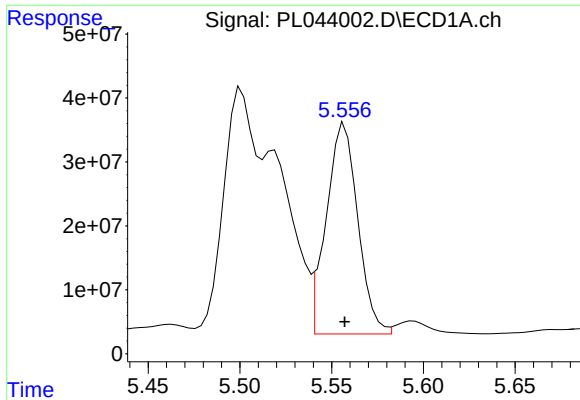

#26 Chlordane-4


R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 394958354
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

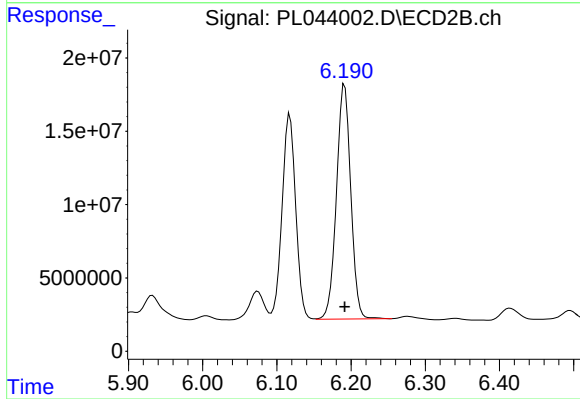


#26 Chlordane-4

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 215344927
Conc: 500.00 ng/ml

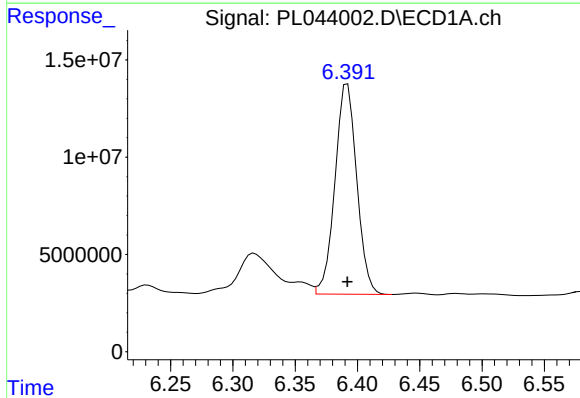


#27 Chlordane-5

R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 131836437
Conc: 500.00 ng/ml

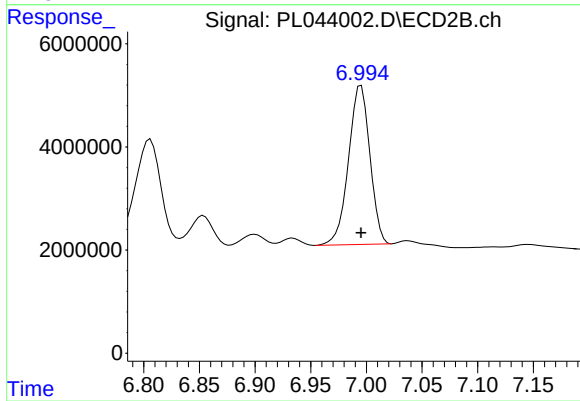

#27 Chlordane-5


R.T.: 6.995 min
Delta R.T.: 0.000 min
Response: 41315692
Conc: 500.00 ng/ml

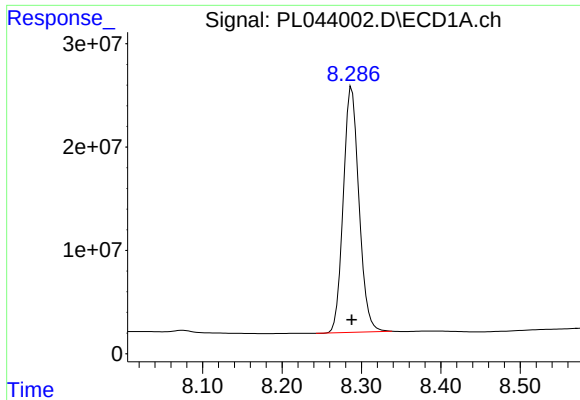

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 326407683
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

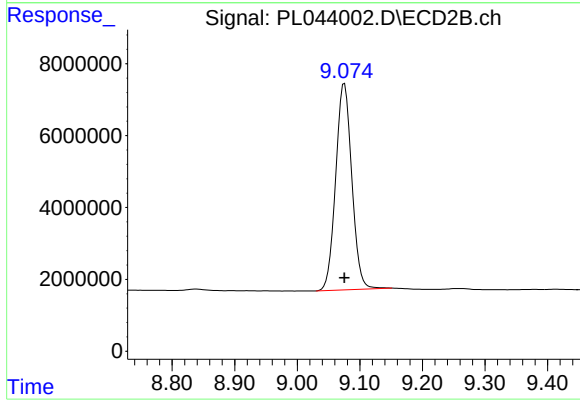

#28 Decachlorobiphenyl

R.T.: 9.075 min
Delta R.T.: 0.000 min
Response: 103209404
Conc: 50.00 ng/ml