

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
 Data File : PL044014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2019 14:37
 Operator : AJ\SJ
 Sample : K1147-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 06:39:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 18 06:10:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	4.007	122.9E6	45954694	21.339	20.772
28)	SA Decachlor...	8.293	9.077	112.7E6	39633804	16.681	18.558
Target Compounds							
6)	B beta-BHC	4.498f	0.000	8466122	0	2.419	N.D. #
8)	B Heptachlo...	0.000	5.878	0	11357331	N.D.	4.814 #
14)	MA Endrin	6.123	0.000	15243697	0	2.251	N.D. #
15)	B Endosulfa...	6.320f	0.000	23105988	0	3.415	N.D. #
16)	A 4,4'-DDD	0.000	6.799f	0	14057070	N.D.	7.680 #
23)	Chlordane-1	4.498	0.000	8466122	0	32.125	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
Data File : PL044014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2019 14:37
Operator : AJ\SJ
Sample : K1147-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 06:39:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
Quant Title : GC Extractables
QLast Update : Fri Jan 18 06:10:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

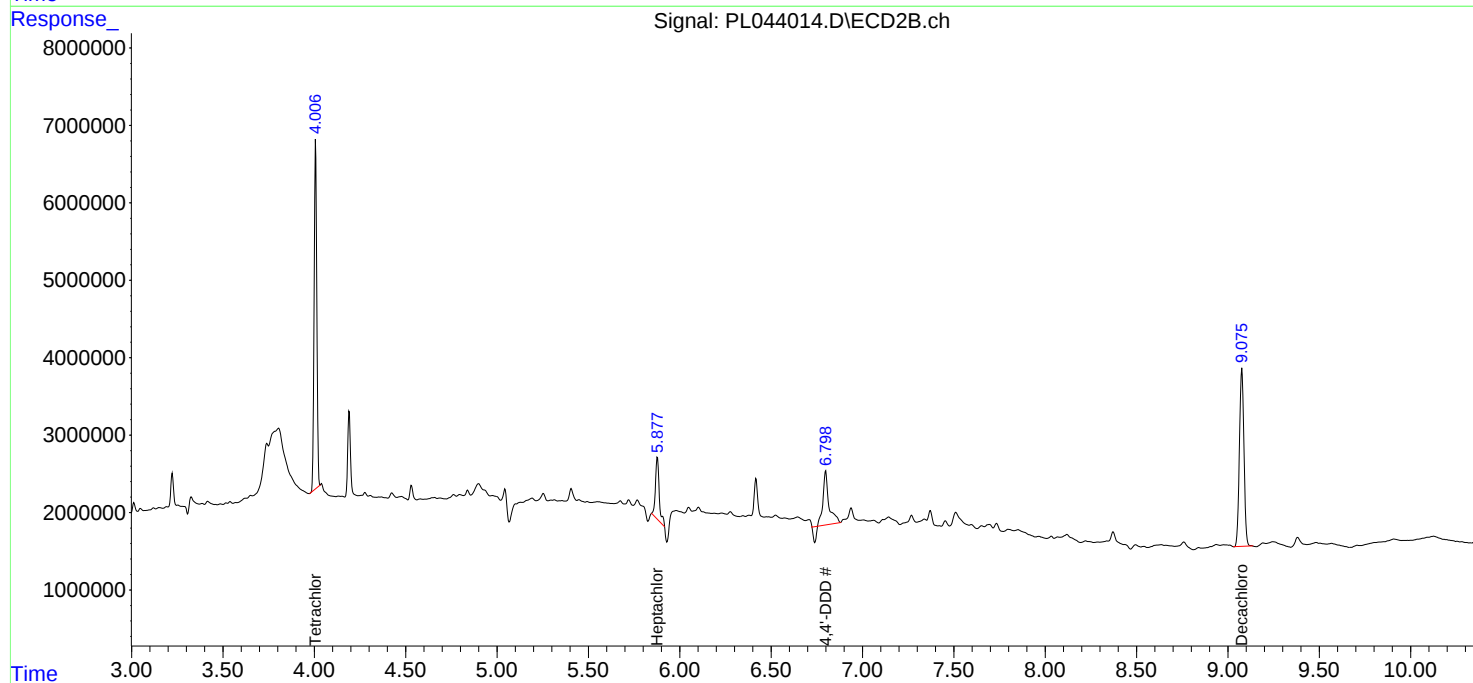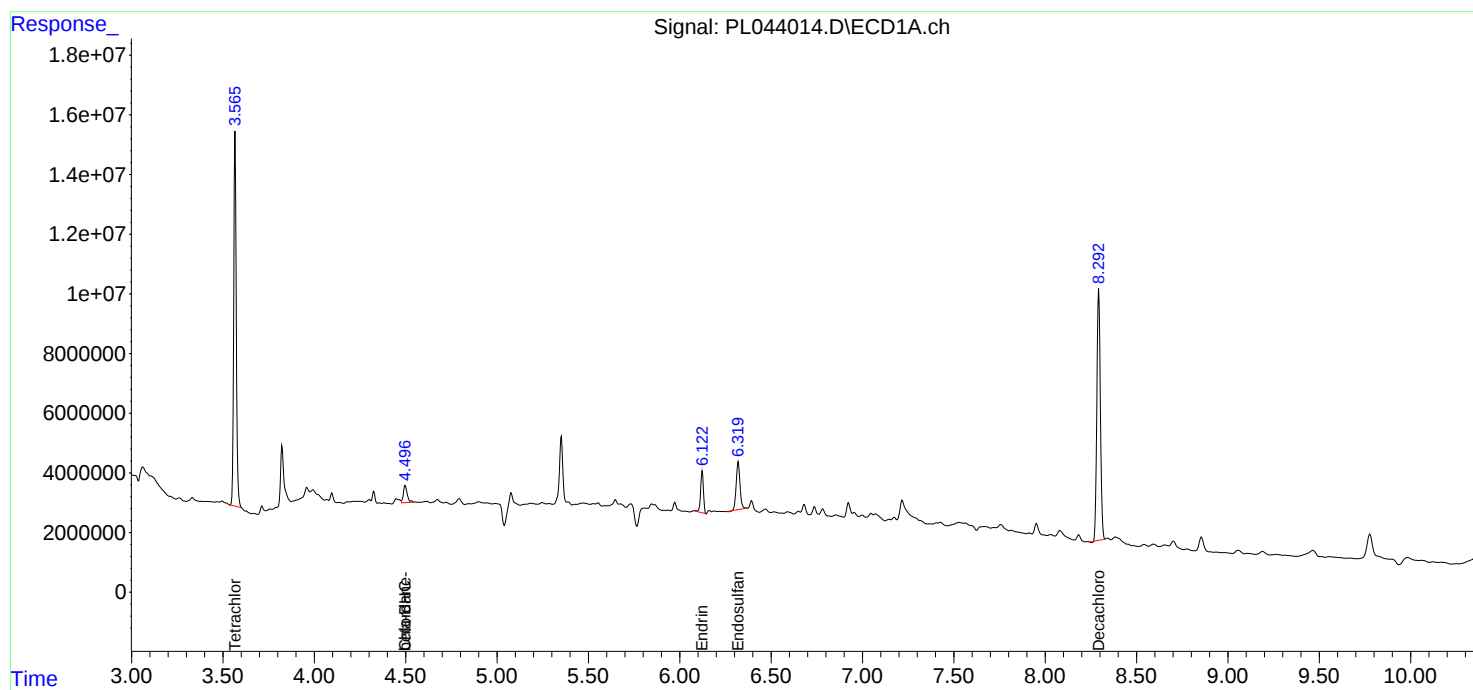


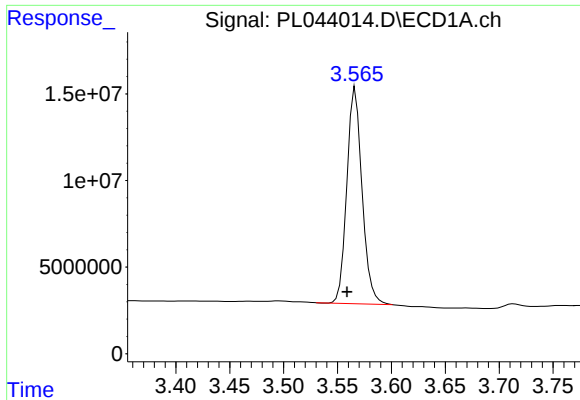

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.008 min
Response: 122946653
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

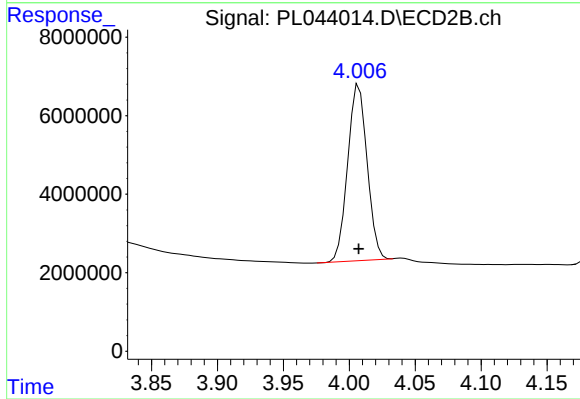


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 45954694
Conc: 20.77 ng/ml

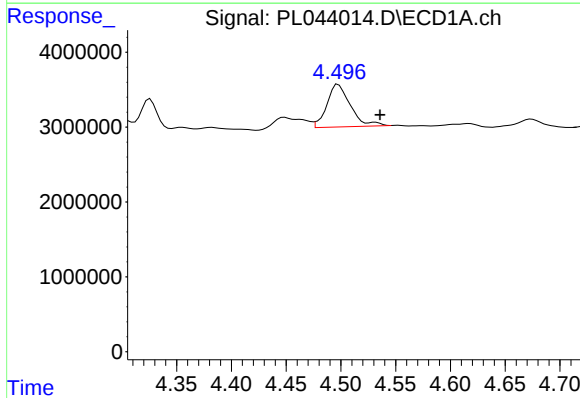


#6 beta-BHC

R.T.: 4.498 min
Delta R.T.: -0.038 min
Response: 8466122
Conc: 2.42 ng/ml

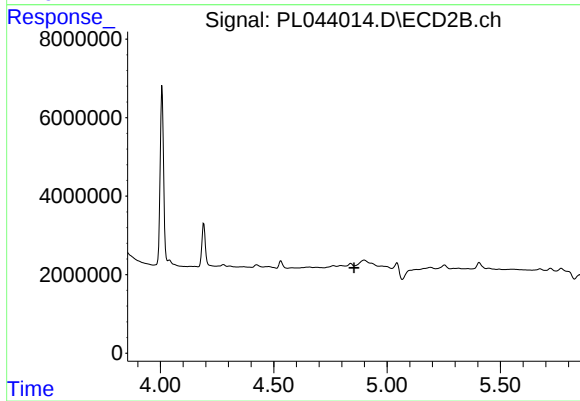

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.854 min
Response: 0
Conc: N.D.

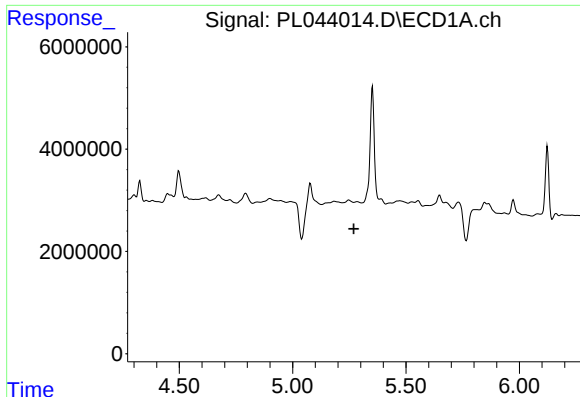

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4

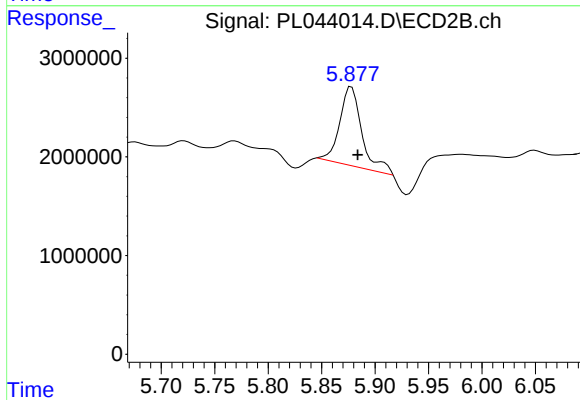


#8 Heptachlor epoxide

R.T.: 5.878 min
Delta R.T.: -0.006 min
Response: 11357331
Conc: 4.81 ng/ml

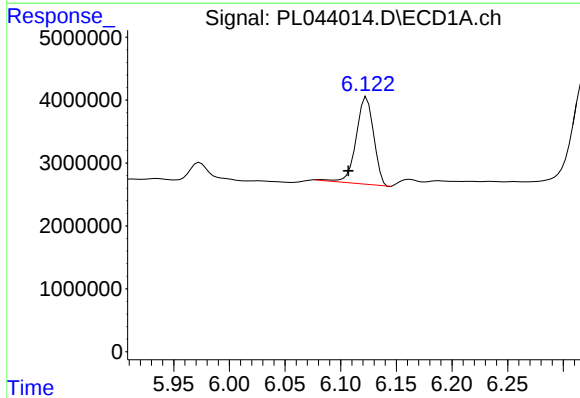


#14 Endrin

R.T.: 6.123 min
Delta R.T.: 0.017 min
Response: 15243697
Conc: 2.25 ng/ml

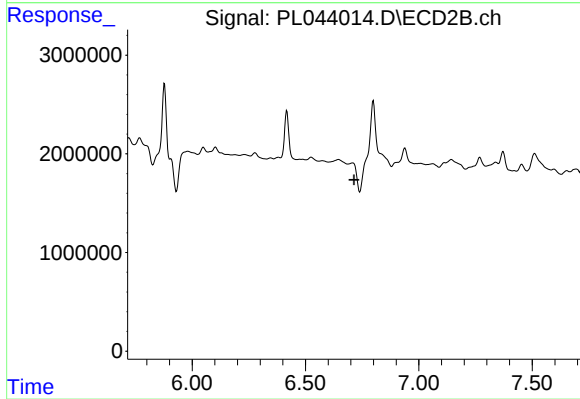

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.715 min
Response: 0
Conc: N.D.

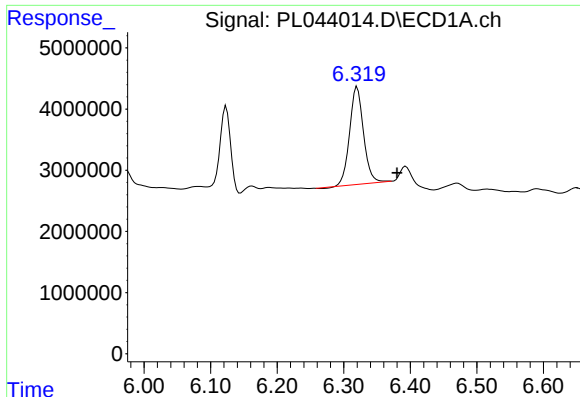

#15 Endosulfan II


R.T.: 6.320 min
Delta R.T.: -0.060 min
Response: 23105988
Conc: 3.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

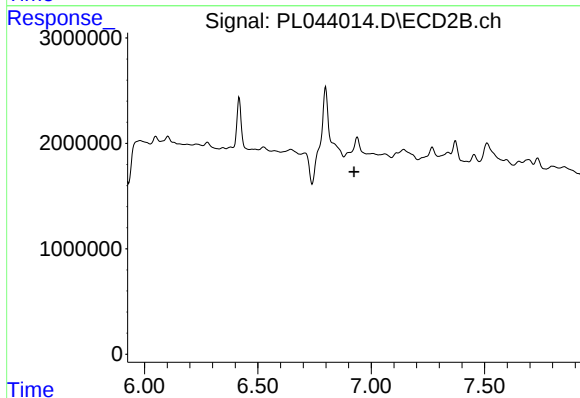


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

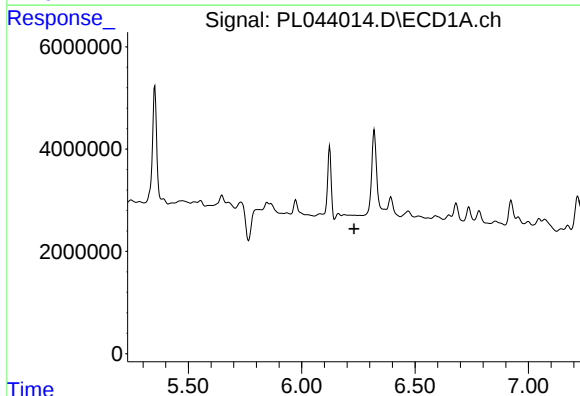


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

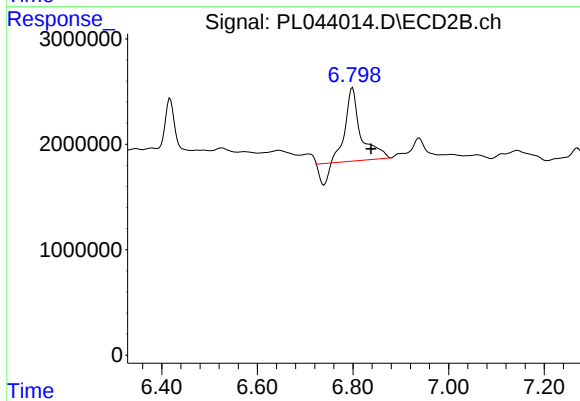

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: -0.039 min
Response: 14057070
Conc: 7.68 ng/ml

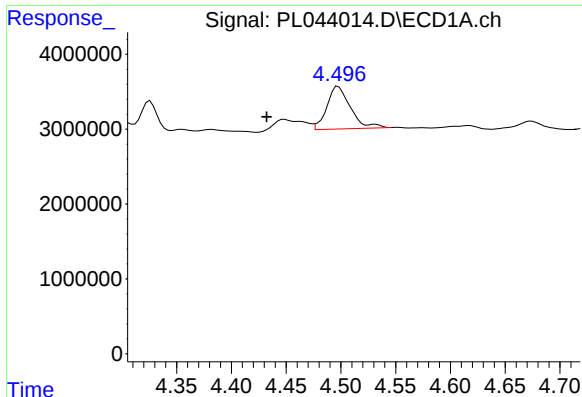

#23 Chlordane-1


R.T.: 4.498 min
Delta R.T.: 0.065 min
Response: 8466122
Conc: 32.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

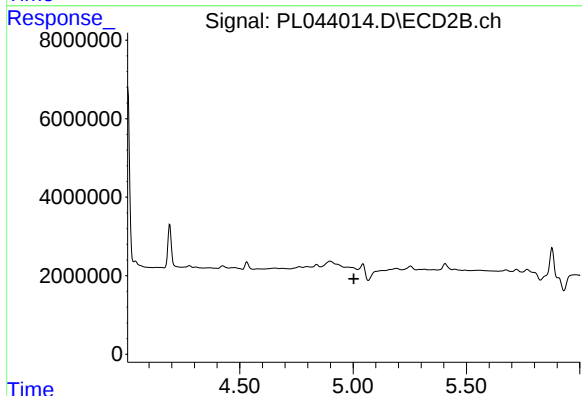


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.003 min
Response: 0
Conc: N.D.

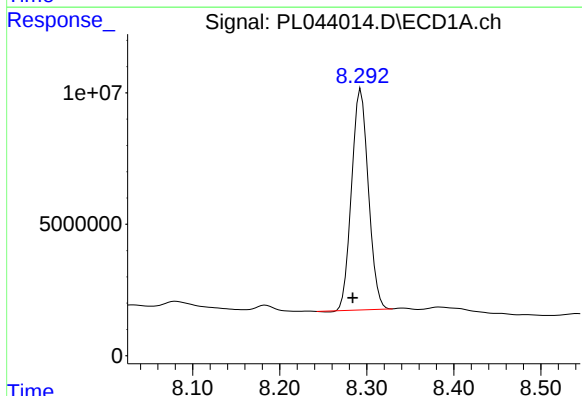

#28 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: 0.009 min
Response: 112692381
Conc: 16.68 ng/ml

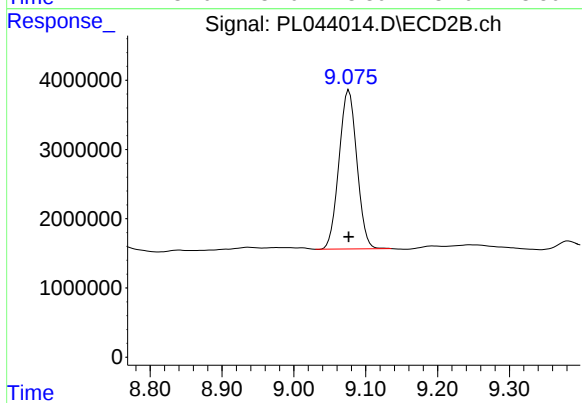

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 39633804
Conc: 18.56 ng/ml