

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
 Data File : PL044045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2019 22:27
 Operator : AJ\SJ
 Sample : K1159-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0115-S-TCLP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 07:10:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 18 06:10:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	4.008	109.7E6	43751733	19.038	19.776
28)	SA Decachlor...	8.295	9.078	69886495	22659186	10.345	10.610
Target Compounds							
6)	B beta-BHC	4.499f	0.000	17412907	0	4.975	N.D. #
15)	B Endosulfa...	6.322f	0.000	26021362	0	3.846	N.D. #
16)	A 4,4'-DDD	0.000	6.799f	0	9903134	N.D.	5.411 #
23)	Chlordane-1	4.499	0.000	17412907	0	66.074	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011719\
Data File : PL044045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2019 22:27
Operator : AJ\SJ
Sample : K1159-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-0115-S-TCLP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 07:10:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011719.M
Quant Title : GC Extractables
QLast Update : Fri Jan 18 06:10:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

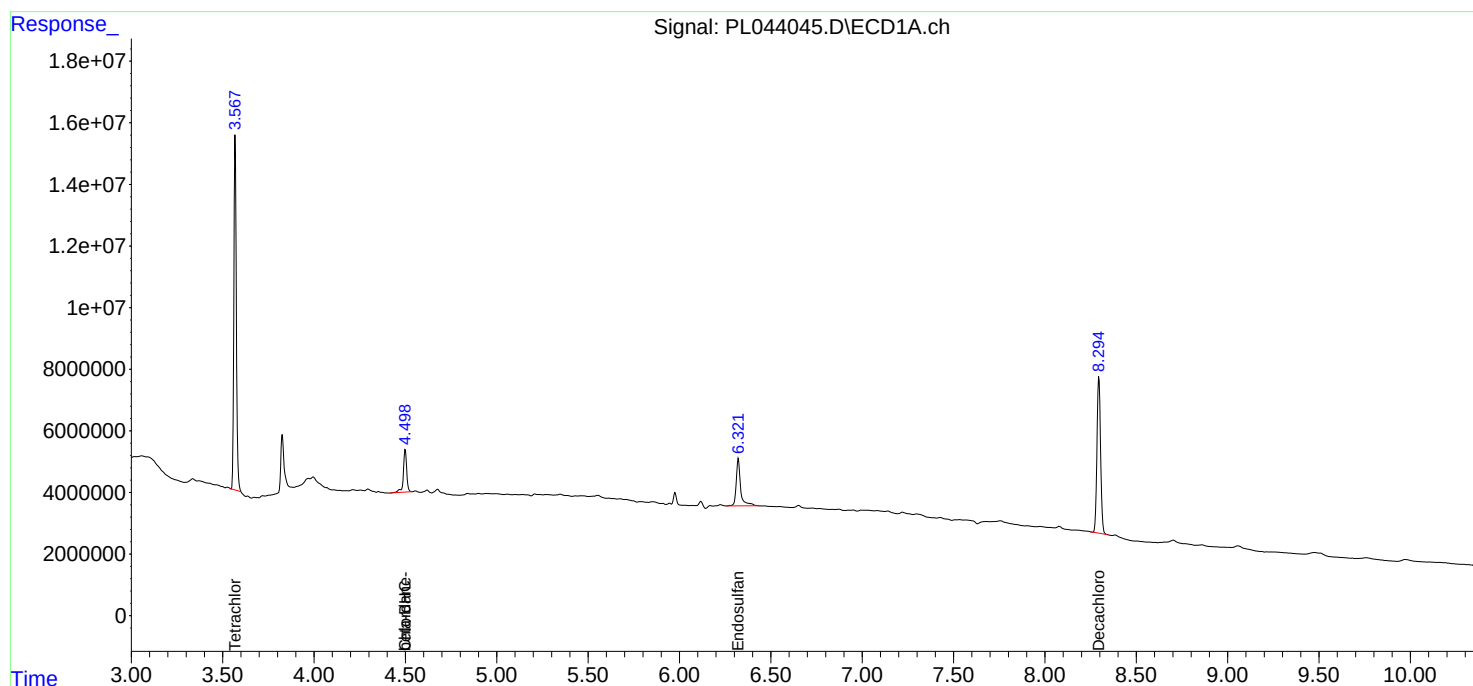


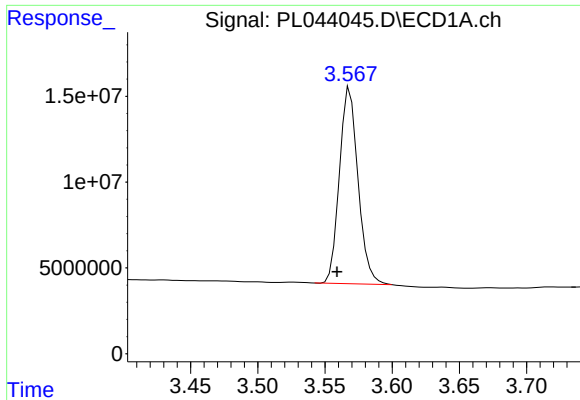

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.010 min
Response: 109689168
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0115-S-TCLP-7

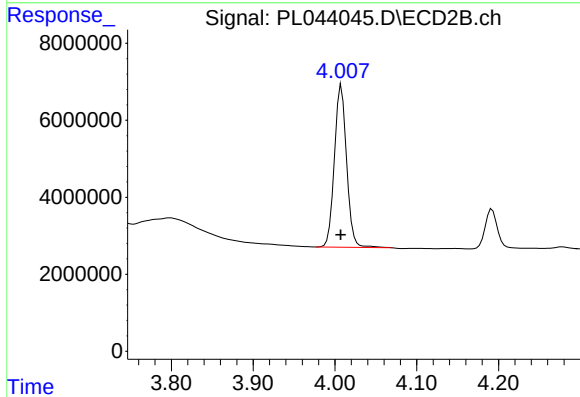


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 43751733
Conc: 19.78 ng/ml

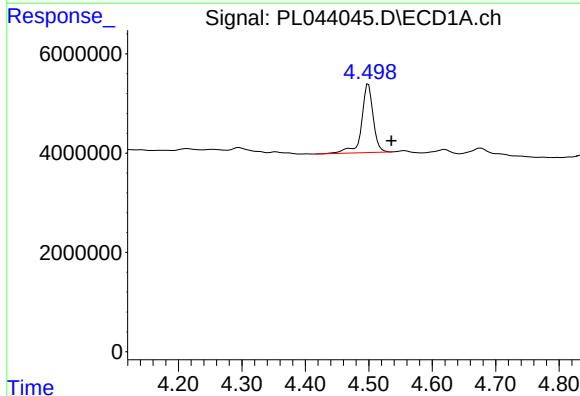


#6 beta-BHC

R.T.: 4.499 min
Delta R.T.: -0.036 min
Response: 17412907
Conc: 4.98 ng/ml

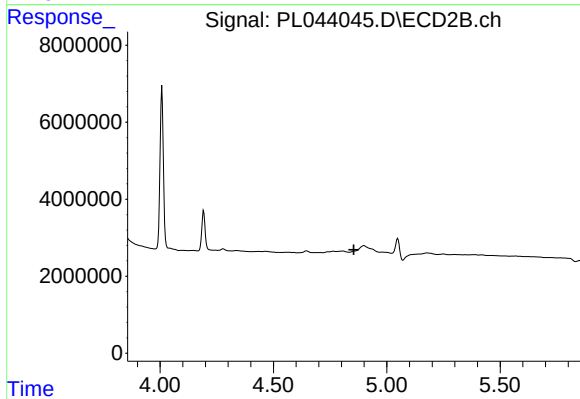

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.854 min
Response: 0
Conc: N.D.

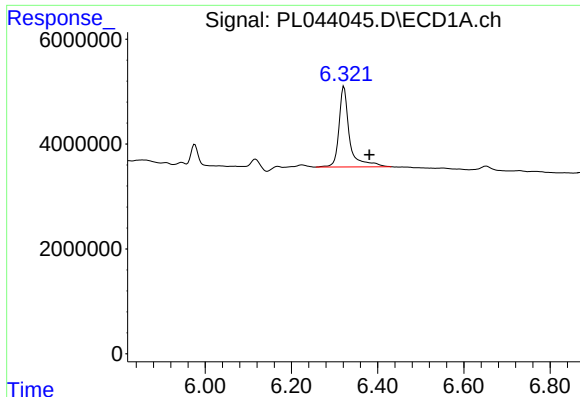

#15 Endosulfan II


R.T.: 6.322 min
Delta R.T.: -0.058 min
Response: 26021362
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0115-S-TCLP-7

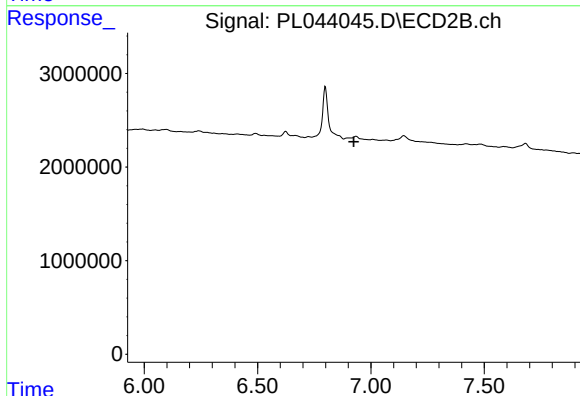


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

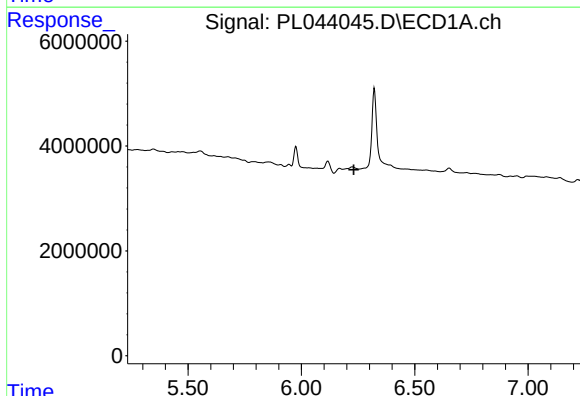


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

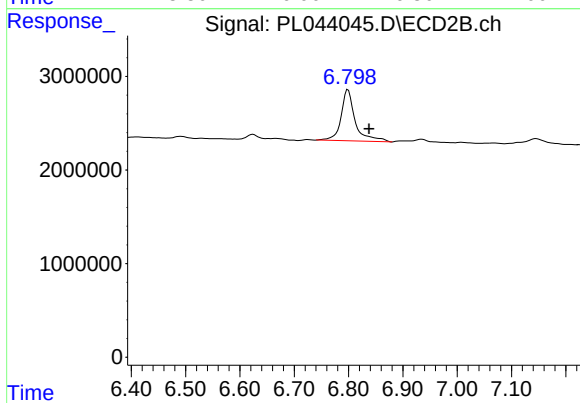

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: -0.038 min
Response: 9903134
Conc: 5.41 ng/ml

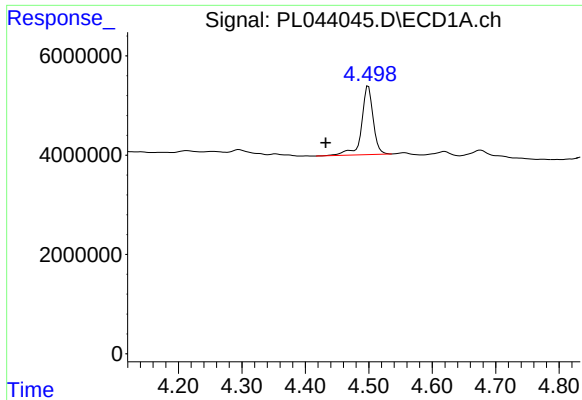

#23 Chlordane-1


R.T.: 4.499 min
Delta R.T.: 0.067 min
Response: 17412907
Conc: 66.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0115-S-TCLP-7

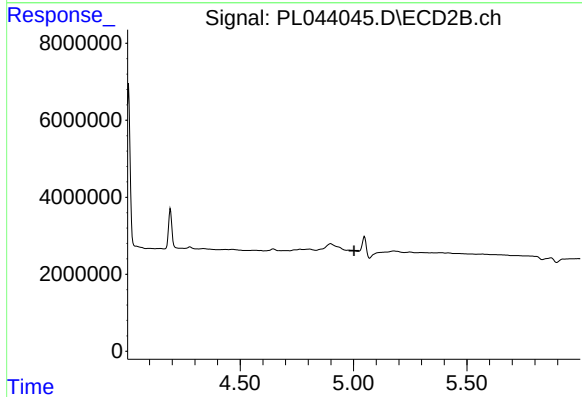


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.003 min
Response: 0
Conc: N.D.

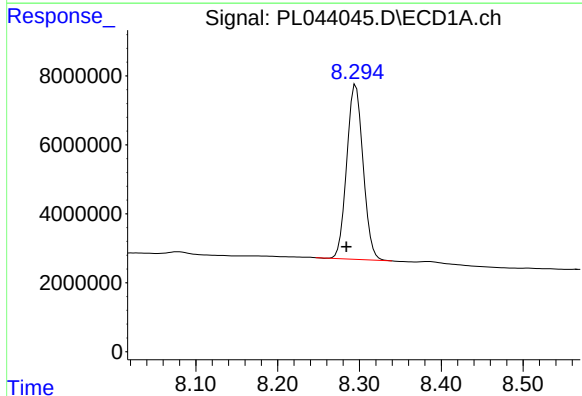

#28 Decachlorobiphenyl

R.T.: 8.295 min
Delta R.T.: 0.011 min
Response: 69886495
Conc: 10.34 ng/ml

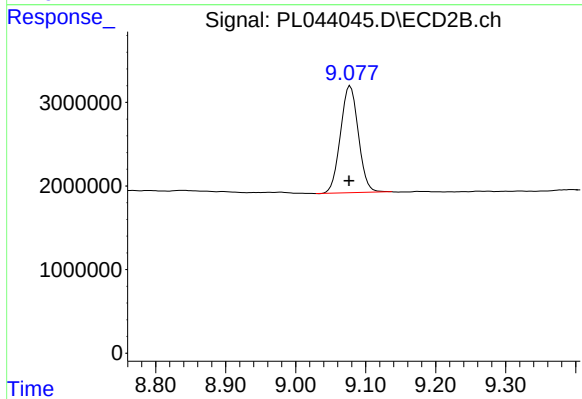

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.002 min
Response: 22659186
Conc: 10.61 ng/ml