

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011720\
 Data File : PL055820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2020 14:45
 Operator : AJ\MA
 Sample : L1008-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-011620

Manual Integrations
 APPROVED

mohammad
 1/20/2020 10:38:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:32:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	126.2E6	33109665	13.662	12.498
28)	SA Decachlor...	8.233	8.954	124.5E6	30028537	14.180	14.443
Target Compounds							
10)	B gamma-Chl...	5.424	6.040	6149040	2087935	0.459m	0.742m#
11)	B alpha-Chl...	5.485	6.113	6318398	3774509	0.481m	1.343m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011720\
Data File : PL055820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2020 14:45
Operator : AJ\MA
Sample : L1008-08
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
CL-01-011620


Manual Integrations
APPROVED

mohammad
1/20/2020 10:38:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:32:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

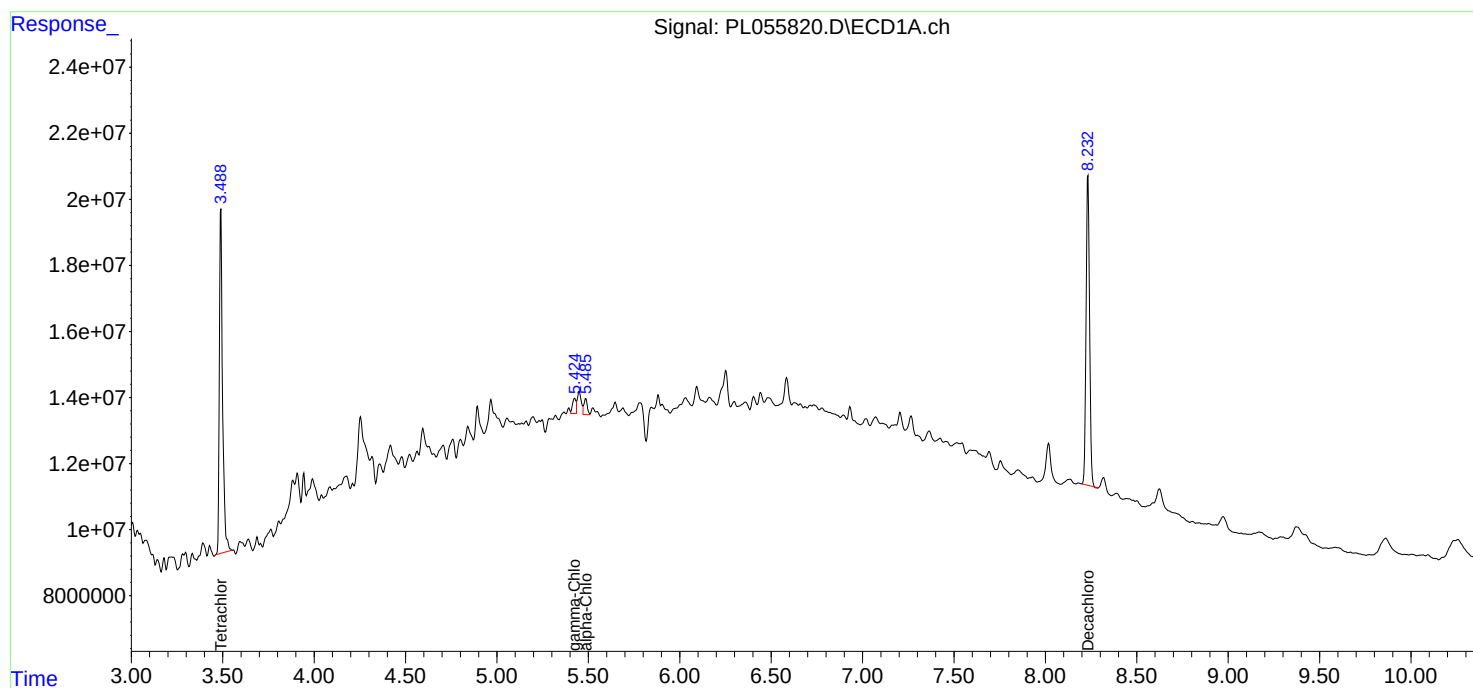

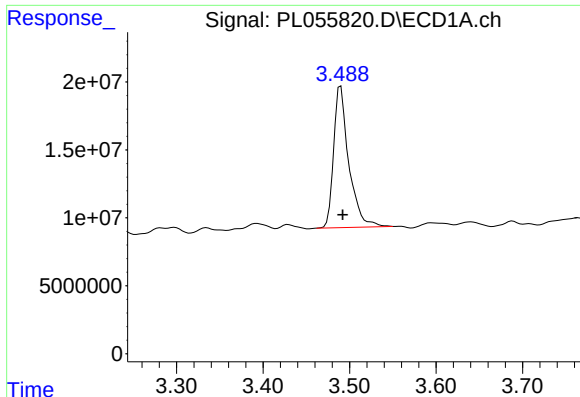


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: -0.002 min
Response: 126246485
Conc: 13.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-011620


Manual Integrations
APPROVED

mohammad
1/20/2020 10:38:07 AM

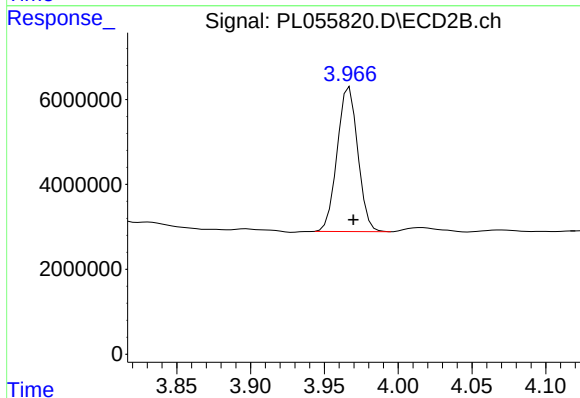


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.003 min
Response: 33109665
Conc: 12.50 ng/ml

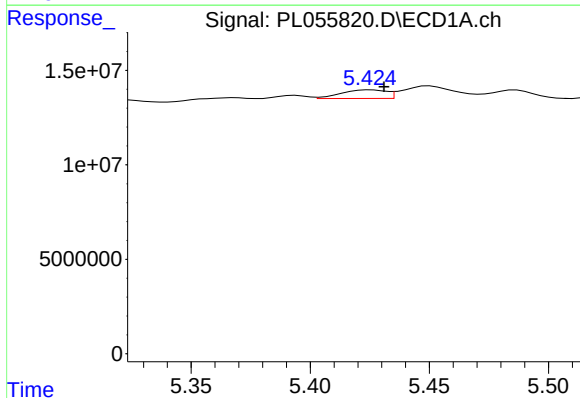


#10 gamma-Chlordane

R.T.: 5.424 min
Delta R.T.: -0.007 min
Response: 6149040
Conc: 0.46 ng/ml m

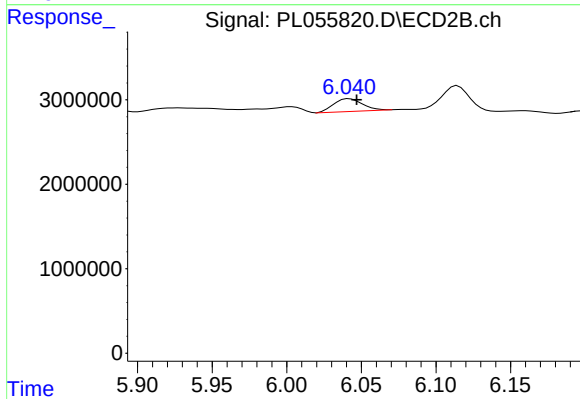

#10 gamma-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.007 min
Response: 2087935
Conc: 0.74 ng/ml m

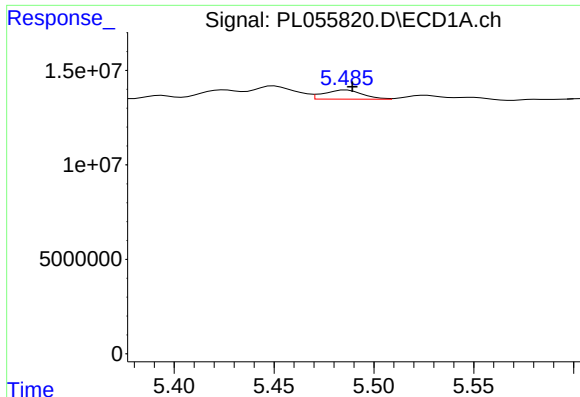


#11 alpha-Chlordane

R.T.: 5.485 min
Delta R.T.: -0.004 min
Response: 6318398
Conc: 0.48 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-01-011620


Manual Integrations
APPROVED

mohammad
1/20/2020 10:38:07 AM

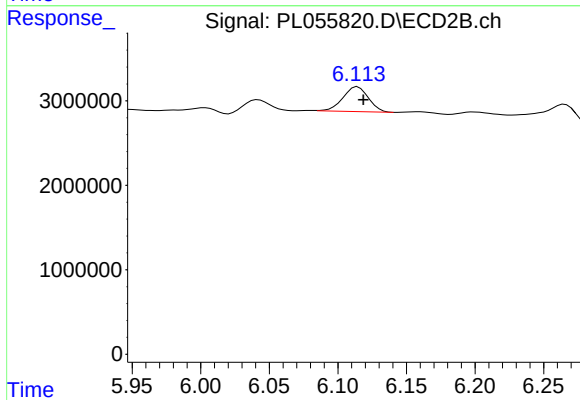


#11 alpha-Chlordane

R.T.: 6.113 min
Delta R.T.: -0.005 min
Response: 3774509
Conc: 1.34 ng/ml m

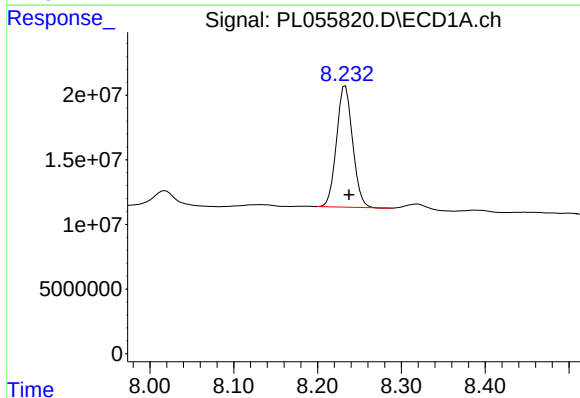

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: -0.004 min
Response: 124528500
Conc: 14.18 ng/ml

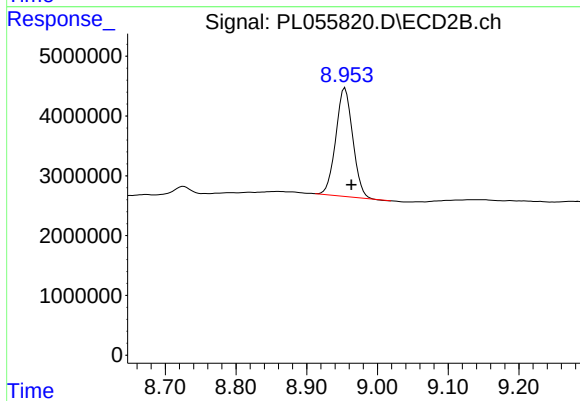

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.009 min
Response: 30028537
Conc: 14.44 ng/ml