

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
 Data File : PL072019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 12:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:29:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 00:27:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.554	5.495	10043891	29382538	18.091	18.091
28)	SA Decachlor...	10.323	11.395	17226487	30305554	19.390	18.782
Target Compounds							
7)	B delta-BHC	0.000	7.020f	0	818356	N.D.	0.333 #
11)	B alpha-Chl...	0.000	8.282f	0	207402	N.D.	0.105 #
13)	MA Dieldrin	0.000	8.657	0	270659	N.D.	0.138 #
15)	B Endosulfa...	8.263f	9.154f	371227	443747	0.499	0.259 #
16)	A 4,4'-DDD	0.000	9.042	0	156100	N.D.	0.109 #
17)	MA 4,4'-DDT	0.000	9.346	0	301358	N.D.	0.191 #
19)	B Endosulfa...	0.000	9.501	0	328021	N.D.	0.210 #
21)	B Endrin ke...	0.000	10.024f	0	27647	N.D.	0.017 #
26)	Chlordane-4	0.000	8.282f	0	207402	N.D.	0.625 #
27)	Chlordane-5	0.000	9.191	0	13290	N.D.	0.218 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
Data File : PL072019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 12:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:29:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 00:27:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

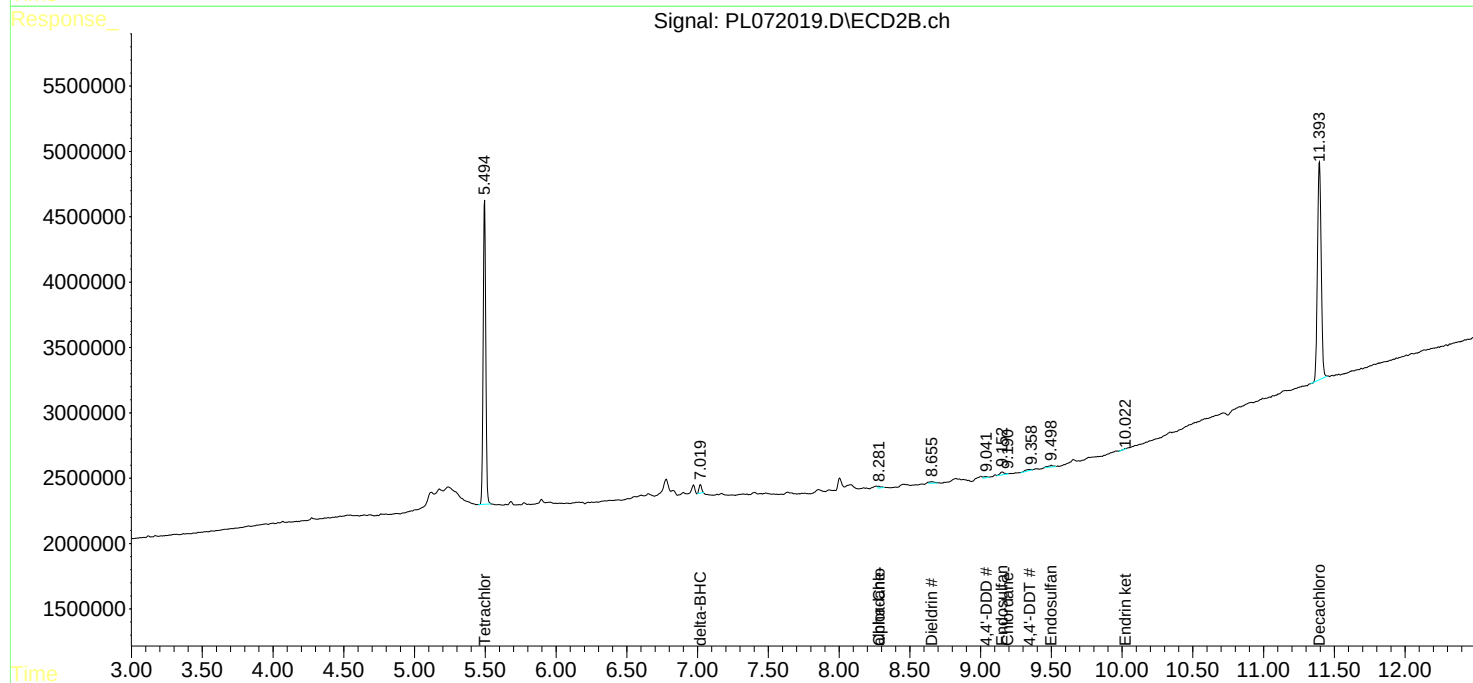


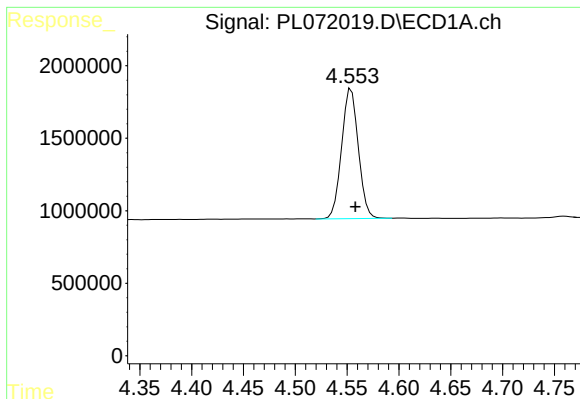

#1 Tetrachloro-m-xylene


R.T.: 4.554 min
Delta R.T.: -0.004 min
Response: 10043891
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

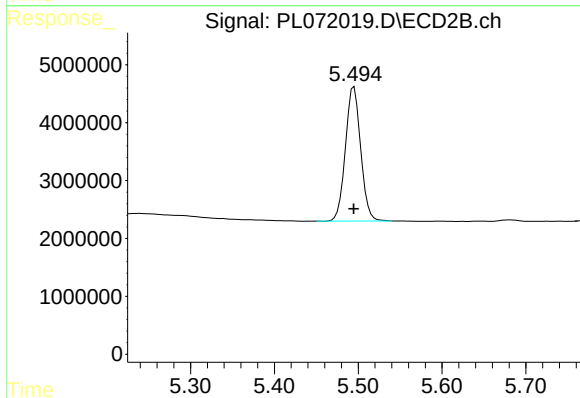


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 29382538
Conc: 18.09 ng/ml

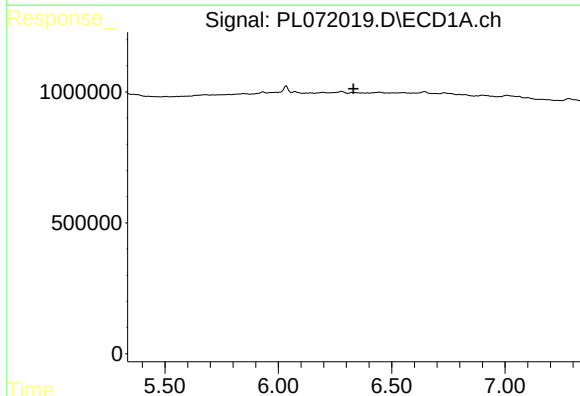


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

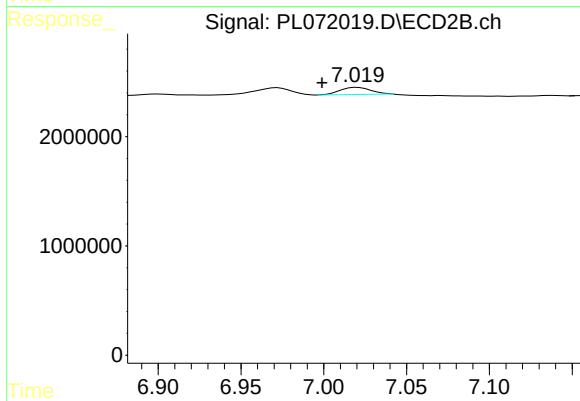

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.021 min
Response: 818356
Conc: 0.33 ng/ml

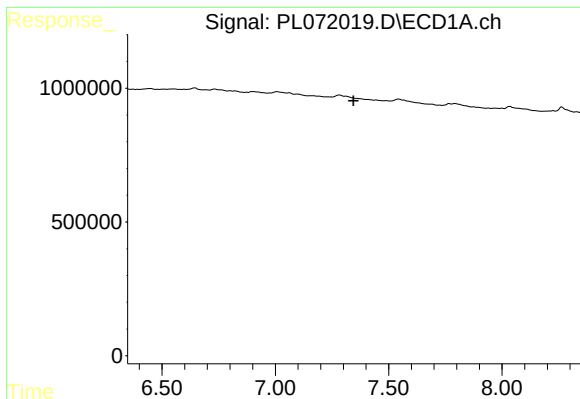

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

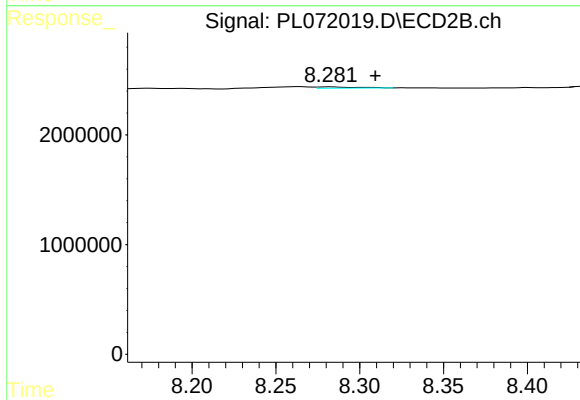


#11 alpha-Chlordane

R.T.: 8.282 min
Delta R.T.: -0.027 min
Response: 207402
Conc: 0.10 ng/ml

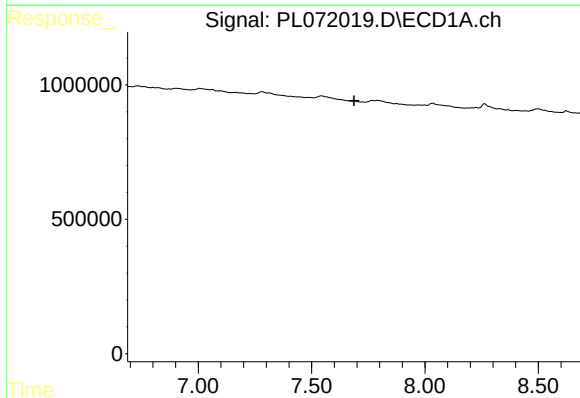


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.687 min
Response: 0
Conc: N.D.

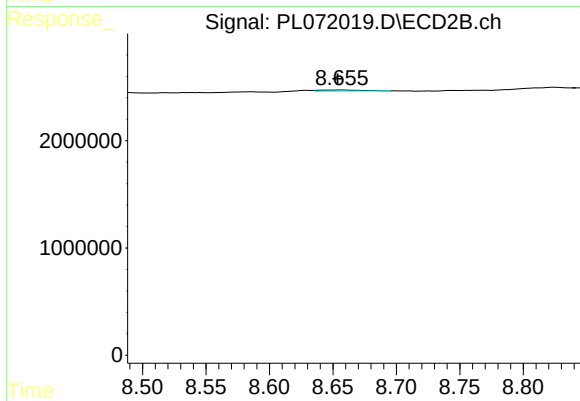

#13 Dieldrin


R.T.: 8.657 min
Delta R.T.: 0.003 min
Response: 270659
Conc: 0.14 ng/ml

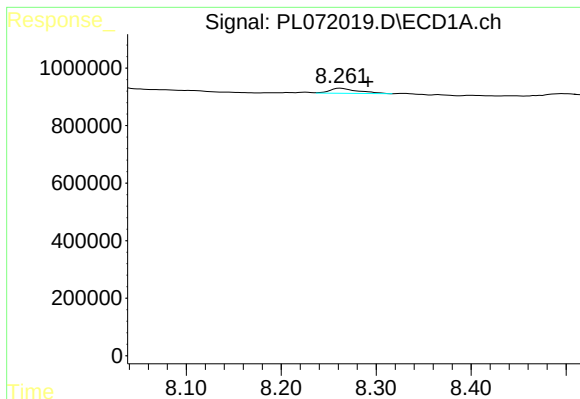

#15 Endosulfan II


R.T.: 8.263 min
Delta R.T.: -0.029 min
Response: 371227
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

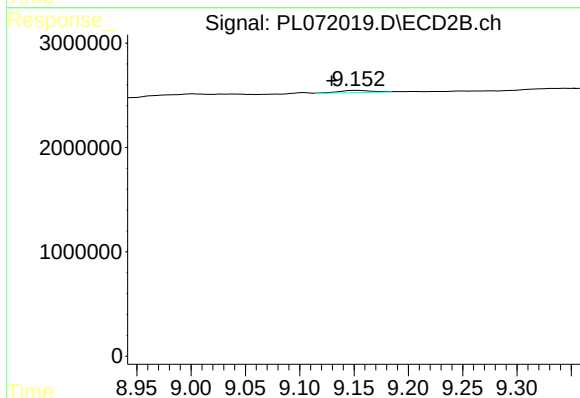


#15 Endosulfan II

R.T.: 9.154 min
Delta R.T.: 0.024 min
Response: 443747
Conc: 0.26 ng/ml

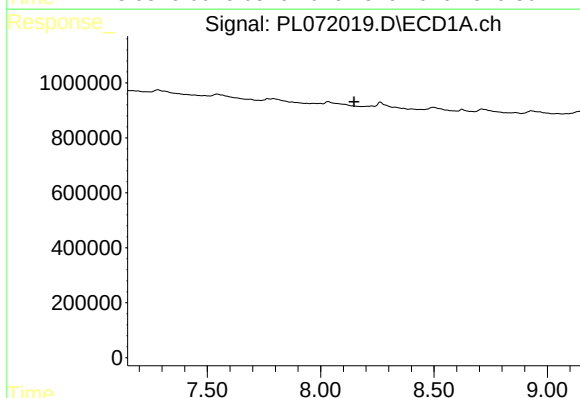


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.

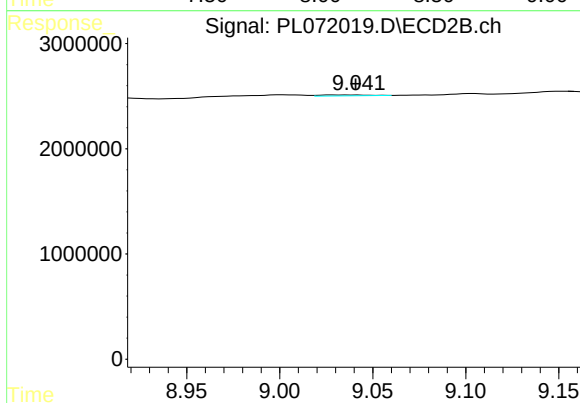

#16 4,4'-DDD


R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 156100
Conc: 0.11 ng/ml

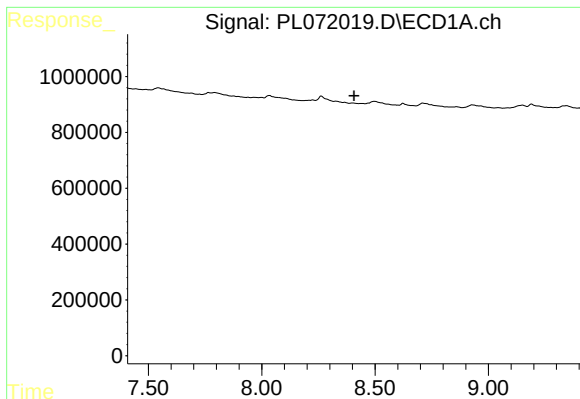

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

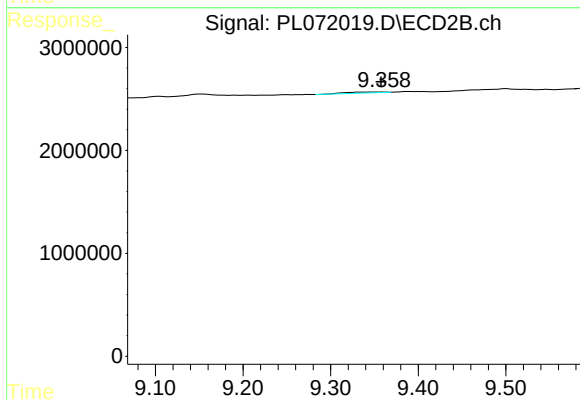


#17 4,4'-DDT

R.T.: 9.346 min
Delta R.T.: -0.012 min
Response: 301358
Conc: 0.19 ng/ml

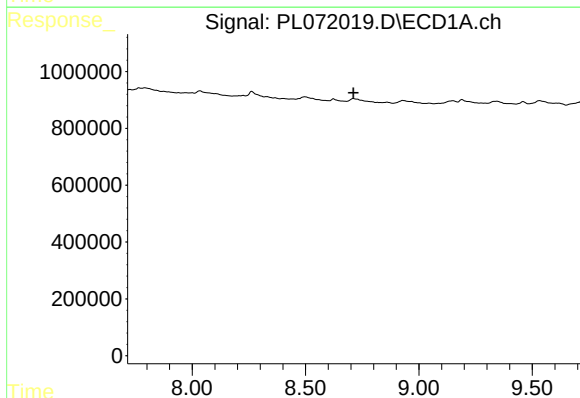


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

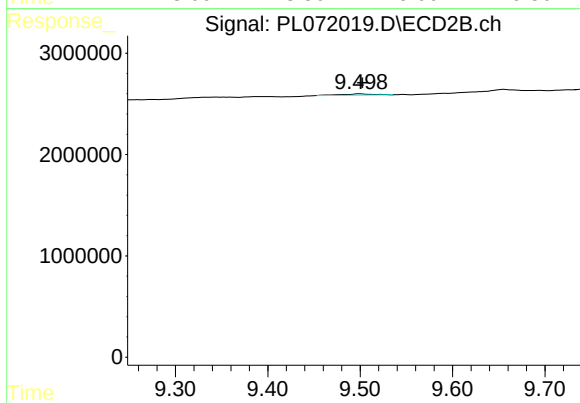

#19 Endosulfan Sulfate


R.T.: 9.501 min
Delta R.T.: -0.002 min
Response: 328021
Conc: 0.21 ng/ml

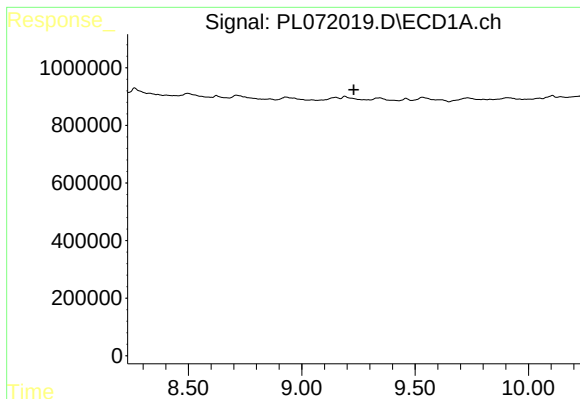

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

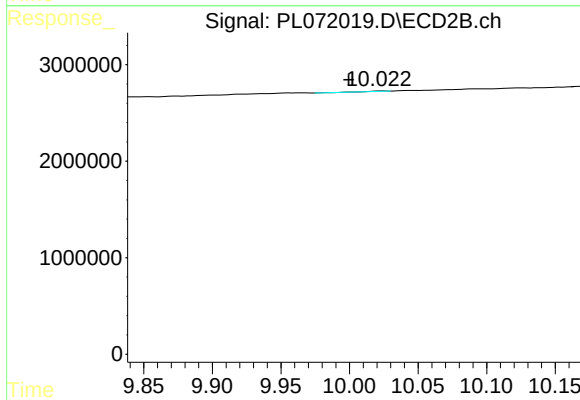


#21 Endrin ketone

R.T.: 10.024 min
Delta R.T.: 0.024 min
Response: 27647
Conc: 0.02 ng/ml

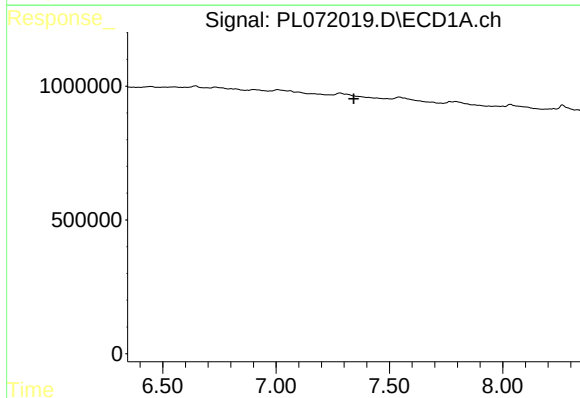


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

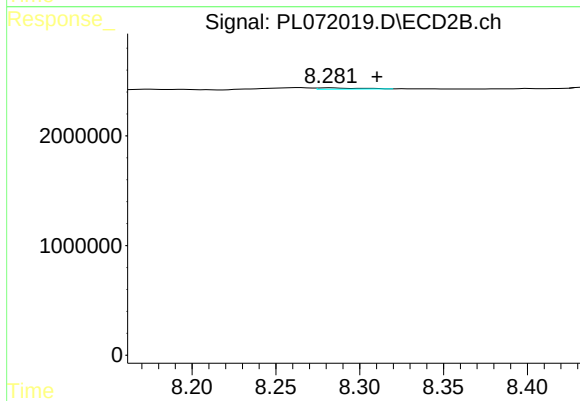

#26 Chlordane-4


R.T.: 8.282 min
Delta R.T.: -0.028 min
Response: 207402
Conc: 0.62 ng/ml

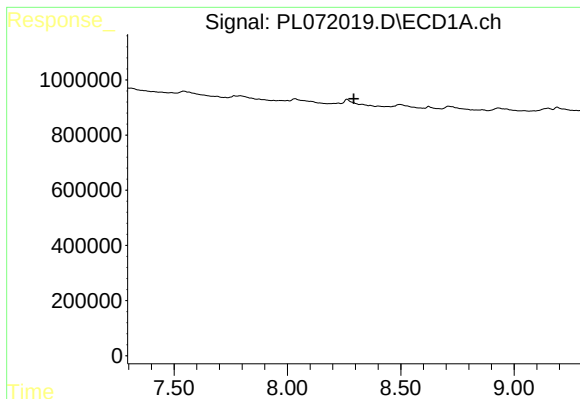

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

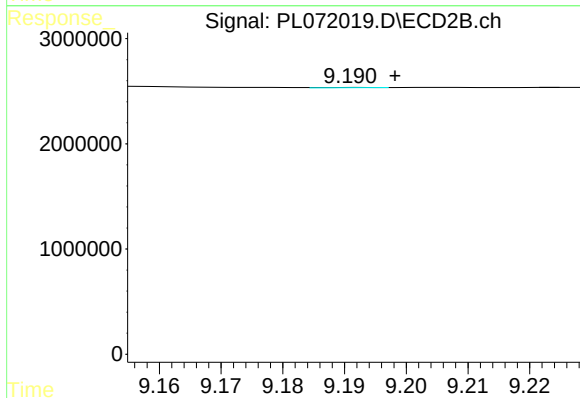


#27 Chlordane-5

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 13290
Conc: 0.22 ng/ml

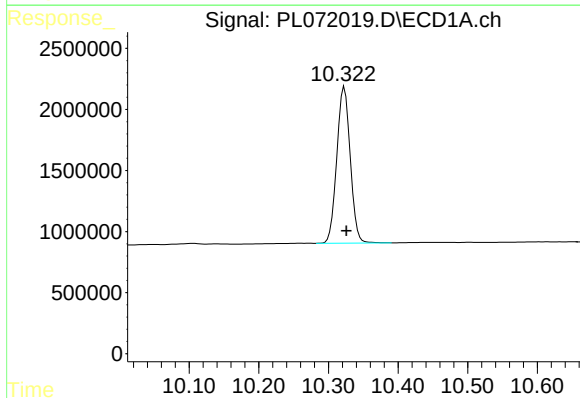

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.003 min
Response: 17226487
Conc: 19.39 ng/ml

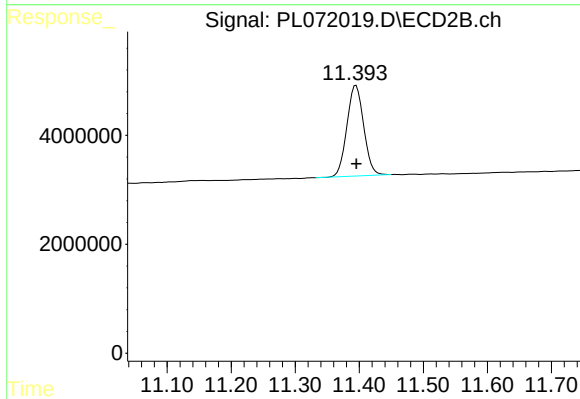

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.000 min
Response: 30305554
Conc: 18.78 ng/ml