

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
 Data File : PL072030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 15:43
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:14:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 00:05:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.495	14459964	41182533	24.637	24.749
28)	SA Decachlor...	10.326	11.396	23208478	42189976	26.487	25.651
Target Compounds							
23)	Chlordane-1	5.884	6.878	4989357	15779692	240.993	240.365
24)	Chlordane-2	6.575	7.472	6860825	17481179	253.319	251.546
25)	Chlordane-3	7.276	8.230	18532233	68216382	241.311	242.721
26)	Chlordane-4	7.344	8.311	20065314	81932576	242.868	245.857
27)	Chlordane-5	8.294	9.199	7134097	14920345	248.641	245.344



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
Data File : PL072030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 15:43
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:14:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 00:05:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

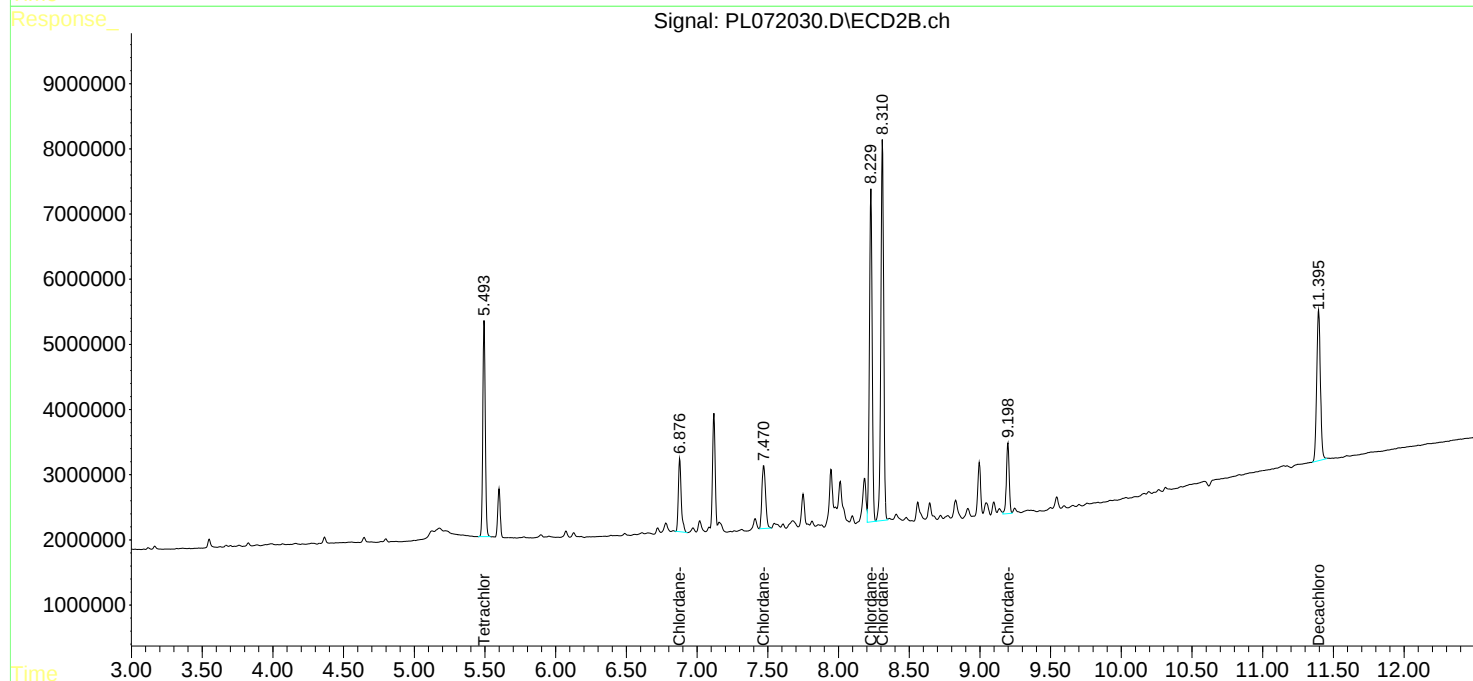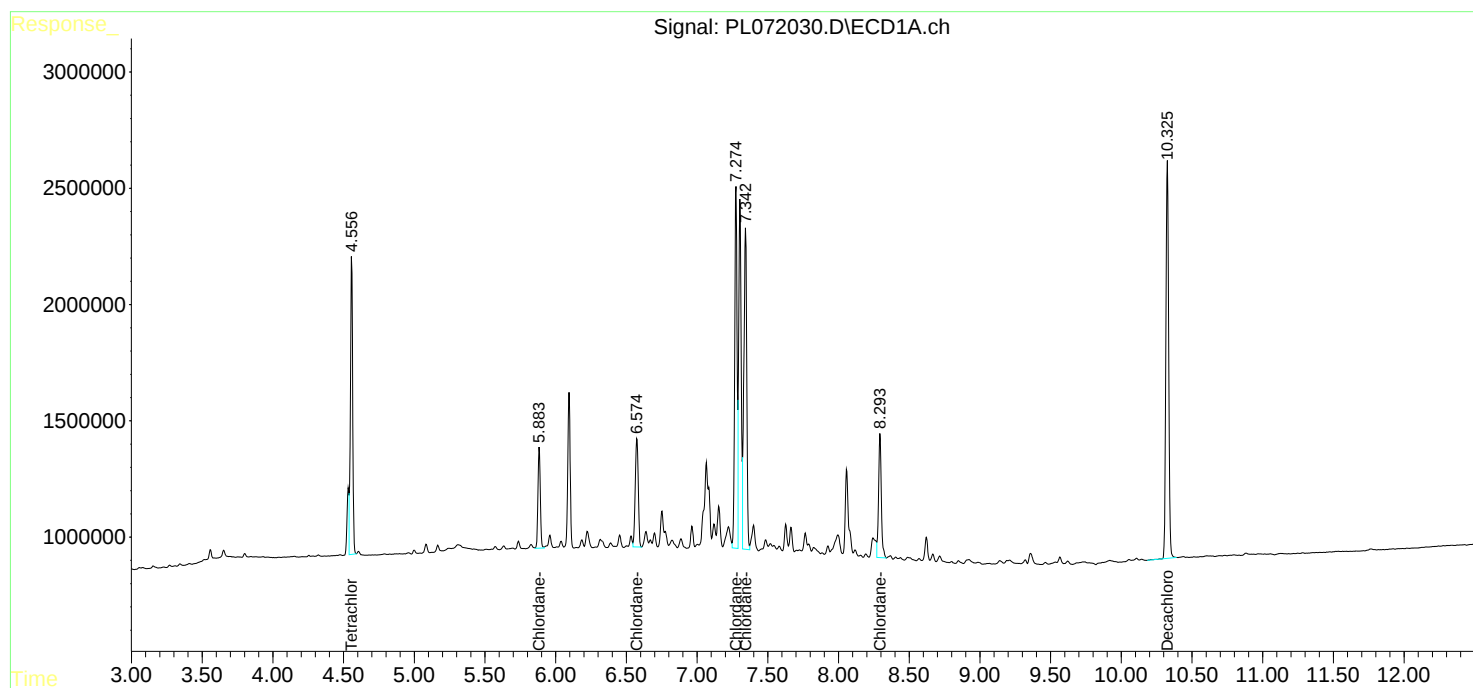


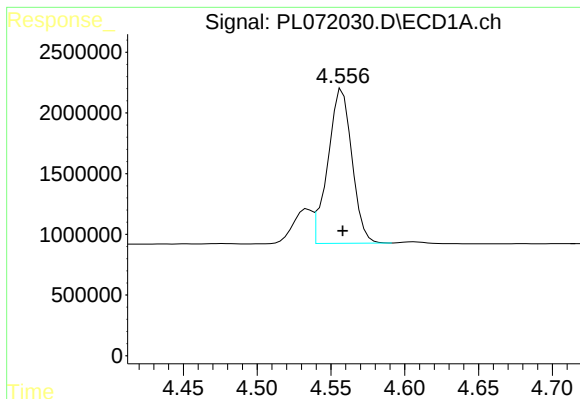

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 14459964
Conc: 24.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

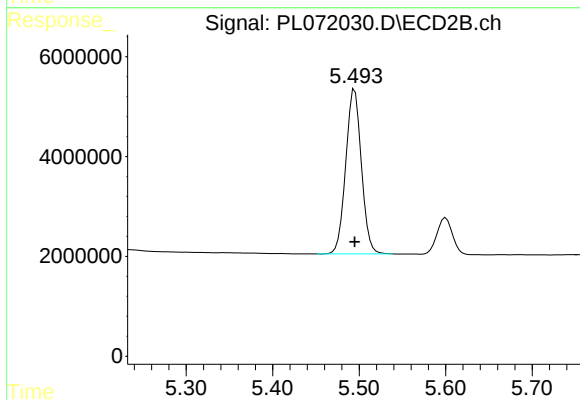


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 41182533
Conc: 24.75 ng/ml

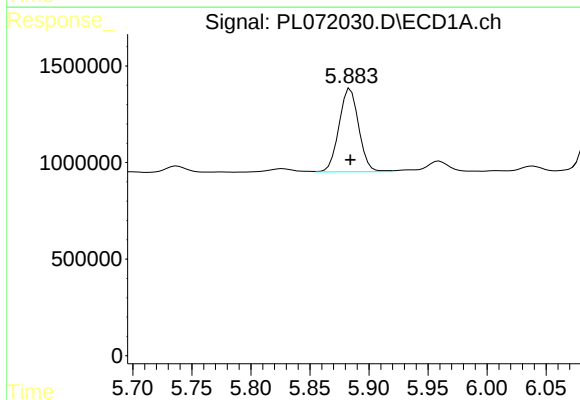


#23 Chlordane-1

R.T.: 5.884 min
Delta R.T.: 0.000 min
Response: 4989357
Conc: 240.99 ng/ml

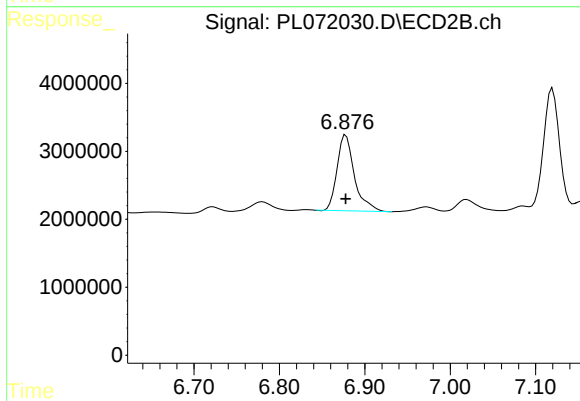

#23 Chlordane-1


R.T.: 6.878 min
Delta R.T.: 0.000 min
Response: 15779692
Conc: 240.36 ng/ml

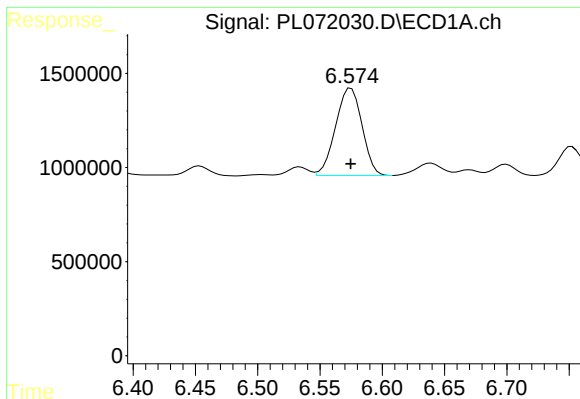

#24 Chlordane-2


R.T.: 6.575 min
Delta R.T.: 0.000 min
Response: 6860825
Conc: 253.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

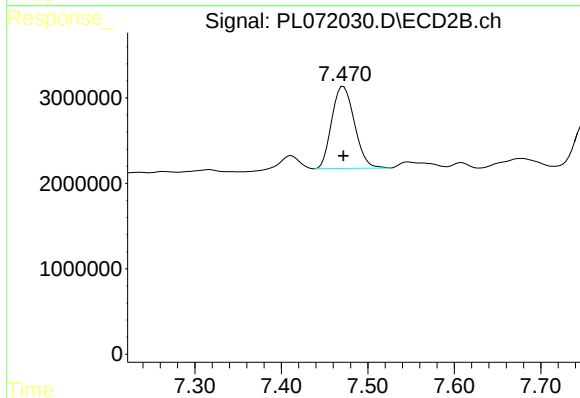


#24 Chlordane-2

R.T.: 7.472 min
Delta R.T.: 0.000 min
Response: 17481179
Conc: 251.55 ng/ml

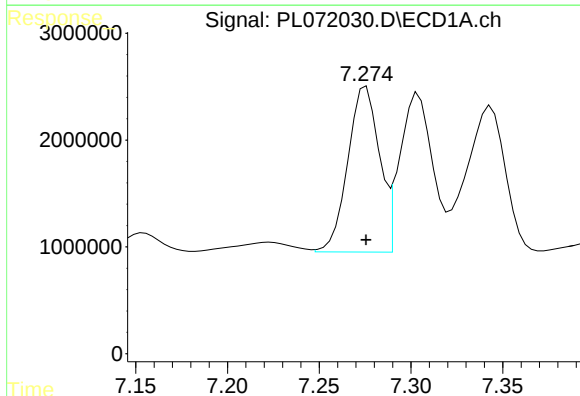


#25 Chlordane-3

R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 18532233
Conc: 241.31 ng/ml

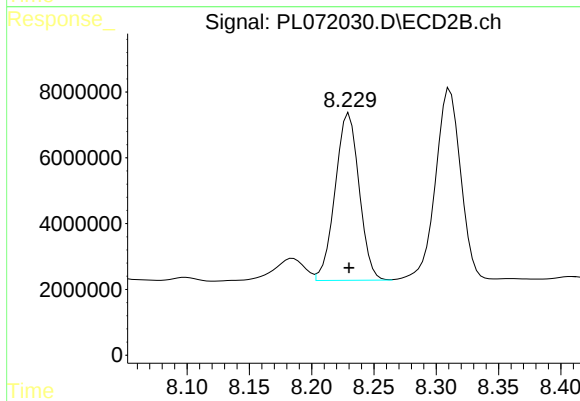

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 68216382
Conc: 242.72 ng/ml

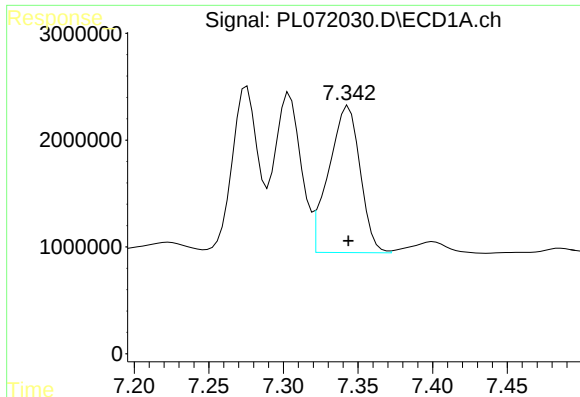

#26 Chlordane-4


R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 20065314
Conc: 242.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

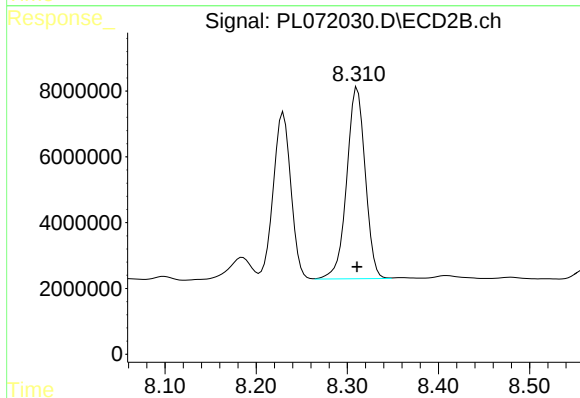


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 81932576
Conc: 245.86 ng/ml

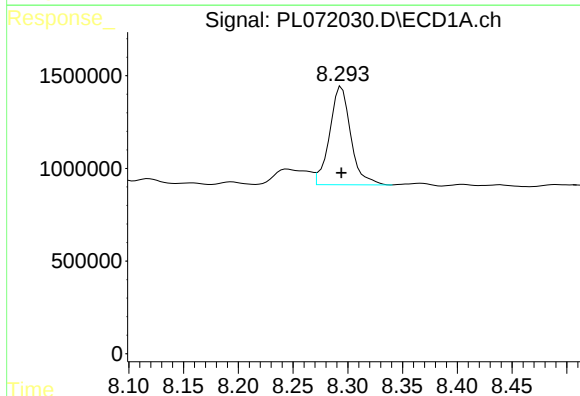


#27 Chlordane-5

R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 7134097
Conc: 248.64 ng/ml

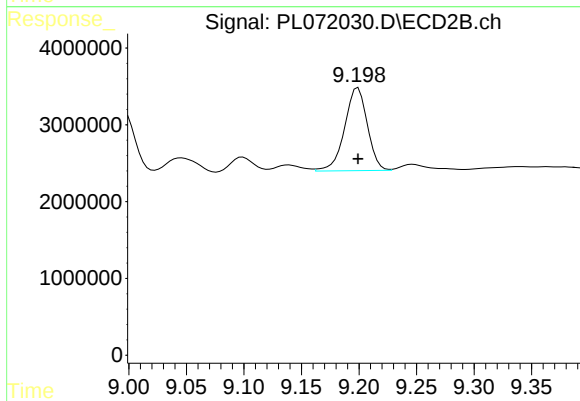

#27 Chlordane-5


R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 14920345
Conc: 245.34 ng/ml

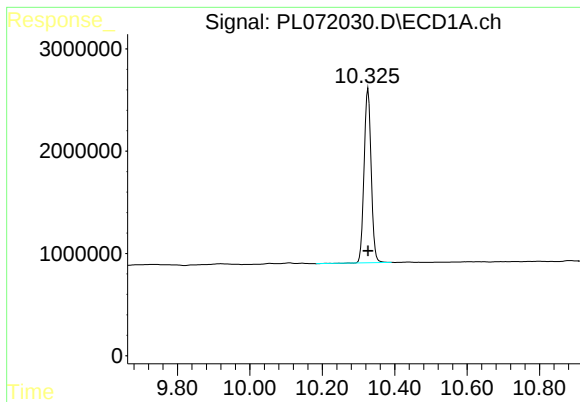

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 23208478
Conc: 26.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

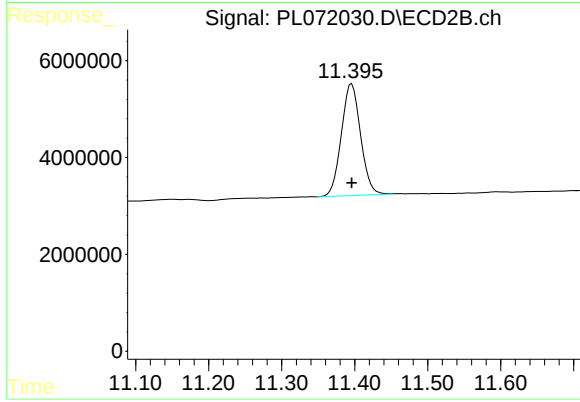

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.000 min
Response: 42189976
Conc: 25.65 ng/ml