

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
 Data File : PL072027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 14:54
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:10:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 00:05:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.495	59357230	168.5E6	100.479	100.436
28)	SA Decachlor...	10.326	11.395	83460014	160.1E6	96.466	97.636
Target Compounds							
23)	Chlordane-1	5.885	6.877	21047396	66976118	1000.586	1006.593
24)	Chlordane-2	6.574	7.471	26475699	68236006	978.444	982.556
25)	Chlordane-3	7.275	8.229	78493190	286.9E6	1007.965	1007.318
26)	Chlordane-4	7.343	8.310	84532202	336.6E6	1006.229	1000.185
27)	Chlordane-5	8.294	9.199	28930468	61807778	1003.763	1002.076



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
Data File : PL072027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 14:54
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:10:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 00:05:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

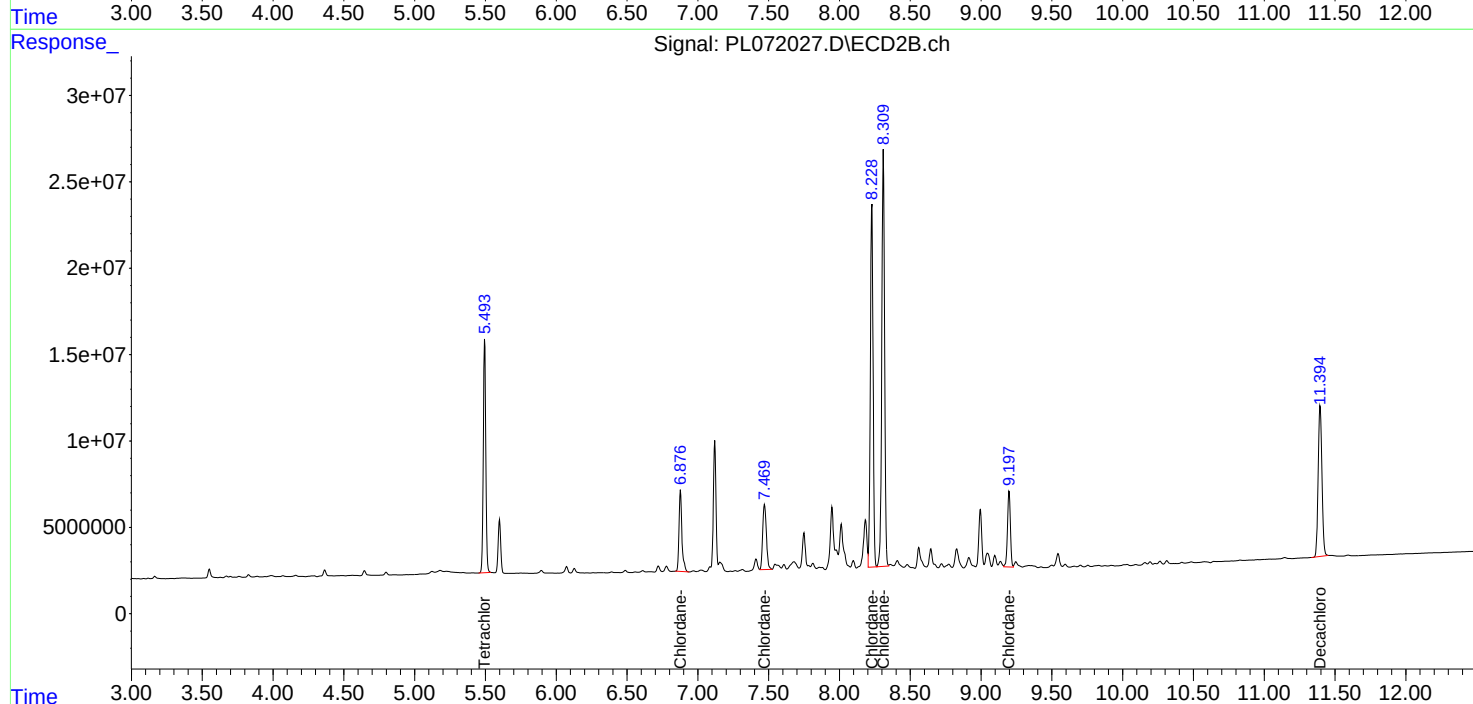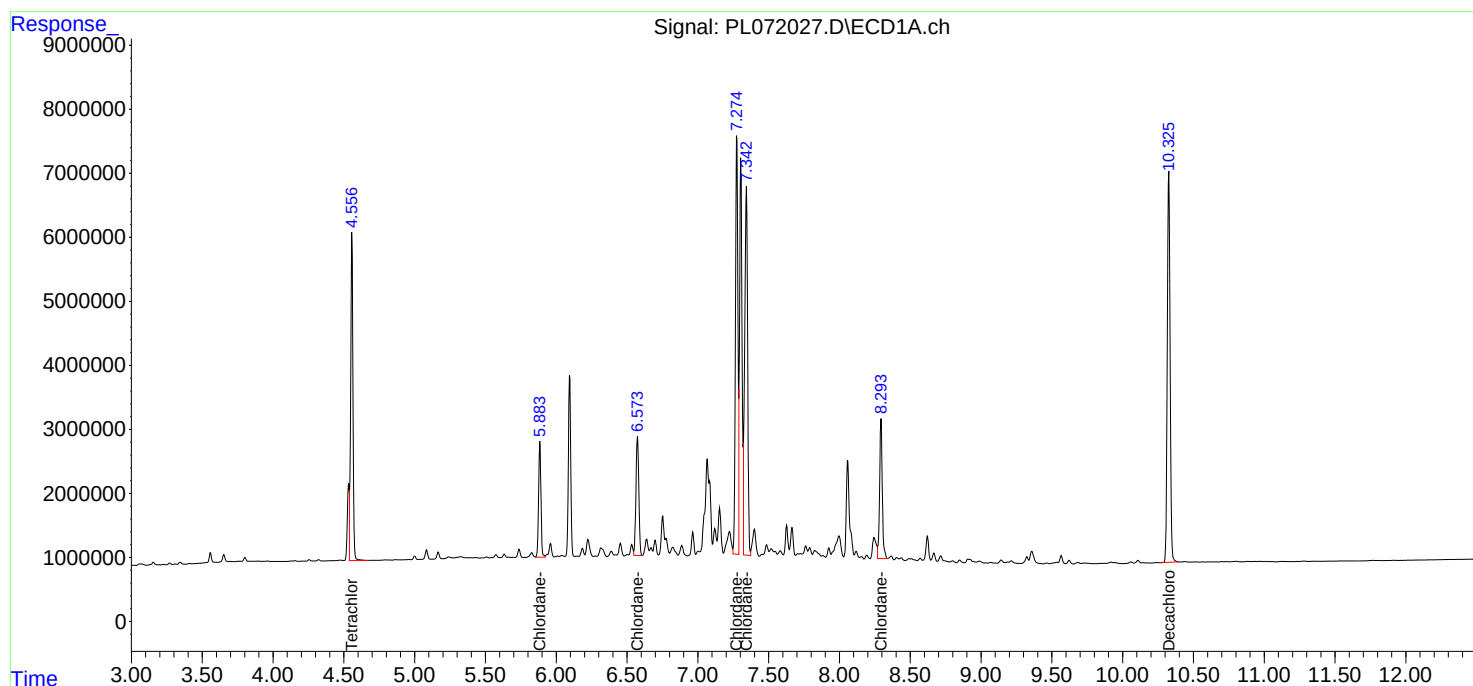


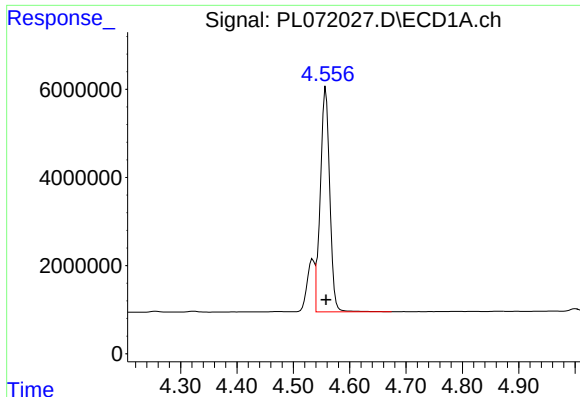

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 59357230
Conc: 100.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

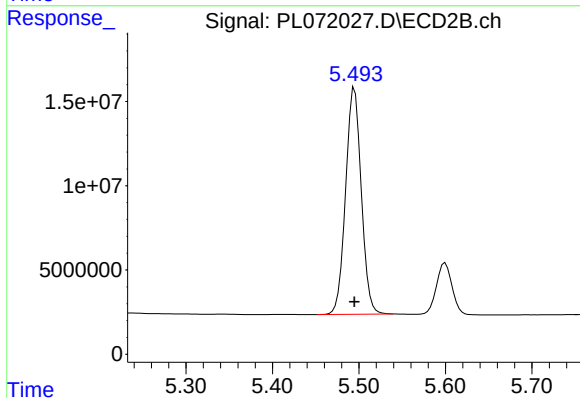


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 168480743
Conc: 100.44 ng/ml

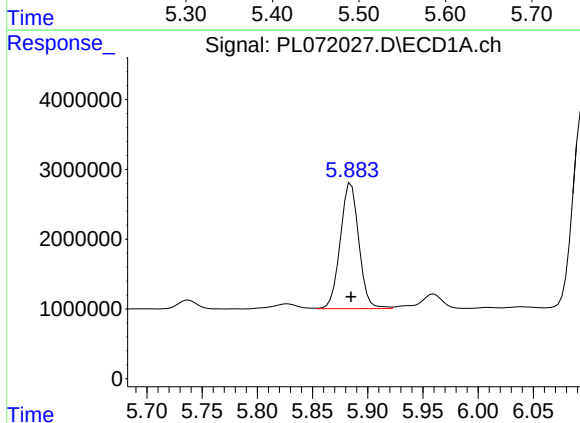


#23 Chlordane-1

R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 21047396
Conc: 1000.59 ng/ml

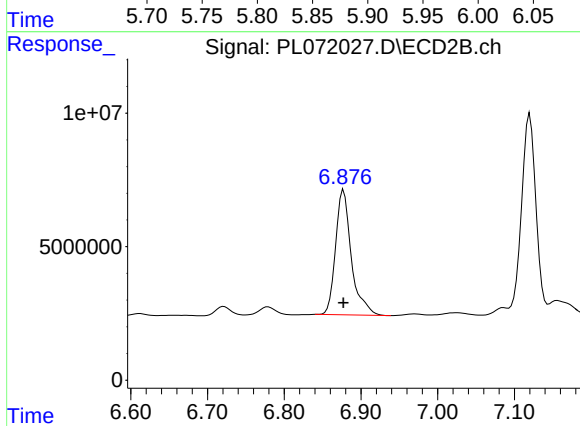

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 66976118
Conc: 1006.59 ng/ml

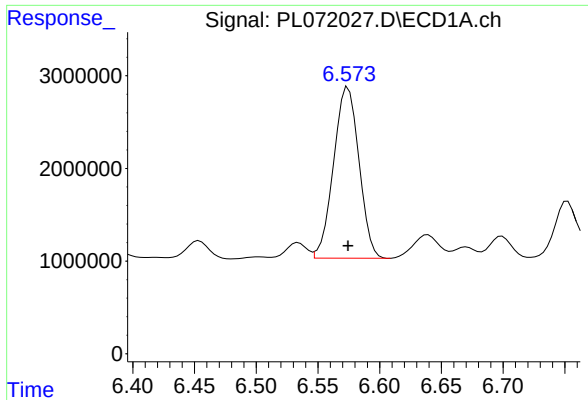

#24 Chlordane-2


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 26475699
Conc: 978.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

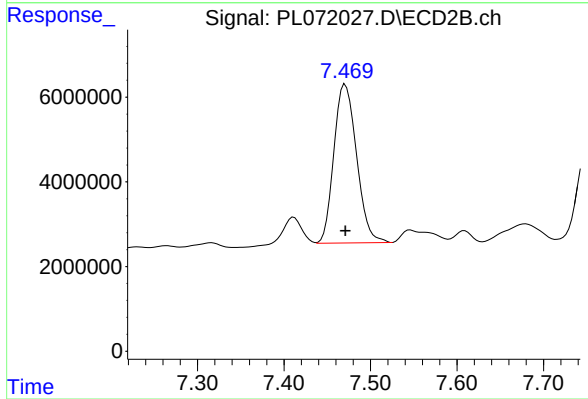


#24 Chlordane-2

R.T.: 7.471 min
Delta R.T.: 0.000 min
Response: 68236006
Conc: 982.56 ng/ml

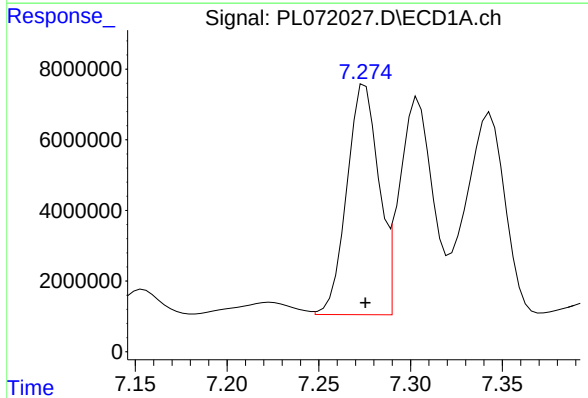


#25 Chlordane-3

R.T.: 7.275 min
Delta R.T.: 0.000 min
Response: 78493190
Conc: 1007.97 ng/ml

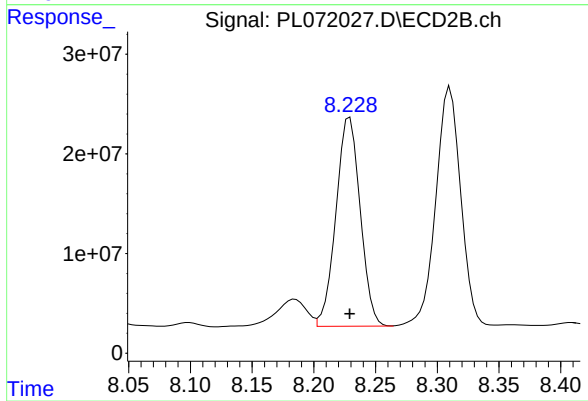

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 286897546
Conc: 1007.32 ng/ml

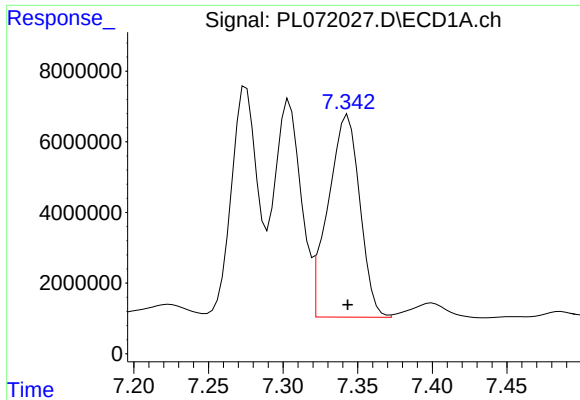

#26 Chlordane-4


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 84532202
Conc: 1006.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

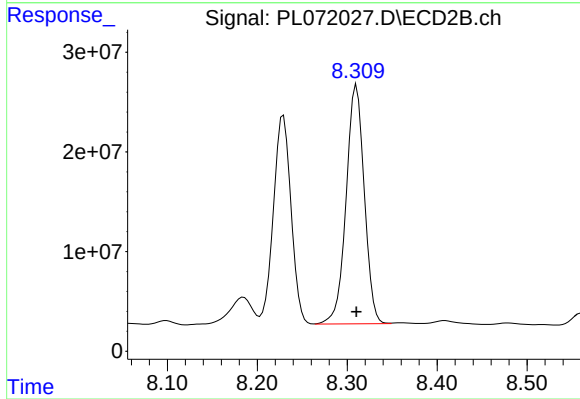


#26 Chlordane-4

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 336559431
Conc: 1000.18 ng/ml

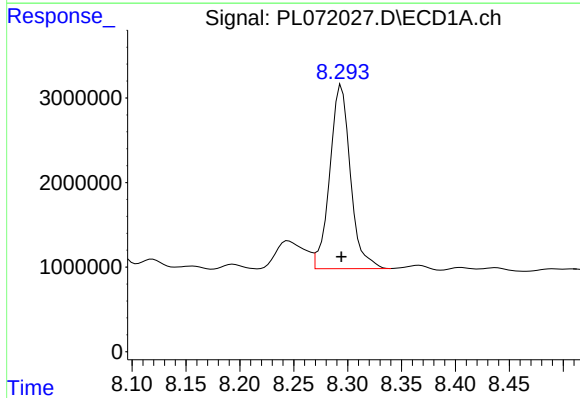


#27 Chlordane-5

R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 28930468
Conc: 1003.76 ng/ml

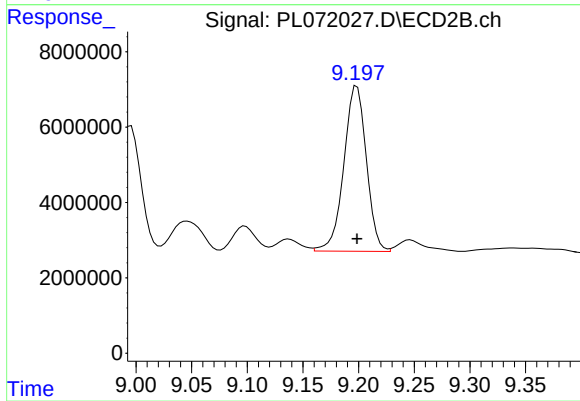

#27 Chlordane-5


R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 61807778
Conc: 1002.08 ng/ml

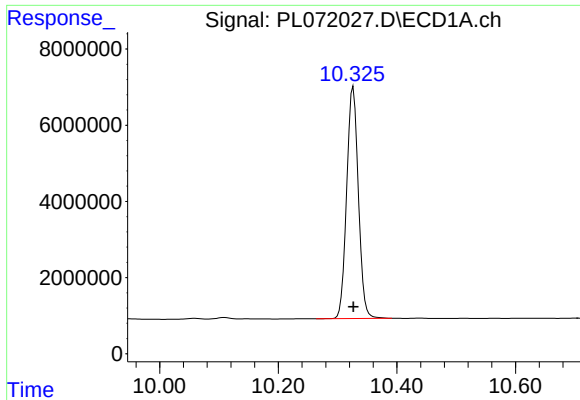

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 83460014
Conc: 96.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

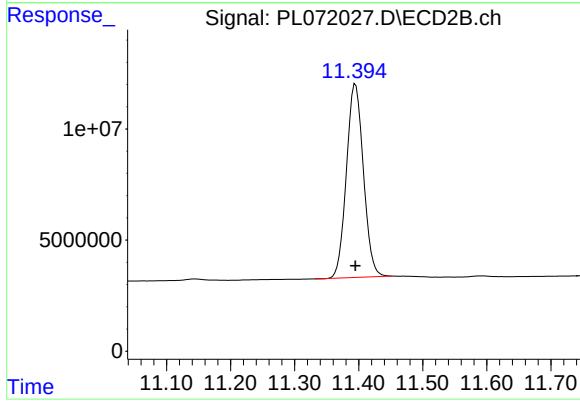

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.000 min
Response: 160121717
Conc: 97.64 ng/ml