

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
 Data File : PL072028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 15:10
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:12:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 00:05:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	44083084	124.0E6	74.748	74.288
28)	SA Decachlor...	10.326	11.395	63468165	120.9E6	73.898	74.128
Target Compounds							
23)	Chlordane-1	5.884	6.877	15589215	49801677	744.047	748.983
24)	Chlordane-2	6.574	7.471	20080229	51870268	744.709	747.930
25)	Chlordane-3	7.275	8.229	57988314	211.3E6	746.427	744.517
26)	Chlordane-4	7.343	8.310	61645673	249.2E6	739.121	743.714
27)	Chlordane-5	8.294	9.198	21441712	45161646	745.946	738.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
Data File : PL072028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 15:10
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:12:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 00:05:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

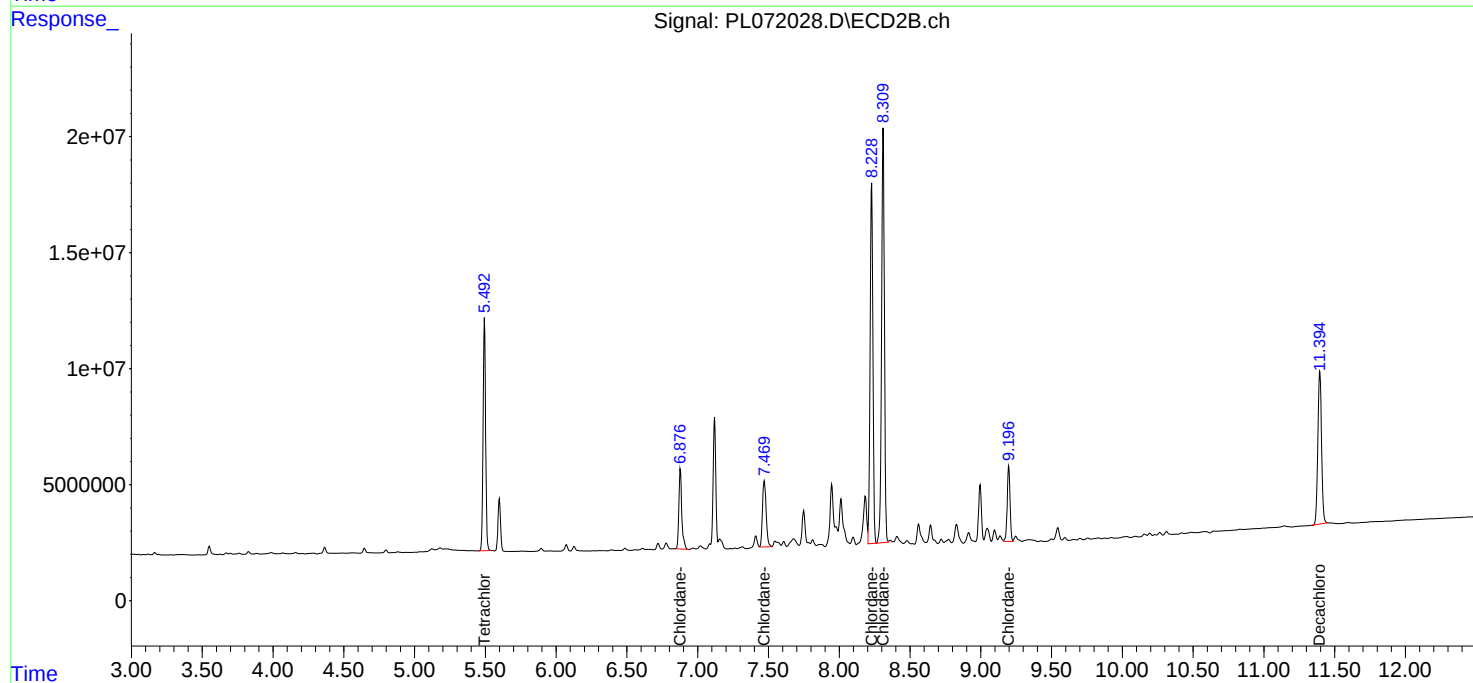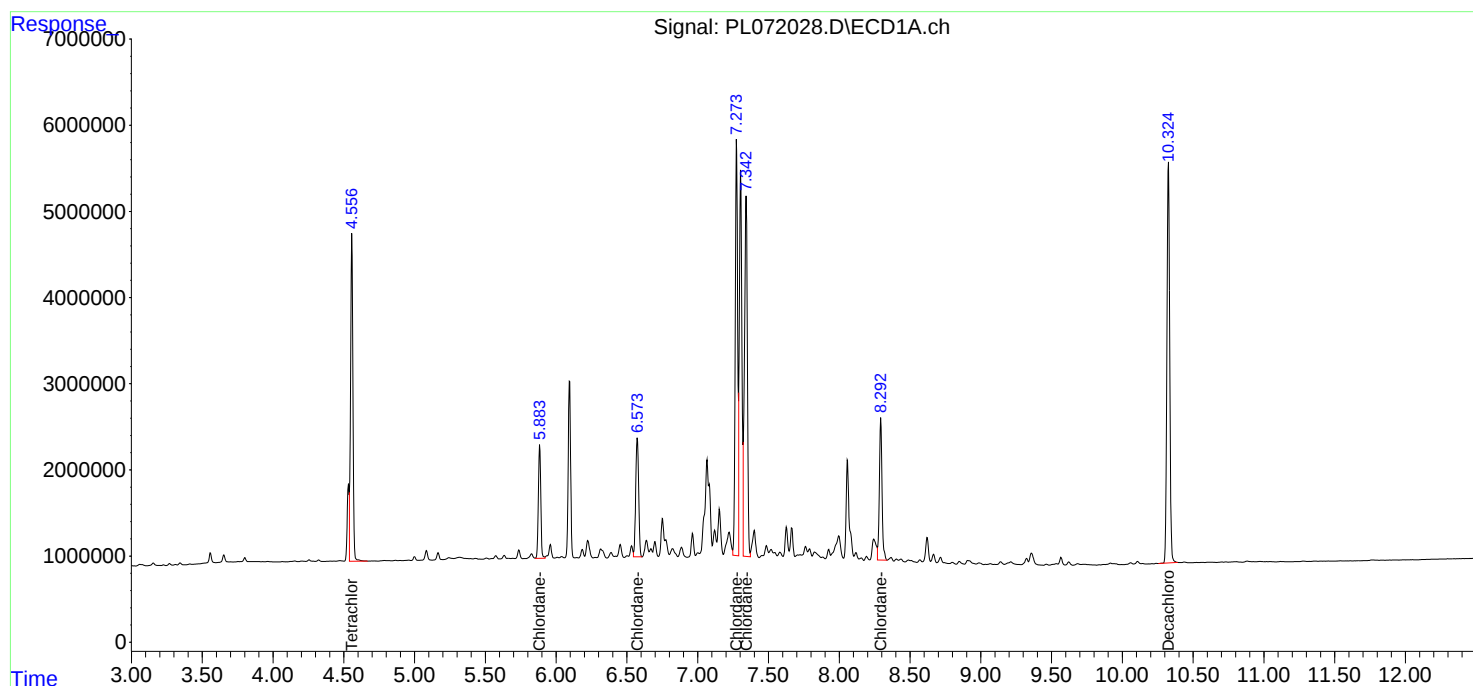


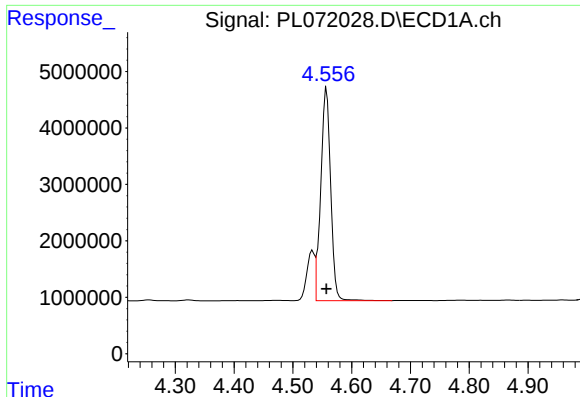

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 44083084
Conc: 74.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

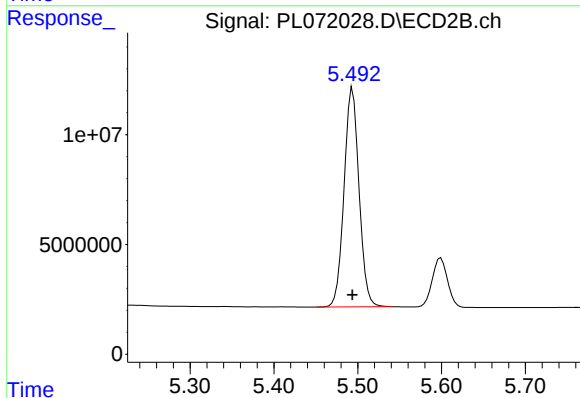


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 124029722
Conc: 74.29 ng/ml

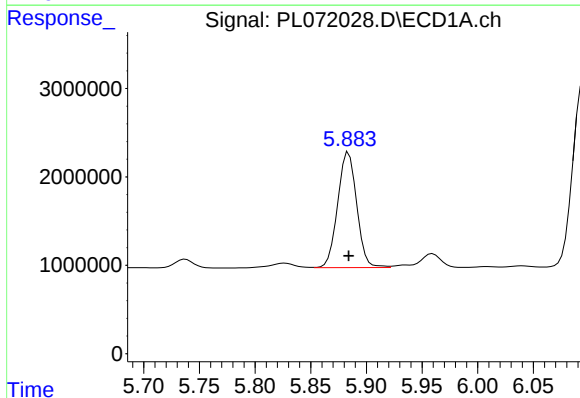


#23 Chlordane-1

R.T.: 5.884 min
Delta R.T.: 0.000 min
Response: 15589215
Conc: 744.05 ng/ml

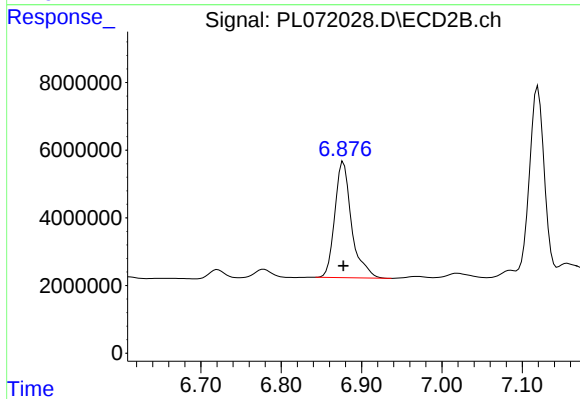

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 49801677
Conc: 748.98 ng/ml

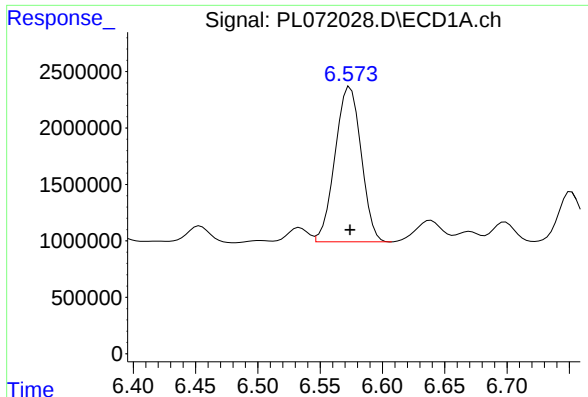

#24 Chlordane-2


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 20080229
Conc: 744.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

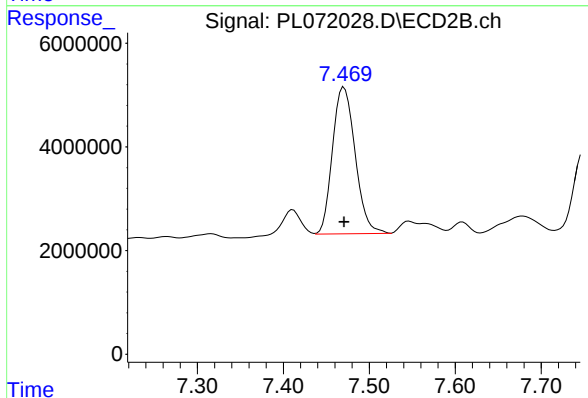


#24 Chlordane-2

R.T.: 7.471 min
Delta R.T.: 0.000 min
Response: 51870268
Conc: 747.93 ng/ml

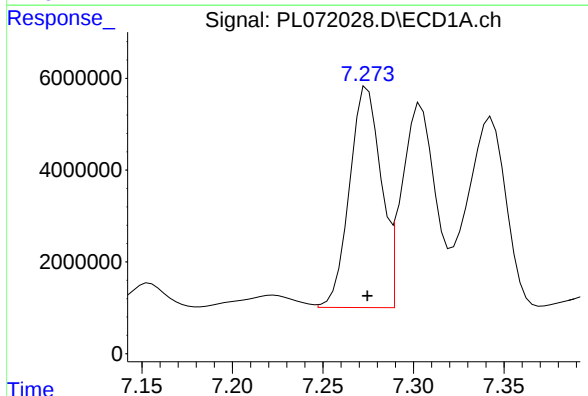


#25 Chlordane-3

R.T.: 7.275 min
Delta R.T.: 0.000 min
Response: 57988314
Conc: 746.43 ng/ml

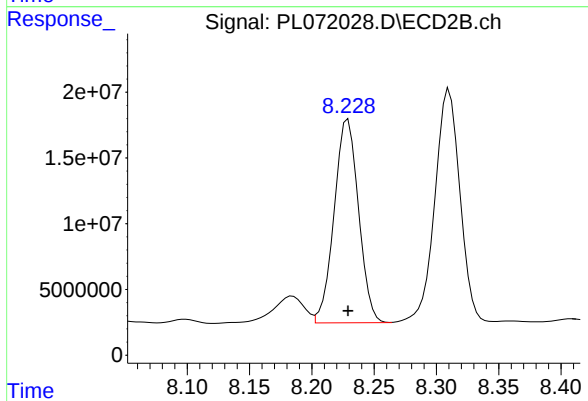

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 211276091
Conc: 744.52 ng/ml

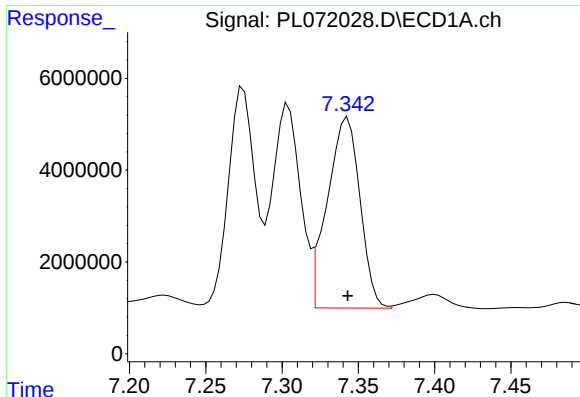

#26 Chlordane-4


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 61645673
Conc: 739.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

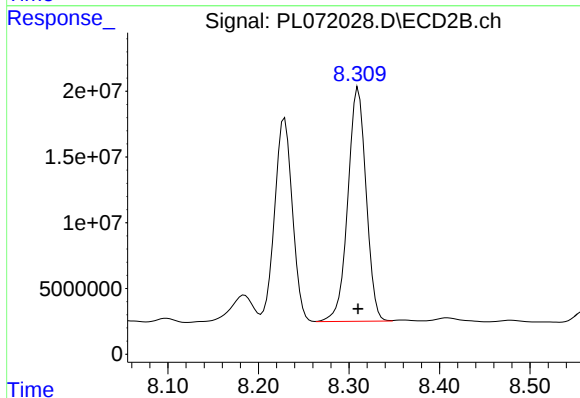


#26 Chlordane-4

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 249213567
Conc: 743.71 ng/ml

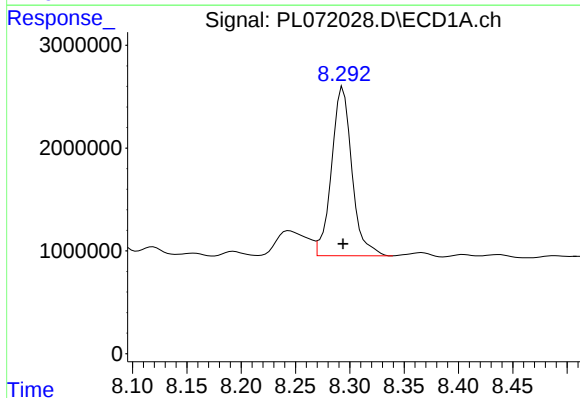


#27 Chlordane-5

R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 21441712
Conc: 745.95 ng/ml

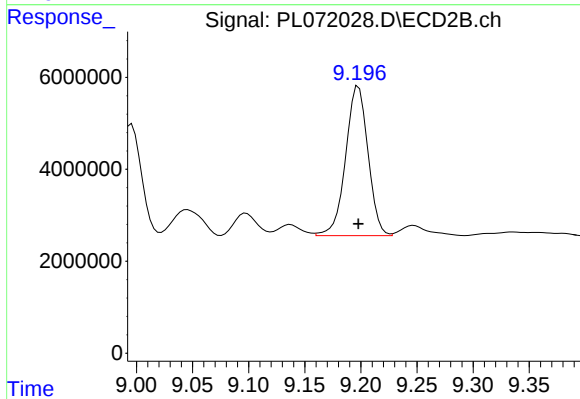

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 45161646
Conc: 738.04 ng/ml

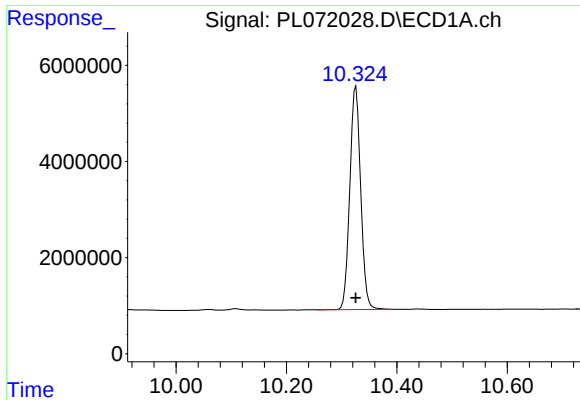

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 63468165
Conc: 73.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

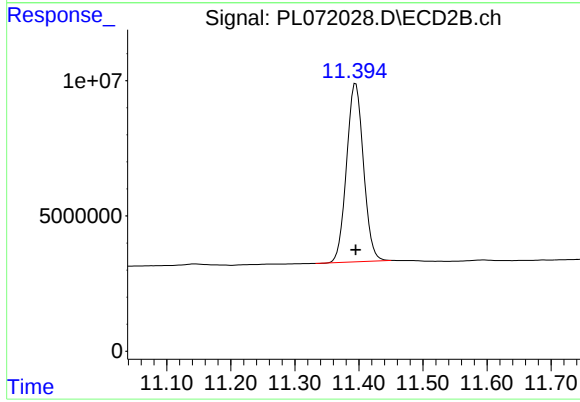

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.000 min
Response: 120867636
Conc: 74.13 ng/ml