

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
 Data File : PL072038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 17:54
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL011722CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:19:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 00:18:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	30300654	84006896	49.768	50.619
28)	SA Decachlor...	10.325	11.394	44676214	84592068	49.116	50.635
Target Compounds							
23)	Chlordane-1	5.884	6.877	10593099	33100296	513.541	507.218
24)	Chlordane-2	6.574	7.471	13924128	35546002	505.635	508.568
25)	Chlordane-3	7.275	8.229	38952116	141.7E6	509.120	510.098
26)	Chlordane-4	7.343	8.310	41699532	169.1E6	505.425	509.248
27)	Chlordane-5	8.293	9.197	14450207	30940757	495.828	507.075



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011722\
Data File : PL072038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 17:54
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL011722CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:19:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 00:18:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

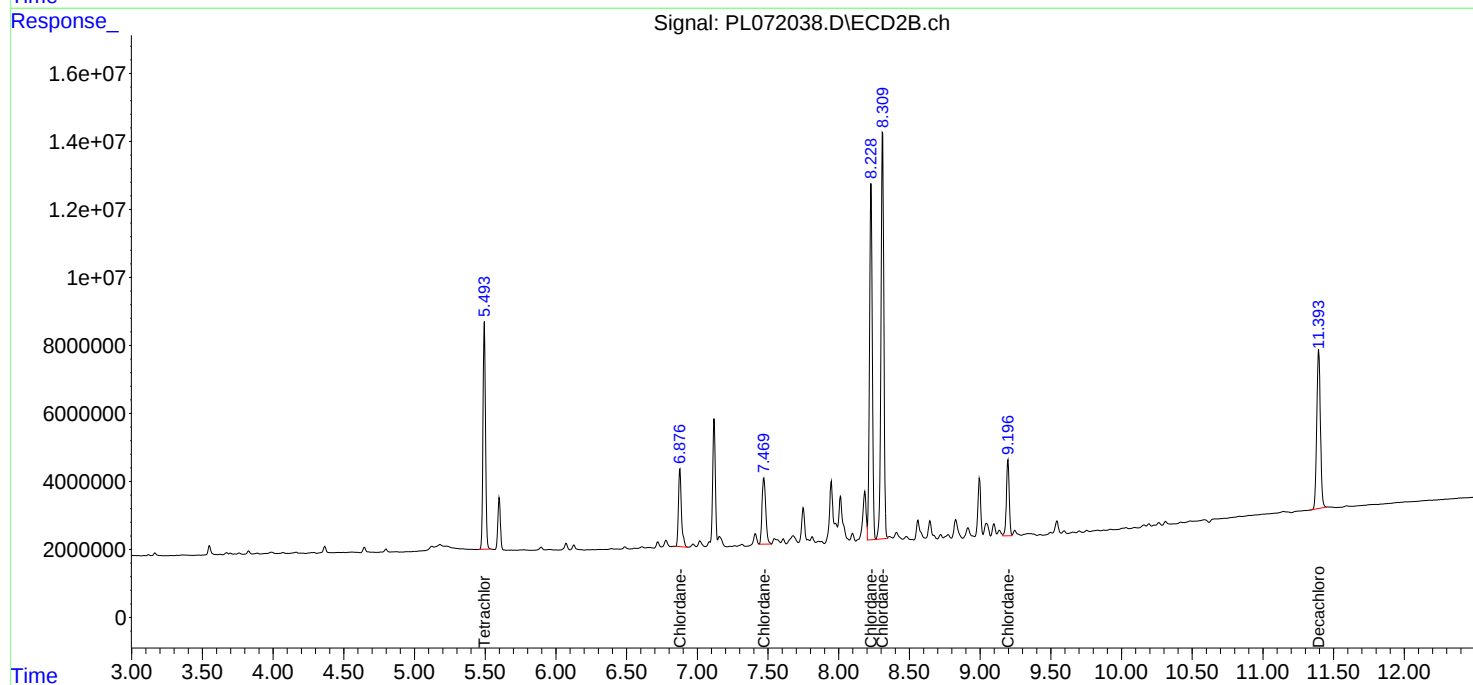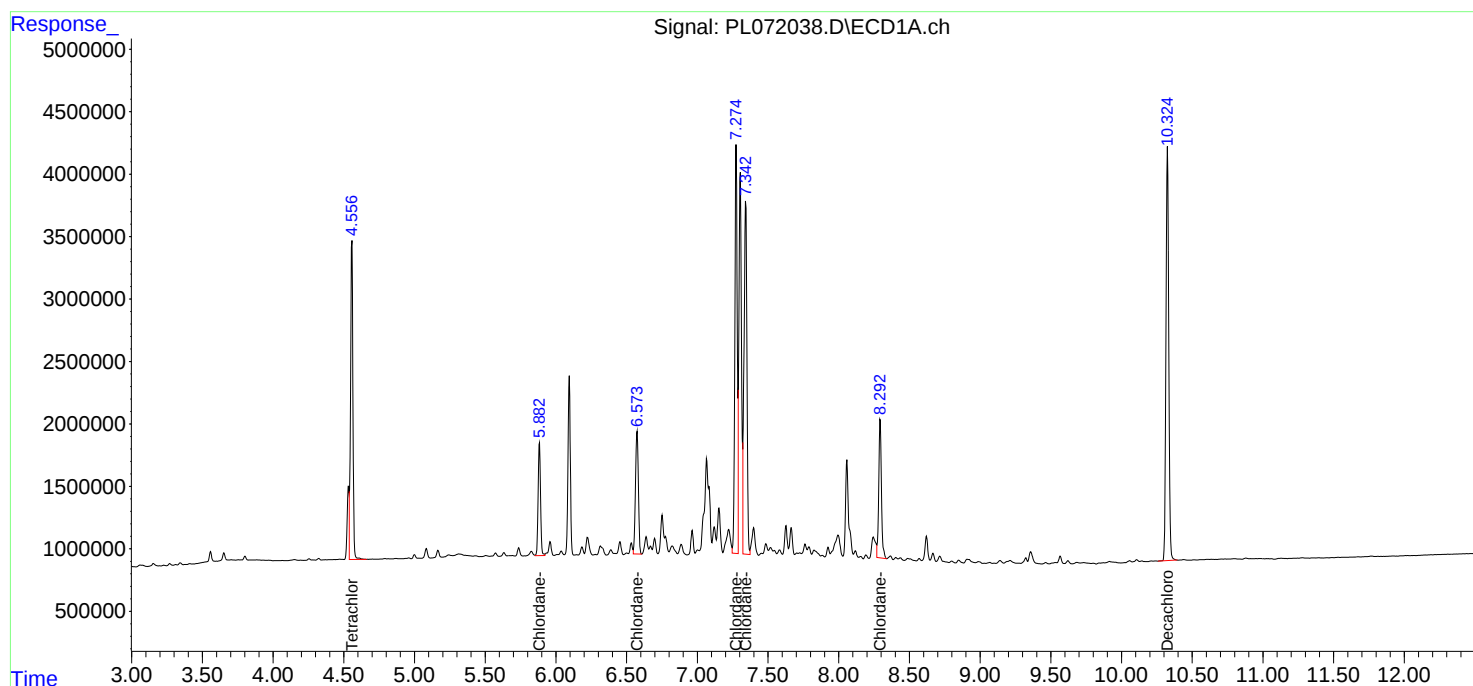


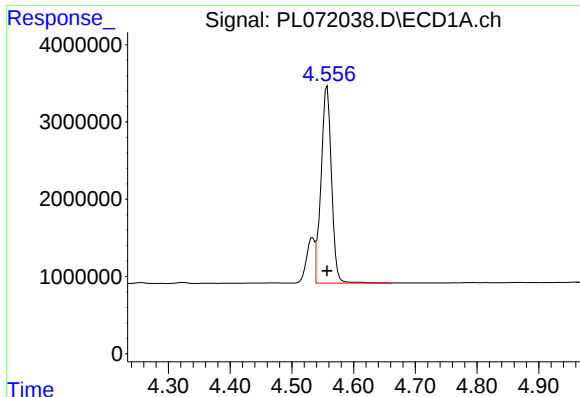

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 30300654
Conc: 49.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011722CHLOR

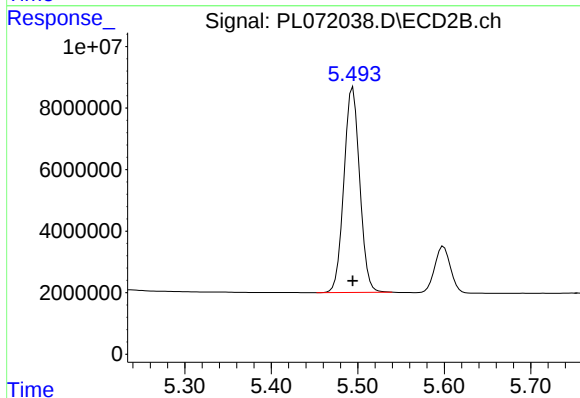


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 84006896
Conc: 50.62 ng/ml

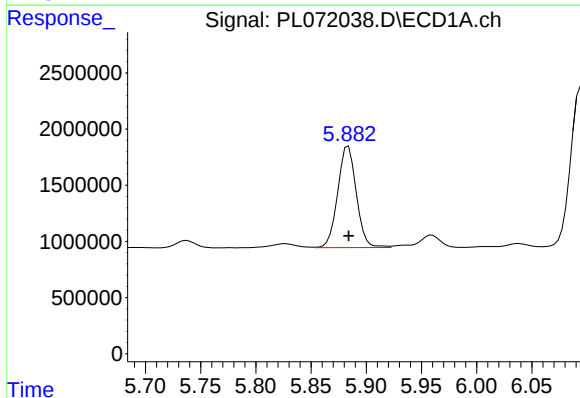


#23 Chlordane-1

R.T.: 5.884 min
Delta R.T.: 0.000 min
Response: 10593099
Conc: 513.54 ng/ml

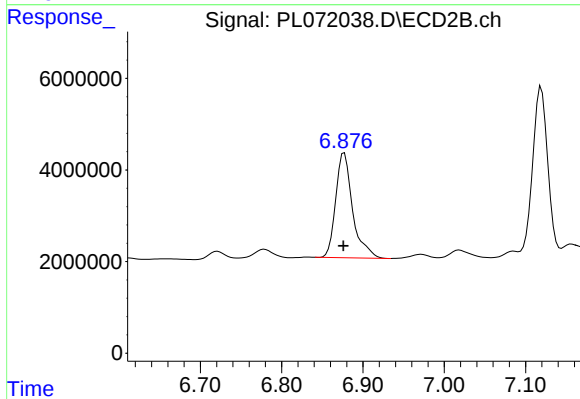

#23 Chlordane-1


R.T.: 6.877 min
Delta R.T.: 0.001 min
Response: 33100296
Conc: 507.22 ng/ml

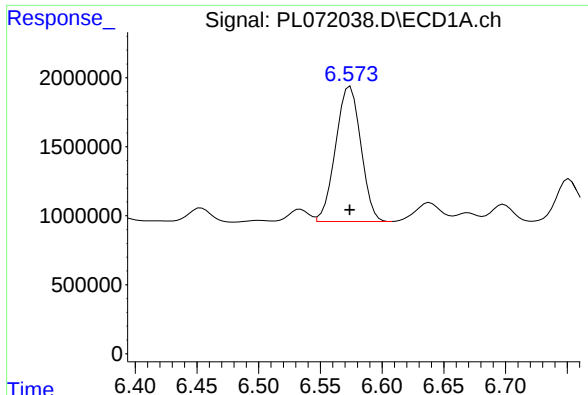

#24 Chlordane-2


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 13924128
Conc: 505.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011722CHLOR

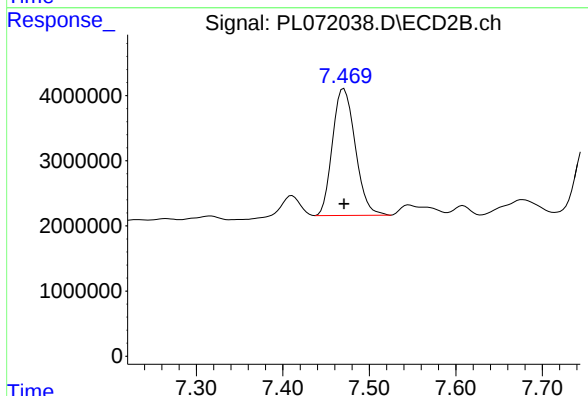


#24 Chlordane-2

R.T.: 7.471 min
Delta R.T.: 0.000 min
Response: 35546002
Conc: 508.57 ng/ml

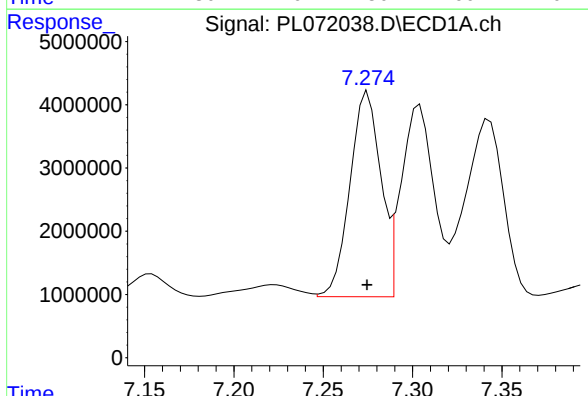


#25 Chlordane-3

R.T.: 7.275 min
Delta R.T.: 0.000 min
Response: 38952116
Conc: 509.12 ng/ml

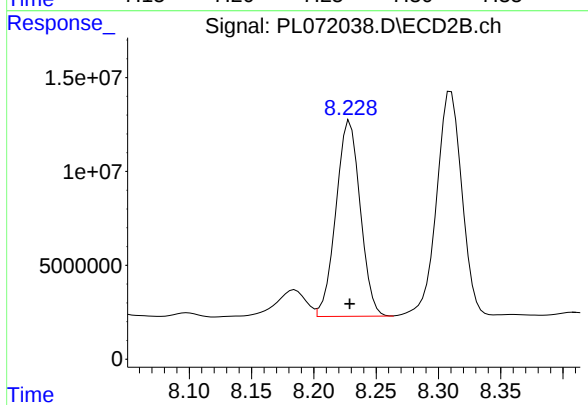

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 141722060
Conc: 510.10 ng/ml

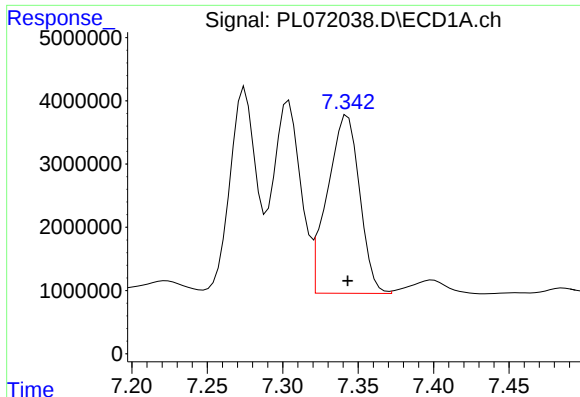

#26 Chlordane-4


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 41699532
Conc: 505.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011722CHLOR

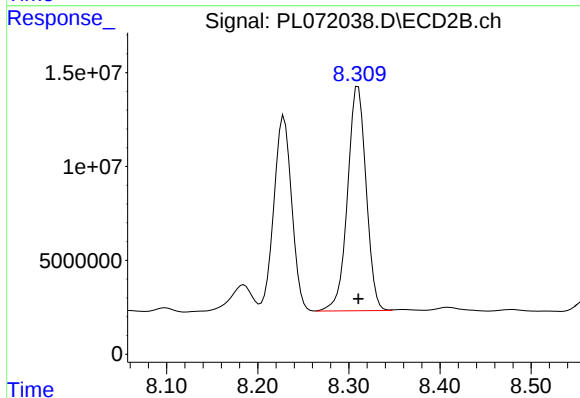


#26 Chlordane-4

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 169106231
Conc: 509.25 ng/ml

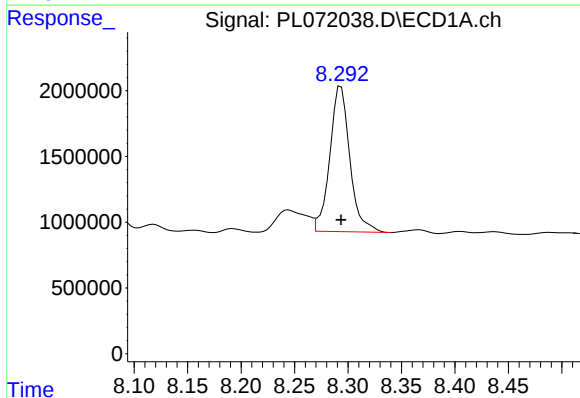


#27 Chlordane-5

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 14450207
Conc: 495.83 ng/ml

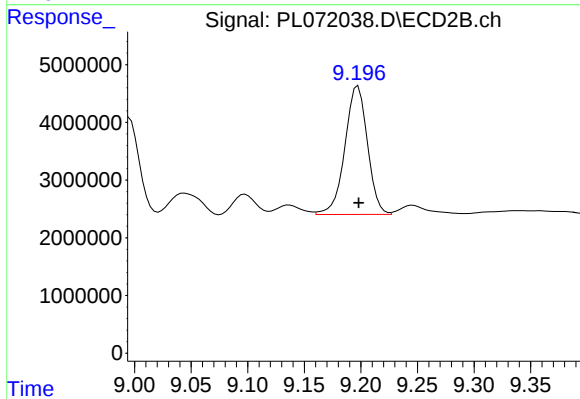

#27 Chlordane-5


R.T.: 9.197 min
Delta R.T.: 0.000 min
Response: 30940757
Conc: 507.07 ng/ml

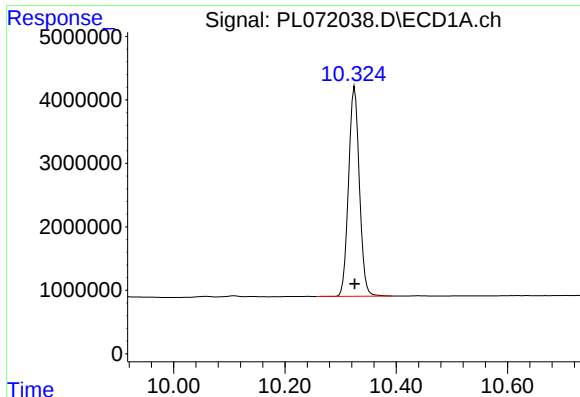

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: 0.000 min
Response: 44676214
Conc: 49.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011722CHLOR

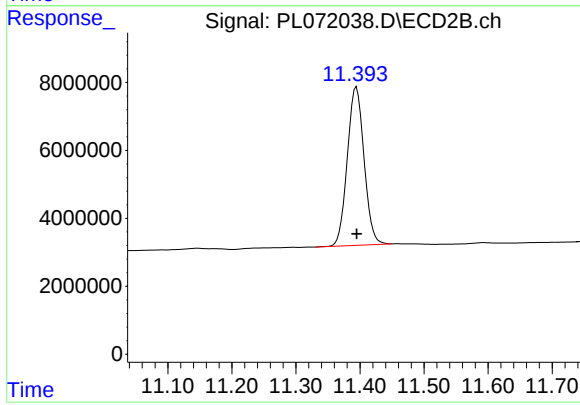

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.000 min
Response: 84592068
Conc: 50.63 ng/ml